

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
 Data File : VX029888.D
 Acq On : 30 Jun 2022 02:54
 Operator : JC/MD
 Sample : N3481-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-21R

Quant Time: Jun 30 06:27:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 05:54:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	232174	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	403314	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	347750	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	145648	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	129270	43.985	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	87.980%
35) Dibromofluoromethane	5.391	113	115657	45.887	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.780%
50) Toluene-d8	8.653	98	457733	48.409	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	96.820%
62) 4-Bromofluorobenzene	11.085	95	152592	45.653	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.300%
Target Compounds						
					Qvalue	
16) Acetone	2.386	43	6199	4.311	ug/l	96
44) Trichloroethene	7.141	130	795	0.272	ug/l	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029888.D
Acq On : 30 Jun 2022 02:54
Operator : JC/MD
Sample : N3481-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-21R

Quant Time: Jun 30 06:27:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 05:54:51 2022
Response via : Initial Calibration




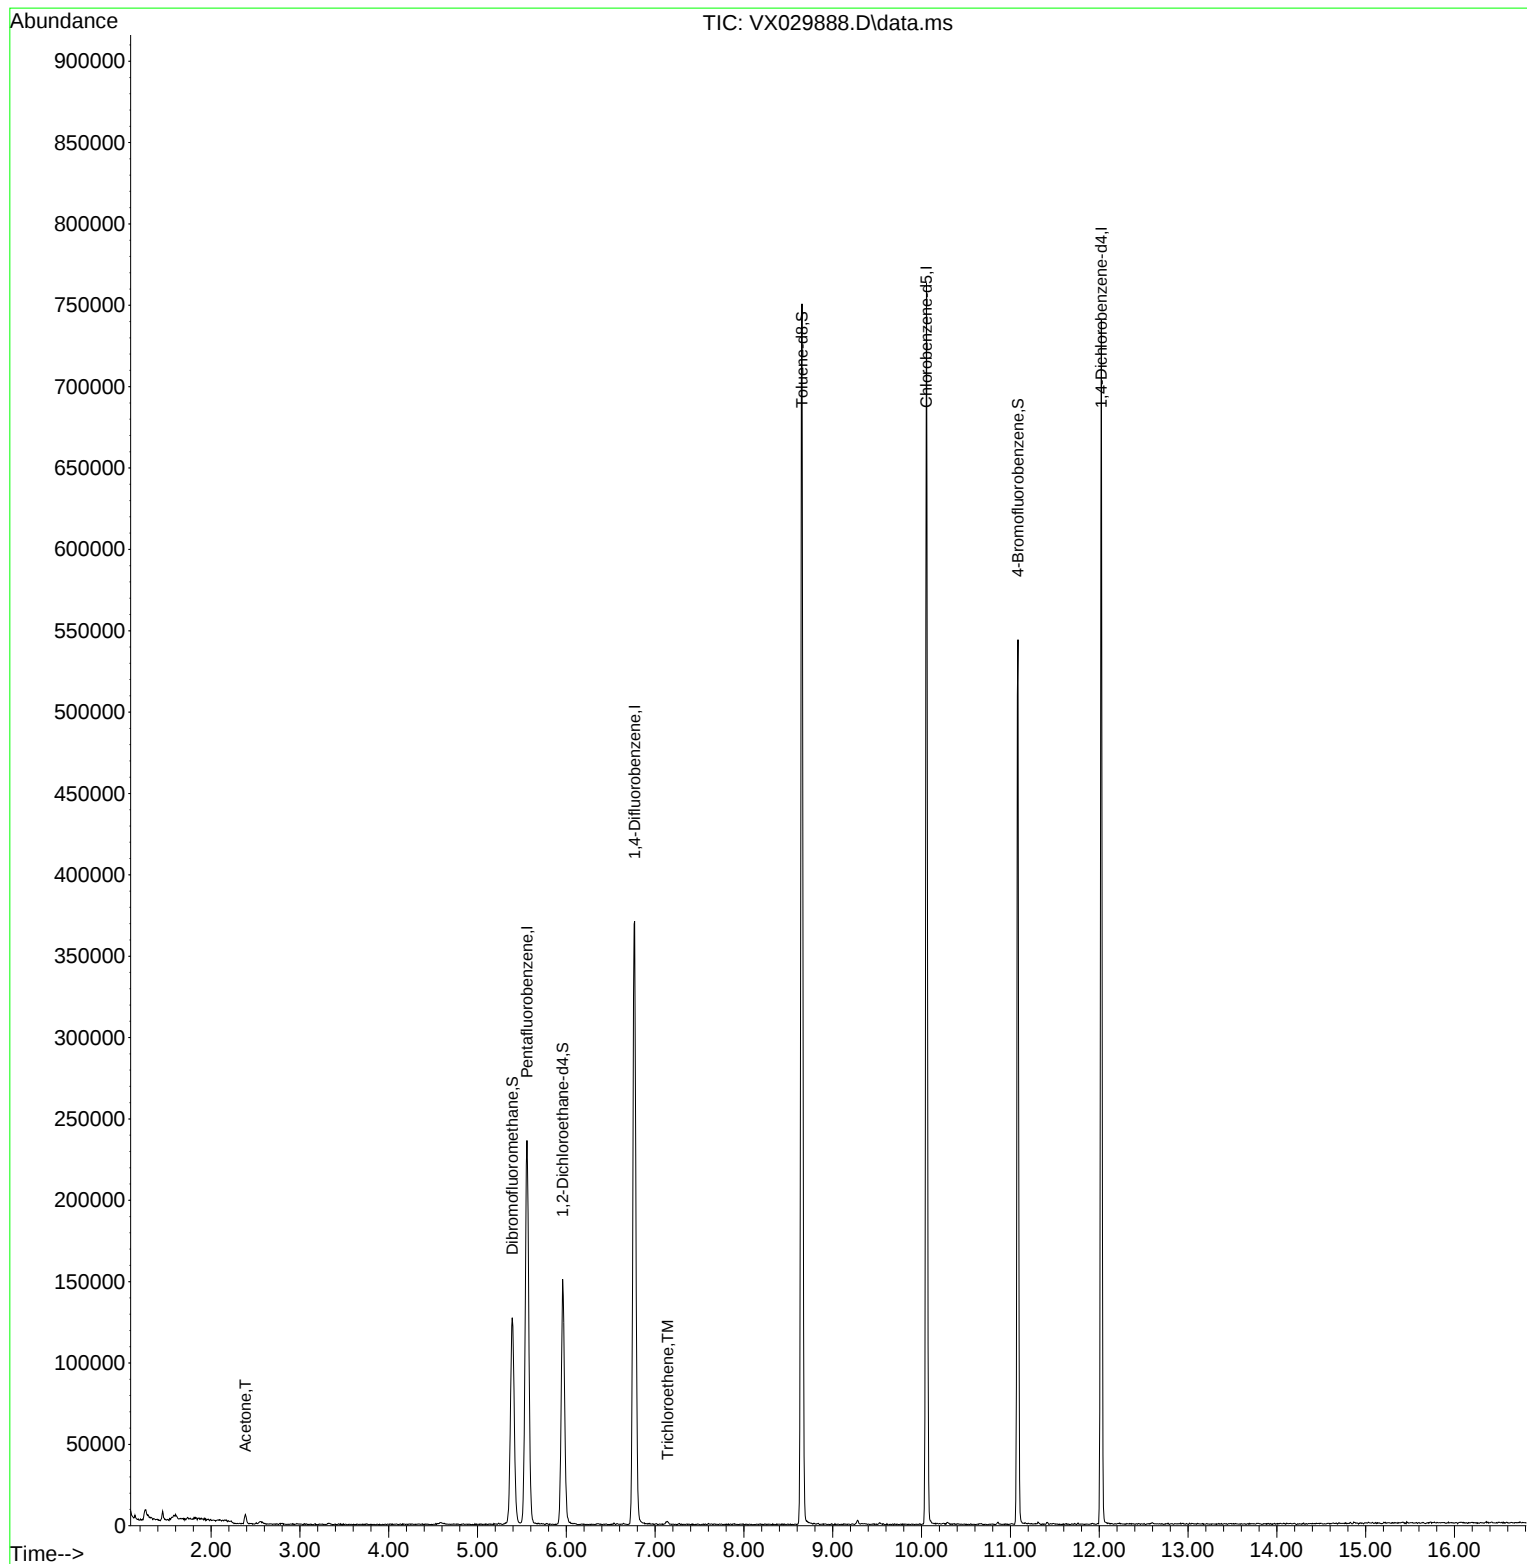




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029888.D
Acq: 30 Jun 2022 02:54




Instrument :
MSVOA_X
ClientSampleId :
MW-21R


Tgt Ion:168 Resp: 232174
Ion Ratio Lower Upper
168 100
99 54.5 44.0 66.0

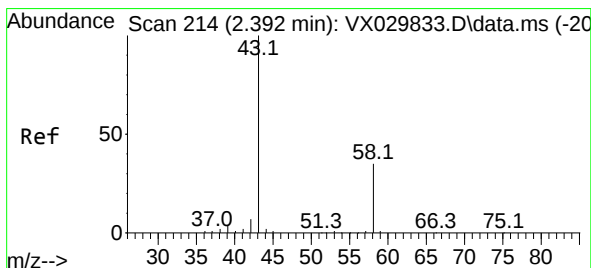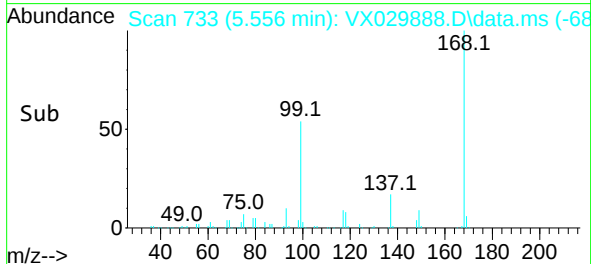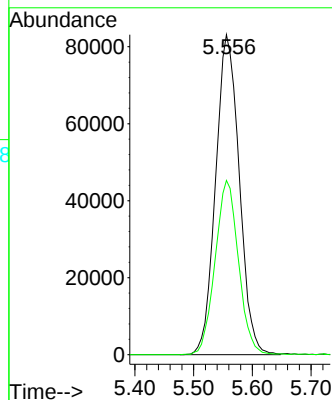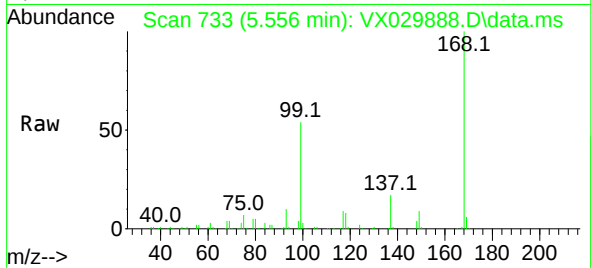

#16
Acetone
Concen: 4.311 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX029888.D
Acq: 30 Jun 2022 02:54

Tgt Ion: 43 Resp: 6199
Ion Ratio Lower Upper
43 100
58 36.8 27.7 41.5

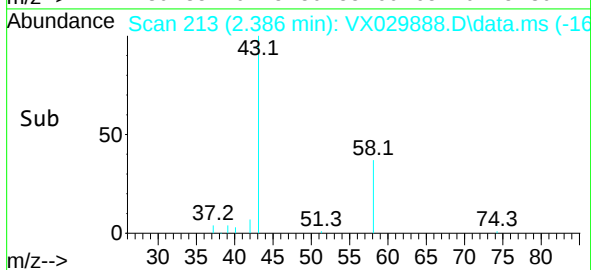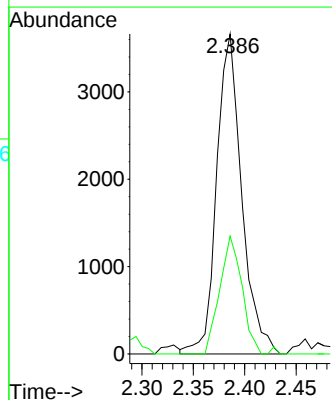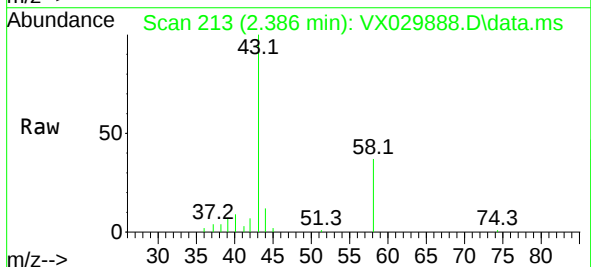

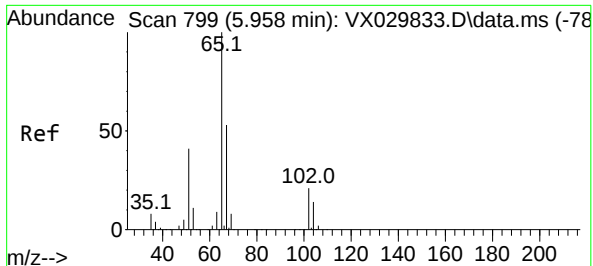

#33

1,2-Dichloroethane-d4

Concen: 43.985 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029888.D

Acq: 30 Jun 2022 02:54

Instrument :

MSVOA_X

ClientSampleId :





MW-21R

Tgt Ion: 65 Resp: 129270

Ion Ratio Lower Upper

65 100

67 56.3 0.0 109.6

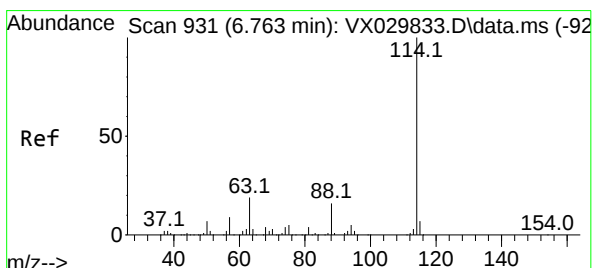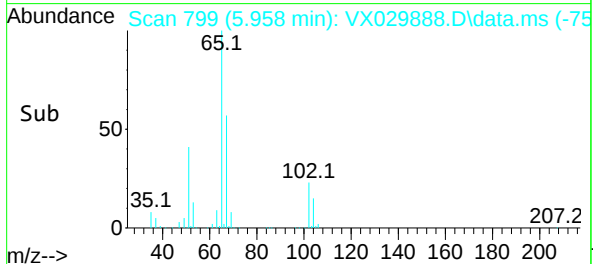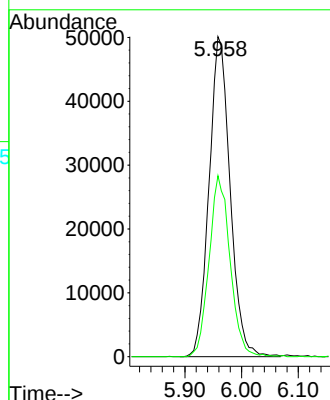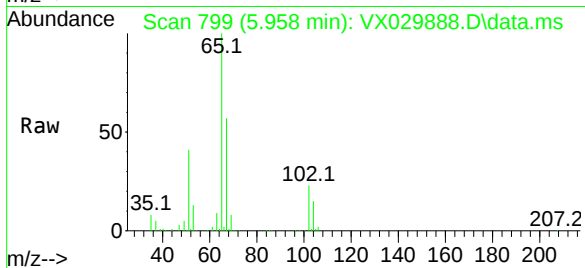

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.006 min

Lab File: VX029888.D

Acq: 30 Jun 2022 02:54




Tgt Ion: 114 Resp: 403314


Ion Ratio Lower Upper

114 100

63 18.8 0.0 38.4

88 14.5 0.0 31.8


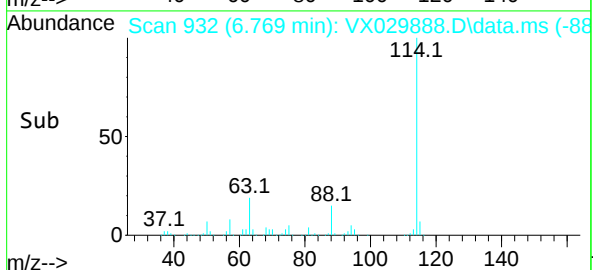
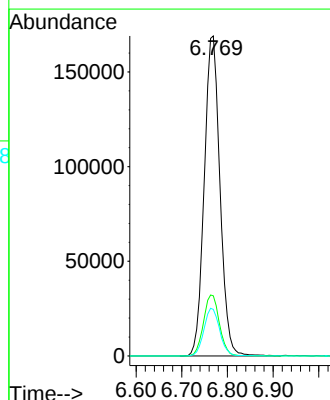
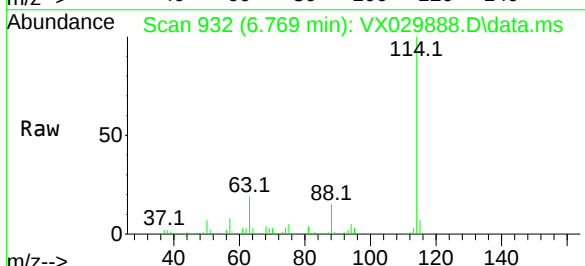


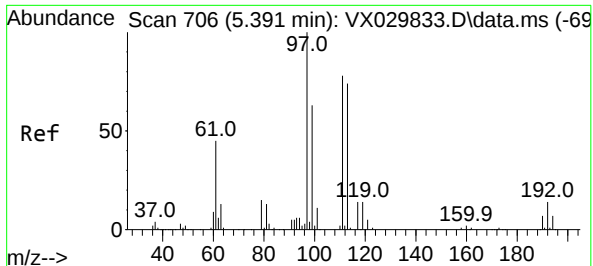

#35
Dibromofluoromethane
Concen: 45.887 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX029888.D
Acq: 30 Jun 2022 02:54




Instrument :
MSVOA_X
ClientSampleId :
MW-21R


Tgt Ion:113 Resp: 115657
Ion Ratio Lower Upper
113 100
111 102.1 83.2 124.8
192 18.9 14.8 22.2

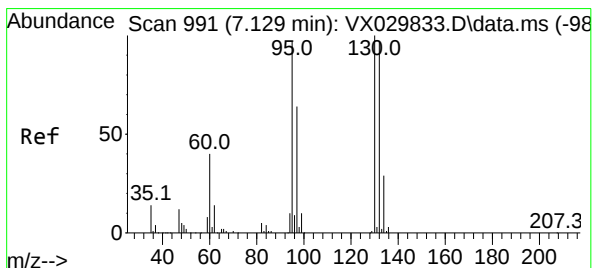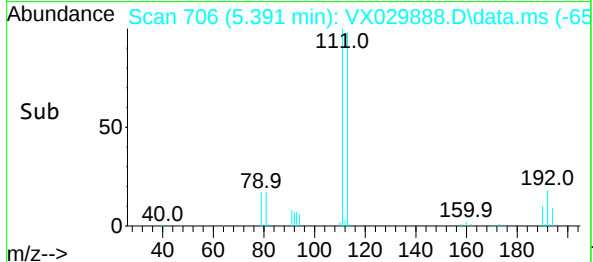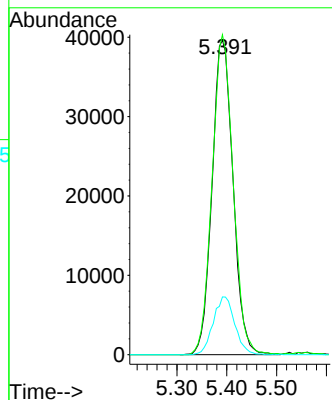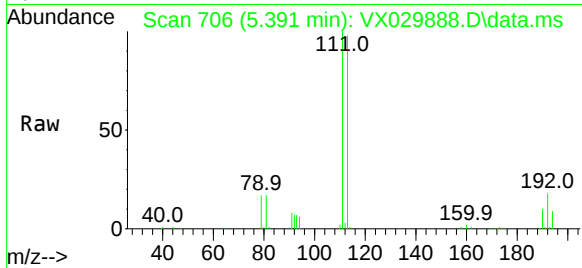

#44
Trichloroethene
Concen: 0.272 ug/l
RT: 7.141 min Scan# 993
Delta R.T. 0.012 min
Lab File: VX029888.D
Acq: 30 Jun 2022 02:54

Tgt Ion:130 Resp: 795
Ion Ratio Lower Upper
130 100
95 81.1 0.0 194.8


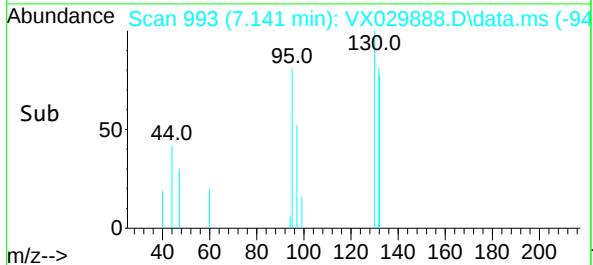
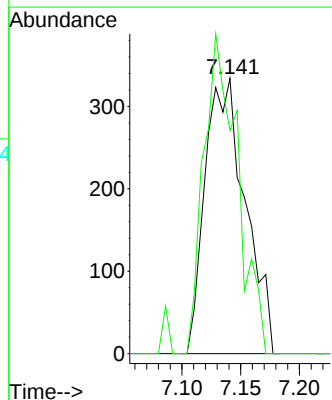
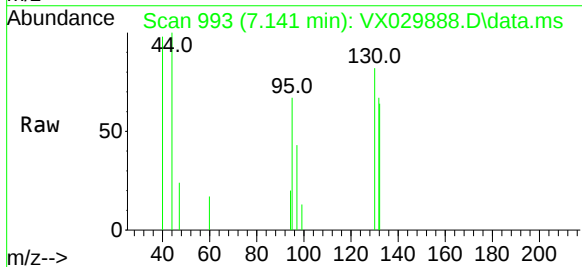


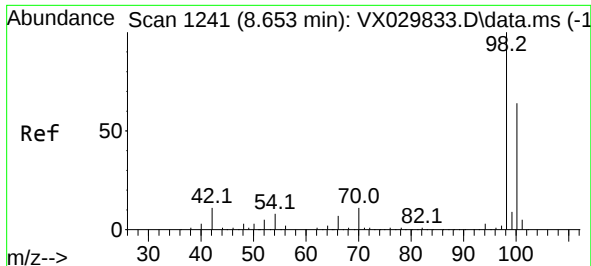

#50
Toluene-d8
Concen: 48.409 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX029888.D
Acq: 30 Jun 2022 02:54




Instrument :
MSVOA_X
ClientSampleId :
MW-21R


Tgt Ion: 98 Resp: 457733
Ion Ratio Lower Upper
98 100
100 65.9 52.3 78.5

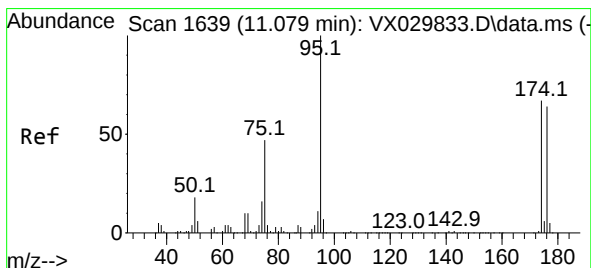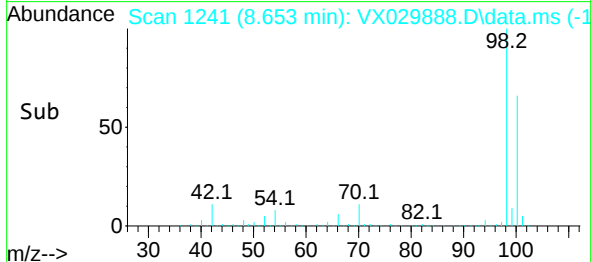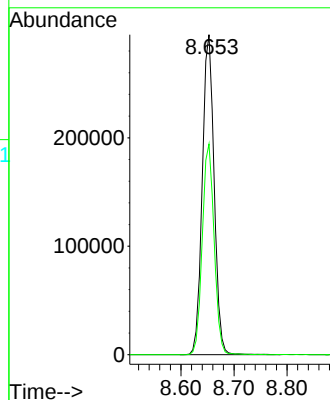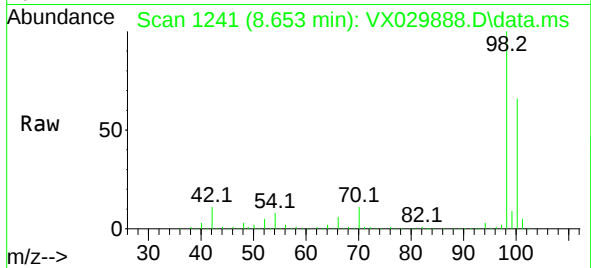

#62
4-Bromofluorobenzene
Concen: 45.653 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX029888.D
Acq: 30 Jun 2022 02:54

Tgt Ion: 95 Resp: 152592
Ion Ratio Lower Upper
95 100
174 74.6 0.0 149.0
176 71.3 0.0 146.0


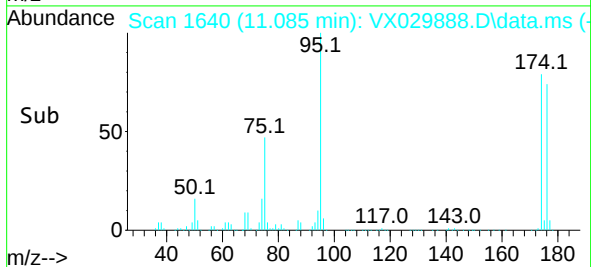
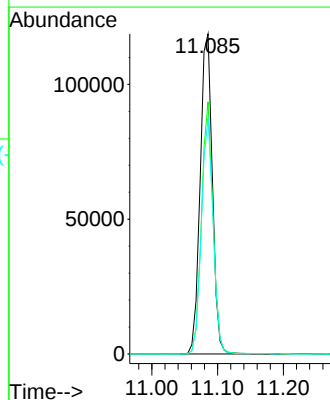
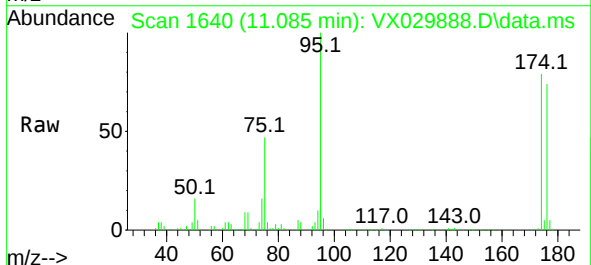


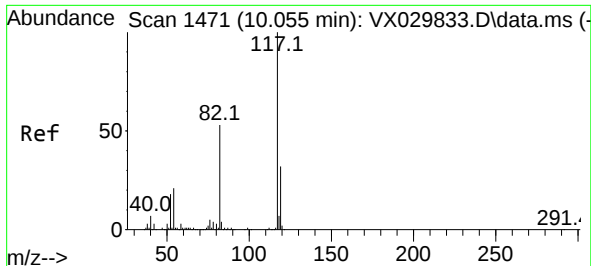

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX029888.D
Acq: 30 Jun 2022 02:54

Instrument :
MSVOA_X
ClientSampleId :
MW-21R

Tgt Ion:117 Resp: 347750
Ion Ratio Lower Upper
117 100
82 52.7 42.7 64.1
119 31.2 25.4 38.2

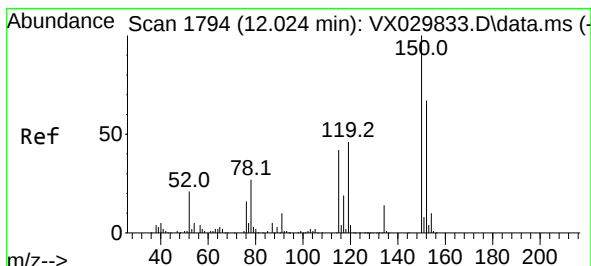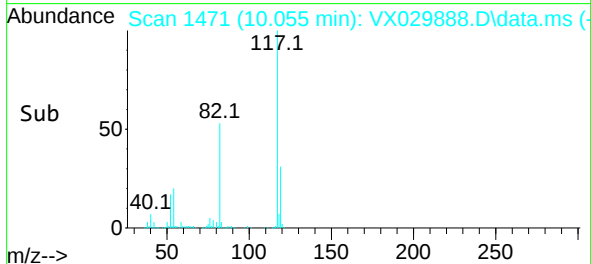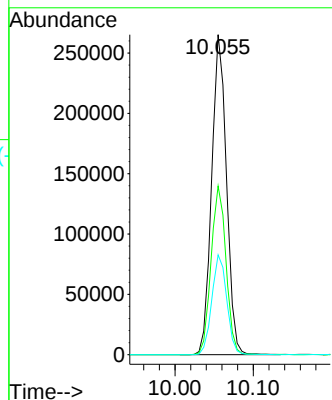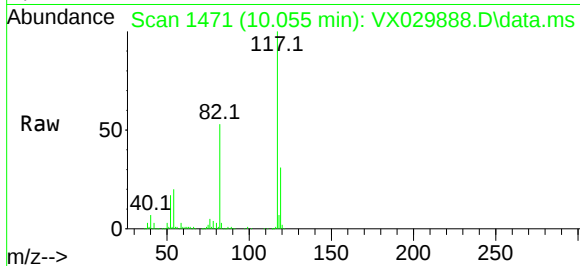

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX029888.D
Acq: 30 Jun 2022 02:54

Tgt Ion:152 Resp: 145648
Ion Ratio Lower Upper
152 100
115 59.8 40.5 121.5
150 159.7 0.0 347.0

