

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
 Data File : VX029872.D
 Acq On : 29 Jun 2022 19:13
 Operator : JC/MD
 Sample : N3485-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE120D3-20220623

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Title : SW846 8260

Signal : TIC: VX029872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	23	29	36	rBV3	6561	16050	1.38%	0.227%
2	2.331	194	204	210	rBV3	15362	30994	2.66%	0.438%
3	5.391	694	706	721	rVV2	123933	361124	30.98%	5.103%
4	5.556	722	733	748	rVB	228017	648664	55.64%	9.166%
5	5.964	788	800	815	rBV2	142803	380572	32.64%	5.378%
6	6.769	919	932	943	rBV	363145	873335	74.91%	12.341%
7	7.129	982	991	1001	rBV	496521	1048465	89.93%	14.815%
8	8.653	1232	1241	1252	rBV	741783	1165809	100.00%	16.474%
9	9.275	1336	1343	1348	rBV2	12077	20026	1.72%	0.283%
10	10.055	1465	1471	1481	rBV	727359	980410	84.10%	13.854%
11	11.085	1633	1640	1648	rBV	533238	693832	59.52%	9.804%
12	12.024	1788	1794	1804	rBV	703576	857592	73.56%	12.118%




Sum of corrected areas: 7076873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029872.D
Acq On : 29 Jun 2022 19:13
Operator : JC/MD
Sample : N3485-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20220623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

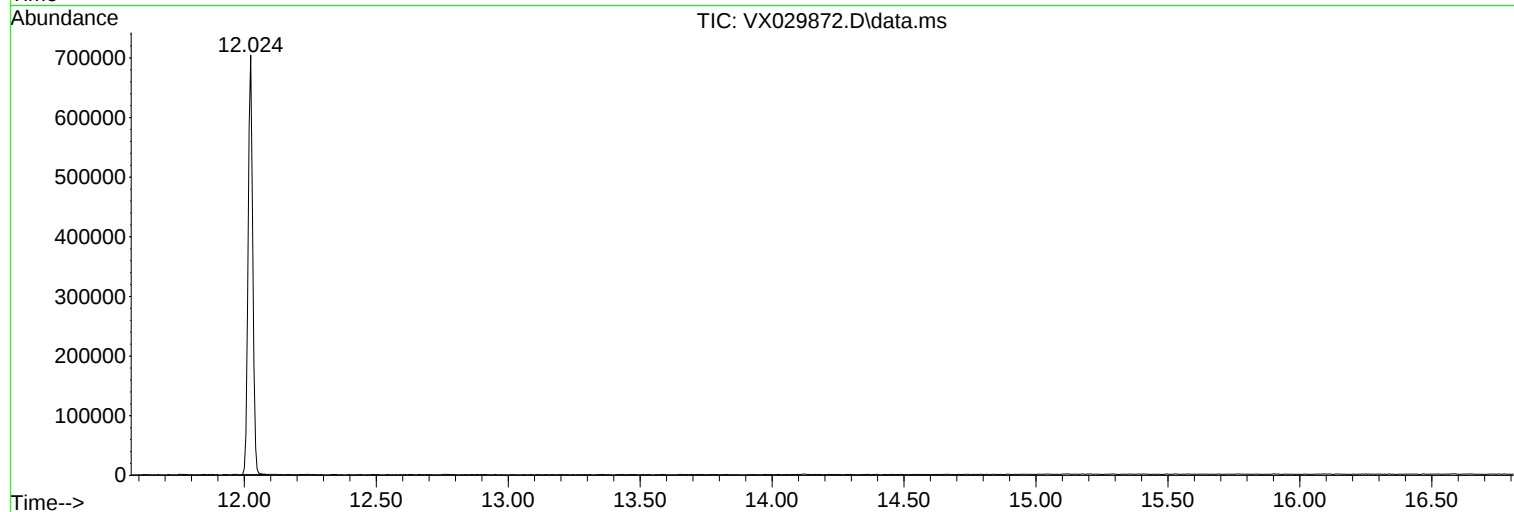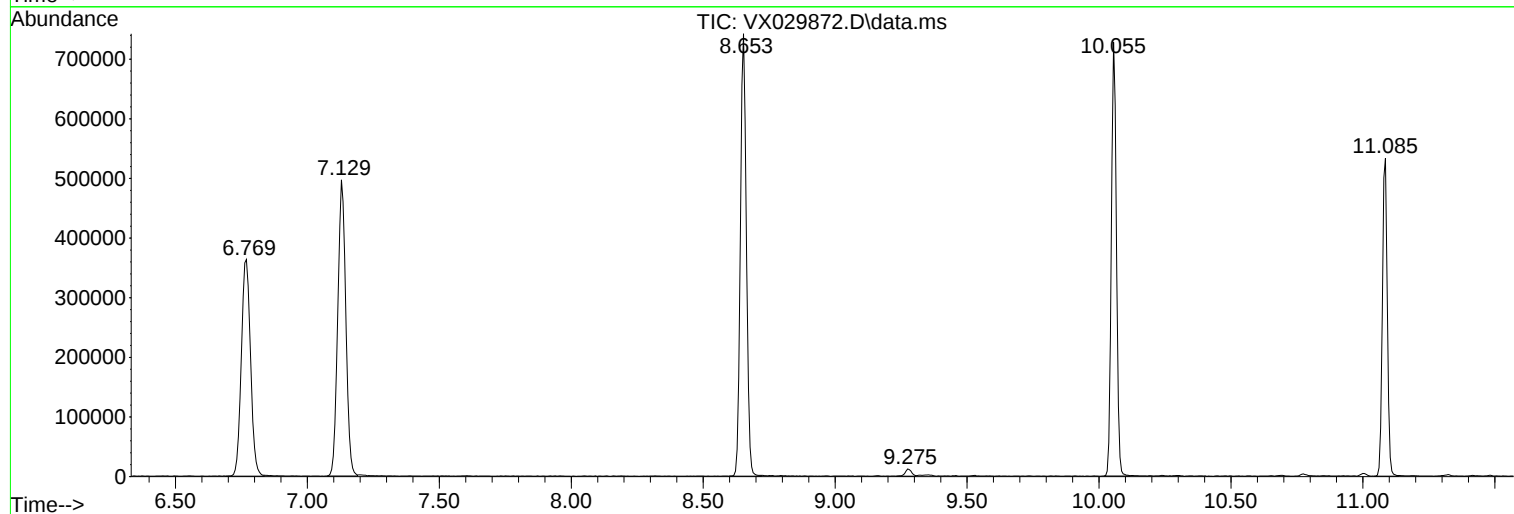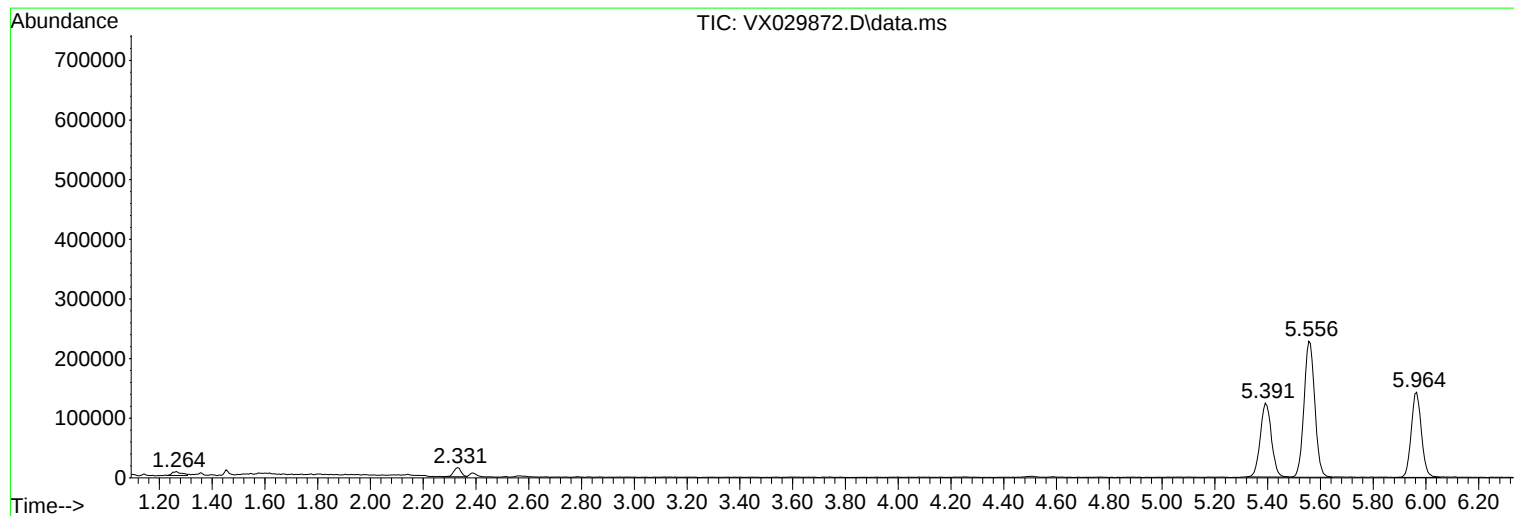

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029872.D
Acq On : 29 Jun 2022 19:13
Operator : JC/MD
Sample : N3485-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20220623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029872.D
Acq On : 29 Jun 2022 19:13
Operator : JC/MD
Sample : N3485-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20220623

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------