

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
 Data File : VX029895.D
 Acq On : 30 Jun 2022 05:37
 Operator : JC/MD
 Sample : N3481-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-28

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M

Title : SW846 8260

Signal : TIC: VX029895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	40	rBV	25658	56334	4.79%	0.888%
2	4.495	550	559	567	rBV2	13695	39325	3.34%	0.620%
3	5.391	692	706	722	rVB	127221	371007	31.53%	5.847%
4	5.556	722	733	746	rBV	230560	652541	55.46%	10.284%
5	5.964	786	800	816	rBV	143682	381829	32.45%	6.018%
6	6.763	920	931	946	rBV	366458	880535	74.84%	13.877%
7	7.129	983	991	1002	rBV3	12770	30288	2.57%	0.477%
8	8.653	1233	1241	1252	rBV	751035	1176562	100.00%	18.543%
9	9.275	1335	1343	1351	rBV	120275	177236	15.06%	2.793%
10	10.055	1465	1471	1484	rBV	740850	1000488	85.03%	15.768%
11	11.085	1634	1640	1648	rBV	533749	702203	59.68%	11.067%
12	12.024	1788	1794	1806	rBV	717486	876771	74.52%	13.818%




Sum of corrected areas: 6345119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029895.D
Acq On : 30 Jun 2022 05:37
Operator : JC/MD
Sample : N3481-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

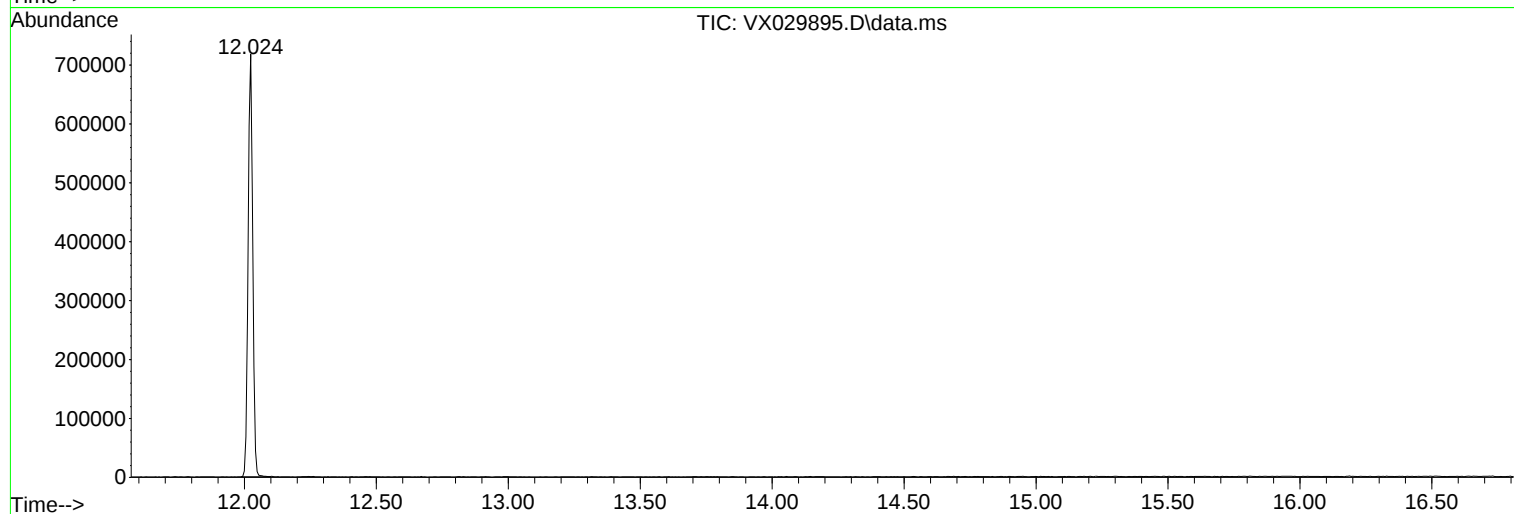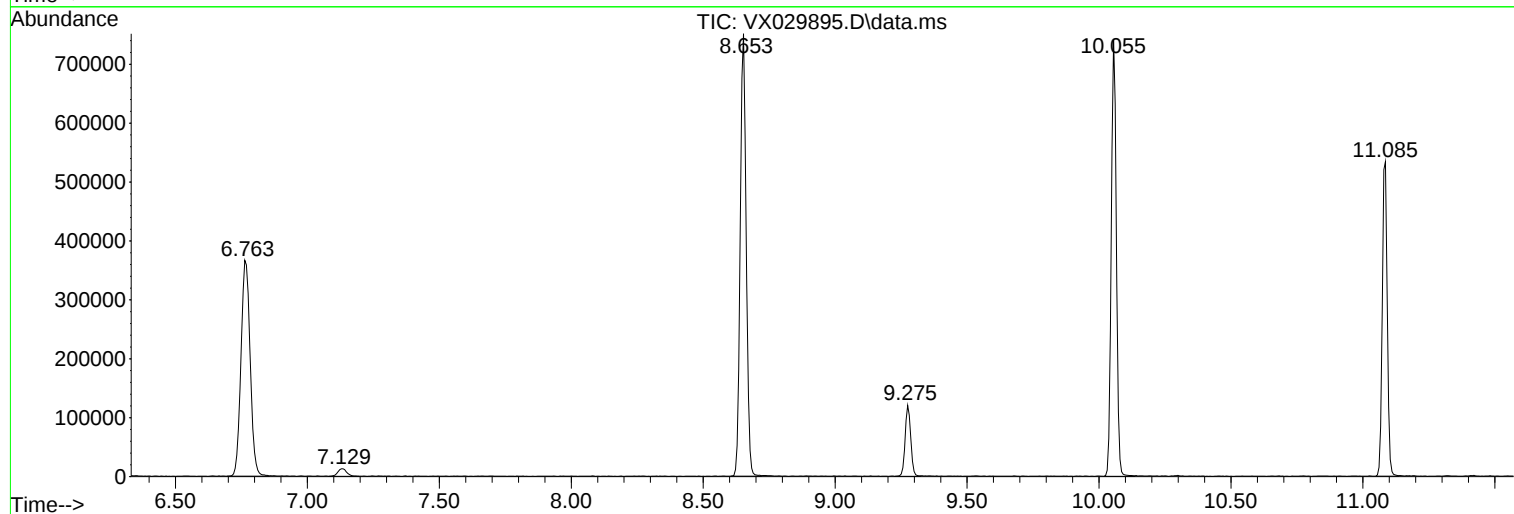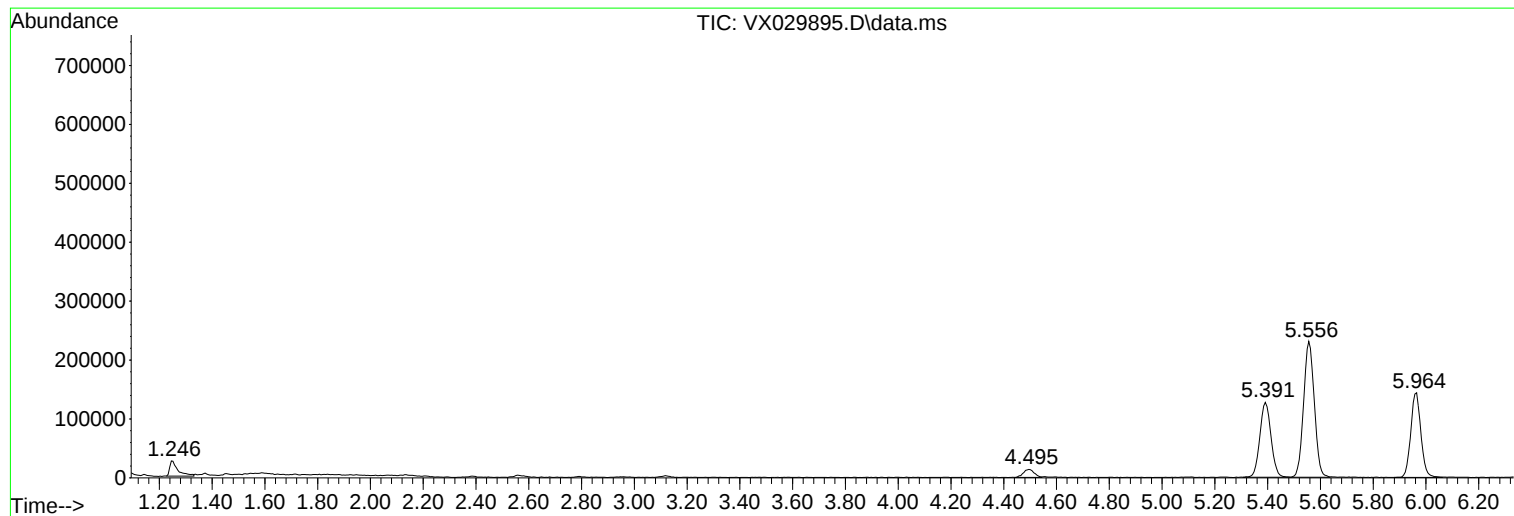

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029895.D
Acq On : 30 Jun 2022 05:37
Operator : JC/MD
Sample : N3481-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029895.D
Acq On : 30 Jun 2022 05:37
Operator : JC/MD
Sample : N3481-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc