


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029847.D
Acq On : 29 Jun 2022 08:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 05:54:51 2022

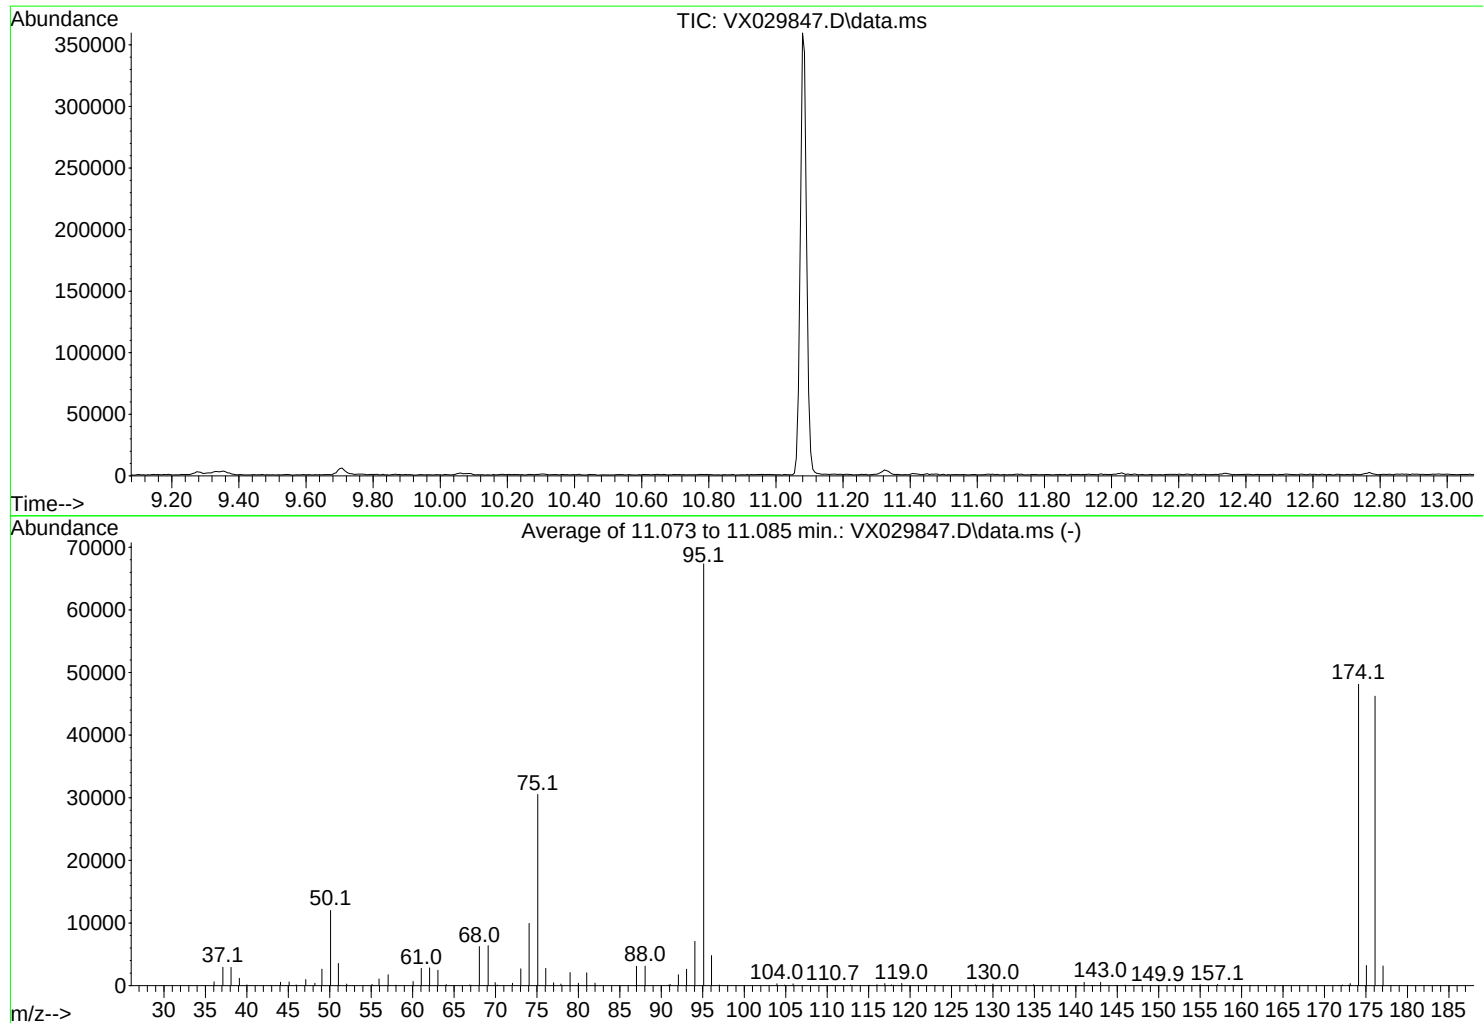

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	12020	PASS
75	95	30	60	45.3	30525	PASS
95	95	100	100	100.0	67352	PASS
96	95	5	9	7.1	4797	PASS
173	174	0.00	2	0.7	337	PASS
174	95	50	100	71.5	48141	PASS
175	174	5	9	6.7	3228	PASS
176	174	95	101	96.0	46229	PASS
177	176	5	9	6.8	3159	PASS