
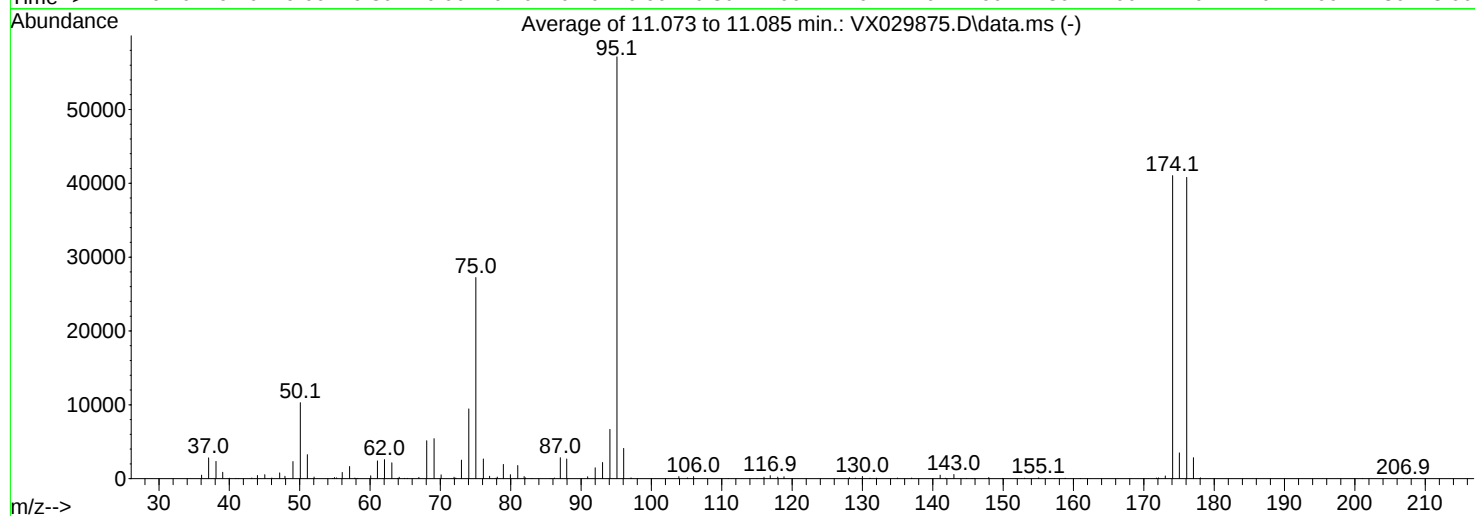


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062922\
Data File : VX029875.D
Acq On : 29 Jun 2022 20:58
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 05:54:51 2022

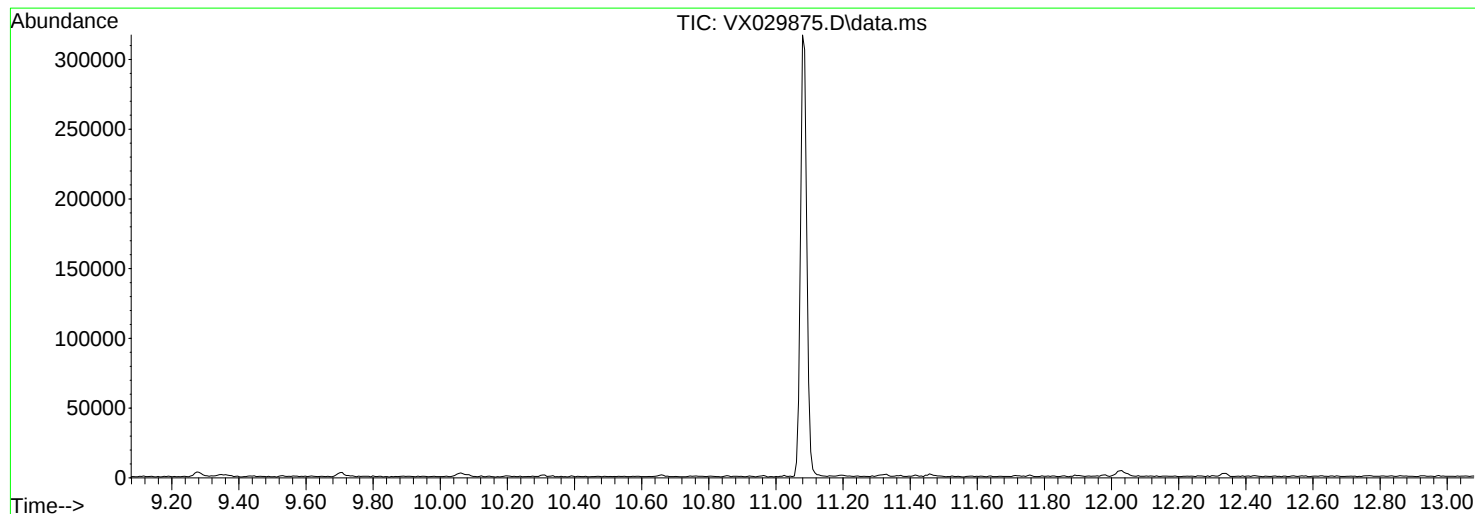

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	10300	PASS
75	95	30	60	47.7	27240	PASS
95	95	100	100	100.0	57125	PASS
96	95	5	9	7.2	4089	PASS
173	174	0.00	2	0.9	369	PASS
174	95	50	100	71.8	41032	PASS
175	174	5	9	8.5	3499	PASS
176	174	95	101	99.5	40811	PASS
177	176	5	9	6.9	2830	PASS