

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062923\
 Data File : VX036371.D
 Acq On : 29 Jun 2023 12:26
 Operator : JC/MD
 Sample : 03451-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Title : SW846 8260

Signal : TIC: VX036371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	41	47	58	rBV	32739	41444	2.85%	0.463%
2	1.746	105	108	116	rVB	11059	17149	1.18%	0.191%
3	2.337	199	205	211	rBV	13050	27837	1.91%	0.311%
4	2.782	269	278	287	rBV	49933	105221	7.23%	1.174%
5	3.099	320	330	342	rVB3	13453	31694	2.18%	0.354%
6	4.489	540	558	574	rBV	192823	534106	36.69%	5.961%
7	5.385	693	705	720	rBV	172704	492751	33.85%	5.499%
8	5.550	720	732	752	rVB	303899	859175	59.02%	9.589%
9	5.952	788	798	811	rBV	188541	496120	34.08%	5.537%
10	6.251	838	847	859	rVB3	5144	15055	1.03%	0.168%
11	6.757	919	930	943	rBV	459328	1095632	75.26%	12.228%
12	7.123	979	990	1001	rBV	47634	103375	7.10%	1.154%
13	8.104	1144	1151	1158	rBV2	14269	28445	1.95%	0.317%
14	8.647	1233	1240	1251	rBV	951253	1455702	100.00%	16.246%
15	9.275	1337	1343	1351	rBV	178550	259604	17.83%	2.897%
16	10.055	1465	1471	1481	rBV	924862	1262878	86.75%	14.094%
17	11.079	1634	1639	1651	rBV	790230	967117	66.44%	10.793%
18	12.018	1788	1793	1803	rBV	924363	1167017	80.17%	13.024%




Sum of corrected areas: 8960322

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062923\
Data File : VX036371.D
Acq On : 29 Jun 2023 12:26
Operator : JC/MD
Sample : 03451-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

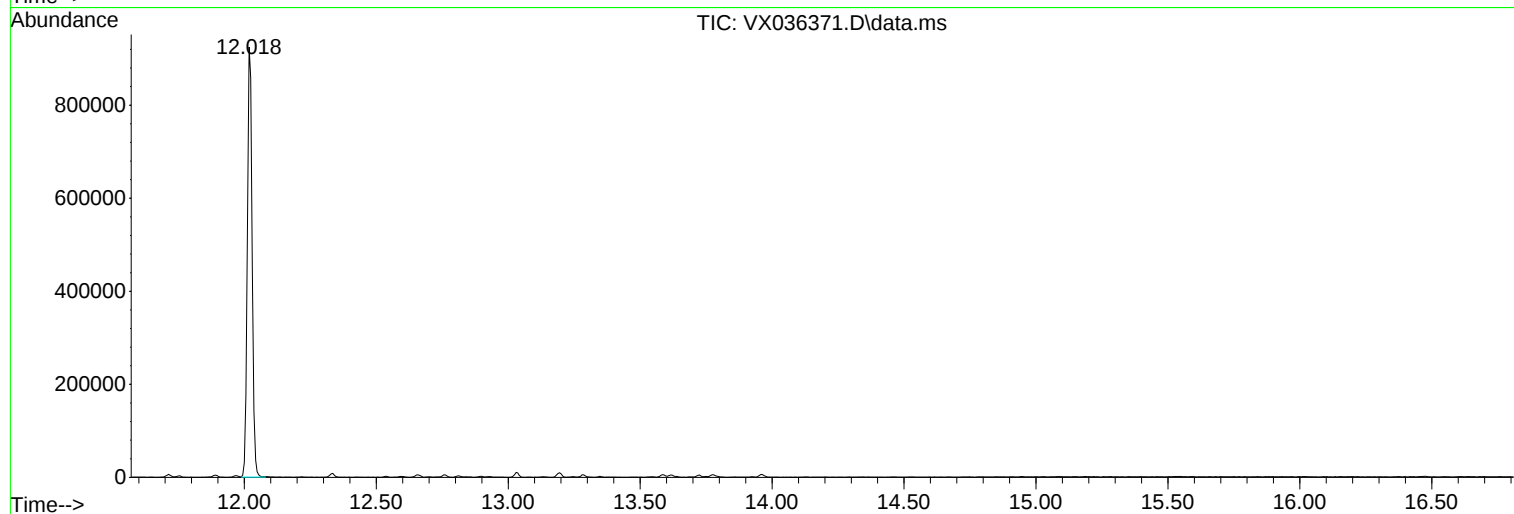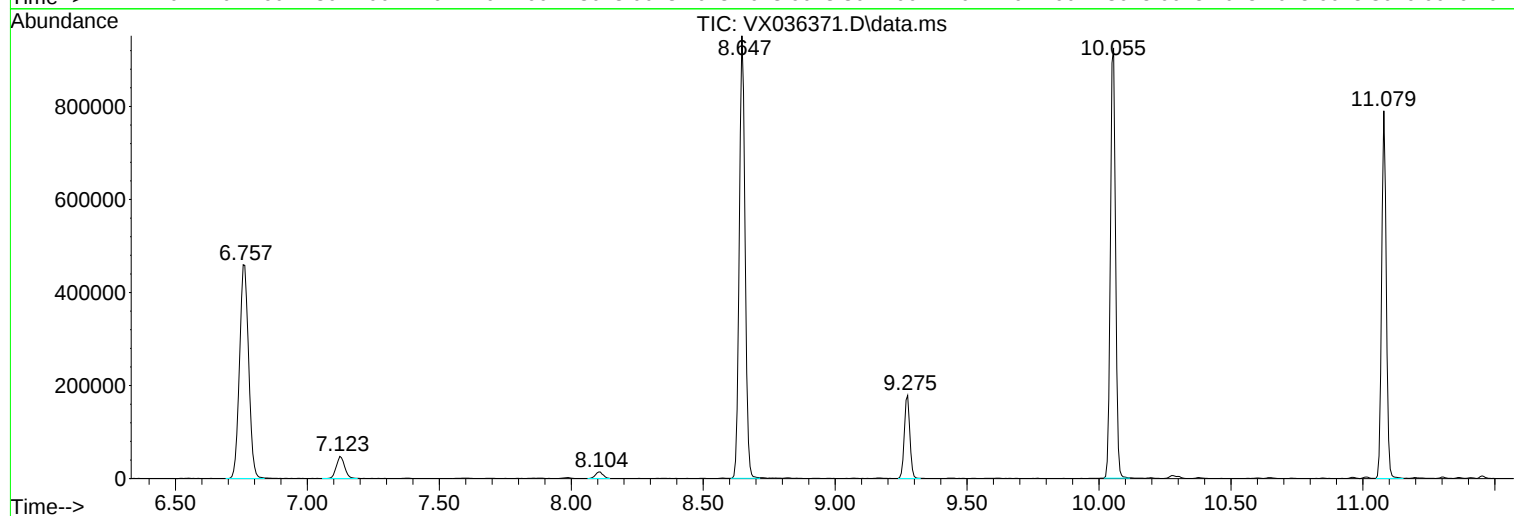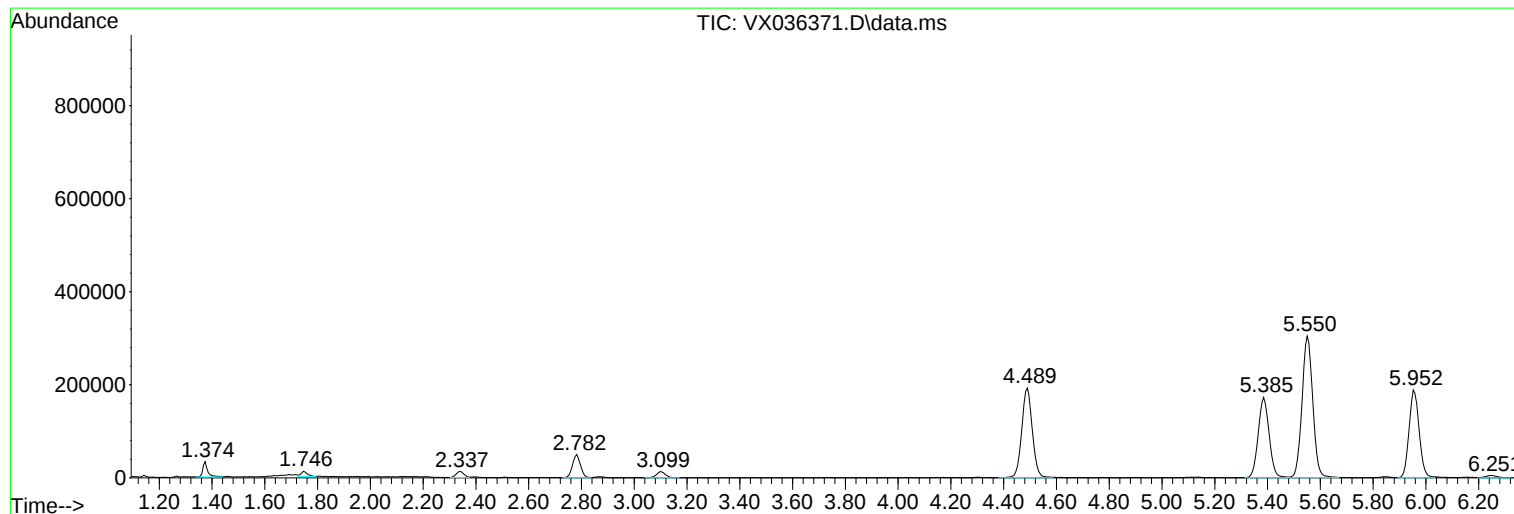

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062923\
Data File : VX036371.D
Acq On : 29 Jun 2023 12:26
Operator : JC/MD
Sample : 03451-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2,3-dimethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.782	6.12 ug/l	105221	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2,3-dimethyl-	86	C6H14	000079-29-8	86
2			Pentane, 2-methyl-	86	C6H14	000107-83-5	50
3			Pentane	72	C5H12	000109-66-0	38
4			Hydroxylamine, O-(3-methylbutyl)-	103	C5H13NO	019411-65-5	10
5			Butanal, 2,2-dimethyl-	100	C6H12O	002094-75-9	10

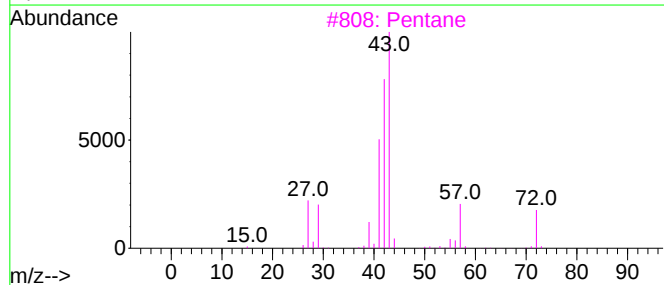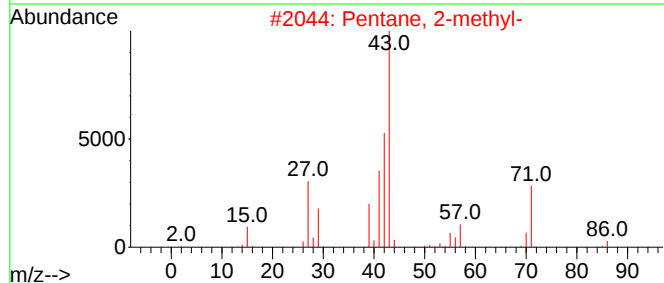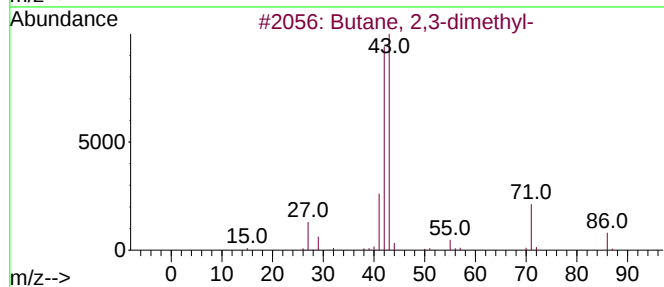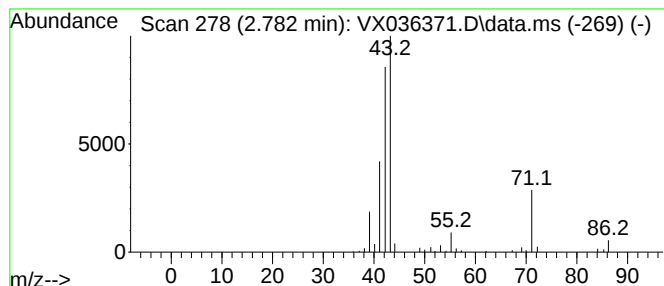

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062923\
Data File : VX036371.D
Acq On : 29 Jun 2023 12:26
Operator : JC/MD
Sample : 03451-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2,3-dim...	2.782	6.1	ug/l	105221	1	5.550	859175	50.0