


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX062923\
Data File : VX036365.D
Acq On : 29 Jun 2023 09:38
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Title : SW846 8260
Last Update : Fri Jun 23 15:03:28 2023

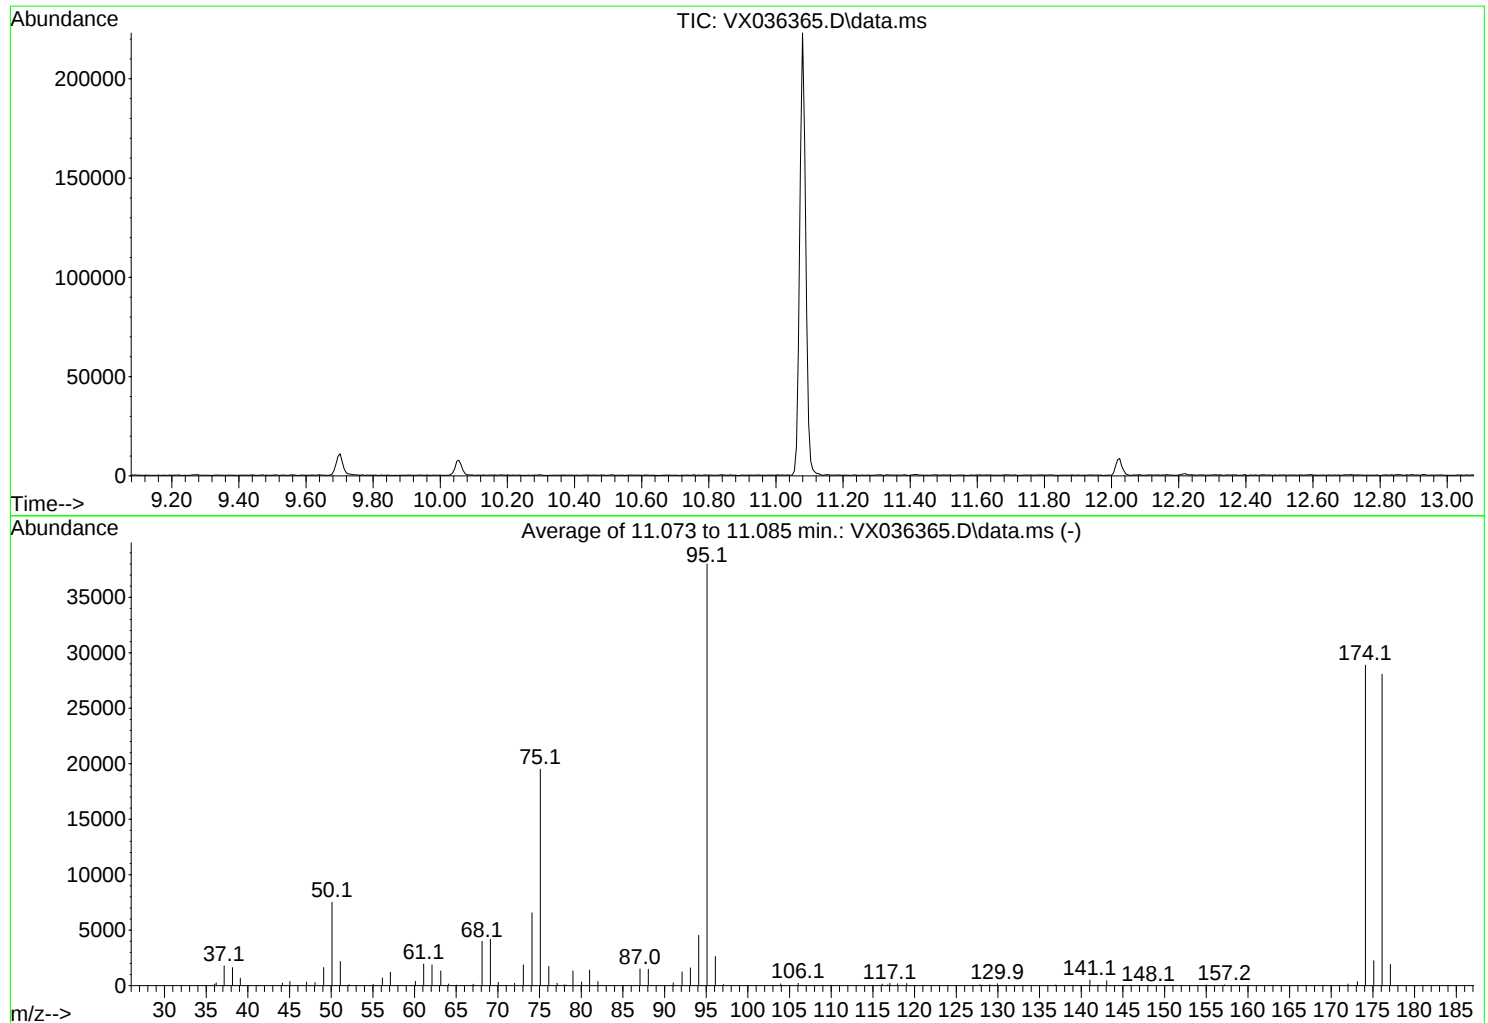

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	7511	PASS
75	95	30	60	51.3	19515	PASS
95	95	100	100	100.0	38013	PASS
96	95	5	9	6.9	2621	PASS
173	174	0.00	2	1.2	343	PASS
174	95	50	100	76.0	28891	PASS
175	174	5	9	7.8	2247	PASS
176	174	95	101	97.1	28067	PASS
177	176	5	9	6.8	1911	PASS