

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063018\
 Data File : VX003081.D
 Acq On : 30 Jun 2018 16:16
 Operator : JC/MD
 Sample : J3675-13
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S73-0020

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	91	rBV	826106	1102985	79.00%	12.158%
2	1.306	108	118	145	rBV	133171	784591	56.20%	8.648%
3	4.611	648	660	671	rBV4	5012	17048	1.22%	0.188%
4	5.507	795	807	821	rBV	176967	499899	35.81%	5.510%
5	5.665	821	833	847	rVV	258231	732040	52.43%	8.069%
6	6.074	888	900	914	rBV2	188961	485118	34.75%	5.347%
7	6.866	1020	1030	1044	rBV	374339	875744	62.73%	9.653%
8	8.720	1326	1334	1350	rBV	876759	1396147	100.00%	15.389%
9	10.116	1556	1563	1580	rBV	788065	1050276	75.23%	11.577%
10	11.140	1725	1731	1741	rBV	784108	983726	70.46%	10.843%
11	12.079	1880	1885	1896	rBV	889406	1144758	81.99%	12.618%


Sum of corrected areas: 9072332

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX063018\
Data File : VX003081.D
Acq On : 30 Jun 2018 16:16
Operator : JC/MD
Sample : J3675-13
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
S73-0020

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

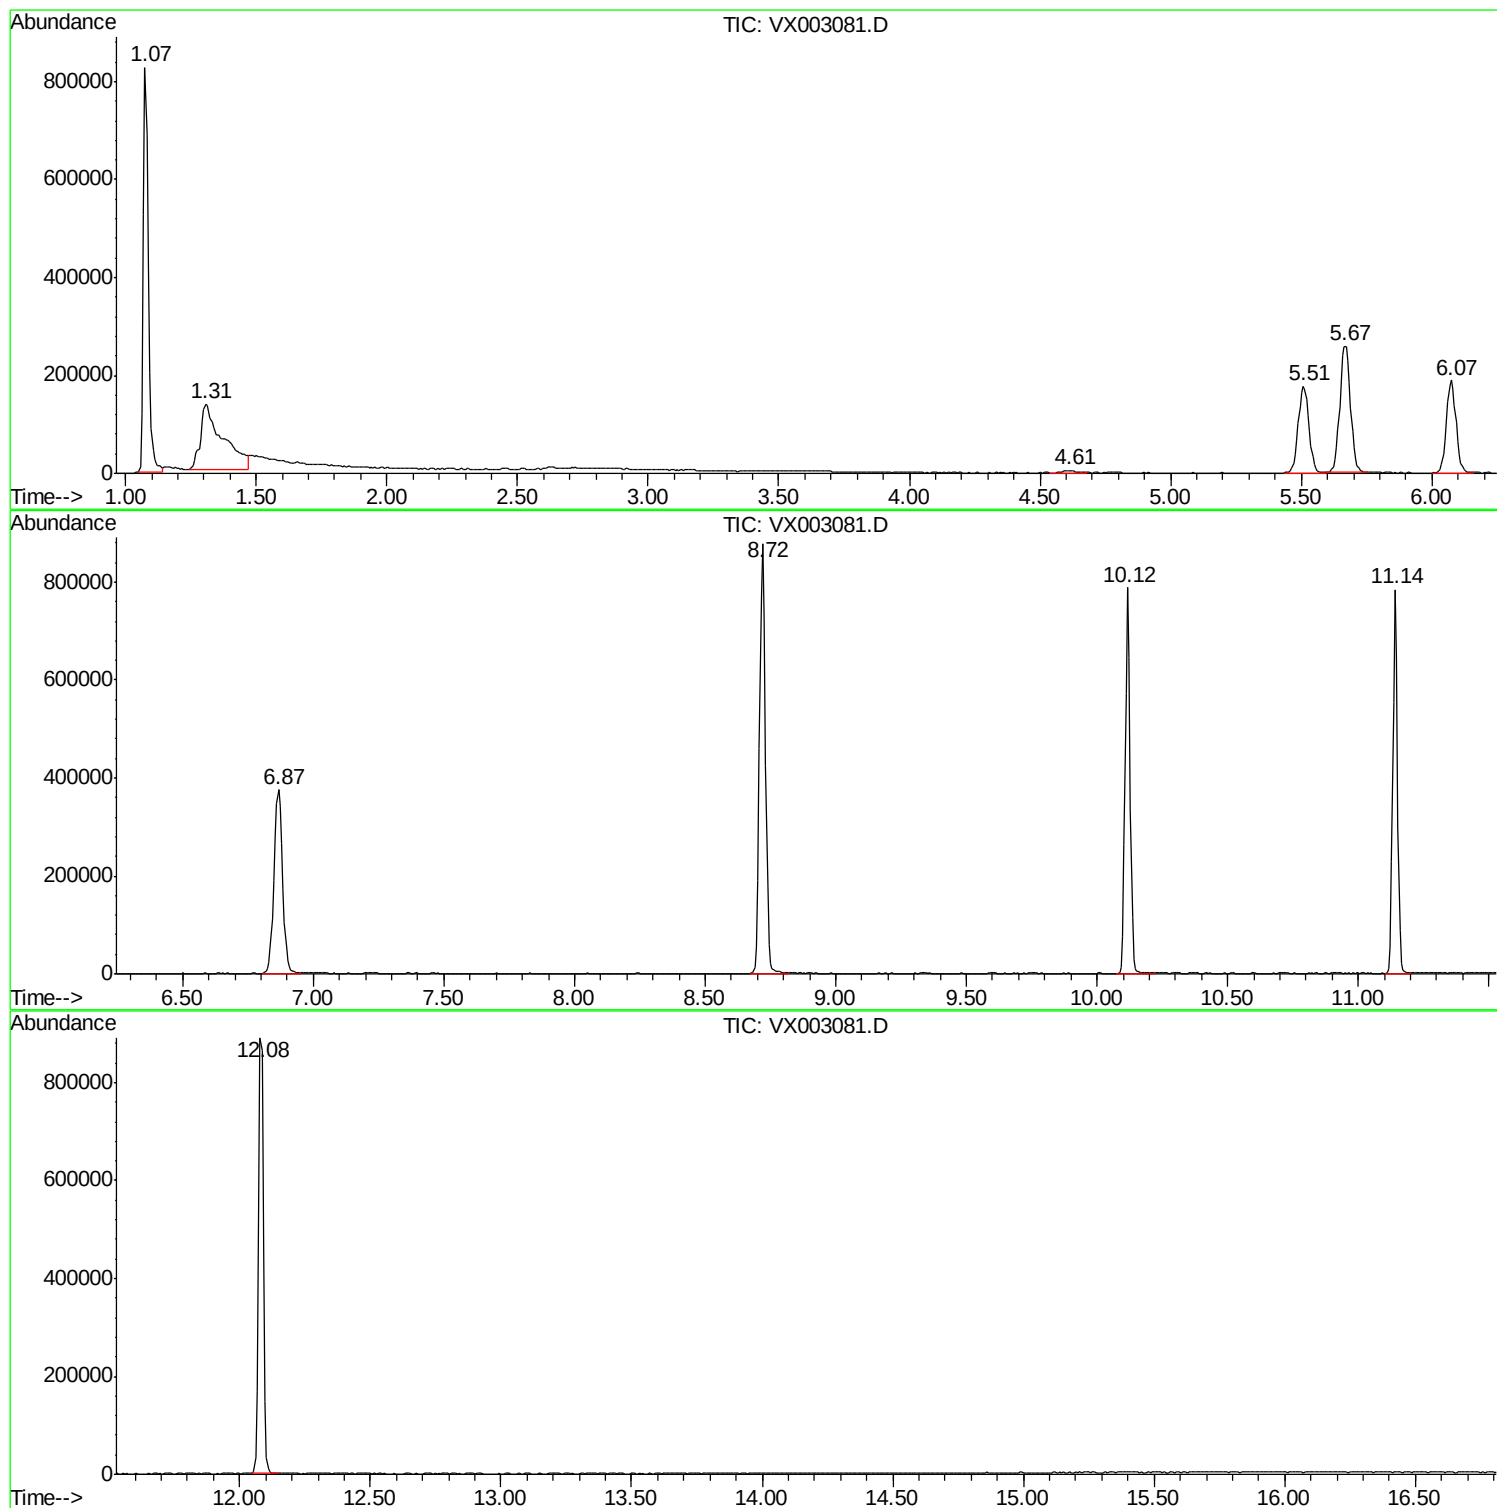

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX063018\
Data File : VX003081.D
Acq On : 30 Jun 2018 16:16
Operator : JC/MD
Sample : J3675-13
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
S73-0020

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.31	53.59 ug/l	784591	Pentafluorobenzene	5.67
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Sulfur dioxide	64 O2S	007446-09-5	83
2	Aminomethanesulfonic acid	111 CH5NO3S	013881-91-9	74
3	L-Alanine, 3-sulfo-	169 C3H7NO5S	000498-40-8	9
4	Ethene, 1,1-difluoro-	64 C2H2F2	000075-38-7	4
5	Ethyl Chloride	64 C2H5Cl	000075-00-3	3

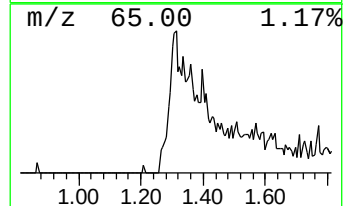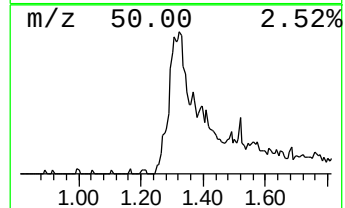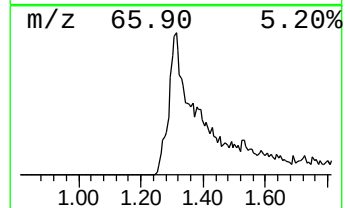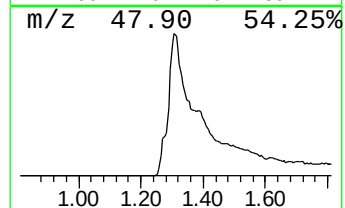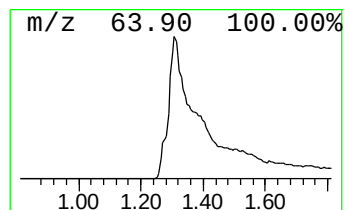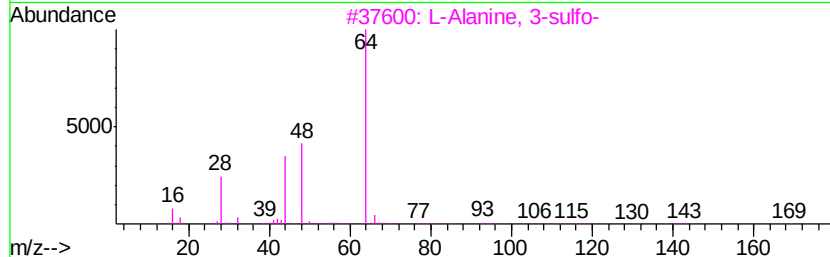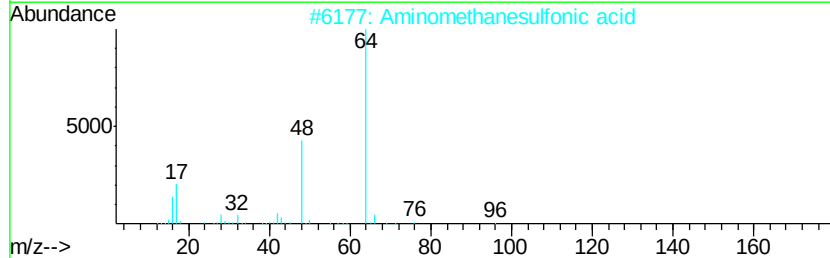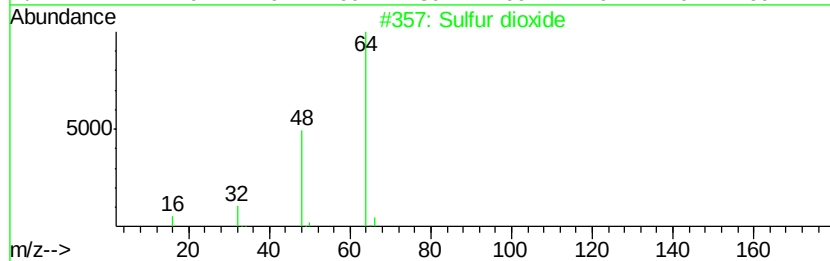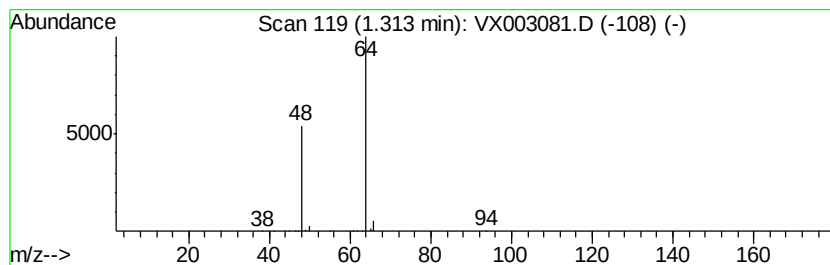

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX063018\
Data File : VX003081.D
Acq On : 30 Jun 2018 16:16
Operator : JC/MD
Sample : J3675-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S73-0020

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.31	53.6	ug/l	784591	1	5.67	732040	50.0