

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX063018\
 Data File : VX003084.D
 Acq On : 30 Jun 2018 17:36
 Operator : JC/MD
 Sample : J3716-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S22-0037

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	94	rBV	521955	760260	26.51%	3.044%
2	1.276	108	113	120	rBV	60541	100336	3.50%	0.402%
3	1.788	192	197	207	rVB	103938	150277	5.24%	0.602%
4	2.001	227	232	243	rVB	55685	82767	2.89%	0.331%
5	2.843	363	370	374	rBV2	41839	92940	3.24%	0.372%
6	2.885	374	377	386	rVB	28211	56156	1.96%	0.225%
7	3.172	415	424	432	rVB	34650	78190	2.73%	0.313%
8	3.519	473	481	494	rBV	21774	47755	1.67%	0.191%
9	4.397	614	625	639	rVB	126410	380603	13.27%	1.524%
10	5.507	796	807	813	rBV	181608	519742	18.12%	2.081%
11	5.580	813	819	826	rVV	135918	411956	14.37%	1.650%
12	5.671	826	834	854	rVB	275917	830592	28.96%	3.326%
13	5.934	864	877	890	rBV6	15461	56074	1.96%	0.225%
14	6.074	890	900	917	rVV	188057	492294	17.17%	1.971%
15	6.257	920	930	938	rVV4	16437	51528	1.80%	0.206%
16	6.354	939	946	955	rVV4	21859	63133	2.20%	0.253%
17	6.452	955	962	973	rVB2	28098	78062	2.72%	0.313%
18	6.866	1021	1030	1050	rBV	384753	907679	31.65%	3.635%
19	7.464	1115	1128	1141	rBV	213168	490110	17.09%	1.963%
20	7.732	1166	1172	1183	rVB	21768	45673	1.59%	0.183%
21	8.177	1238	1245	1255	rBV4	14676	39652	1.38%	0.159%
22	8.665	1319	1325	1328	rBV	16034	29357	1.02%	0.118%
23	8.720	1328	1334	1349	rVV	942463	1455505	50.75%	5.828%
24	9.043	1381	1387	1396	rVB2	22697	38125	1.33%	0.153%
25	10.116	1557	1563	1571	rBV	826349	1078573	37.61%	4.319%
26	10.256	1580	1586	1594	rVB	385630	508347	17.73%	2.036%
27	10.360	1595	1603	1615	rBV	2159472	2867757	100.00%	11.483%
28	11.024	1705	1712	1721	rBV	404405	525434	18.32%	2.104%
29	11.140	1725	1731	1738	rBV	866764	1074093	37.45%	4.301%
30	11.366	1758	1768	1774	rBV	350503	441087	15.38%	1.766%
31	11.439	1774	1780	1787	rVV	1254864	2271187	79.20%	9.094%
32	11.512	1787	1792	1799	rVB	749027	945532	32.97%	3.786%
33	11.670	1812	1818	1827	rBV	843709	1030499	35.93%	4.126%
34	11.811	1836	1841	1847	rBV	2280806	2681986	93.52%	10.739%

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX063018\
Data File : VX003084.D
Acq On : 30 Jun 2018 17:36
Operator : JC/MD
Sample : J3716-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0037

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Title : SW846 8260

35	11.951	1861	1864	1868	rVB	38203	47264	1.65%	0.189%
36	12.030	1872	1877	1880	rBV	70717	88870	3.10%	0.356%
37	12.079	1880	1885	1891	rVV	1036713	1324672	46.19%	5.304%
38	12.146	1891	1896	1904	rVB	877881	1018943	35.53%	4.080%
39	12.304	1915	1922	1925	rBV	162207	237700	8.29%	0.952%
40	12.378	1929	1934	1943	rVB3	90300	146751	5.12%	0.588%
41	12.463	1943	1948	1953	rBV	24461	31420	1.10%	0.126%
42	12.524	1953	1958	1963	rBV	63675	78957	2.75%	0.316%
43	12.591	1964	1969	1971	rBV	55760	80261	2.80%	0.321%
44	12.615	1971	1973	1977	rVV	70207	71446	2.49%	0.286%
45	12.670	1977	1982	1985	rVV	78480	93154	3.25%	0.373%
46	12.707	1985	1988	1992	rVB	27775	33423	1.17%	0.134%
47	12.762	1992	1997	2004	rBV2	72037	125700	4.38%	0.503%
48	12.908	2016	2021	2026	rVB2	46038	63983	2.23%	0.256%
49	12.981	2026	2033	2036	rBV	44721	58495	2.04%	0.234%
50	13.024	2036	2040	2045	rVB	72433	90706	3.16%	0.363%
51	13.347	2089	2093	2100	rVB2	121611	171215	5.97%	0.686%
52	13.481	2111	2115	2121	rVB	57523	74328	2.59%	0.298%
53	13.841	2166	2174	2180	rBV	169742	235746	8.22%	0.944%
54	14.700	2305	2315	2320	rBV	92994	122880	4.28%	0.492%
55	14.841	2332	2338	2346	rBV	66680	94533	3.30%	0.379%


Sum of corrected areas: 24973708

Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX063018\
Data File : VX003084.D
Acq On : 30 Jun 2018 17:36
Operator : JC/MD
Sample : J3716-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0037

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

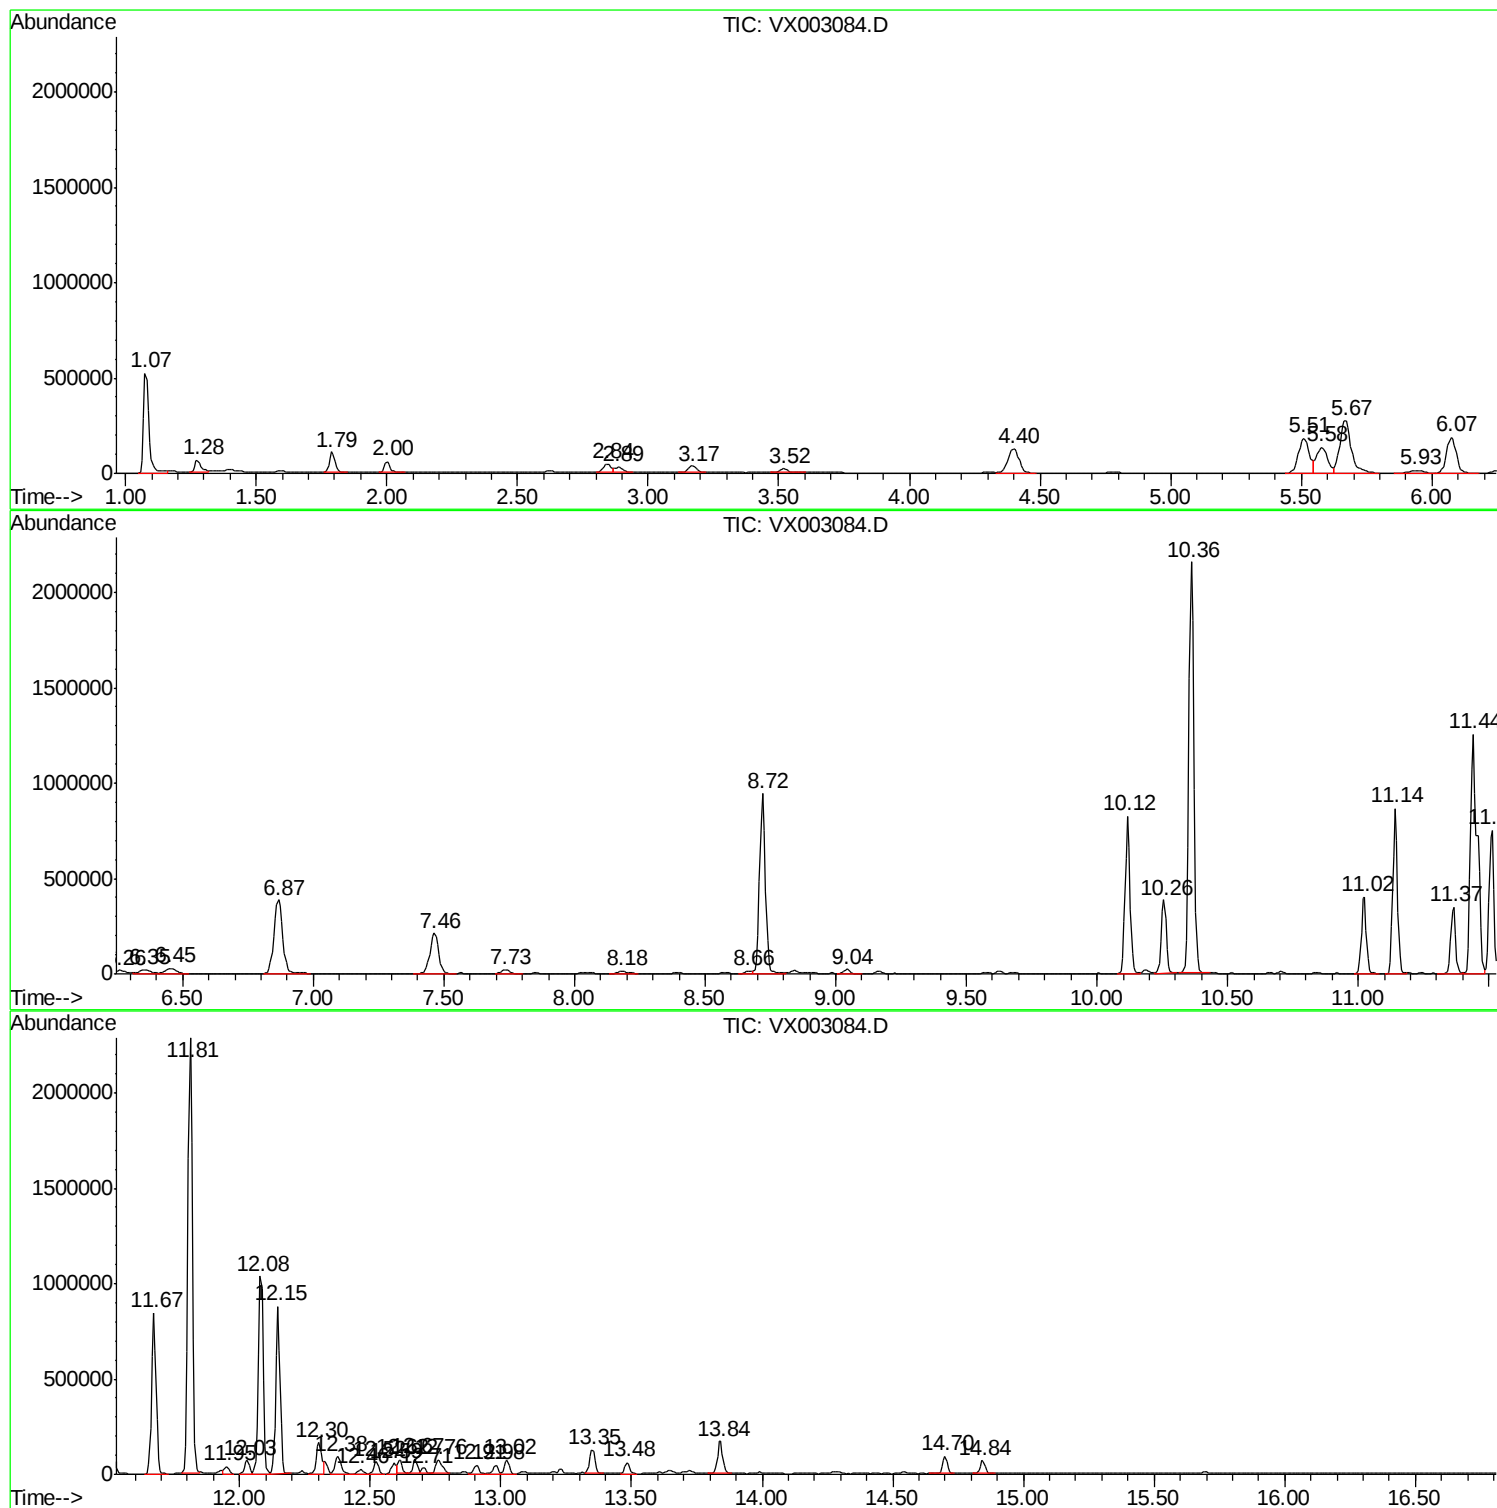

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063018\
Data File : VX003084.D
Acq On : 30 Jun 2018 17:36
Operator : JC/MD
Sample : J3716-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0037

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063018\
Data File : VX003084.D
Acq On : 30 Jun 2018 17:36
Operator : JC/MD
Sample : J3716-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0037

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc