

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063018\
 Data File : VX003087.D
 Acq On : 30 Jun 2018 18:56
 Operator : JC/MD
 Sample : J3738-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S22-0042

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	94	rBV	567012	822613	52.52%	5.812%
2	1.276	108	113	115	rBV	45639	66793	4.26%	0.472%
3	1.318	115	120	129	rVV2	45902	168384	10.75%	1.190%
4	2.623	330	334	340	rVB	12709	20282	1.29%	0.143%
5	5.507	795	807	822	rBV	188145	538026	34.35%	3.801%
6	5.671	822	834	854	rVB	281068	821373	52.44%	5.803%
7	6.074	887	900	916	rBV	199936	516323	32.97%	3.648%
8	6.348	933	945	956	rVB	36608	117801	7.52%	0.832%
9	6.866	1020	1030	1042	rBV	404801	942262	60.16%	6.657%
10	7.452	1117	1126	1134	rVB7	8421	22534	1.44%	0.159%
11	7.580	1140	1147	1152	rBV2	10180	22125	1.41%	0.156%
12	7.641	1152	1157	1161	rVV2	11895	25524	1.63%	0.180%
13	7.848	1184	1191	1200	rVB3	16004	34020	2.17%	0.240%
14	8.055	1211	1225	1235	rBV2	70333	169447	10.82%	1.197%
15	8.183	1238	1246	1253	rVV	97935	197235	12.59%	1.394%
16	8.256	1253	1258	1262	rVV	17991	33225	2.12%	0.235%
17	8.390	1272	1280	1285	rBV3	17902	36243	2.31%	0.256%
18	8.451	1285	1290	1295	rVV3	8351	16366	1.04%	0.116%
19	8.537	1295	1304	1308	rVV3	9717	22794	1.46%	0.161%
20	8.720	1318	1334	1349	rBV	991136	1566255	100.00%	11.066%
21	8.842	1349	1354	1358	rVV2	34948	60128	3.84%	0.425%
22	8.884	1358	1361	1371	rVB2	10671	20351	1.30%	0.144%
23	9.043	1381	1387	1398	rVB	78275	127451	8.14%	0.900%
24	9.165	1398	1407	1413	rBV	30418	52075	3.32%	0.368%
25	9.445	1443	1453	1457	rBV2	9648	17534	1.12%	0.124%
26	9.573	1467	1474	1480	rBV3	27702	51309	3.28%	0.363%
27	9.683	1485	1492	1496	rBV	143270	228298	14.58%	1.613%
28	9.823	1509	1515	1519	rVV4	11396	19752	1.26%	0.140%
29	9.896	1519	1527	1541	rVB5	24787	54966	3.51%	0.388%
30	10.116	1558	1563	1569	rBV	864580	1138266	72.67%	8.042%
31	10.256	1579	1586	1591	rBV	209851	290253	18.53%	2.051%
32	10.366	1595	1604	1609	rVV2	108621	202715	12.94%	1.432%
33	10.414	1609	1612	1620	rVV	13881	27047	1.73%	0.191%
34	10.518	1624	1629	1635	rVB	18586	26835	1.71%	0.190%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063018\
 Data File : VX003087.D
 Acq On : 30 Jun 2018 18:56
 Operator : JC/MD
 Sample : J3738-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S22-0042

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

35	10.646	1640	1650	1658	rBV7	35008	95405	6.09%	0.674%
36	10.719	1658	1662	1671	rVB4	9404	16362	1.04%	0.116%
37	10.817	1671	1678	1679	rBV4	15677	25749	1.64%	0.182%
38	10.835	1679	1681	1688	rVB	20207	26292	1.68%	0.186%
39	10.920	1688	1695	1703	rBV5	22358	45402	2.90%	0.321%
40	11.024	1706	1712	1717	rBV	208789	279193	17.83%	1.973%
41	11.140	1725	1731	1736	rBV	886371	1113243	71.08%	7.865%
42	11.189	1736	1739	1742	rVV3	19587	25891	1.65%	0.183%
43	11.280	1746	1754	1762	rVV3	38086	61021	3.90%	0.431%
44	11.365	1762	1768	1778	rVV	204448	267623	17.09%	1.891%
45	11.457	1778	1783	1794	rVB	78080	108798	6.95%	0.769%
46	11.670	1812	1818	1827	rVV	411034	516083	32.95%	3.646%
47	11.774	1827	1835	1837	rVV4	11190	18857	1.20%	0.133%
48	11.810	1837	1841	1852	rVB	60559	85032	5.43%	0.601%
49	11.914	1852	1858	1861	rBV4	10884	19886	1.27%	0.140%
50	11.951	1861	1864	1869	rVB	25056	33661	2.15%	0.238%
51	12.079	1880	1885	1894	rBV	1038146	1336212	85.31%	9.441%
52	12.237	1906	1911	1915	rVB	19892	27717	1.77%	0.196%
53	12.304	1915	1922	1927	rVV2	99898	124754	7.97%	0.881%
54	12.371	1927	1933	1940	rVB2	31426	54492	3.48%	0.385%
55	12.463	1944	1948	1953	rBV	24103	31879	2.04%	0.225%
56	12.524	1953	1958	1963	rVV	39238	51311	3.28%	0.363%
57	12.591	1963	1969	1971	rVV	35945	49192	3.14%	0.348%
58	12.615	1971	1973	1976	rVV	25761	29009	1.85%	0.205%
59	12.670	1978	1982	1985	rVV	45035	59325	3.79%	0.419%
60	12.707	1985	1988	1993	rVV2	33304	53394	3.41%	0.377%
61	12.762	1993	1997	2005	rVV2	87804	161021	10.28%	1.138%
62	12.853	2005	2012	2015	rVV3	15877	39693	2.53%	0.280%
63	12.896	2017	2019	2025	rVB3	18039	25681	1.64%	0.181%
64	12.981	2030	2033	2036	rVB2	29776	34118	2.18%	0.241%
65	13.024	2036	2040	2046	rVB	51936	68392	4.37%	0.483%
66	13.085	2046	2050	2056	rVB2	31969	45344	2.90%	0.320%
67	13.158	2056	2062	2066	rBV2	15432	30448	1.94%	0.215%
68	13.201	2066	2069	2072	rBV	16627	18007	1.15%	0.127%
69	13.310	2083	2087	2089	rBV2	27236	34847	2.22%	0.246%
70	13.347	2089	2093	2099	rVV2	144474	227958	14.55%	1.611%
71	13.432	2104	2107	2110	rVV	14952	16643	1.06%	0.118%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063018\
Data File : VX003087.D
Acq On : 30 Jun 2018 18:56
Operator : JC/MD
Sample : J3738-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0042

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Title : SW846 8260

72	13.481	2110	2115	2120	rVB3	24684	37073	2.37%	0.262%
73	13.639	2137	2141	2147	rBV4	24739	47955	3.06%	0.339%
74	13.731	2153	2156	2160	rVB2	17043	26607	1.70%	0.188%
75	13.841	2170	2174	2181	rVB	55075	83467	5.33%	0.590%
76	13.926	2181	2188	2192	rVB6	9384	22840	1.46%	0.161%
77	13.987	2192	2198	2203	rBV4	14246	27822	1.78%	0.197%
78	14.273	2240	2245	2252	rBV4	17089	26175	1.67%	0.185%
79	14.438	2268	2272	2275	rVB2	12624	16547	1.06%	0.117%
80	14.548	2284	2290	2294	rBV3	16855	27997	1.79%	0.198%
81	14.737	2317	2321	2326	rVB3	14617	19402	1.24%	0.137%
82	14.847	2334	2339	2347	rBV	58833	83364	5.32%	0.589%


Sum of corrected areas: 14153789

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX063018\
Data File : VX003087.D
Acq On : 30 Jun 2018 18:56
Operator : JC/MD
Sample : J3738-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0042

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

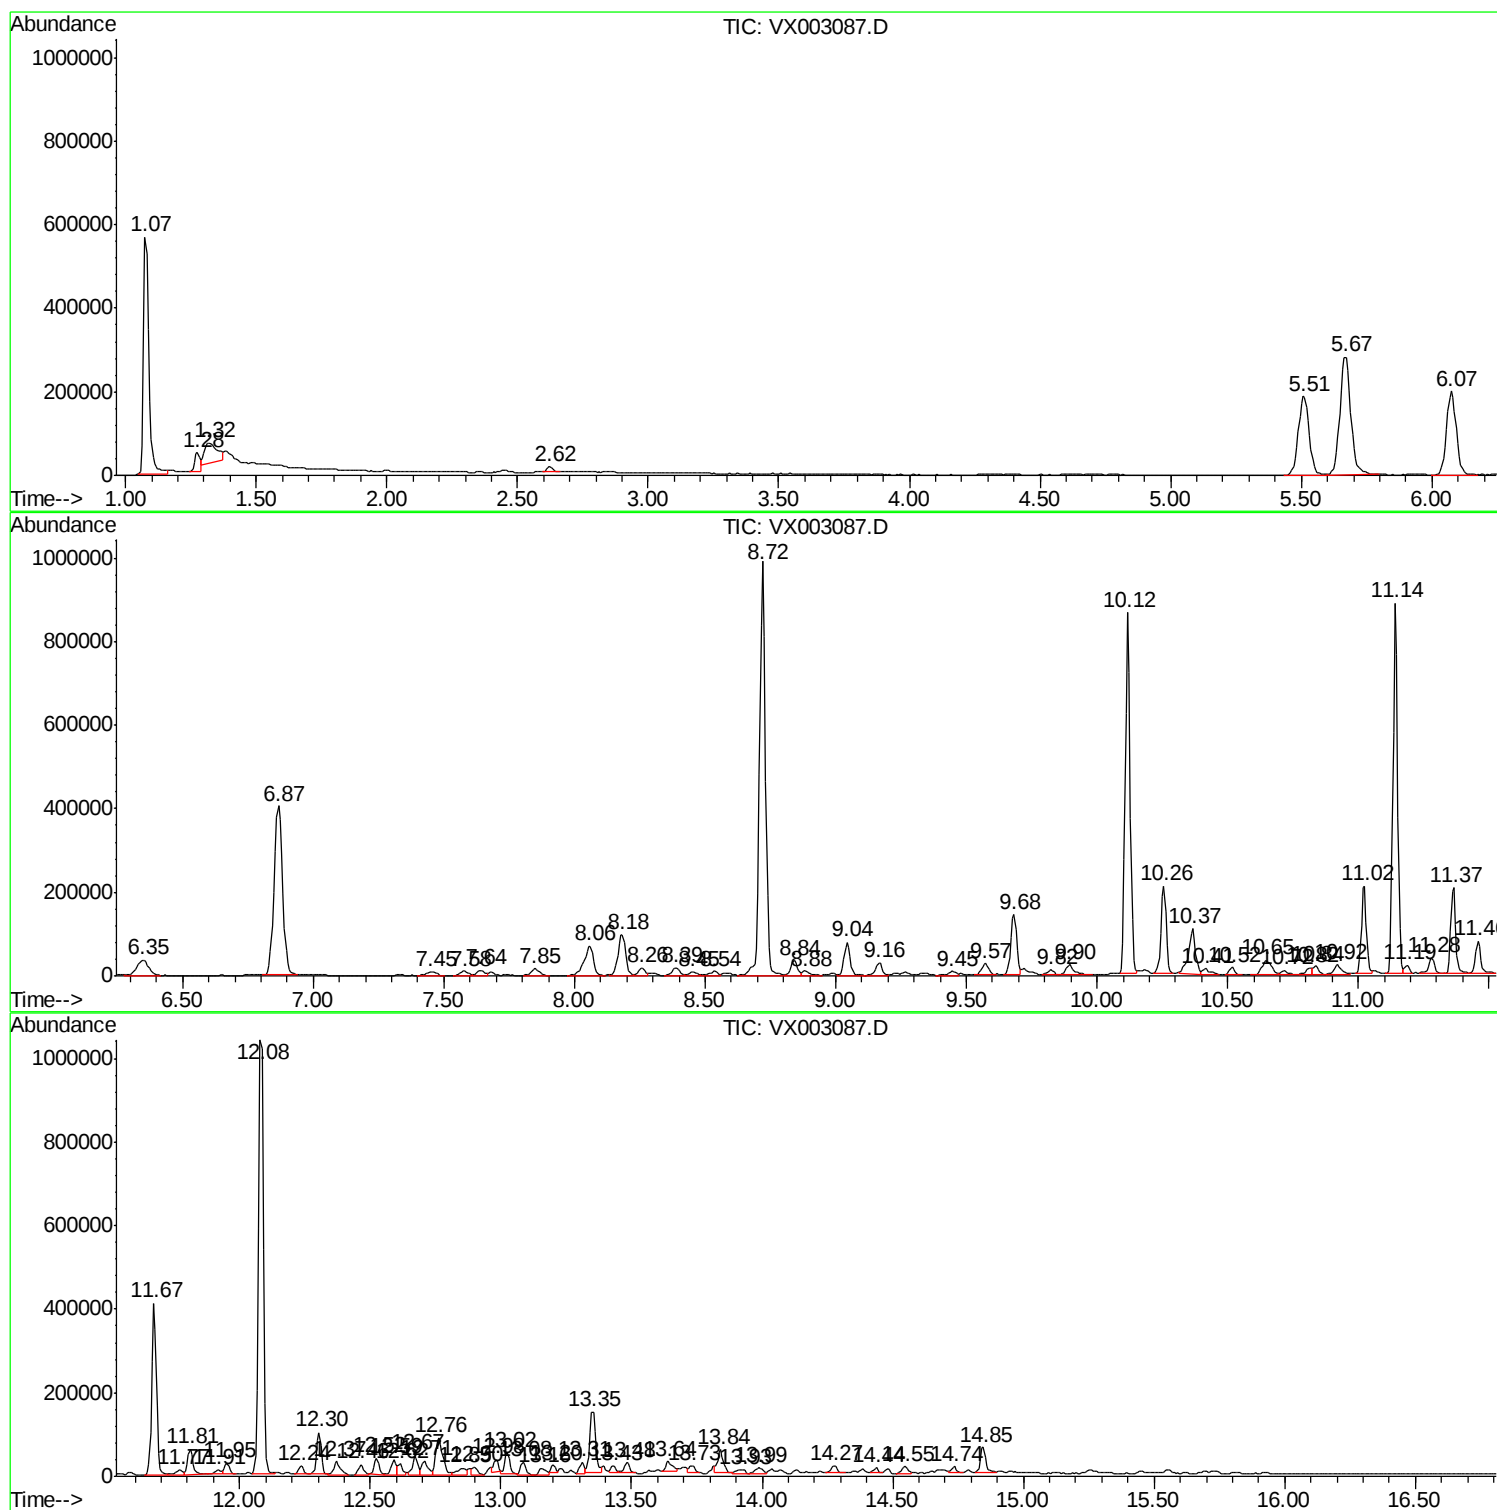

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX063018\
Data File : VX003087.D
Acq On : 30 Jun 2018 18:56
Operator : JC/MD
Sample : J3738-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0042

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX063018\
Data File : VX003087.D
Acq On : 30 Jun 2018 18:56
Operator : JC/MD
Sample : J3738-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0042

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc