

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063018\
 Data File : VX003089.D
 Acq On : 30 Jun 2018 19:49
 Operator : JC/MD
 Sample : J3738-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S22-0041

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	94	rBV	1200572	1541677	8.56%	1.538%
2	1.301	114	117	128	rVB	104245	295990	1.64%	0.295%
3	1.788	192	197	207	rVB	749393	1050025	5.83%	1.048%
4	2.843	361	370	376	rBV	543302	1245209	6.91%	1.242%
5	3.172	414	424	437	rVB	399694	926981	5.14%	0.925%
6	4.306	596	610	619	rBV	149432	455215	2.53%	0.454%
7	5.507	796	807	815	rBV	172458	508011	2.82%	0.507%
8	5.672	826	834	837	rBV	233964	592088	3.29%	0.591%
9	5.727	838	843	863	rVB	415257	1199157	6.65%	1.196%
10	5.946	866	879	891	rBV5	190067	661527	3.67%	0.660%
11	6.074	891	900	909	rBV	177354	461888	2.56%	0.461%
12	6.263	919	931	938	rBV2	356335	1118121	6.20%	1.116%
13	6.354	938	946	956	rVV3	579223	1746639	9.69%	1.743%
14	6.452	956	962	975	rVB2	72000	200272	1.11%	0.200%
15	6.867	1019	1030	1054	rBV	373161	896220	4.97%	0.894%
16	7.458	1116	1127	1138	rVB3	316873	802960	4.46%	0.801%
17	7.854	1184	1192	1200	rVB2	140037	294498	1.63%	0.294%
18	8.055	1211	1225	1237	rVB3	333108	945756	5.25%	0.944%
19	8.183	1237	1246	1254	rBV	468301	966262	5.36%	0.964%
20	8.391	1275	1280	1286	rVB3	151678	282877	1.57%	0.282%
21	8.513	1295	1300	1308	rBV3	85131	196536	1.09%	0.196%
22	8.671	1319	1326	1329	rBV3	257766	482870	2.68%	0.482%
23	8.720	1329	1334	1348	rVV	931593	1550590	8.60%	1.547%
24	8.842	1348	1354	1359	rVV	392052	664924	3.69%	0.663%
25	9.043	1381	1387	1394	rVB	583037	918812	5.10%	0.917%
26	9.165	1399	1407	1413	rBV	269653	445043	2.47%	0.444%
27	9.573	1469	1474	1479	rBV3	180499	279890	1.55%	0.279%
28	9.628	1479	1483	1487	rVB	136327	180434	1.00%	0.180%
29	9.683	1487	1492	1496	rBV	494021	738524	4.10%	0.737%
30	10.116	1558	1563	1568	rVB	769559	1004162	5.57%	1.002%
31	10.189	1568	1575	1580	rBV	214991	310098	1.72%	0.309%
32	10.256	1580	1586	1595	rBV	13550872	18019914	100.00%	17.979%
33	10.366	1595	1604	1610	rVV	10817017	13729204	76.19%	13.698%
34	10.646	1641	1650	1657	rBV2	93914	244348	1.36%	0.244%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063018\
 Data File : VX003089.D
 Acq On : 30 Jun 2018 19:49
 Operator : JC/MD
 Sample : J3738-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S22-0041

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

35	10.841	1678	1682	1690	rVB2	128195	181652	1.01%	0.181%
36	11.024	1706	1712	1717	rBV	2926900	3835741	21.29%	3.827%
37	11.140	1725	1731	1736	rBV	843798	1070704	5.94%	1.068%
38	11.366	1763	1768	1778	rVB	2444438	3102990	17.22%	3.096%
39	11.457	1778	1783	1788	rBV	2543330	2989109	16.59%	2.982%
40	11.671	1813	1818	1828	rBV	3214964	3971746	22.04%	3.963%
41	11.811	1836	1841	1846	rVB	4116035	4738607	26.30%	4.728%
42	11.921	1852	1859	1861	rBV2	133499	218588	1.21%	0.218%
43	11.951	1861	1864	1871	rVB	465231	585169	3.25%	0.584%
44	12.079	1879	1885	1891	rVB2	1062794	1590897	8.83%	1.587%
45	12.146	1891	1896	1901	rBV	2019509	2348491	13.03%	2.343%
46	12.238	1906	1911	1915	rVB	176830	223860	1.24%	0.223%
47	12.305	1916	1922	1927	rBV	2220506	2773857	15.39%	2.768%
48	12.372	1927	1933	1942	rVB2	392037	602226	3.34%	0.601%
49	12.463	1942	1948	1953	rBV	321372	406049	2.25%	0.405%
50	12.524	1953	1958	1964	rBV	841503	1031079	5.72%	1.029%
51	12.591	1964	1969	1971	rBV	405129	505492	2.81%	0.504%
52	12.616	1971	1973	1976	rVV	225010	220059	1.22%	0.220%
53	12.670	1977	1982	1985	rVV	707974	839189	4.66%	0.837%
54	12.707	1985	1988	1992	rVV	365989	458789	2.55%	0.458%
55	12.762	1992	1997	2004	rVB2	982774	1535752	8.52%	1.532%
56	12.902	2016	2020	2025	rVB2	192860	293661	1.63%	0.293%
57	12.981	2025	2033	2036	rVV	574679	755228	4.19%	0.753%
58	13.024	2036	2040	2046	rVV	478776	598374	3.32%	0.597%
59	13.231	2071	2074	2077	rVB	199995	215829	1.20%	0.215%
60	13.347	2089	2093	2099	rVB2	1805807	2423895	13.45%	2.418%
61	13.481	2111	2115	2121	rVB	488736	619410	3.44%	0.618%
62	13.646	2138	2142	2147	rBV3	179464	319371	1.77%	0.319%
63	13.725	2153	2155	2163	rVB3	211796	335349	1.86%	0.335%
64	13.841	2164	2174	2182	rBV	2792293	3666342	20.35%	3.658%
65	14.280	2241	2246	2252	rVB2	109813	213101	1.18%	0.213%
66	14.701	2303	2315	2325	rBV	1139299	1420381	7.88%	1.417%
67	14.841	2333	2338	2347	rBV	721210	964027	5.35%	0.962%
68	15.694	2469	2478	2481	rBV	132896	217696	1.21%	0.217%


Sum of corrected areas: 100229432

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX063018\
Data File : VX003089.D
Acq On : 30 Jun 2018 19:49
Operator : JC/MD
Sample : J3738-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0041

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

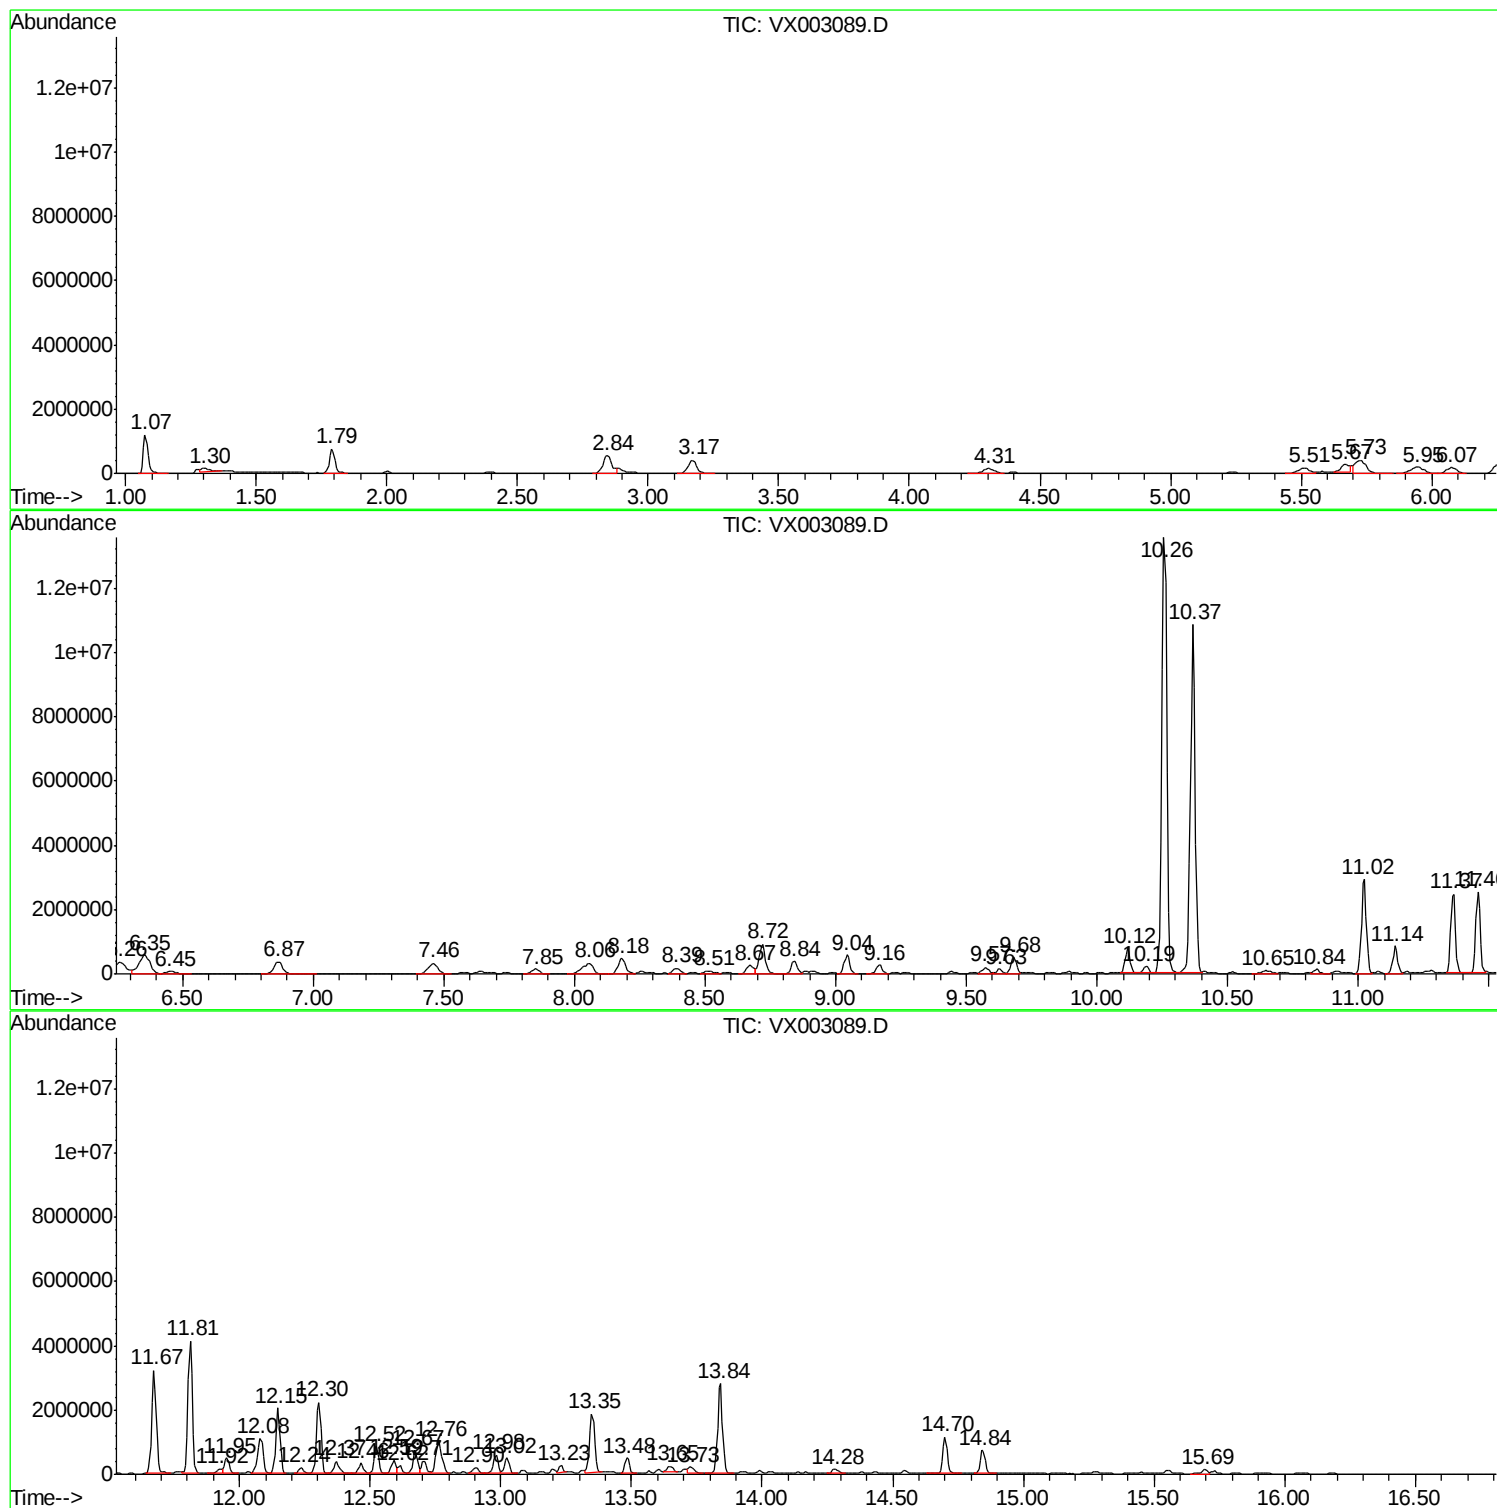

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX063018\
Data File : VX003089.D
Acq On : 30 Jun 2018 19:49
Operator : JC/MD
Sample : J3738-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0041

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX063018\
Data File : VX003089.D
Acq On : 30 Jun 2018 19:49
Operator : JC/MD
Sample : J3738-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S22-0041

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc