

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063018\
 Data File : VX003106.D
 Acq On : 01 Jul 2018 04:40
 Operator : JC/MD
 Sample : J3800-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

Signal : TIC: VX003105.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	91	rBV	885416	1179372	81.13%	13.271%
2	1.276	108	113	114	rBV	25167	33312	2.29%	0.375%
3	1.306	114	118	127	rVV	22273	74944	5.16%	0.843%
4	2.623	328	334	342	rVB	12240	22282	1.53%	0.251%
5	4.605	648	659	672	rBV	26447	76210	5.24%	0.858%
6	5.507	796	807	820	rBV2	182997	517190	35.58%	5.820%
7	5.665	820	833	852	rVB	273389	767934	52.82%	8.642%
8	6.074	890	900	918	rBV	192459	498233	34.27%	5.607%
9	6.866	1020	1030	1045	rBV	391016	911191	62.68%	10.254%
10	8.720	1326	1334	1349	rBV	941390	1453740	100.00%	16.359%
11	10.116	1556	1563	1575	rBV	820266	1094520	75.29%	12.317%
12	11.140	1725	1731	1742	rBV	836929	1039073	71.48%	11.693%
13	12.079	1879	1885	1896	rBV	950810	1218551	83.82%	13.712%


Sum of corrected areas: 8886552

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX063018\
Data File : VX003106.D
Acq On : 01 Jul 2018 04:40
Operator : JC/MD
Sample : J3800-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

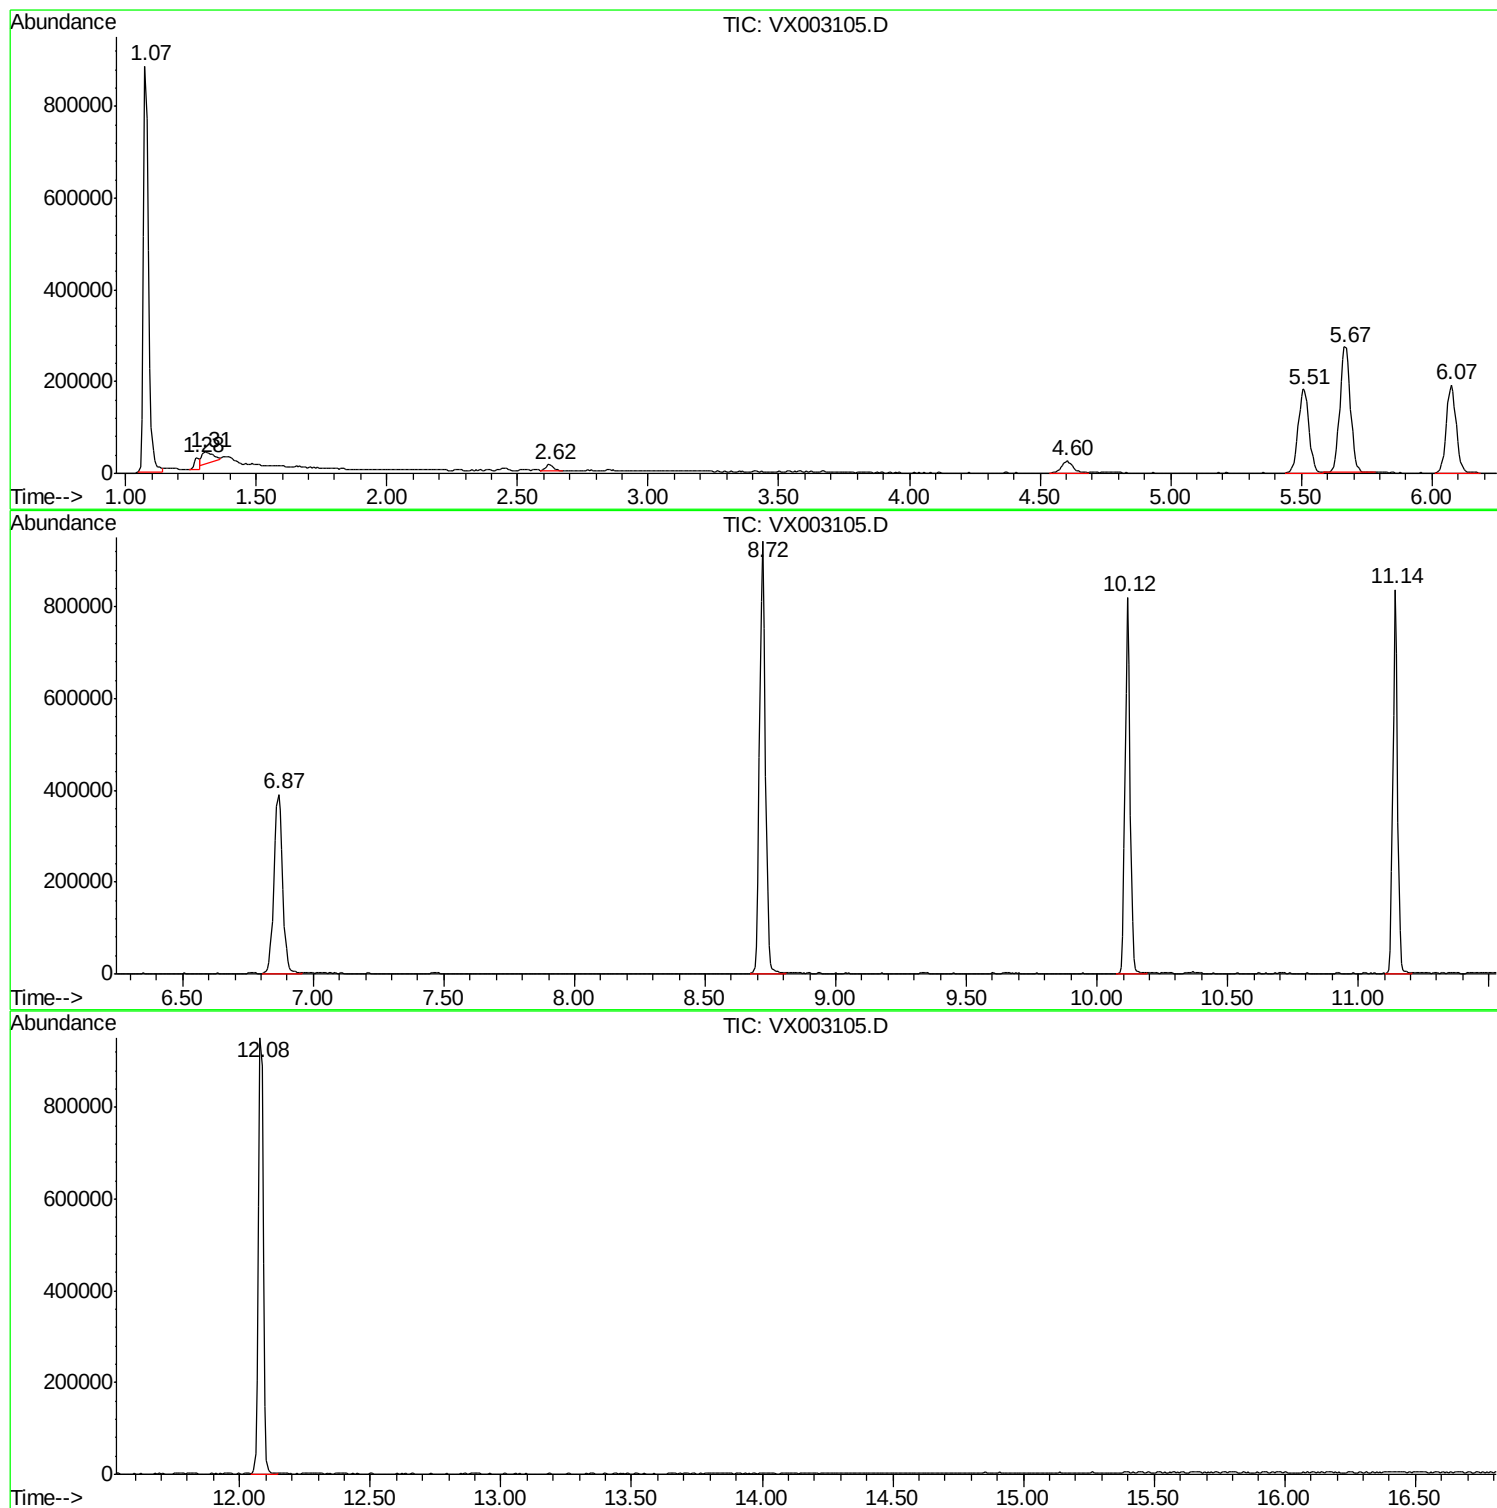

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX063018\
Data File : VX003106.D
Acq On : 01 Jul 2018 04:40
Operator : JC/MD
Sample : J3800-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX063018\
Data File : VX003106.D
Acq On : 01 Jul 2018 04:40
Operator : JC/MD
Sample : J3800-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-11

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc