

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063018\
 Data File : VX003107.D
 Acq On : 01 Jul 2018 05:07
 Operator : JC/MD
 Sample : J3800-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-14

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

Signal : TIC: VX003106.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	92	rBV	1266693	1607529	100.00%	15.737%
2	1.294	108	116	129	rBV	195061	745808	46.39%	7.301%
3	2.623	329	334	340	rBV	26369	48859	3.04%	0.478%
4	5.507	795	807	822	rBV	195488	553503	34.43%	5.419%
5	5.666	822	833	847	rVV	289751	812375	50.54%	7.953%
6	6.074	889	900	915	rBV	196787	514372	32.00%	5.035%
7	6.867	1019	1030	1042	rBV	400400	940142	58.48%	9.203%
8	8.720	1326	1334	1343	rBV	973679	1491319	92.77%	14.599%
9	10.116	1554	1563	1577	rBV	841813	1129489	70.26%	11.057%
10	11.140	1725	1731	1745	rBV	867753	1074561	66.85%	10.519%
11	12.079	1880	1885	1896	rBV	980663	1268224	78.89%	12.415%
12	15.639	2464	2469	2476	rBV	17891	28868	1.80%	0.283%


Sum of corrected areas: 10215049

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX063018\
Data File : VX003107.D
Acq On : 01 Jul 2018 05:07
Operator : JC/MD
Sample : J3800-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-14

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

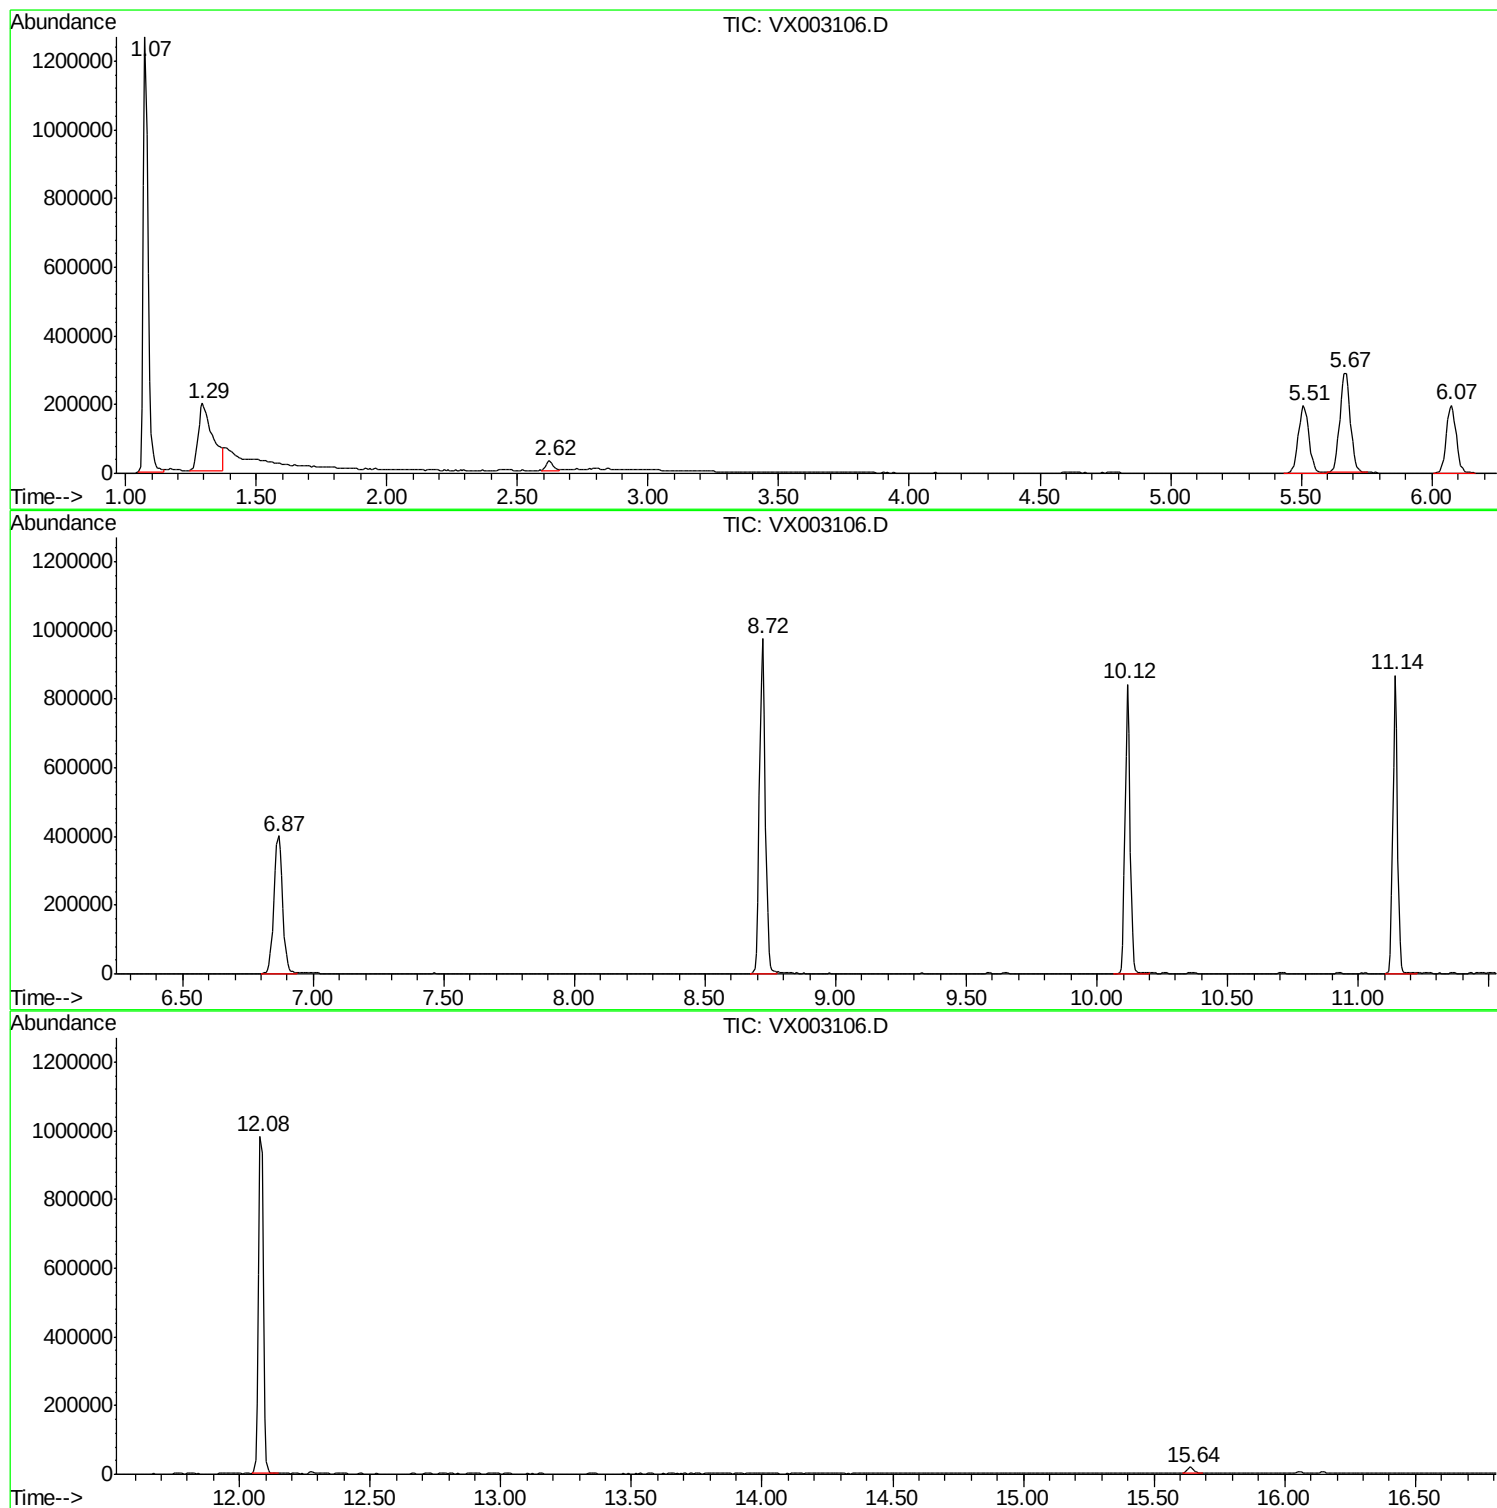

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX063018\
Data File : VX003107.D
Acq On : 01 Jul 2018 05:07
Operator : JC/MD
Sample : J3800-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-14










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Sulfur dioxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.29	45.90 ug/l	745808	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Sulfur dioxide	64	O2S	007446-09-5	83
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5		Ethyl Chloride	64	C2H5Cl	000075-00-3	3

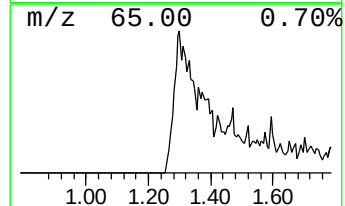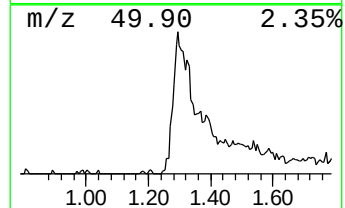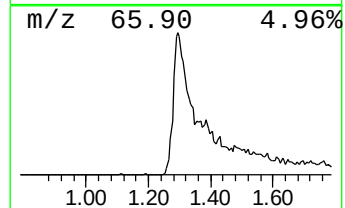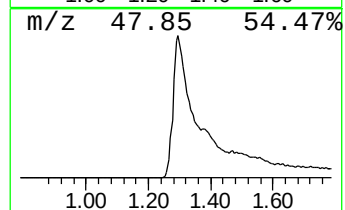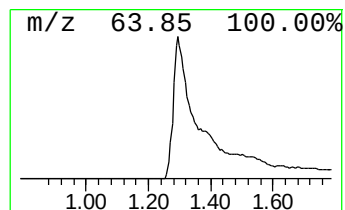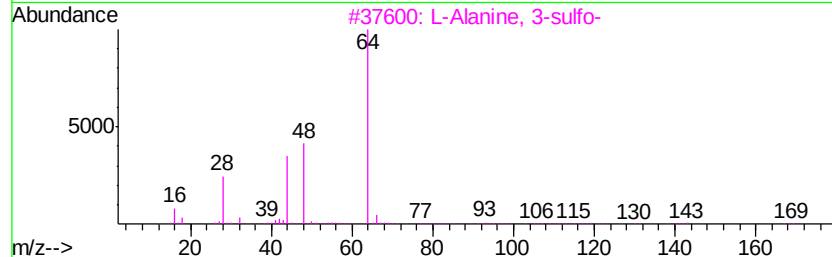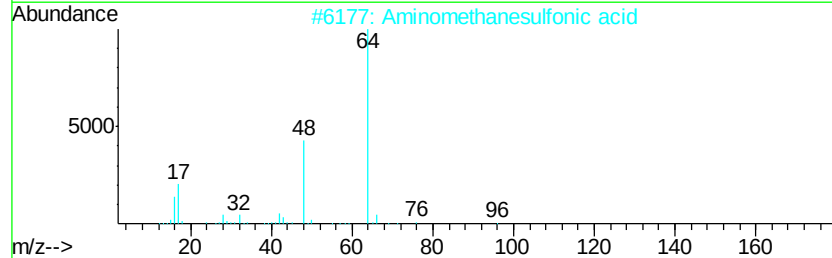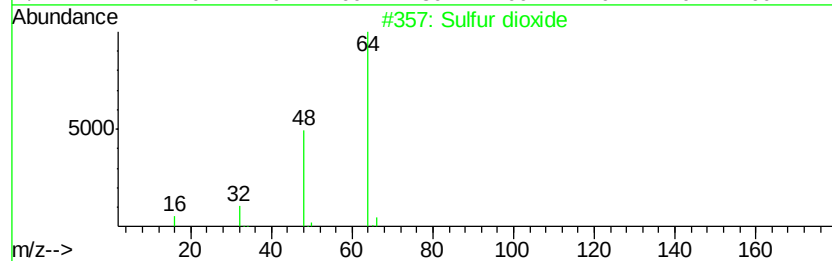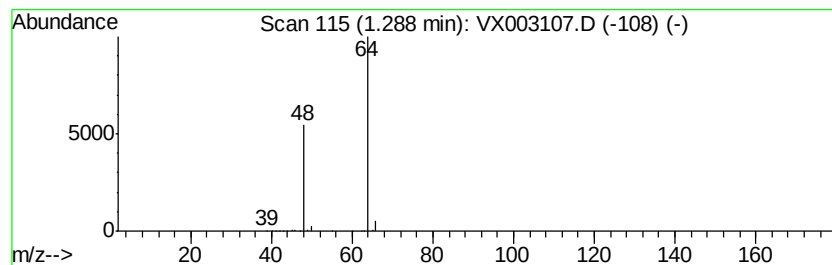

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX063018\
Data File : VX003107.D
Acq On : 01 Jul 2018 05:07
Operator : JC/MD
Sample : J3800-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-14

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.29	45.9	ug/l	745808	1	5.67	812375	50.0