

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063020\
 Data File : VX017074.D
 Acq On : 01 Jul 2020 03:24
 Operator : JC/SP
 Sample : PB129852ZHE#10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB129852ZHE#10

Quant Time: Jul 01 08:23:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 29 17:10:38 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	229031	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	395971	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	423954	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	219654	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	154400	54.68	ug/l	0.00
Spiked Amount			Recovery	=	109.36%	
35) Dibromofluoromethane	5.47	113	133208	53.18	ug/l	0.00
Spiked Amount			Recovery	=	106.36%	
50) Toluene-d8	8.70	98	495886	53.54	ug/l	0.00
Spiked Amount			Recovery	=	107.08%	
62) 4-Bromofluorobenzene	11.12	95	205716	56.82	ug/l	0.00
Spiked Amount			Recovery	=	113.64%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
8) Diethyl Ether	2.17	74	544	0.802	ug/l	87
11) Tert butyl alcohol	3.00	59	2034	3.776	ug/l #	79
12) 1,1-Dichloroethene	2.36	96	700	0.309	ug/l #	5
13) Acrolein	2.28	56	451	1.401	ug/l	93
16) Acetone	2.42	43	11642	11.022	ug/l	92
18) Methyl Acetate	2.75	43	3196	1.159	ug/l #	89
20) Methylene Chloride	2.84	84	12377	4.395	ug/l	96
25) 2-Butanone	4.65	43	4640	2.636	ug/l	92
29) Tetrahydrofuran	5.10	42	315	0.271	ug/l #	36
31) Cyclohexane	5.63	56	4800	1.259	ug/l #	14
36) 1,1-Dichloropropene	5.63	75	16659	4.451	ug/l #	51
38) Carbon Tetrachloride	5.63	117	22215	5.389	ug/l #	20
43) Isopropyl Acetate	6.42	43	58804	9.320	ug/l	99
44) Trichloroethene	7.20	130	506	Below Cal		86
48) Methyl methacrylate	7.65	41	3951	1.318	ug/l #	15
49) 1,4-Dioxane	7.74	88	51	0.751	ug/l #	1
51) 4-Methyl-2-Pentanone	8.60	43	55720	14.815	ug/l #	53
54) cis-1,3-Dichloropropene	8.59	75	25919	5.515	ug/l #	63
56) Ethyl methacrylate	9.29	69	1443	0.361	ug/l #	1
57) 1,3-Dichloropropane	9.52	76	5221	1.100	ug/l #	46
59) 2-Hexanone	9.52	43	64683	23.548	ug/l #	51
74) N-amyl acetate	10.80	43	3030	0.494	ug/l #	52
76) 1,2,3-Trichloropropane	11.12	75	104137	24.109	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.49	105	2814	0.236	ug/l	96
81) trans-1,4-Dichloro-2-buten	11.12	75	104137	62.434	ug/l #	13
88) 1,4-Dichlorobenzene	12.01	146	571	Below Cal		86
94) Hexachlorobutadiene	13.77	225	149	0.928	ug/l	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 746

Delta R.T. -0.00 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :


PB129852ZHE#10

Tot Ion:168 Resp: 229031

Ion Ratio Lower Upper




168 100

99 54.0 42.6 64.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

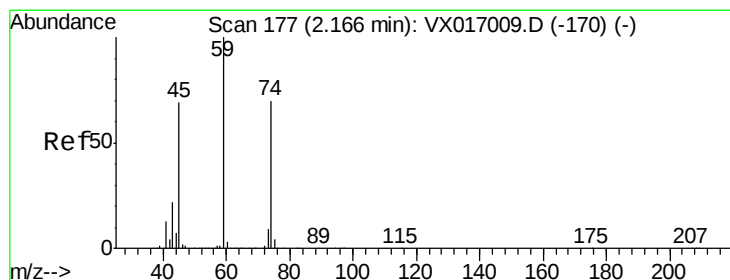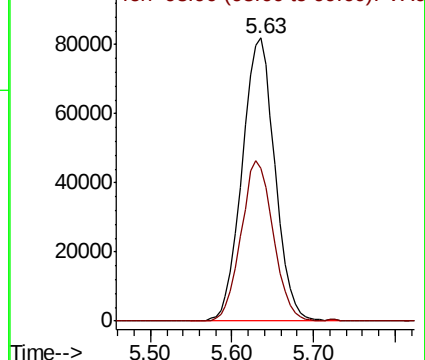

#8

Diethyl Ether

Concen: 0.802 ug/l

RT: 2.17 min Scan# 177

Delta R.T. -0.00 min

Lab File: VX017074.D


Acq: 01 Jul 2020 03:24

Tgt Ion: 74 Resp: 544

Ion Ratio Lower Upper



74 100


45 86.6 49.8 149.3



Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

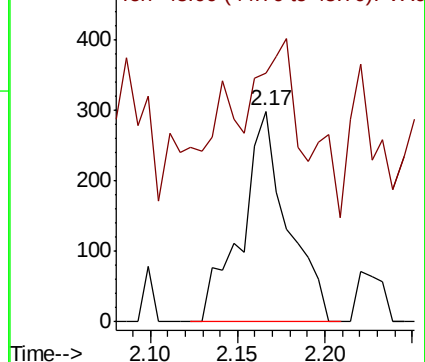




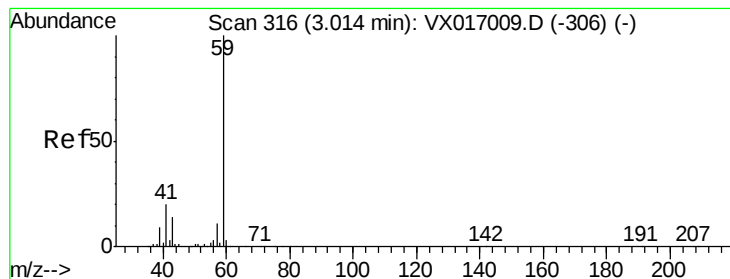


#11

Tert butyl alcohol
Concen: 3.776 ug/l
RT: 3.00 min Scan# 313
Delta R.T. -0.02 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24

Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#10




Tot Ion: 59 Resp: 2034
Ion Ratio Lower Upper
59 100
57 2.2 8.2 12.2#

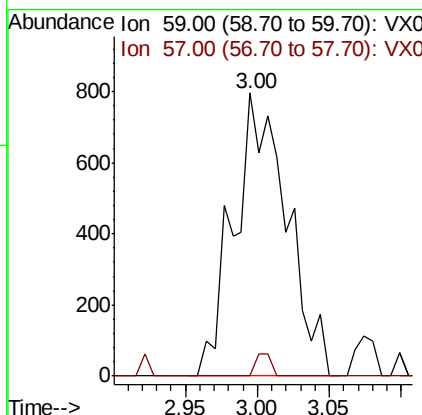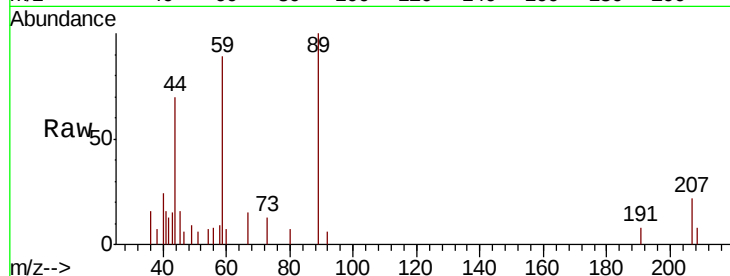


#12

1,1-Dichloroethene
Concen: 0.309 ug/l
RT: 2.36 min Scan# 209
Delta R.T. 0.01 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24

Tgt Ion: 96 Resp: 700
Ion Ratio Lower Upper
96 100
61 26.3 126.3 189.5#
98 0.0 51.0 76.6#

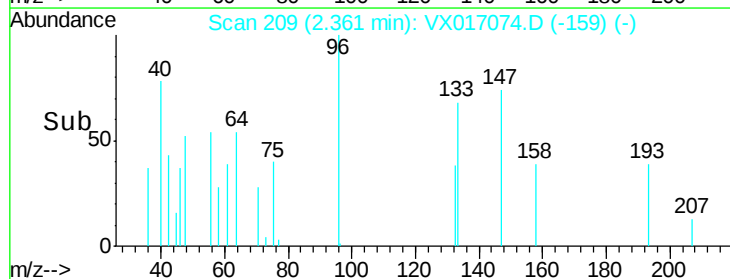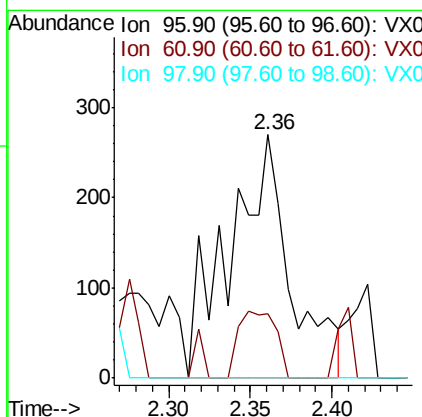



#13

Acrolein

Concen: 1.401 ug/l

RT: 2.28 min Scan# 195

Delta R.T. 0.01 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :


PB129852ZHE#10

Tot Ion: 56 Resp: 451

Ion Ratio Lower Upper




56 100

55 75.4 55.7 83.5

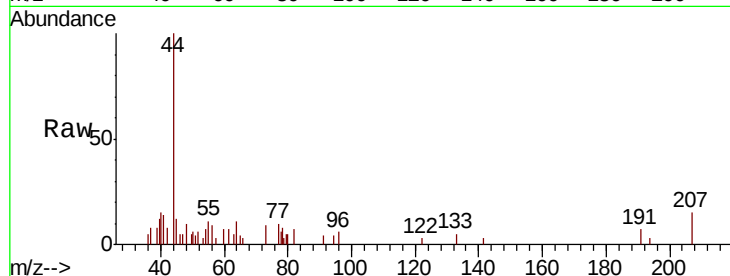

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

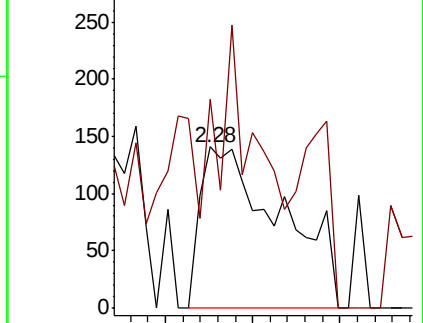

#16

Acetone

Concen: 11.022 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX017074.D


Acq: 01 Jul 2020 03:24

Tgt Ion: 43 Resp: 11642

Ion Ratio Lower Upper



43 100


58 27.8 25.7 38.5



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




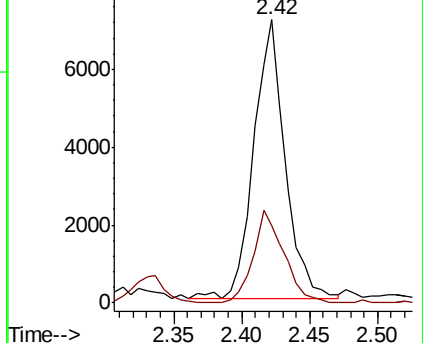




#18
Methyl Acetate
Concen: 1.159 ug/l
RT: 2.75 min Scan# 273
Delta R.T. 0.01 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24




Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#10


Tot Ion: 43 Resp: 3196
Ion Ratio Lower Upper
43 100
74 29.5 19.3 28.9#

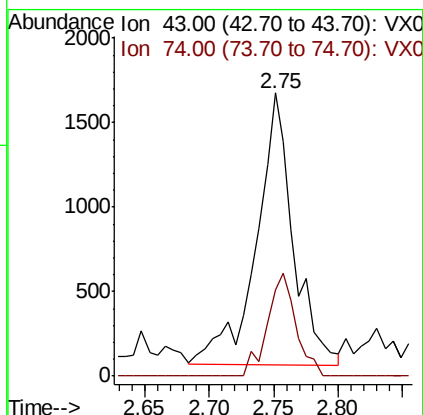

#20
Methylene Chloride
Concen: 4.395 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24

Tgt Ion: 84 Resp: 12377
Ion Ratio Lower Upper
84 100
49 122.7 94.7 142.1
51 38.0 28.6 42.8
86 61.0 50.5 75.7



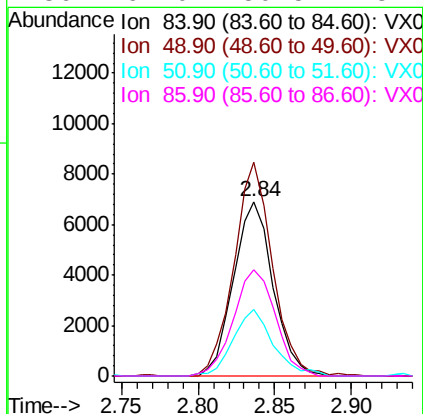





#25
2-Butanone
Concen: 2.636 ug/l
RT: 4.65 min Scan# 585
Delta R.T. 0.02 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24




Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#10


Tot Ion: 43 Resp: 4640
Ion Ratio Lower Upper
43 100
72 21.9 20.8 31.2

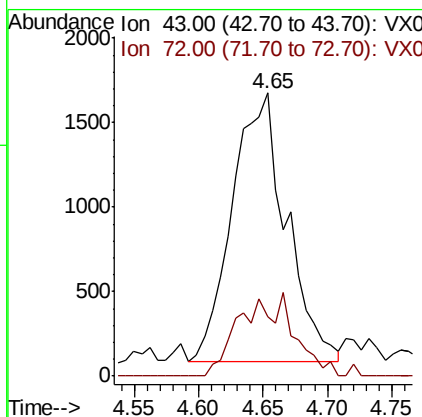

#29
Tetrahydrofuran
Concen: 0.271 ug/l
RT: 5.10 min Scan# 659
Delta R.T. 0.02 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24

Tgt Ion: 42 Resp: 315
Ion Ratio Lower Upper
42 100
72 112.1 35.3 52.9#
71 53.7 33.1 49.7#

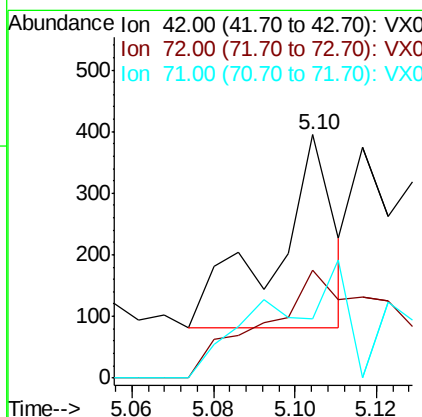

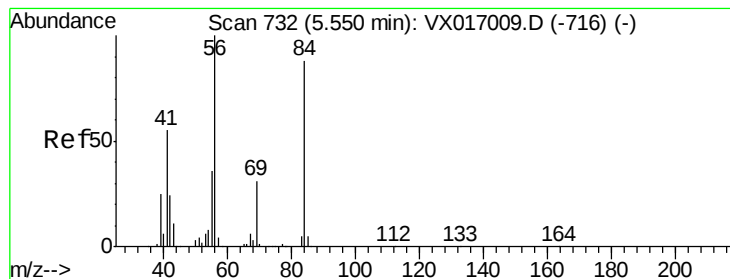

#31

Cyclohexane

Concen: 1.259 ug/l

RT: 5.63 min Scan# 746

Delta R.T. 0.08 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :

PB129852ZHE#10


Tot Ion: 56 Resp: 4800

Ion Ratio Lower Upper

56 100

69 168.1 25.0 37.4#




84 112.0 69.1 103.7#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

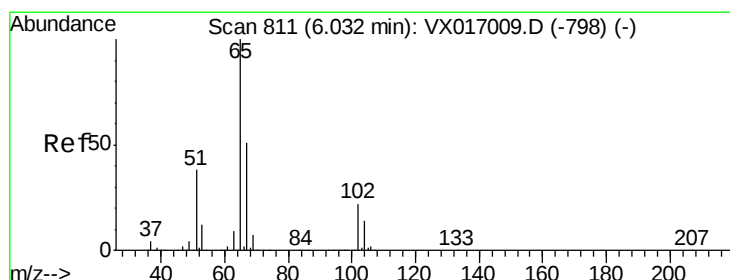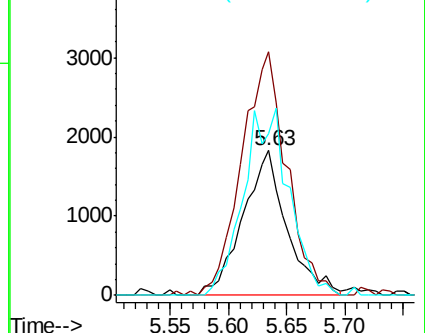

#33

1,2-Dichloroethane-d4

Concen: 54.684 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX017074.D


Acq: 01 Jul 2020 03:24

Tgt Ion: 65 Resp: 154400

Ion Ratio Lower Upper



65 100


67 51.1 0.0 103.8



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

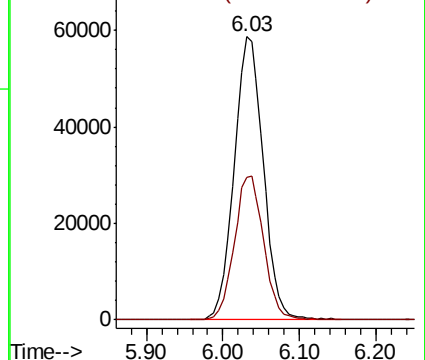

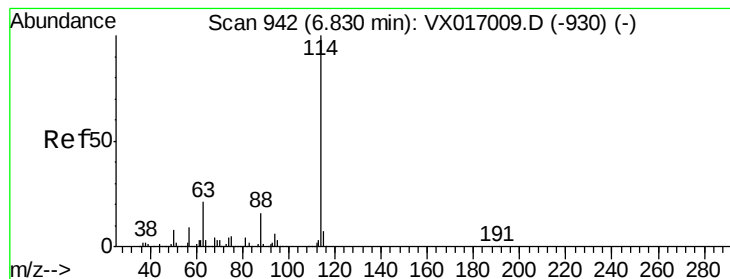

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 943

Delta R.T. 0.01 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :

PB129852ZHE#10


Tot Ion:114 Resp: 395971

Ion Ratio Lower Upper

114 100

63 19.4 0.0 41.4




88 15.4 0.0 32.4



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

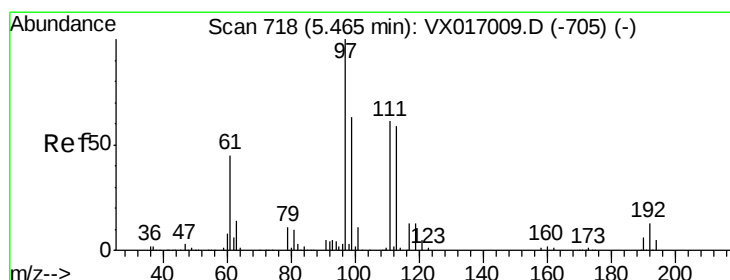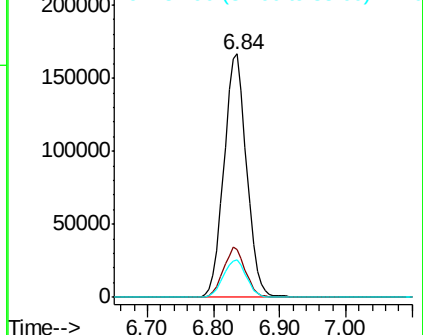

#35

Dibromofluoromethane

Concen: 53.181 ug/l

RT: 5.47 min Scan# 719

Delta R.T. 0.01 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24


Tgt Ion:113 Resp: 133208

Ion Ratio Lower Upper

113 100

111 101.3 81.9 122.9



192 20.5 16.7 25.1




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

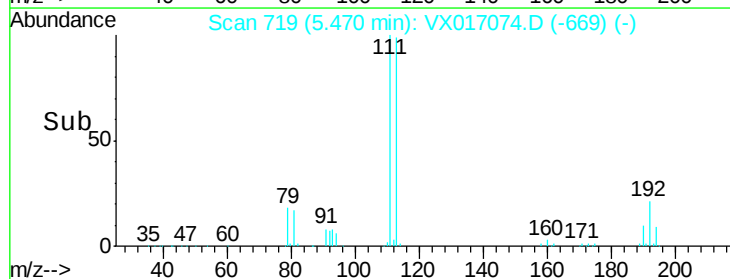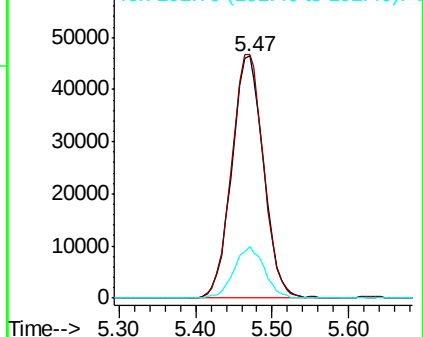

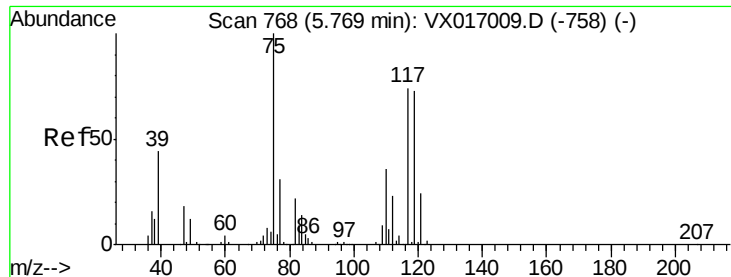

#36

1,1-Dichloropropene

Concen: 4.451 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.14 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :

PB129852ZHE#10


Tot Ion: 75 Resp: 16659

Ion Ratio Lower Upper

75 100

110 10.1 18.1 54.1#




77 0.5 24.6 37.0#

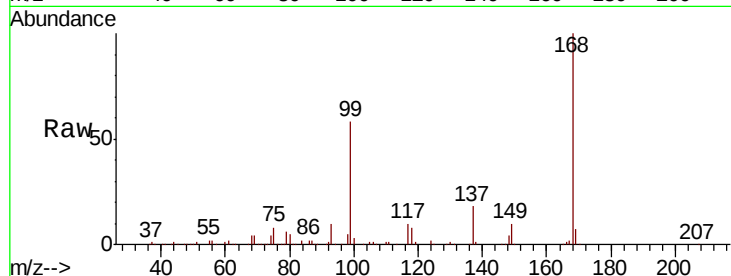

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

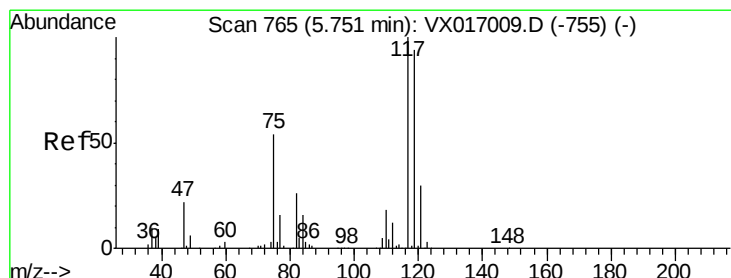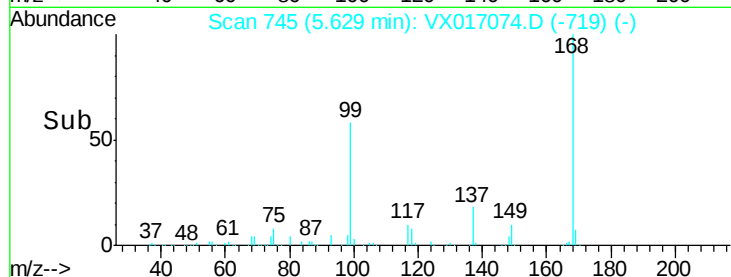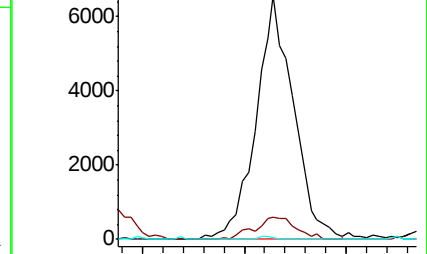

#38

Carbon Tetrachloride

Concen: 5.389 ug/l

RT: 5.63 min Scan# 746

Delta R.T. -0.12 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24


Tgt Ion:117 Resp: 22215

Ion Ratio Lower Upper

117 100

119 8.7 75.4 113.0#



121 0.0 23.8 35.6#

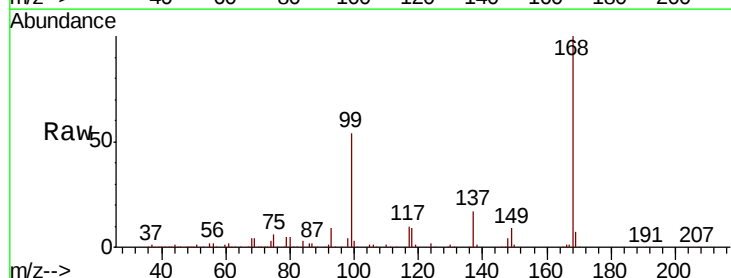


Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

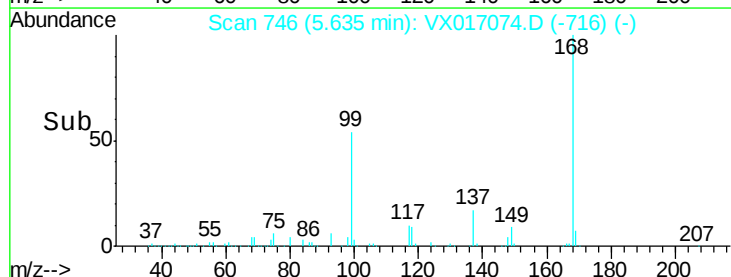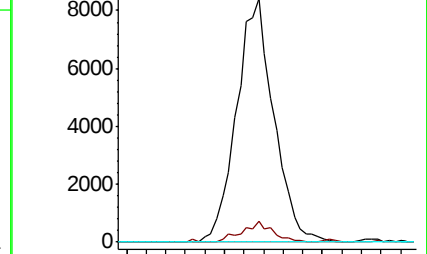

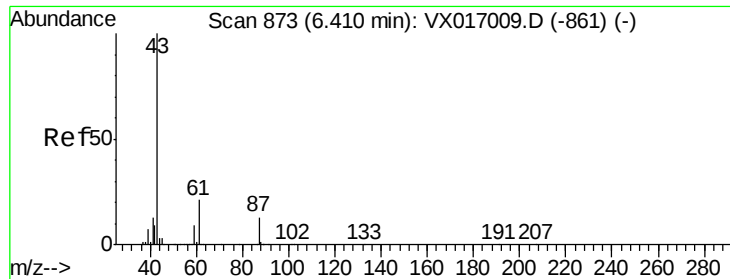

#43

Isopropyl Acetate

Concen: 9.320 ug/l

RT: 6.42 min Scan# 874

Delta R.T. 0.01 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :

PB129852ZHE#10


Tot Ion: 43 Resp: 58804

Ion Ratio Lower Upper

43 100

61 20.9 16.2 24.2




87 13.6 10.7 16.1



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

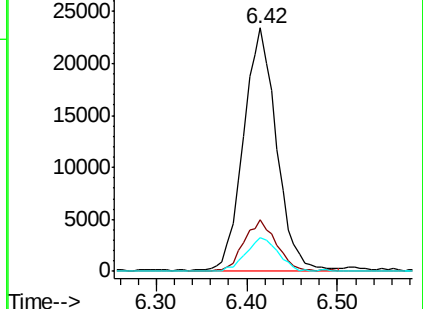

#48

Methyl methacrylate

Concen: 1.318 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.09 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24


Tgt Ion: 41 Resp: 3951

Ion Ratio Lower Upper

41 100

69 0.0 65.8 98.8#



39 0.0 42.5 63.7#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

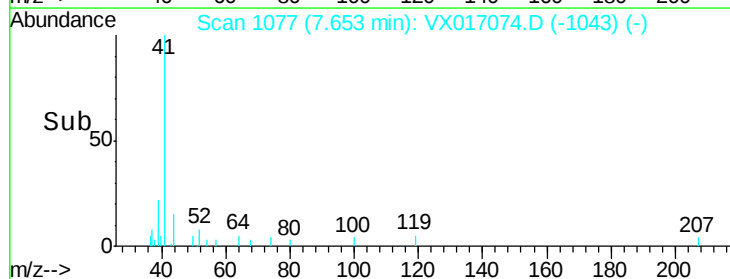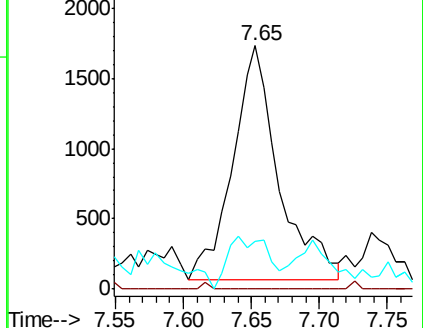


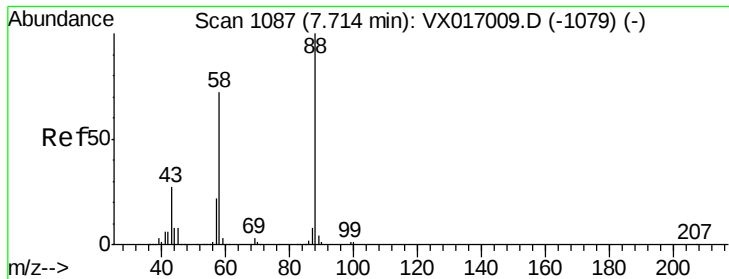




#49
1,4-Dioxane
Concen: 0.751 ug/l
RT: 7.74 min Scan# 1092
Delta R.T. 0.03 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24

Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#10

Tot Ion: 88 Resp: 51
Ion Ratio Lower Upper
88 100
43 0.0 25.8 38.8#
58 1078.4 54.8 82.2#

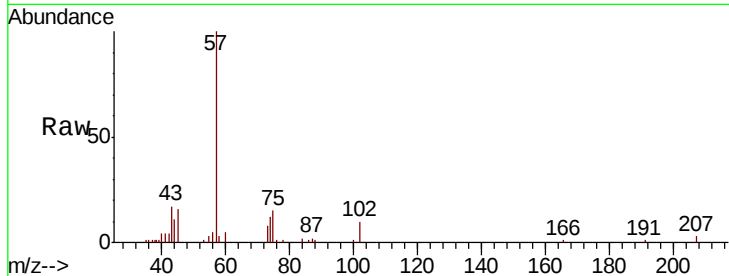


Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0

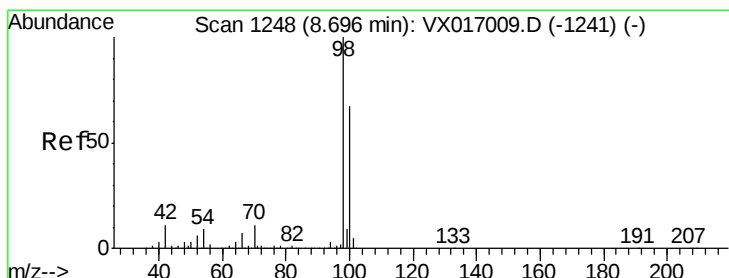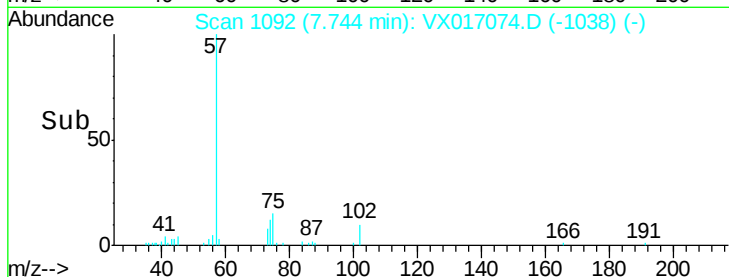
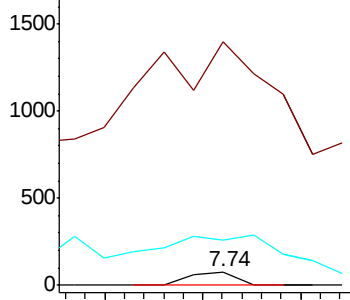



#50
Toluene-d8
Concen: 53.539 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24

Tgt Ion: 98 Resp: 495886
Ion Ratio Lower Upper
98 100
100 66.4 53.8 80.6

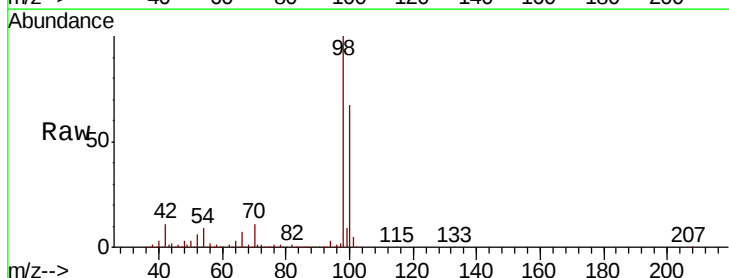

Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): V

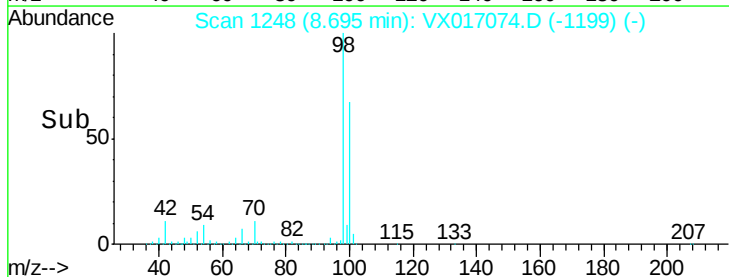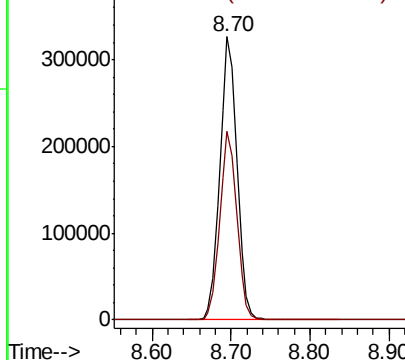



#51

4-Methyl-2-Pentanone

Concen: 14.815 ug/l

RT: 8.60 min Scan# 1232

Delta R.T. -0.02 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :





PB129852ZHE#10

Tot Ion: 43 Resp: 55720

Ion Ratio Lower Upper

43 100

58 10.7 31.9 47.9#

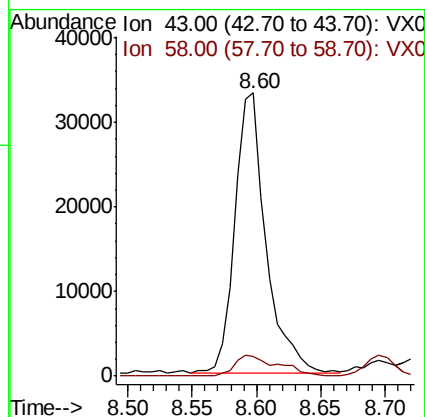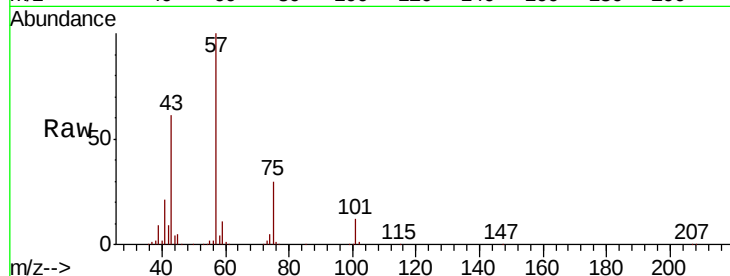

#54

cis-1,3-Dichloropropene

Concen: 5.515 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24




Tgt Ion: 75 Resp: 25919


Ion Ratio Lower Upper

75 100

77 1.0 25.2 37.8#

39 30.4 37.4 56.2#

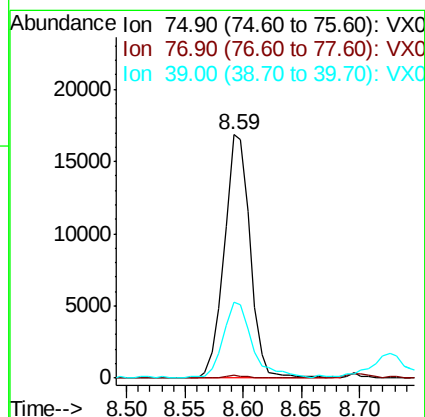

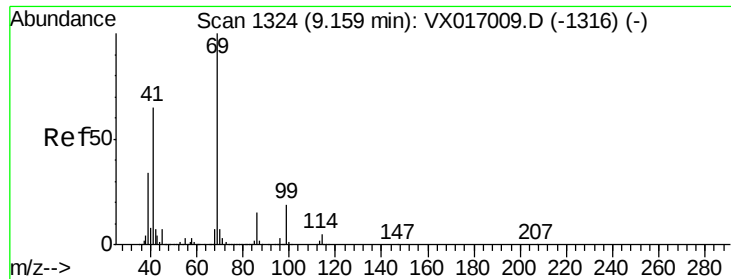

#56

Ethyl methacrylate

Concen: 0.361 ug/l

RT: 9.29 min Scan# 1345

Delta R.T. 0.13 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :

PB129852ZHE#10


Tot Ion: 69 Resp: 1443

Ion Ratio Lower Upper

69 100

41 3312.4 53.6 80.4#




39 1369.2 28.2 42.2#

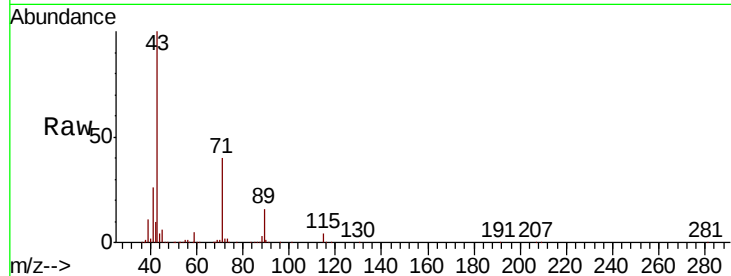

Abundance Ion 69.00 (68.70 to 69.70): VX0

Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

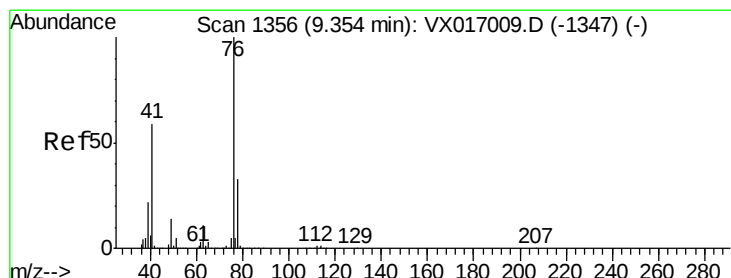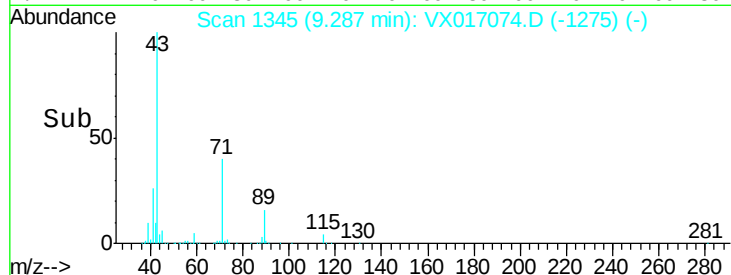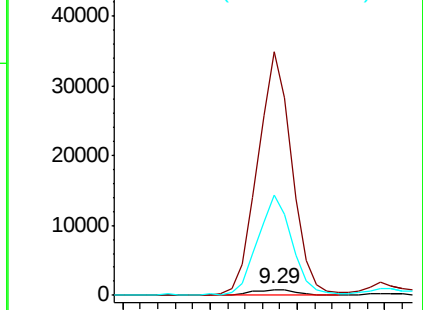

#57

1,3-Dichloropropane

Concen: 1.100 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX017074.D


Acq: 01 Jul 2020 03:24

Tgt Ion: 76 Resp: 5221

Ion Ratio Lower Upper



76 100


78 2.1 25.9 38.9#

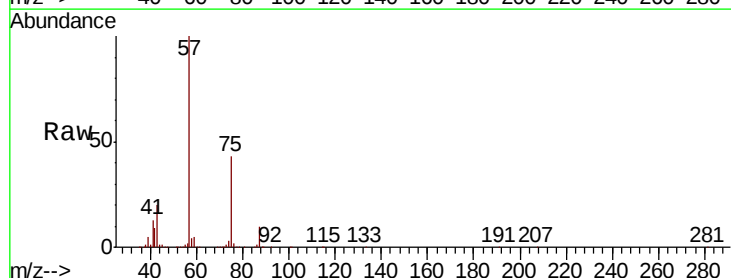

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0



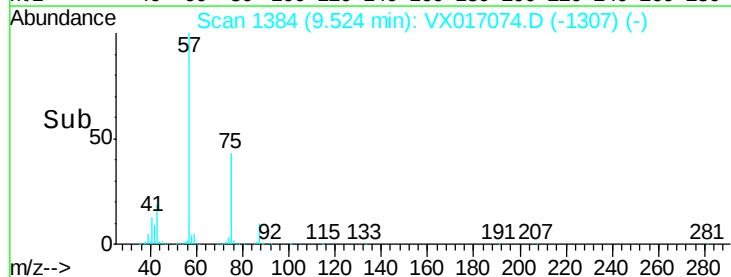
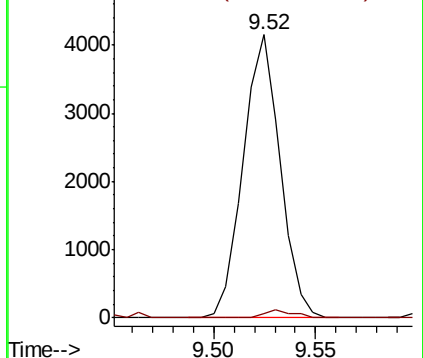




#59
2-Hexanone
Concen: 23.548 ug/l
RT: 9.52 min Scan# 1384
Delta R.T. 0.05 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24




Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#10


Tot Ion: 43 Resp: 64683
Ion Ratio Lower Upper
43 100
58 19.8 27.9 83.6#

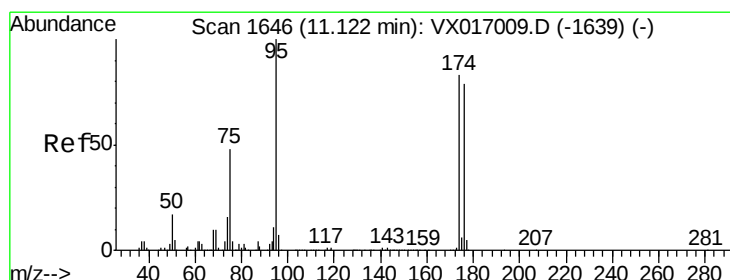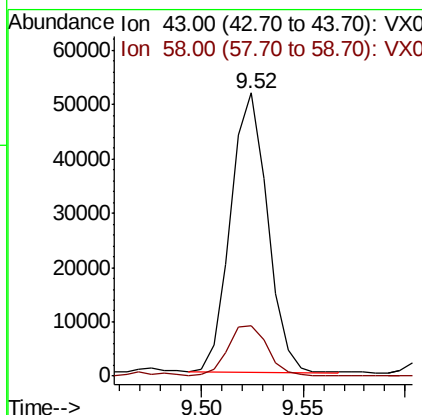

#62
4-Bromofluorobenzene
Concen: 56.816 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24

Tgt Ion: 95 Resp: 205716
Ion Ratio Lower Upper
95 100
174 84.4 0.0 164.0
176 79.6 0.0 157.6



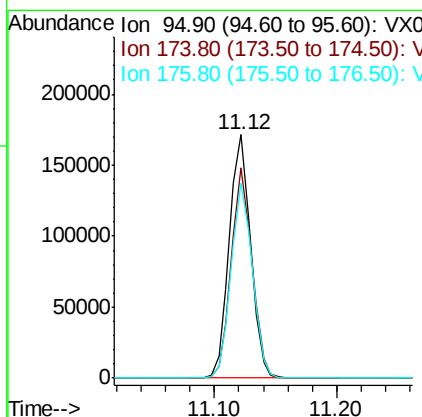





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24




Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#10


Tot Ion:117 Resp: 423954
Ion Ratio Lower Upper
117 100
82 52.2 42.6 63.8
119 32.7 25.4 38.2

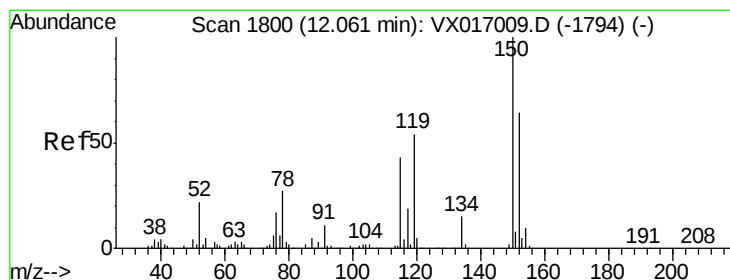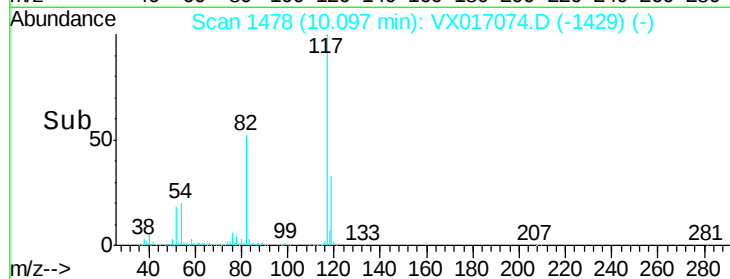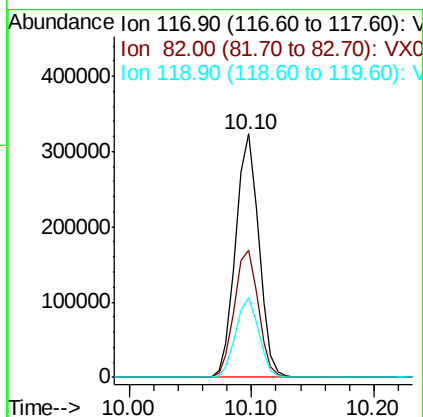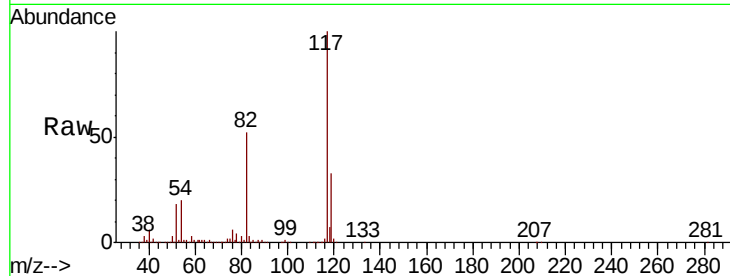

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX017074.D
Acq: 01 Jul 2020 03:24

Tgt Ion:152 Resp: 219654
Ion Ratio Lower Upper
152 100
115 57.4 40.9 122.7
150 156.4 0.0 351.6

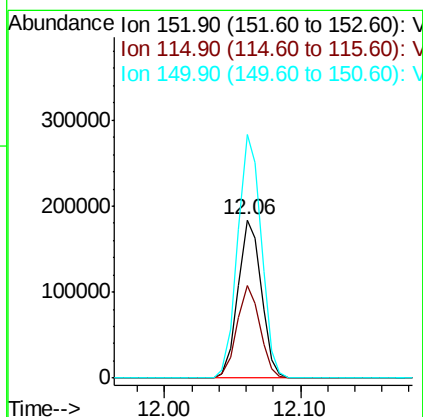

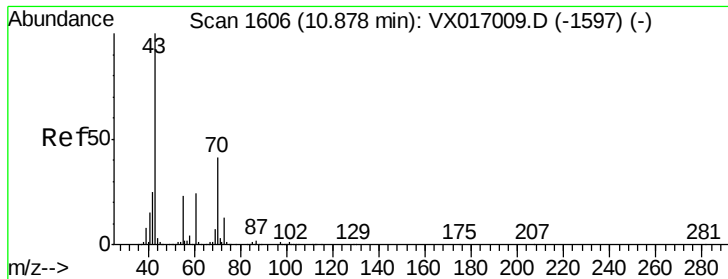

#74

N-amvl acetate

Concen: 0.494 ug/l

RT: 10.80 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :

PB129852ZHE#10

Tot Ion: 43 Resp: 3030


Ion Ratio Lower Upper

43 100

70 0.0 34.2 51.2#

55 16.9 19.2 28.8#

61 0.0 19.6 29.4#



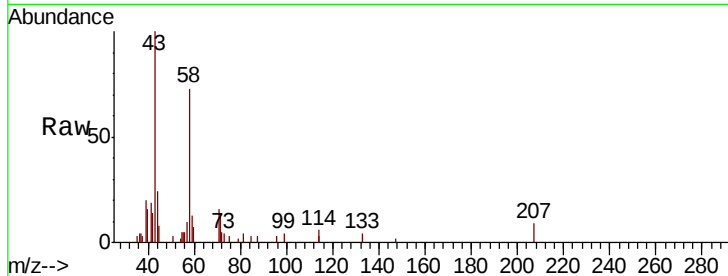


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

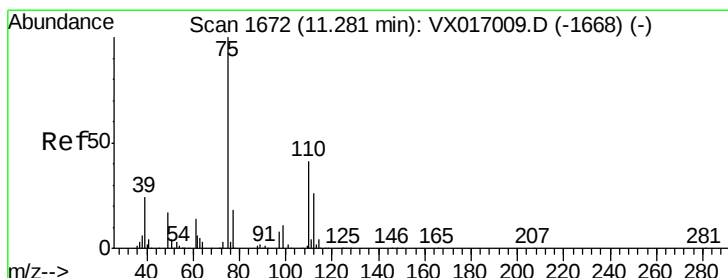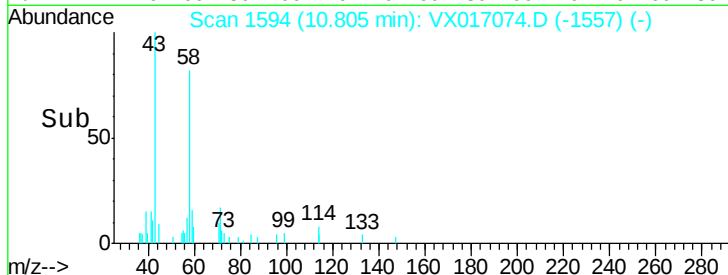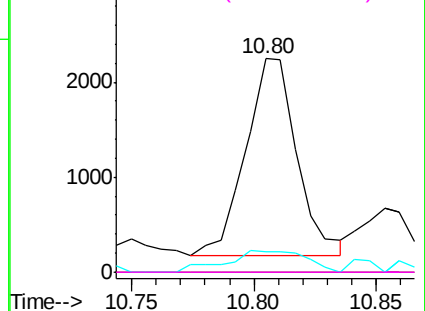

#76

1,2,3-Trichloropropane

Concen: 24.109 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017074.D


Acq: 01 Jul 2020 03:24

Tgt Ion: 75 Resp: 104137

Ion Ratio Lower Upper



75 100


77 1.2 20.2 60.6#

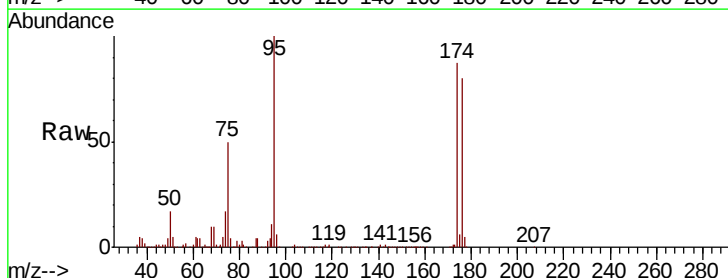

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



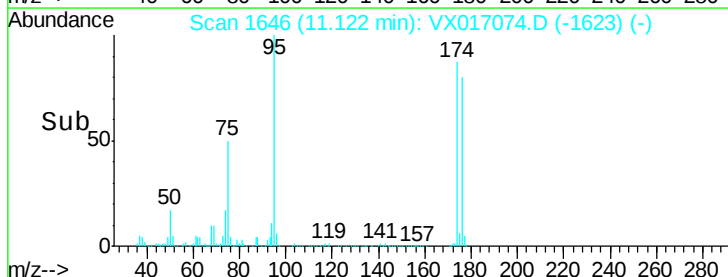
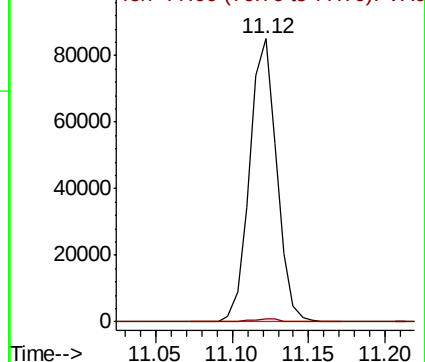


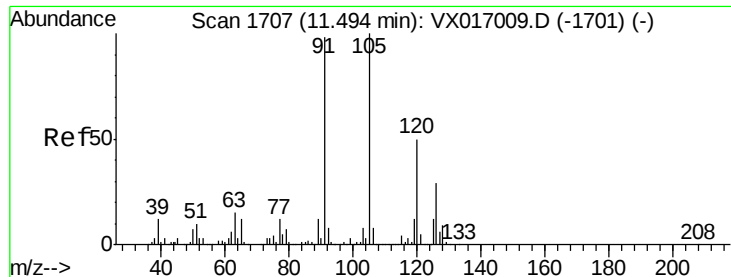

#80
 1,3,5-Trimethylbenzene
 Concen: 0.236 ug/l
 RT: 11.49 min Scan# 1707
 Delta R.T. -0.00 min
 Lab File: VX017074.D
 Acq: 01 Jul 2020 03:24




Instrument :
 MSVOA_X
 ClientSampleId :
 PB129852ZHE#10


Tot Ion:105 Resp: 2814
 Ion Ratio Lower Upper
 105 100
 120 47.1 24.9 74.6

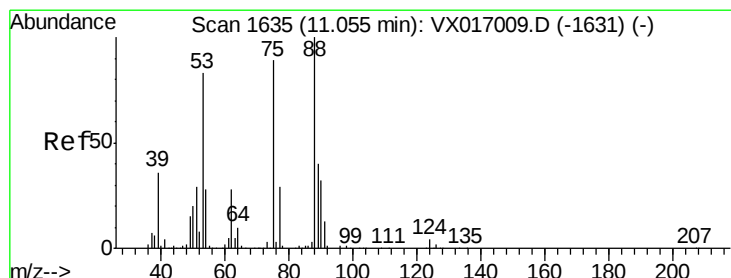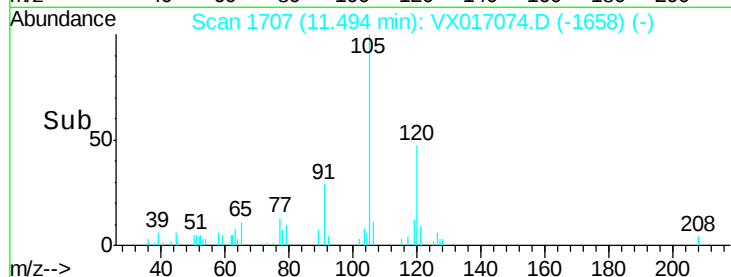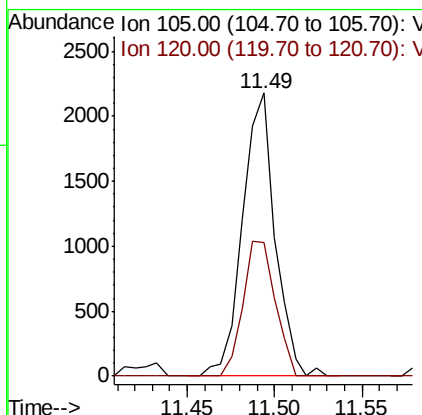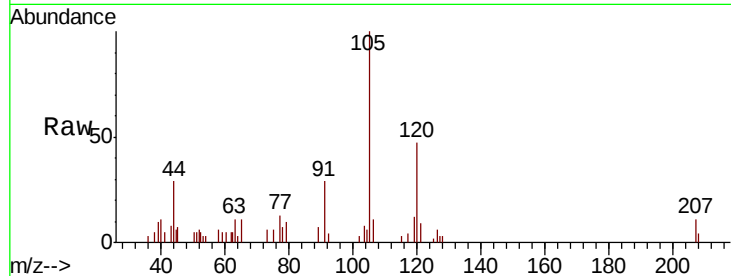

#81
 trans-1,4-Dichloro-2-butene
 Concen: 62.434 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. 0.07 min
 Lab File: VX017074.D
 Acq: 01 Jul 2020 03:24

Tgt Ion: 75 Resp: 104137
 Ion Ratio Lower Upper
 75 100
 53 0.2 72.4 108.6#
 89 0.0 37.0 55.4#

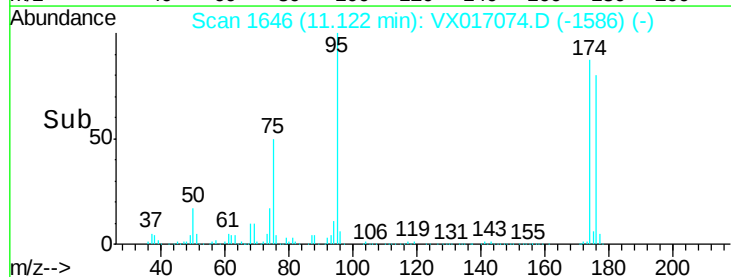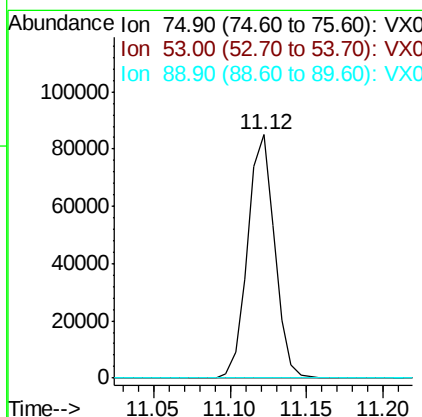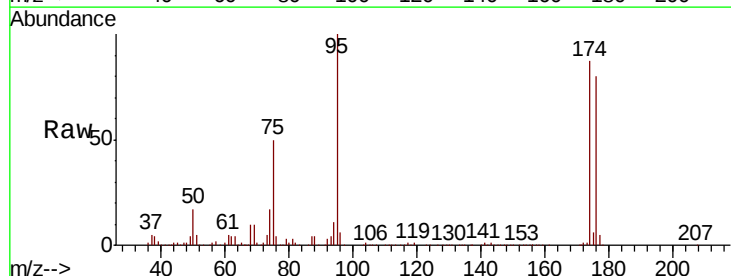

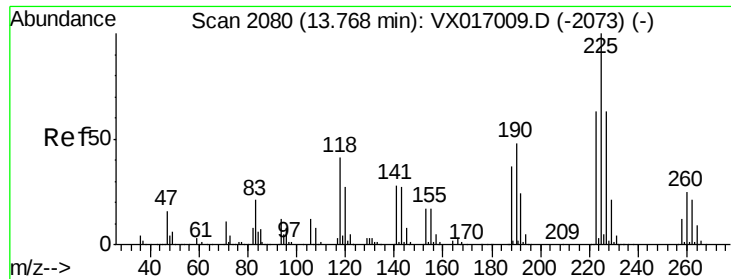

#94

Hexachlorobutadiene

Concen: 0.928 ug/l

RT: 13.77 min Scan# 2081

Delta R.T. 0.01 min

Lab File: VX017074.D

Acq: 01 Jul 2020 03:24

Instrument :

MSVOA_X

ClientSampleId :

PB129852ZHE#10


Tot Ion:225 Resp: 149

Ion Ratio Lower Upper

225 100

223 61.7 32.5 97.5

227 45.6 33.1 99.2

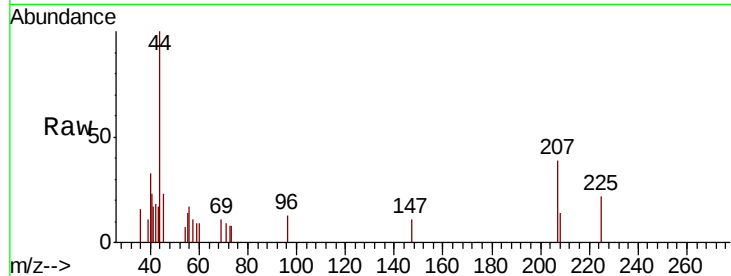

Abundance Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

