

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX063020\
 Data File : VX017069.D
 Acq On : 01 Jul 2020 01:30
 Operator : JC/SP
 Sample : PB129852ZHE#05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB129852ZHE#05

Quant Time: Jul 01 08:48:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 29 17:10:38 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	225948	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	392122	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	413359	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	215538	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	150341	53.97	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.94%	
35) Dibromofluoromethane	5.47	113	129045	52.02	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.04%	
50) Toluene-d8	8.70	98	493943	53.85	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.70%	
62) 4-Bromofluorobenzene	11.12	95	207800	57.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	115.92%	
Target Compounds						
16) Acetone	2.42	43	15111	14.502	ug/l	98
18) Methyl Acetate	2.76	43	3617	1.330	ug/l	96
20) Methylene Chloride	2.84	84	6289	1.878	ug/l #	91
43) Isopropyl Acetate	6.42	43	76636	12.265	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX063020\
Data File : VX017069.D
Acq On : 01 Jul 2020 01:30
Operator : JC/SP
Sample : PB129852ZHE#05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#05

Quant Time: Jul 01 08:48:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 29 17:10:38 2020
Response via : Initial Calibration

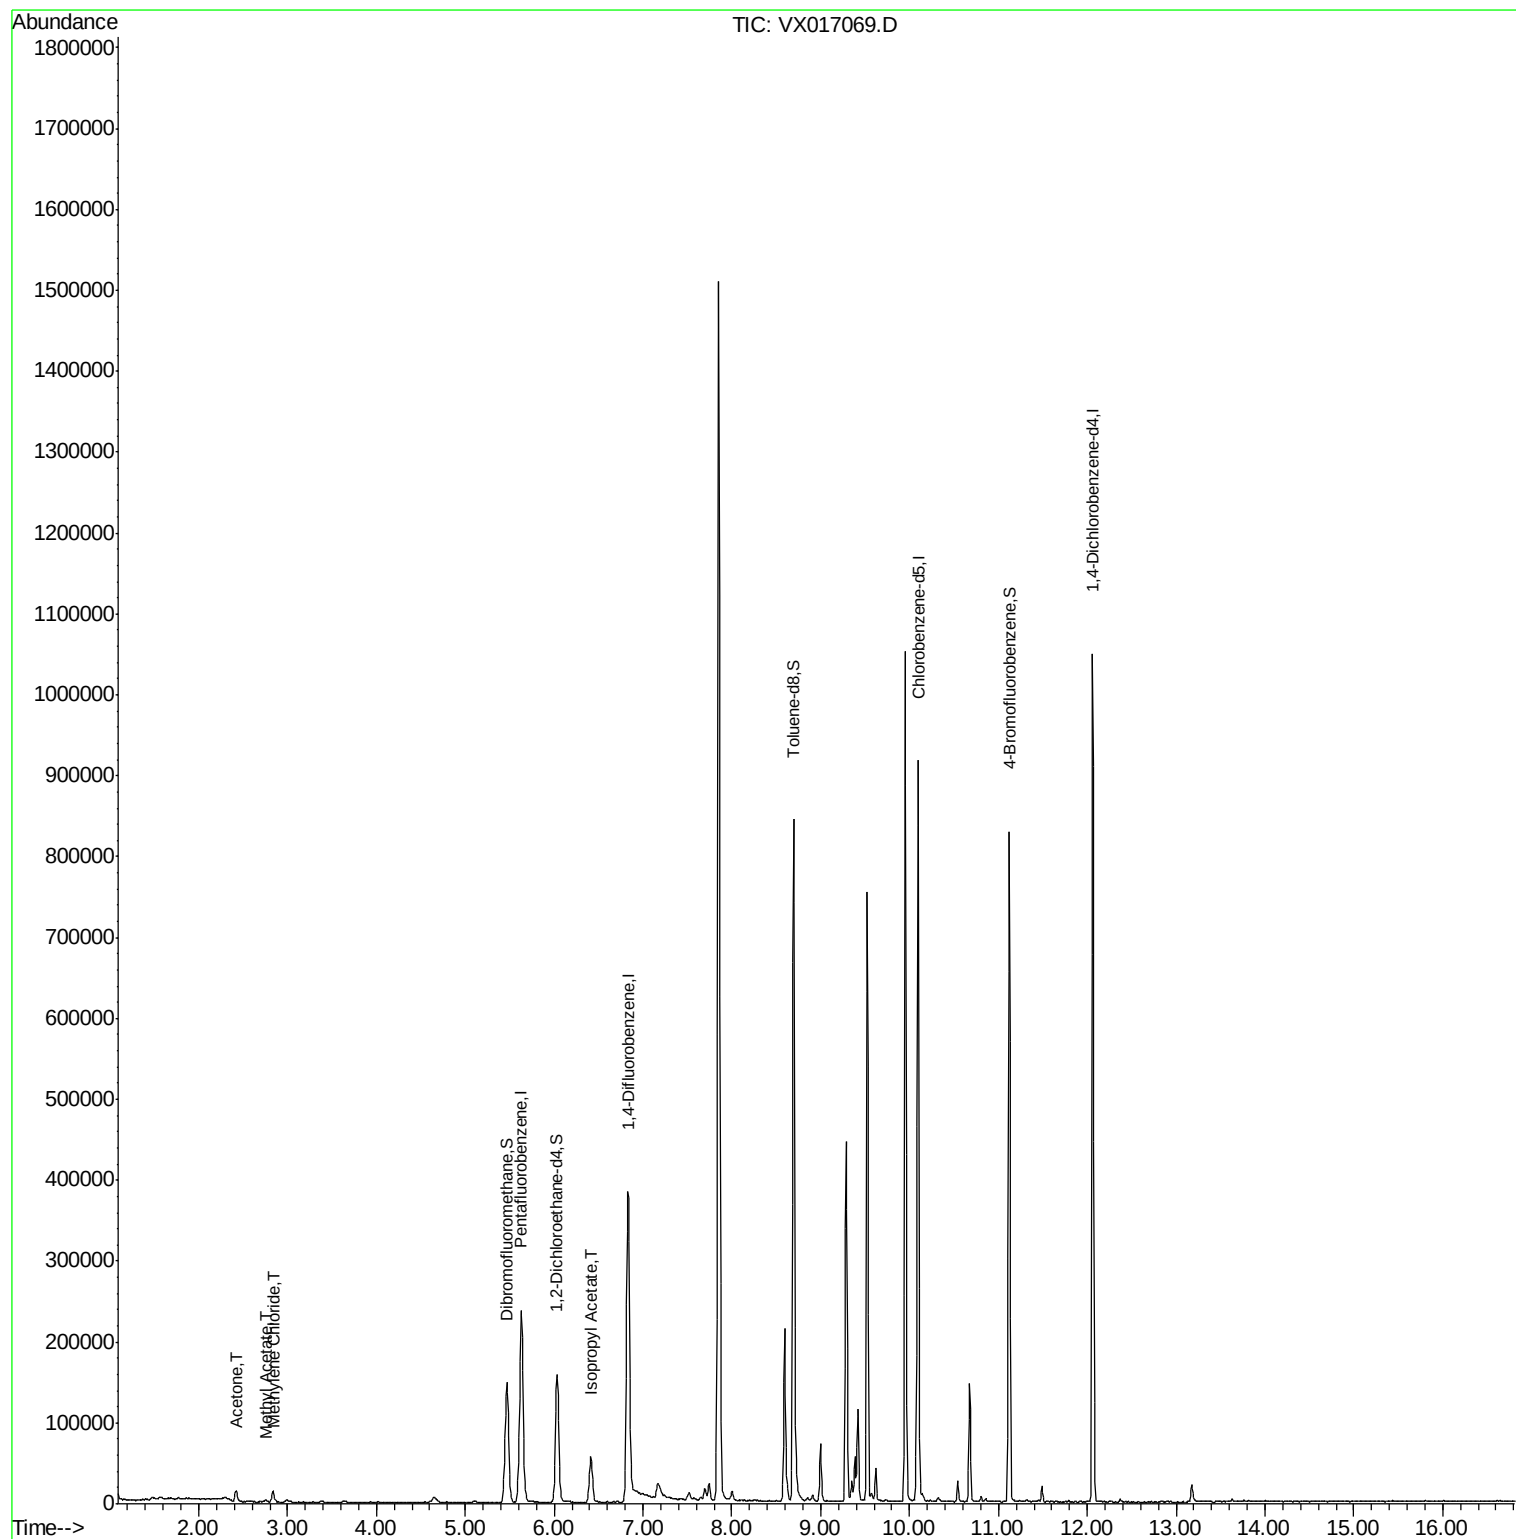

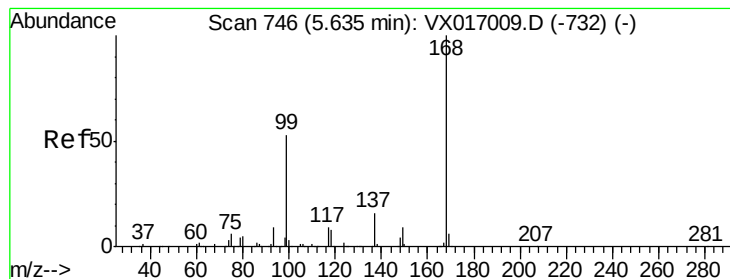

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017069.D

Acq: 01 Jul 2020 01:30

Instrument :

MSVOA_X

ClientSampleId :


PB129852ZHE#05

Tot Ion:168 Resp: 225948

Ion Ratio Lower Upper




168 100

99 57.9 42.6 64.0

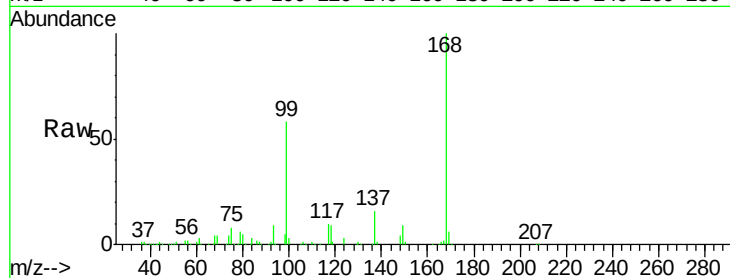

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

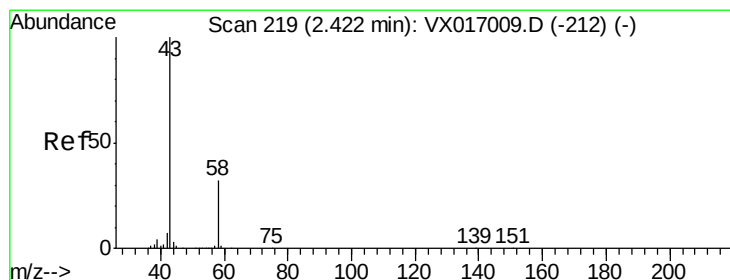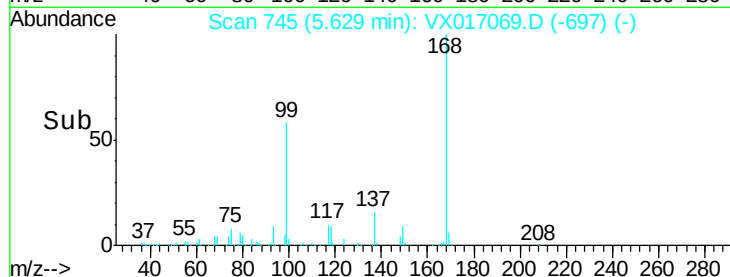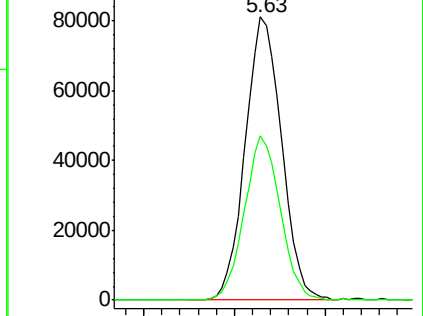

#16

Acetone

Concen: 14.502 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX017069.D


Acq: 01 Jul 2020 01:30

Tgt Ion: 43 Resp: 15111

Ion Ratio Lower Upper



43 100


58 33.0 25.7 38.5

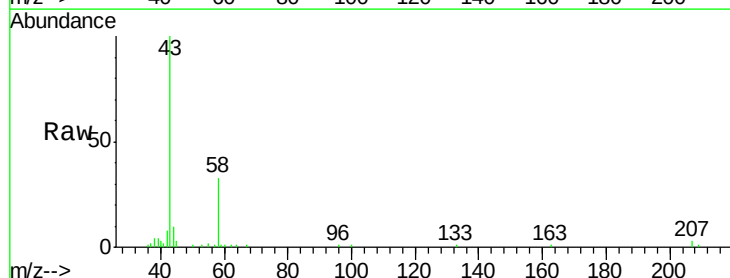

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



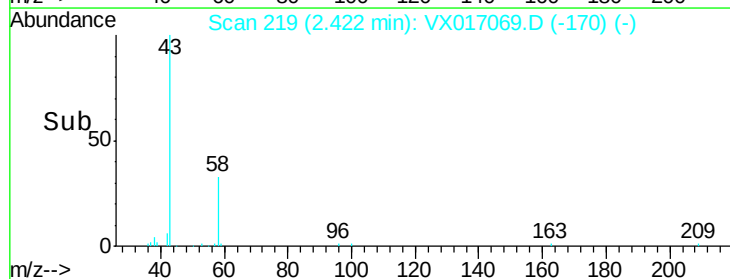
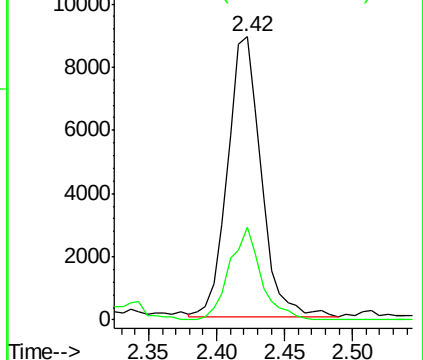


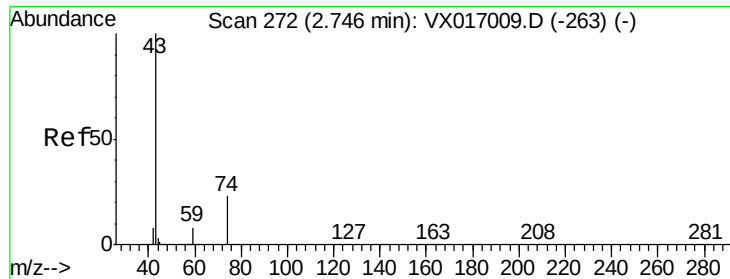

#18
Methyl Acetate
Concen: 1.330 ug/l
RT: 2.76 min Scan# 274
Delta R.T. 0.01 min
Lab File: VX017069.D
Acq: 01 Jul 2020 01:30




Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#05


Tot Ion: 43 Resp: 3617
Ion Ratio Lower Upper
43 100
74 26.2 19.3 28.9

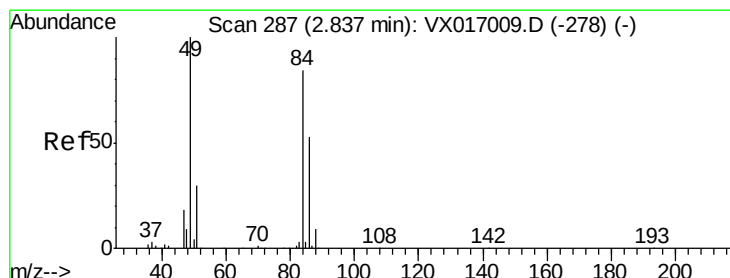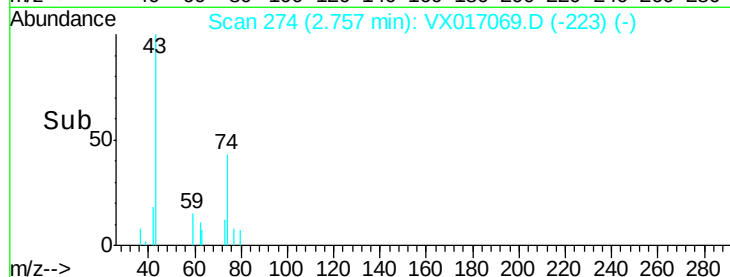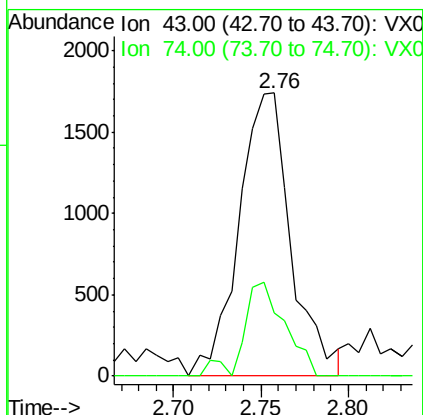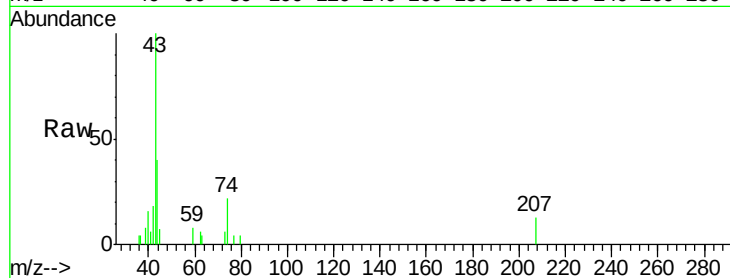

#20
Methylene Chloride
Concen: 1.878 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017069.D
Acq: 01 Jul 2020 01:30

Tgt Ion: 84 Resp: 6289
Ion Ratio Lower Upper
84 100
49 131.9 94.7 142.1
51 43.1 28.6 42.8#
86 63.5 50.5 75.7


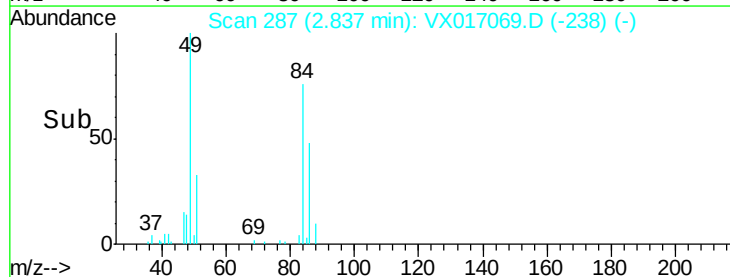
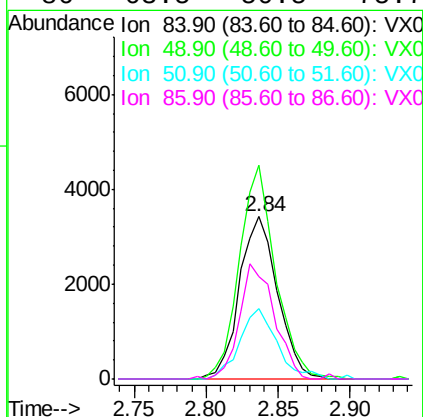
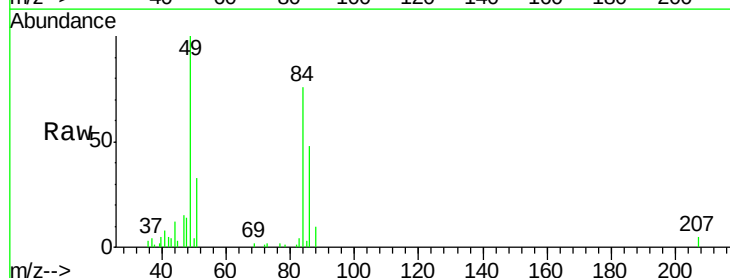


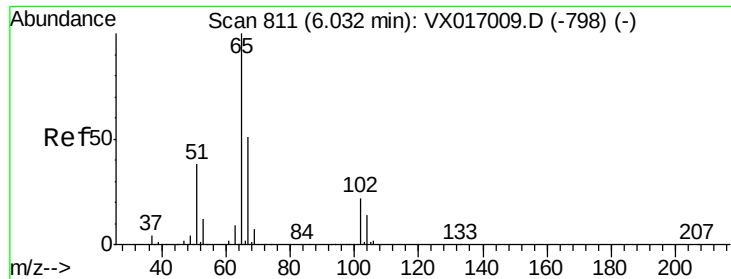

#33
 1,2-Dichloroethane-d4
 Concen: 53.973 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: VX017069.D
 Acq: 01 Jul 2020 01:30




Instrument :
 MSVOA_X
 ClientSampleId :
 PB129852ZHE#05


Tot Ion: 65 Resp: 150341
 Ion Ratio Lower Upper
 65 100
 67 51.8 0.0 103.8

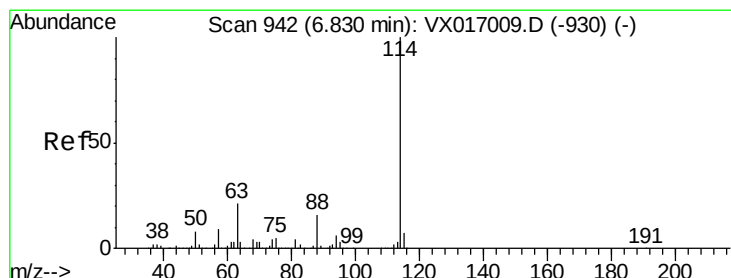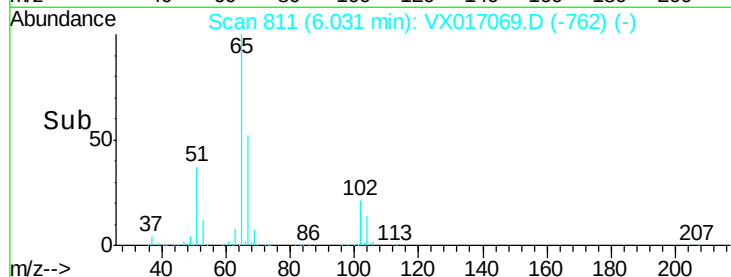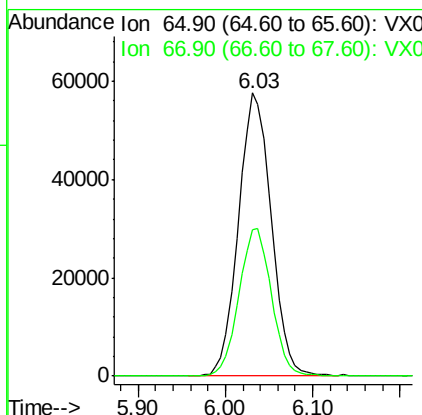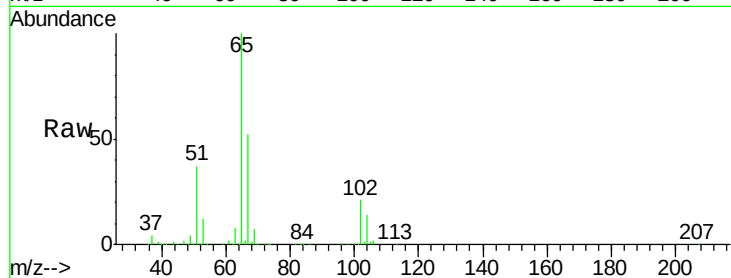

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. -0.00 min
 Lab File: VX017069.D
 Acq: 01 Jul 2020 01:30

Tgt Ion: 114 Resp: 392122
 Ion Ratio Lower Upper
 114 100
 63 19.9 0.0 41.4
 88 16.0 0.0 32.4

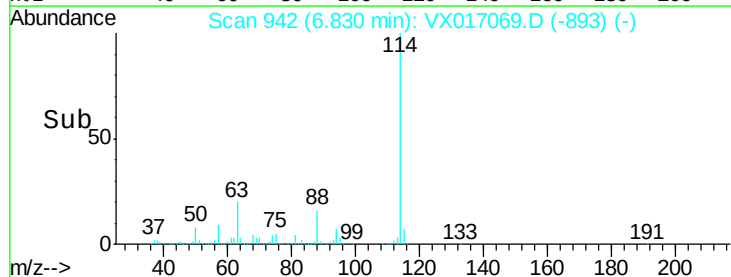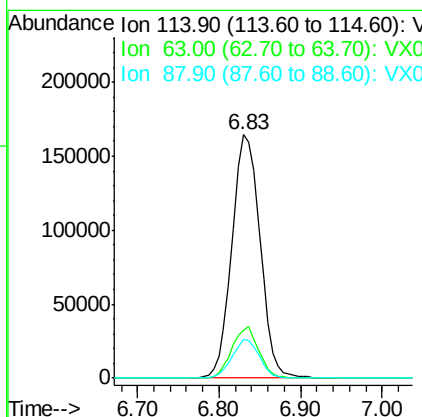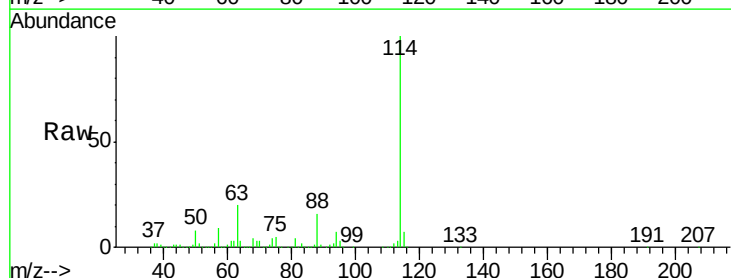

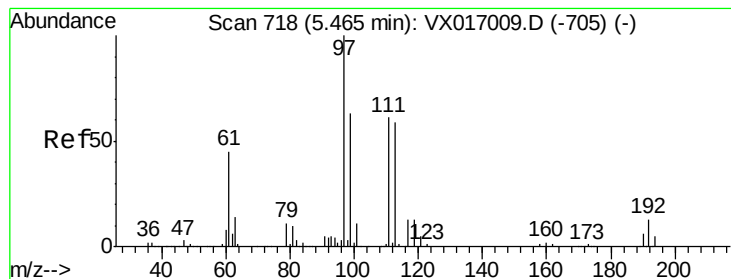

#35

Dibromofluoromethane

Concen: 52.025 ug/l

RT: 5.47 min Scan# 719

Delta R.T. 0.01 min

Lab File: VX017069.D

Acq: 01 Jul 2020 01:30

Instrument :

MSVOA_X

ClientSampleId :

PB129852ZHE#05


Tot Ion:113 Resp: 129045

Ion Ratio Lower Upper

113 100

111 102.9 81.9 122.9




192 21.3 16.7 25.1

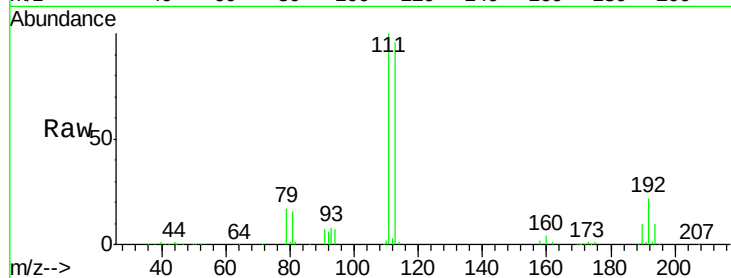

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

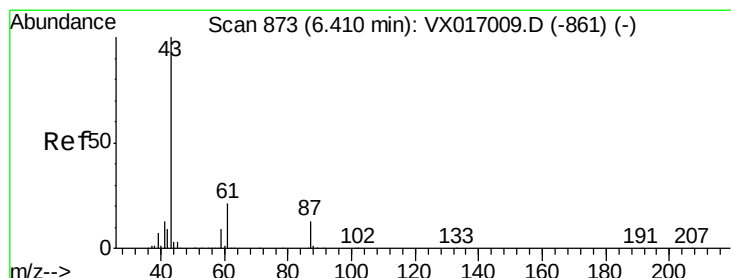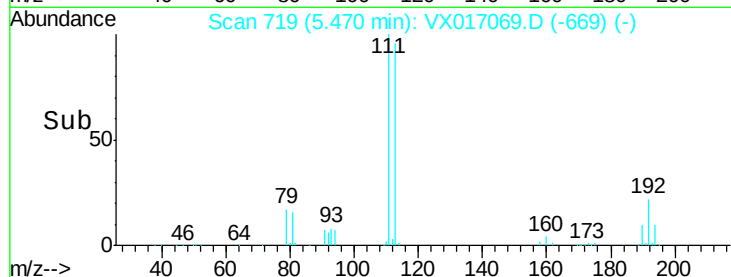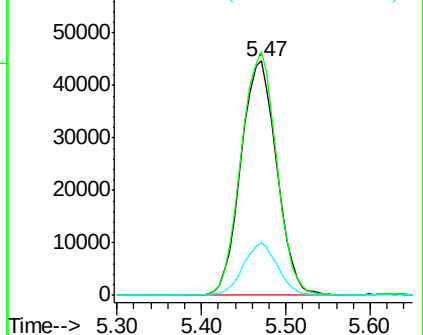

#43

Isopropyl Acetate

Concen: 12.265 ug/l

RT: 6.42 min Scan# 874

Delta R.T. 0.01 min

Lab File: VX017069.D

Acq: 01 Jul 2020 01:30


Tgt Ion: 43 Resp: 76636

Ion Ratio Lower Upper

43 100

61 20.1 16.2 24.2



87 14.4 10.7 16.1

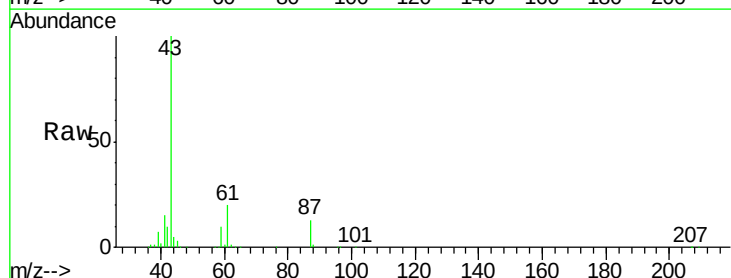


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

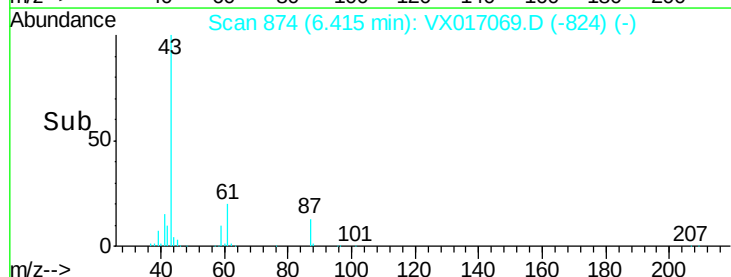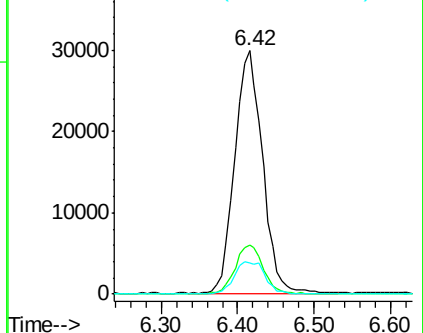

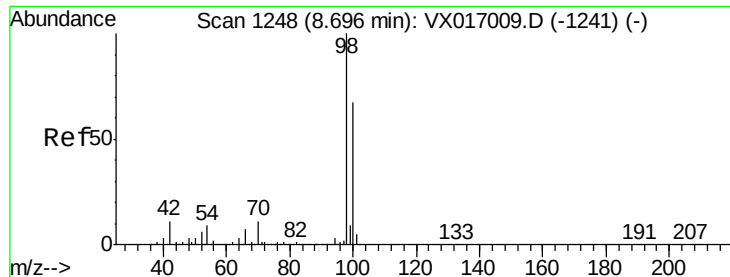

#50

Toluene-d8

Concen: 53.852 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017069.D

Acq: 01 Jul 2020 01:30

Instrument :

MSVOA_X

ClientSampleId :


PB129852ZHE#05

Tot Ion: 98 Resp: 493943

Ion Ratio Lower Upper




98 100

100 66.4 53.8 80.6

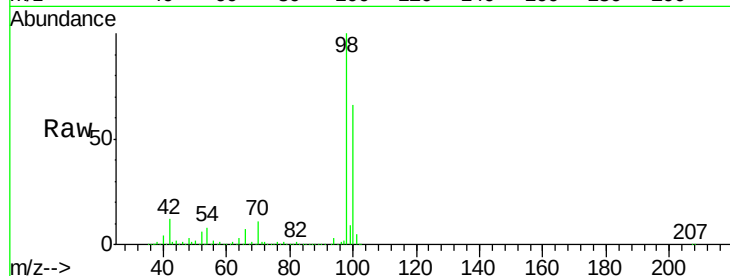

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

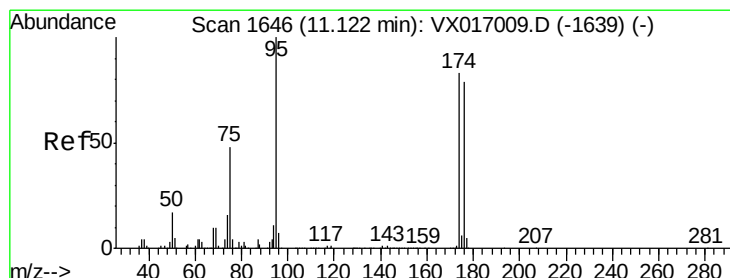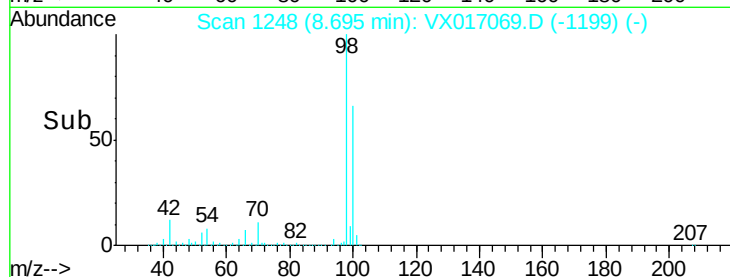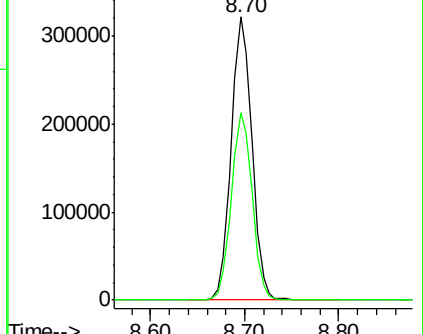

#62

4-Bromofluorobenzene

Concen: 57.955 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX017069.D

Acq: 01 Jul 2020 01:30


Tgt Ion: 95 Resp: 207800

Ion Ratio Lower Upper

95 100

174 82.1 0.0 164.0



176 78.4 0.0 157.6

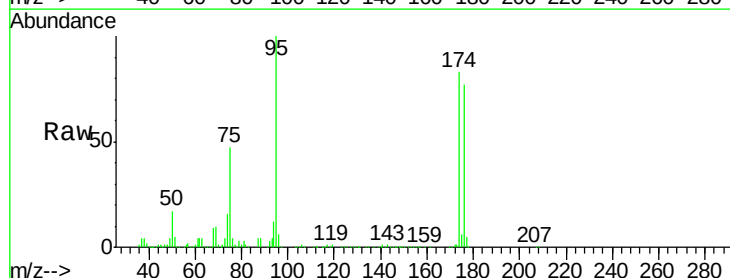


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

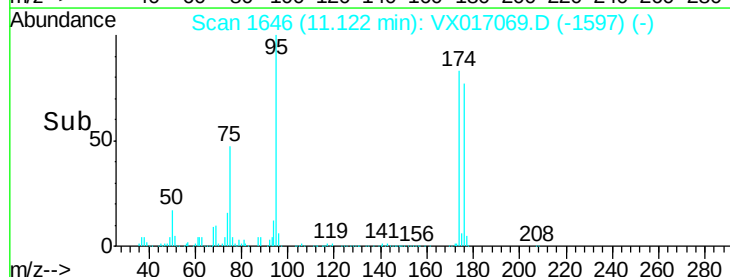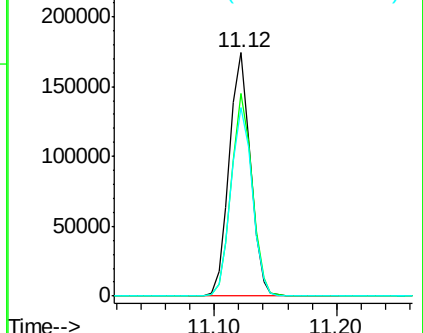


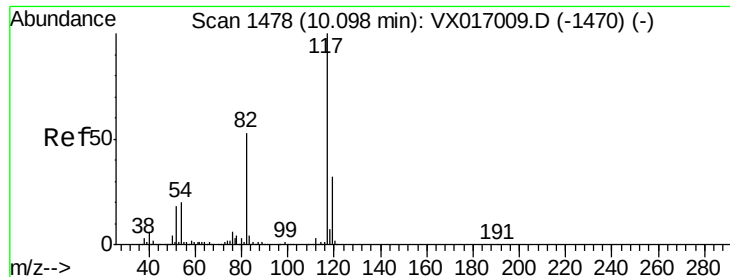




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017069.D
Acq: 01 Jul 2020 01:30

Instrument :
MSVOA_X
ClientSampleId :
PB129852ZHE#05

Tot Ion:117 Resp: 413359
Ion Ratio Lower Upper
117 100
82 54.1 42.6 63.8
119 32.4 25.4 38.2

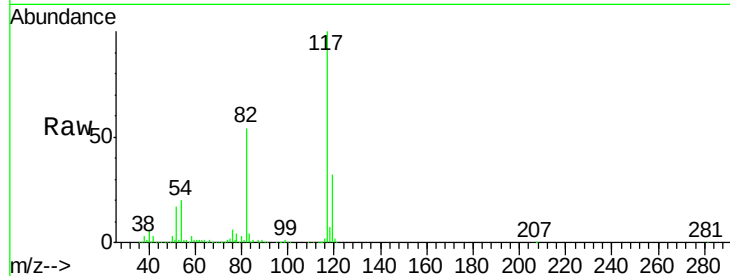


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

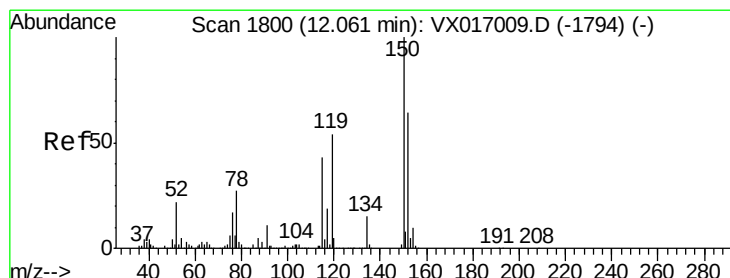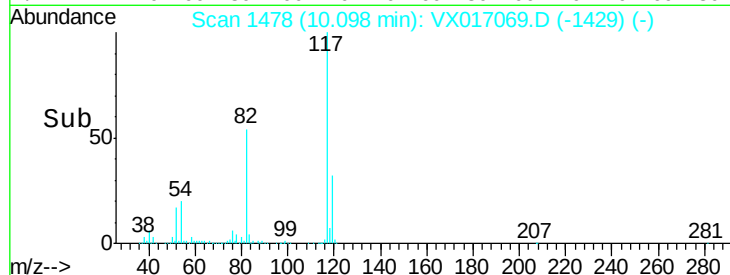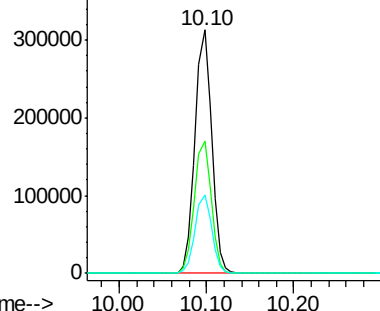

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX017069.D
Acq: 01 Jul 2020 01:30

Tgt Ion:152 Resp: 215538
Ion Ratio Lower Upper
152 100
115 57.7 40.9 122.7
150 158.1 0.0 351.6

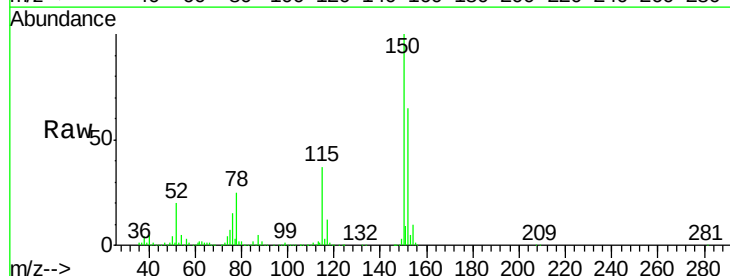

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

