

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
 Data File : VX023030.D
 Acq On : 30 Jun 2021 13:46
 Operator : JC/MD
 Sample : M2872-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX023030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	34	rBV2	11103	10937	2.65%	0.525%
2	1.569	74	79	83	rVB4	3149	5787	1.40%	0.278%
3	2.550	232	240	248	rVB2	2806	5172	1.25%	0.248%
4	5.397	695	707	720	rBV2	45200	128962	31.22%	6.196%
5	5.562	723	734	746	rVB2	74847	205983	49.86%	9.896%
6	5.964	788	800	812	rBV	62156	161729	39.15%	7.770%
7	6.769	922	932	943	rBV	129502	305825	74.03%	14.693%
8	8.653	1233	1241	1254	rBV	270775	413113	100.00%	19.848%
9	10.055	1465	1471	1482	rBV	254911	344378	83.36%	16.545%
10	11.085	1634	1640	1646	rBV	185824	230984	55.91%	11.097%
11	12.024	1789	1794	1802	rVB	222385	268555	65.01%	12.902%


Sum of corrected areas: 2081425

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023030.D
Acq On : 30 Jun 2021 13:46
Operator : JC/MD
Sample : M2872-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

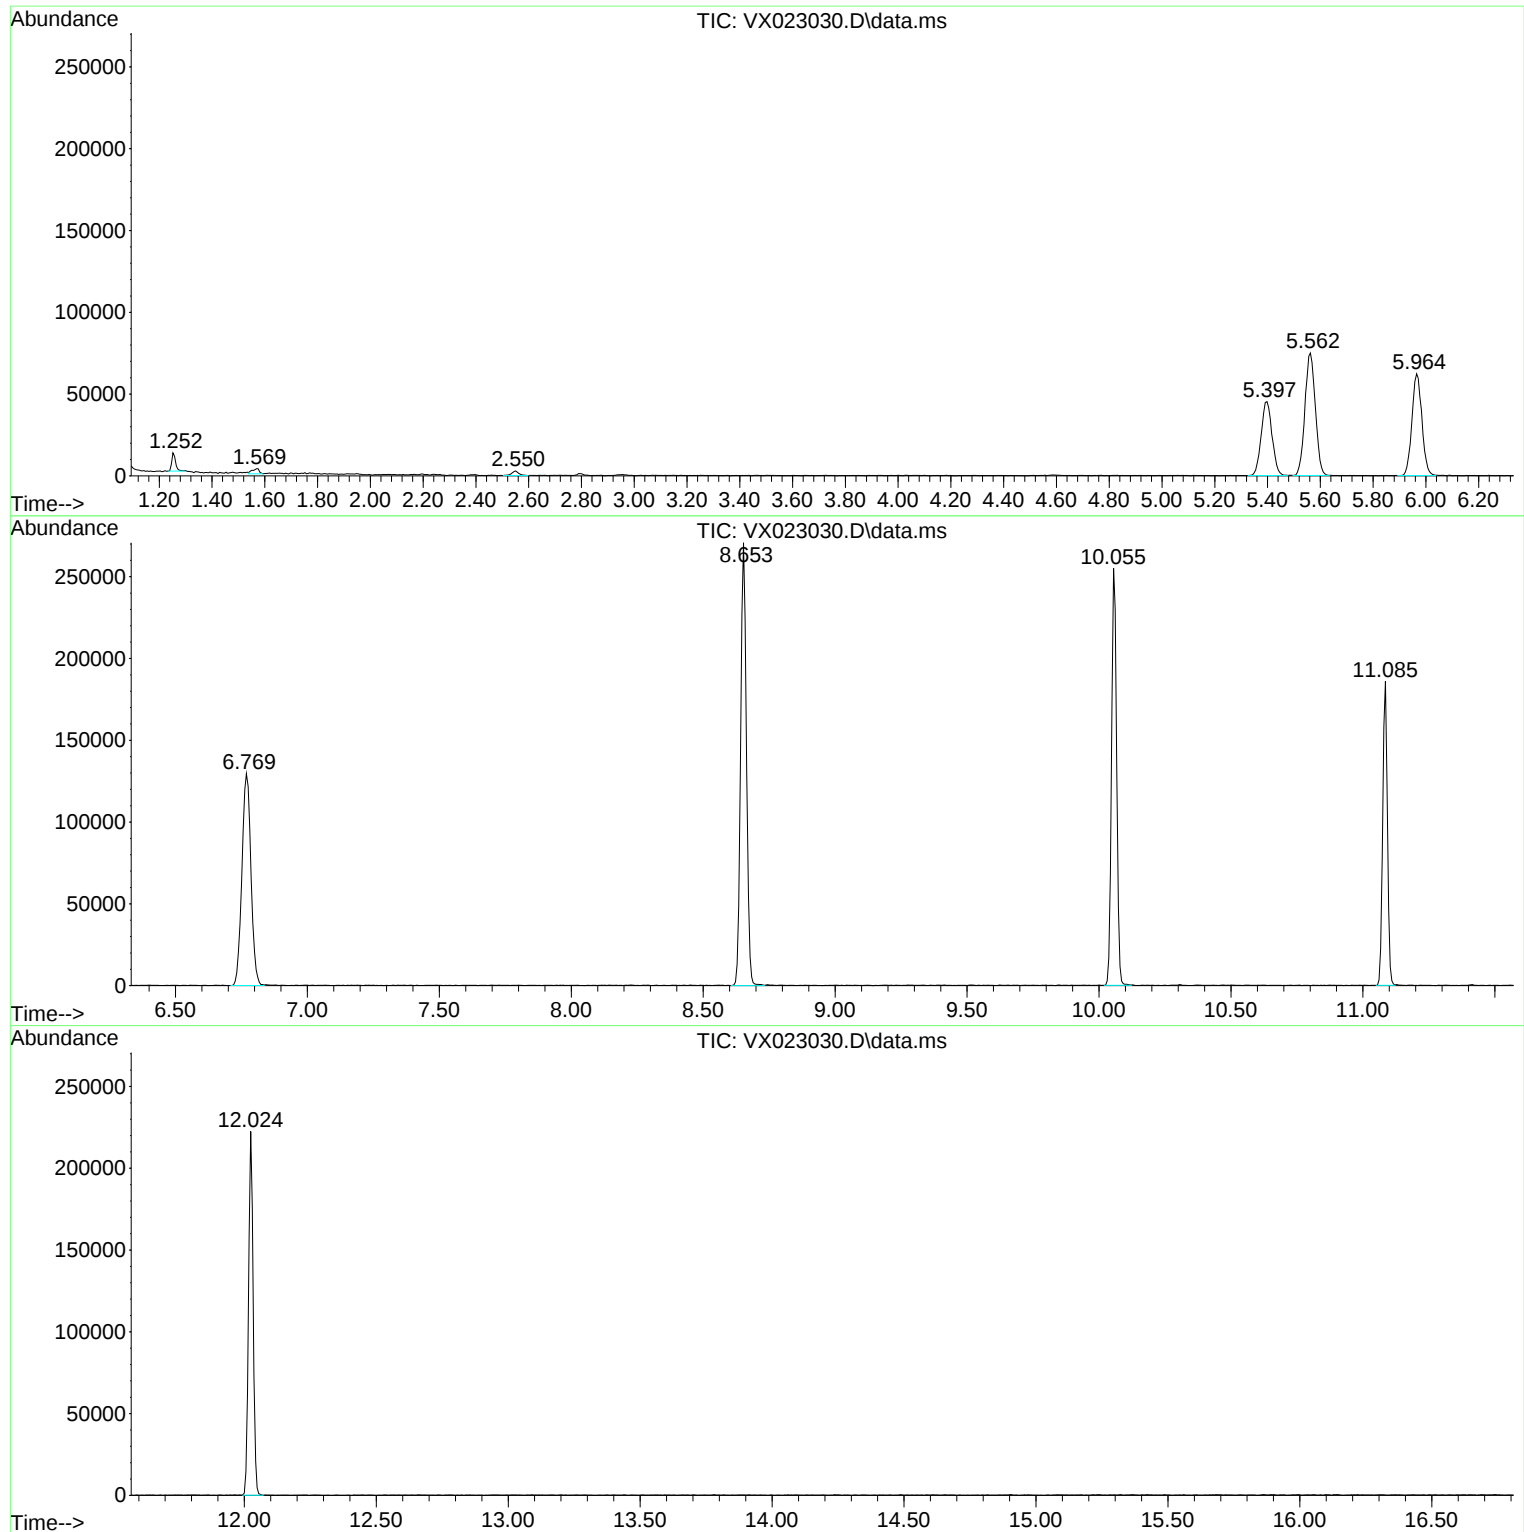

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023030.D
Acq On : 30 Jun 2021 13:46
Operator : JC/MD
Sample : M2872-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023030.D
Acq On : 30 Jun 2021 13:46
Operator : JC/MD
Sample : M2872-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
