

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
 Data File : VX023044.D
 Acq On : 30 Jun 2021 19:15
 Operator : JC/MD
 Sample : M2898-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EB-01-062921

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Title : SW846 8260

Signal : TIC: VX023044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	35	rBV3	4262	7725	1.85%	0.321%
2	2.386	208	213	222	rVB	6944	11268	2.70%	0.468%
3	2.550	234	240	251	rVB	2762	5278	1.27%	0.219%
4	2.794	274	280	286	rBV3	3347	6662	1.60%	0.277%
5	5.397	696	707	721	rVB2	44534	125210	30.01%	5.200%
6	5.562	723	734	747	rVB3	72412	205363	49.22%	8.529%
7	5.964	789	800	813	rBV	59194	158245	37.93%	6.572%
8	6.769	922	932	947	rBV	127091	301792	72.33%	12.534%
9	8.653	1234	1241	1255	rVB	268152	417233	100.00%	17.328%
10	10.055	1466	1471	1479	rBV	270905	360654	86.44%	14.978%
11	11.085	1634	1640	1648	rBV	205216	264877	63.48%	11.001%
12	12.024	1788	1794	1801	rBV	269896	327138	78.41%	13.586%
13	12.591	1873	1887	1892	rBV10	3176	9451	2.27%	0.393%
14	13.390	2014	2018	2021	rBV3	5031	7268	1.74%	0.302%
15	13.707	2062	2070	2075	rBV8	3172	8617	2.07%	0.358%
16	13.847	2089	2093	2095	rVV	5991	6602	1.58%	0.274%
17	13.902	2099	2102	2111	rVB9	2252	4734	1.13%	0.197%
18	14.615	2216	2219	2225	rVB2	13067	13781	3.30%	0.572%
19	14.969	2273	2277	2284	rVB9	4625	9745	2.34%	0.405%
20	15.103	2294	2299	2301	rBV5	3577	6206	1.49%	0.258%
21	15.213	2314	2317	2322	rVV	16052	20521	4.92%	0.852%
22	15.280	2325	2328	2333	rBV6	3185	4309	1.03%	0.179%
23	15.420	2348	2351	2357	rVB5	10248	16310	3.91%	0.677%
24	15.566	2370	2375	2384	rVB6	10510	19468	4.67%	0.809%
25	15.688	2390	2395	2400	rBV9	6323	12989	3.11%	0.539%
26	15.743	2401	2404	2409	rVB3	12862	19015	4.56%	0.790%
27	15.822	2412	2417	2420	rBV6	4698	7727	1.85%	0.321%
28	16.091	2457	2461	2466	rBV8	2592	6347	1.52%	0.264%
29	16.273	2489	2491	2494	rBV4	3152	4473	1.07%	0.186%
30	16.438	2513	2518	2519	rBV4	2671	4391	1.05%	0.182%
31	16.560	2535	2538	2543	rVV7	4567	7430	1.78%	0.309%
32	16.609	2543	2546	2552	rVB8	4258	9217	2.21%	0.383%
33	16.712	2558	2563	2569	rVB3	10242	17801	4.27%	0.739%




Sum of corrected areas: 2407847

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023044.D
Acq On : 30 Jun 2021 19:15
Operator : JC/MD
Sample : M2898-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-062921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

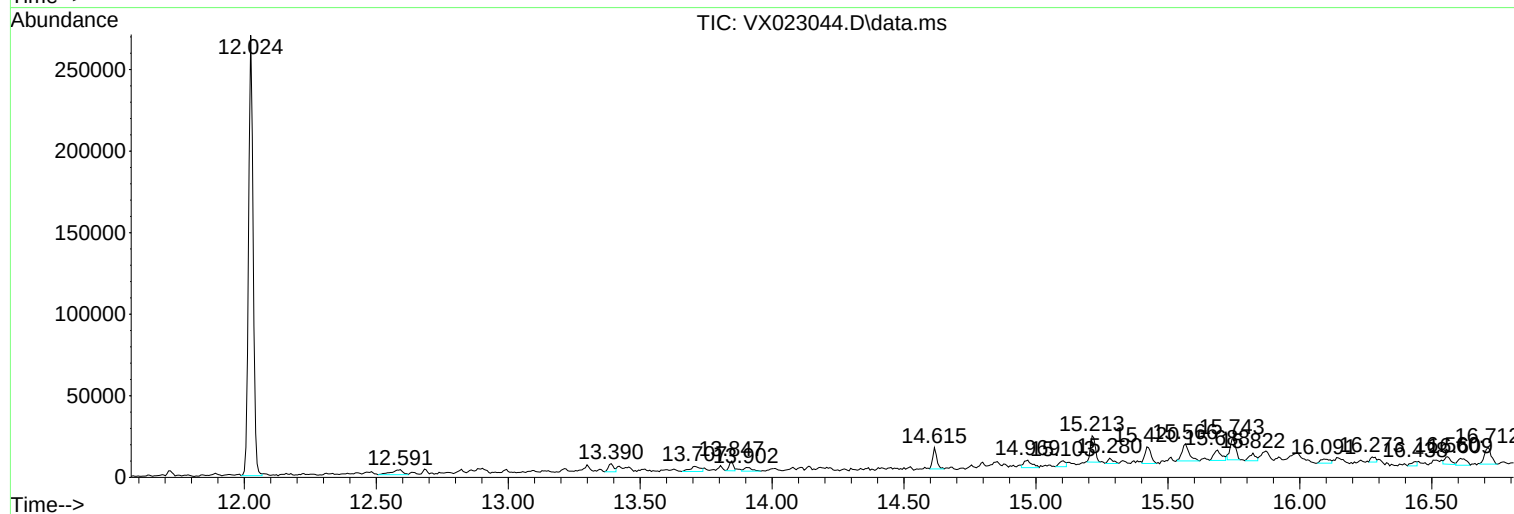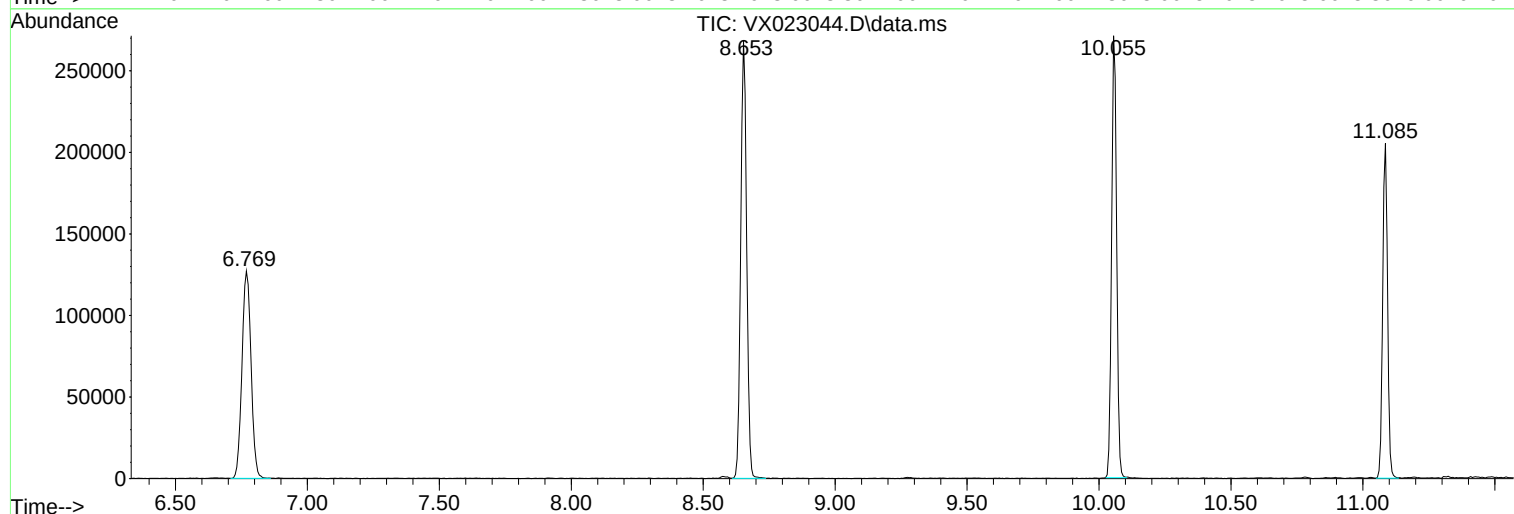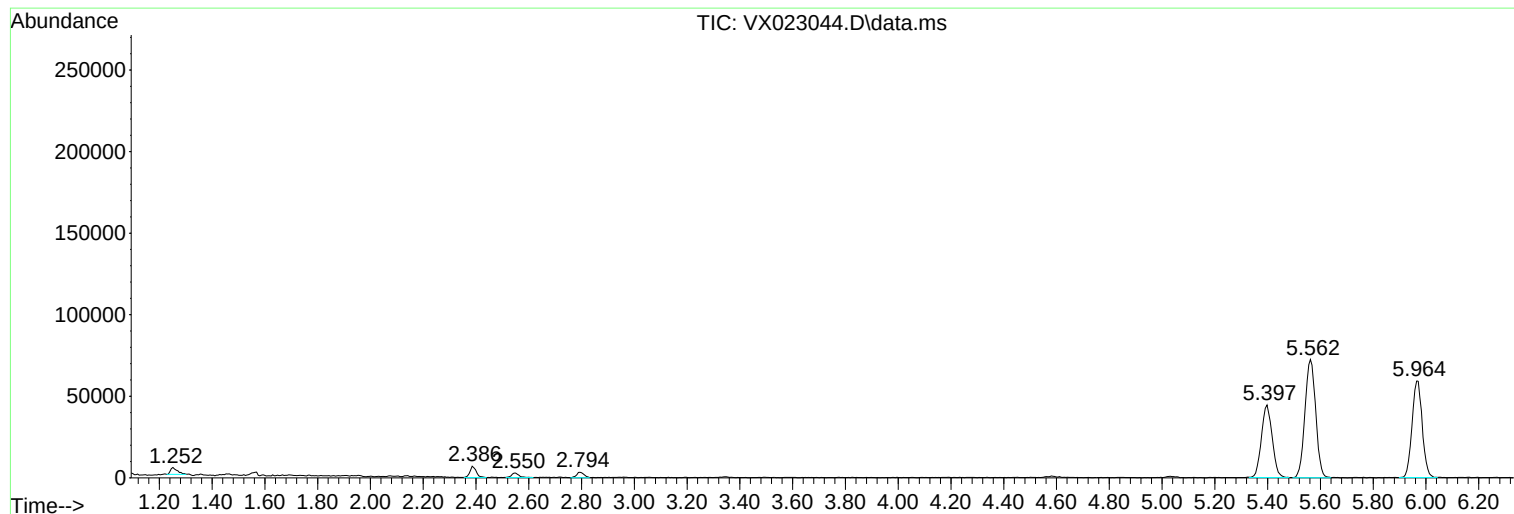

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023044.D
Acq On : 30 Jun 2021 19:15
Operator : JC/MD
Sample : M2898-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-062921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023044.D
Acq On : 30 Jun 2021 19:15
Operator : JC/MD
Sample : M2898-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EB-01-062921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
