

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
 Data File : VX023046.D
 Acq On : 30 Jun 2021 20:02
 Operator : JC/MD
 Sample : M2898-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-10A-062921-FD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX023046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.148	7	10	12	rBV	111028	91794	22.54%	3.697%
2	1.166	12	13	19	rVB	20333	17392	4.27%	0.701%
3	1.270	23	30	42	rBV	38145	144648	35.52%	5.826%
4	1.374	44	47	51	rVB	29811	31289	7.68%	1.260%
5	2.130	169	171	181	rVB8	1892	4682	1.15%	0.189%
6	2.550	231	240	247	rBV4	2285	6013	1.48%	0.242%
7	4.501	548	560	571	rBV	45151	115724	28.42%	4.661%
8	5.397	695	707	722	rBV2	42065	122008	29.96%	4.914%
9	5.562	722	734	748	rVB2	69894	196755	48.31%	7.925%
10	5.964	790	800	810	rBV2	58621	152069	37.34%	6.125%
11	6.769	922	932	947	rBV	127549	296059	72.70%	11.925%
12	8.653	1234	1241	1249	rBV	267077	407238	100.00%	16.404%
13	10.055	1466	1471	1478	rBV	253130	345084	84.74%	13.900%
14	11.085	1634	1640	1650	rBV	198216	245057	60.18%	9.871%
15	12.024	1789	1794	1804	rBV	244021	301114	73.94%	12.129%
16	15.743	2400	2404	2410	rVB6	2673	5700	1.40%	0.230%




Sum of corrected areas: 2482626

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023046.D
Acq On : 30 Jun 2021 20:02
Operator : JC/MD
Sample : M2898-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10A-062921-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

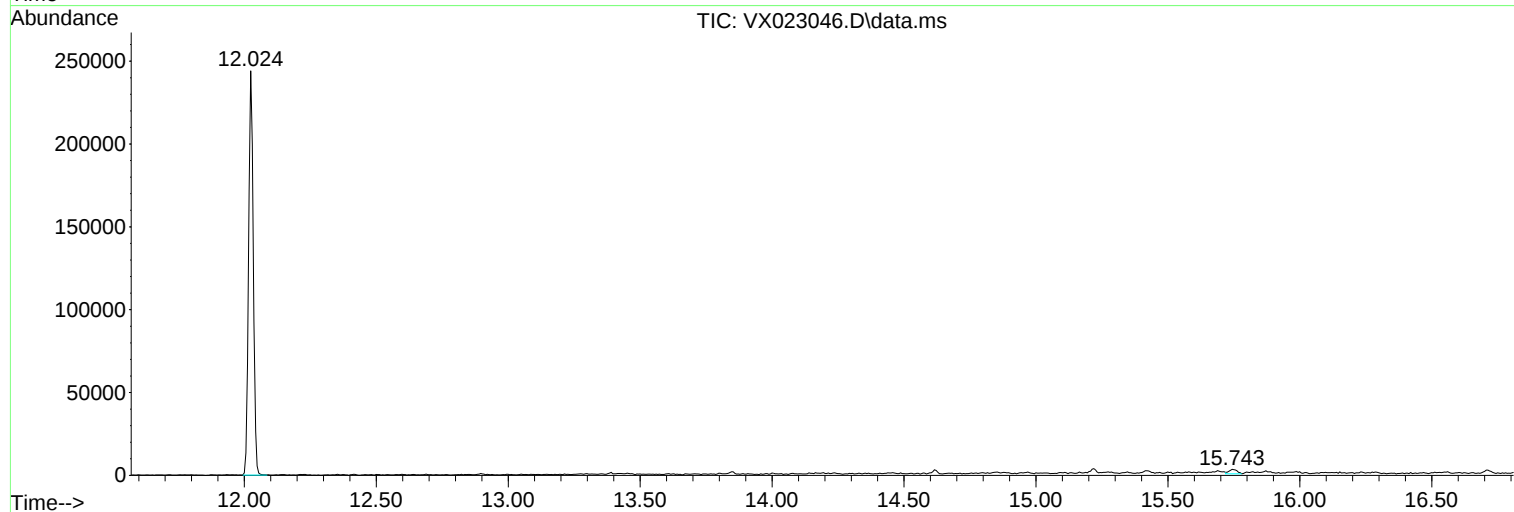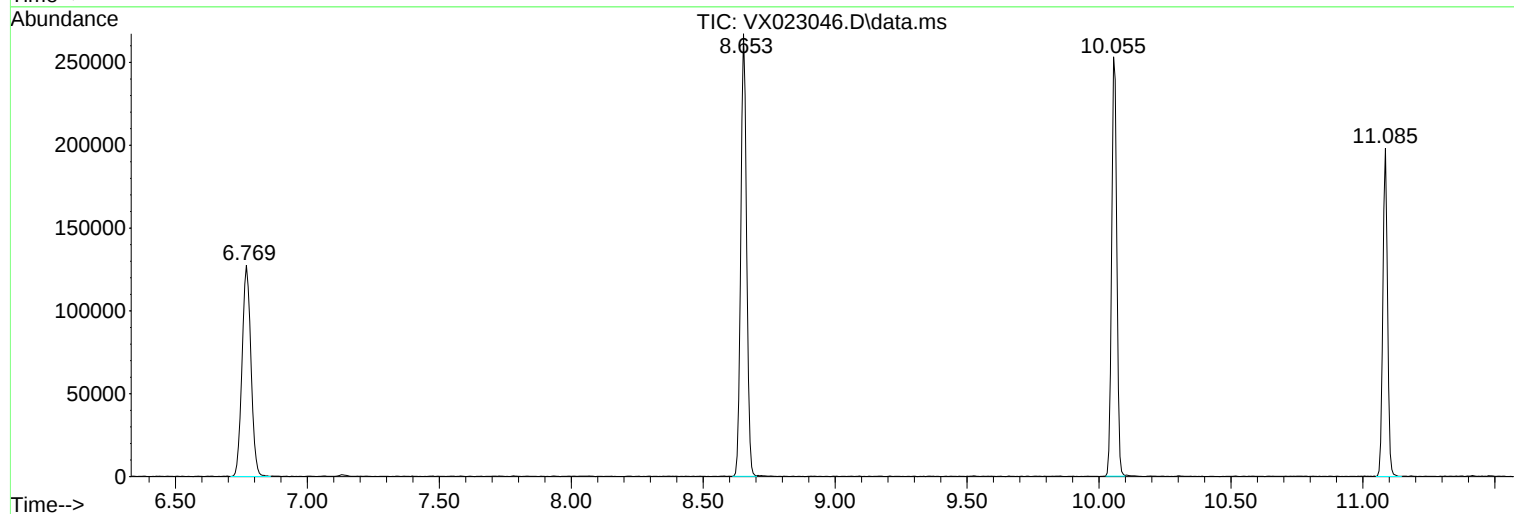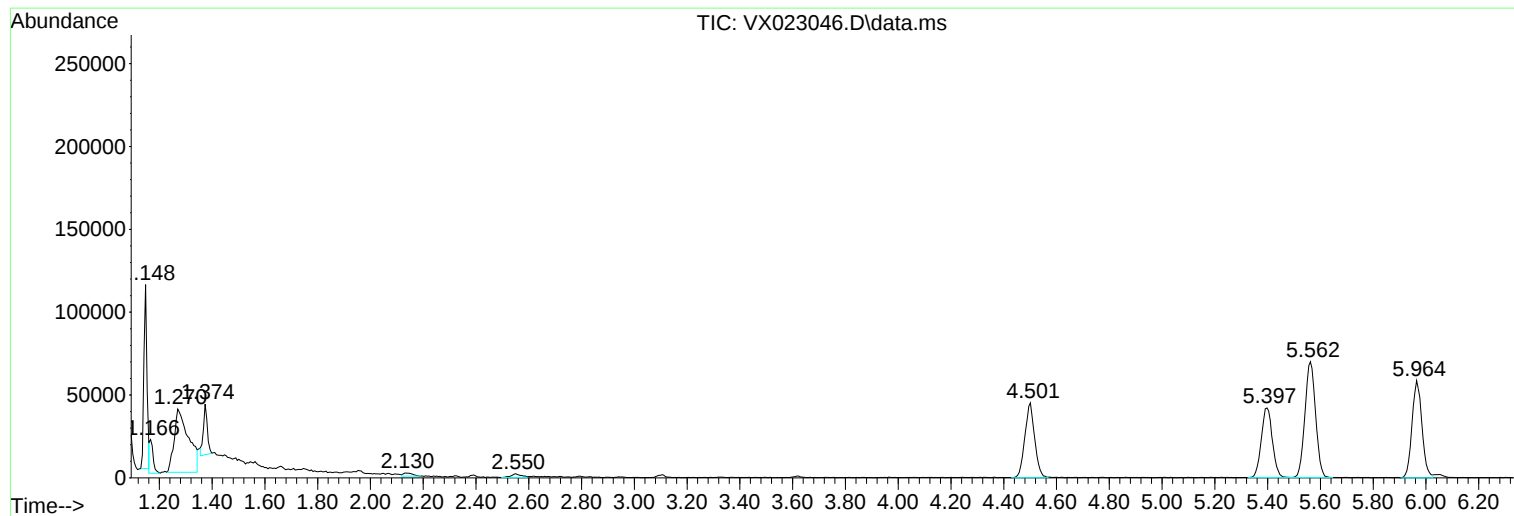

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023046.D
Acq On : 30 Jun 2021 20:02
Operator : JC/MD
Sample : M2898-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10A-062921-FD










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Aminomethanesulfonic acid Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.270	36.76 ug/l	144648	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	83
2			Sulfur dioxide	64	O2S	007446-09-5	83
3			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
4			Ethene, 1,2-difluoro-	64	C2H2F2	001691-13-0	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

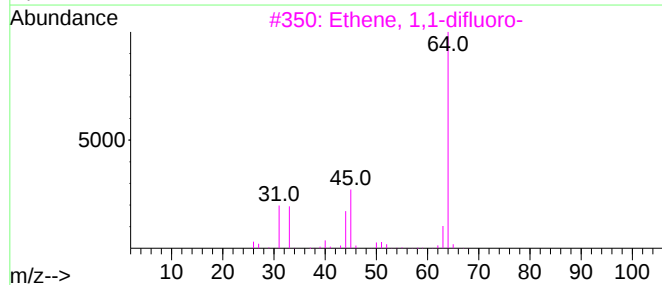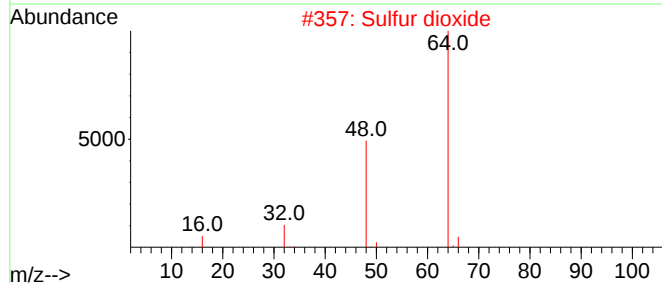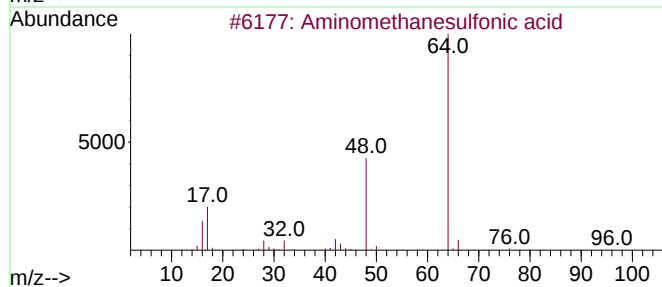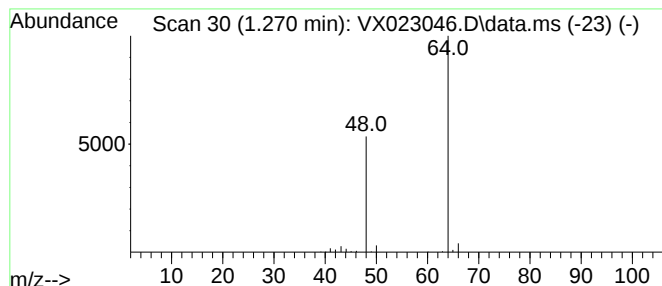

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023046.D
Acq On : 30 Jun 2021 20:02
Operator : JC/MD
Sample : M2898-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10A-062921-FD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Aminomethanesul...	1.270	36.8	ug/l	144648	1	5.562	196755	50.0