

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
 Data File : VX023048.D
 Acq On : 30 Jun 2021 20:49
 Operator : JC/MD
 Sample : M2892-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1R

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX023048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	39	rVB2	12072	20135	5.09%	0.970%
2	1.362	41	45	51	rVB2	4318	4953	1.25%	0.239%
3	1.843	121	124	129	rBV	11627	16199	4.09%	0.781%
4	2.550	232	240	246	rBV	3996	7940	2.01%	0.383%
5	3.130	326	335	343	rVB2	8039	19754	4.99%	0.952%
6	5.397	696	707	719	rBV2	41818	118296	29.89%	5.702%
7	5.562	722	734	746	rBV2	68873	191611	48.41%	9.235%
8	5.964	791	800	814	rBV2	57679	146979	37.14%	7.084%
9	6.769	923	932	943	rBV	123658	287916	72.74%	13.877%
10	8.653	1234	1241	1256	rVB	260315	395795	100.00%	19.076%
11	10.055	1466	1471	1480	rBV	243169	336493	85.02%	16.218%
12	11.085	1634	1640	1648	rBV	193121	242822	61.35%	11.703%
13	12.024	1789	1794	1800	rBV	235777	285904	72.24%	13.780%




Sum of corrected areas: 2074797

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023048.D
Acq On : 30 Jun 2021 20:49
Operator : JC/MD
Sample : M2892-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

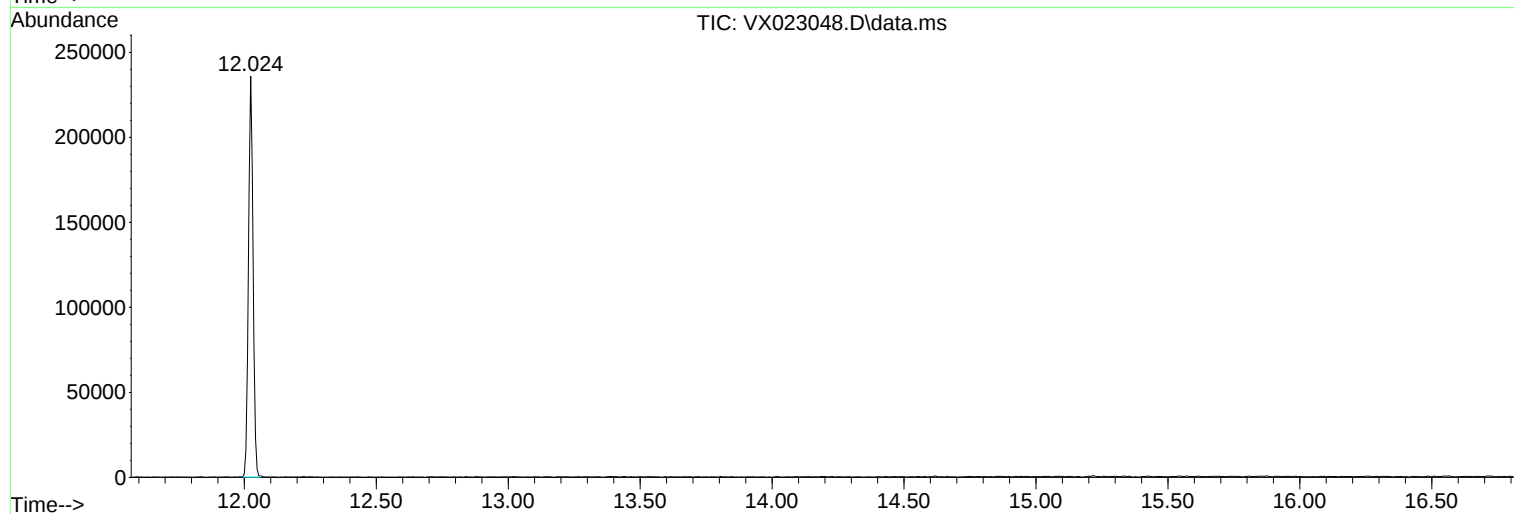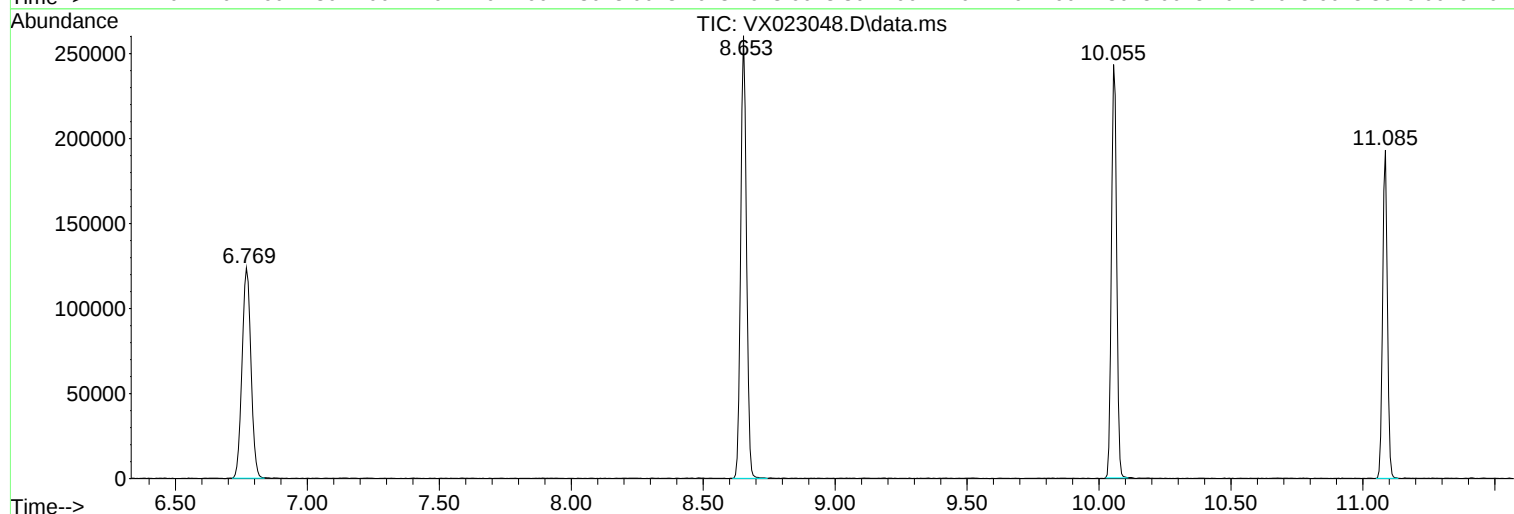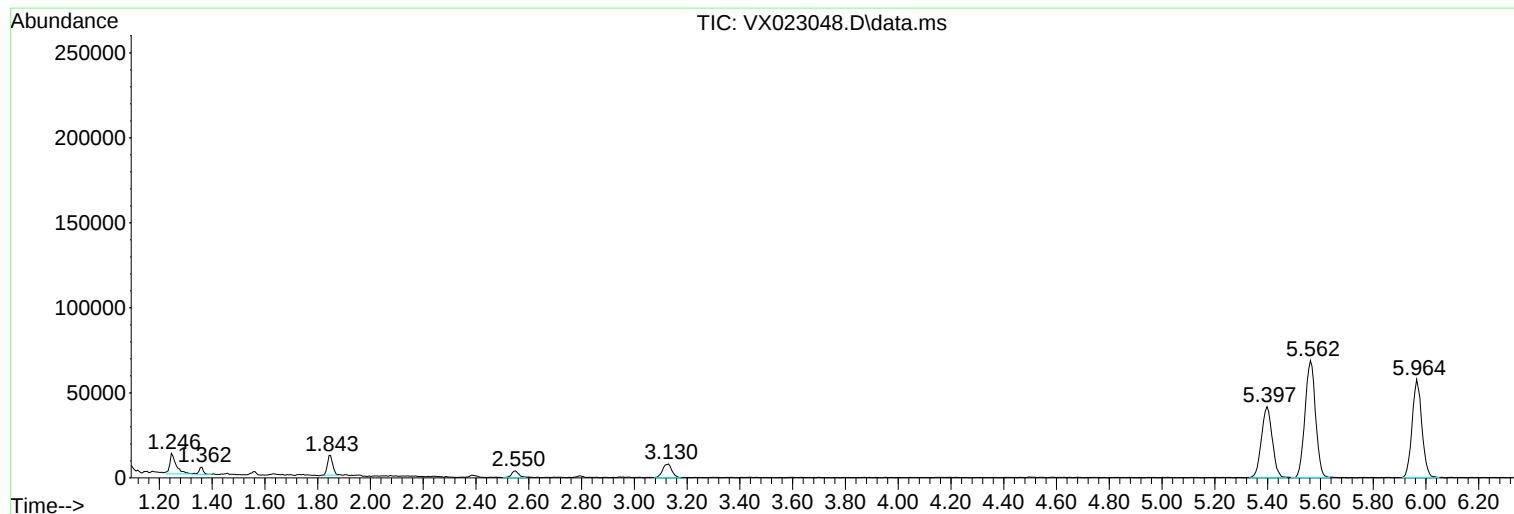

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023048.D
Acq On : 30 Jun 2021 20:49
Operator : JC/MD
Sample : M2892-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1R










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.246	5.25 ug/l	20135	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	74
2			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
3			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

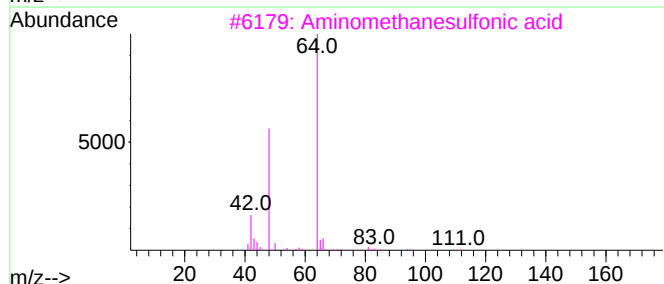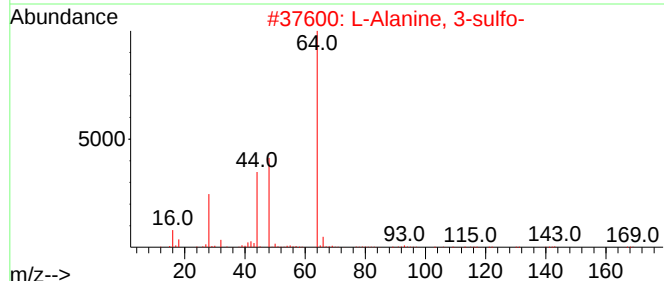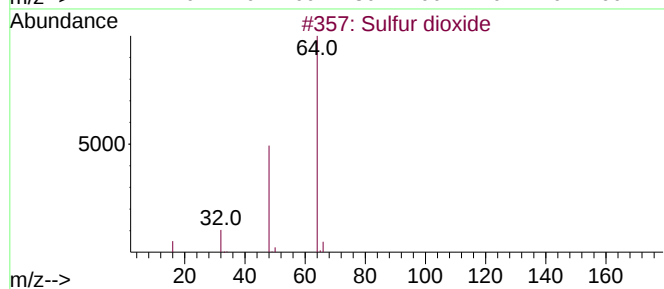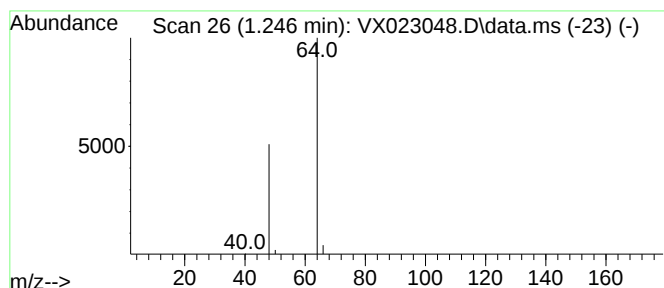

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023048.D
Acq On : 30 Jun 2021 20:49
Operator : JC/MD
Sample : M2892-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.246	5.3	ug/l	20135	1	5.562	191611	50.0