

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
 Data File : VX023063.D
 Acq On : 01 Jul 2021 03:53
 Operator : JC/MD
 Sample : M2845-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 41235

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX023063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.386	207	213	220	rVB2	6410	11601	3.01%	0.580%
2	2.550	235	240	248	rVB	2199	3926	1.02%	0.196%
3	5.025	636	646	661	rBV2	11657	36548	9.47%	1.828%
4	5.397	695	707	721	rBV3	41483	119435	30.94%	5.974%
5	5.562	721	734	747	rVB2	67614	186715	48.37%	9.339%
6	5.970	788	801	814	rBV	57249	151448	39.23%	7.575%
7	6.769	923	932	944	rBV2	119582	279308	72.35%	13.970%
8	8.653	1233	1241	1249	rBV	254011	386052	100.00%	19.308%
9	10.055	1465	1471	1485	rVB	237256	331537	85.88%	16.582%
10	11.085	1634	1640	1646	rBV	180817	224417	58.13%	11.224%
11	12.024	1789	1794	1802	rVB	220769	268404	69.53%	13.424%




Sum of corrected areas: 1999391

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023063.D
Acq On : 01 Jul 2021 03:53
Operator : JC/MD
Sample : M2845-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

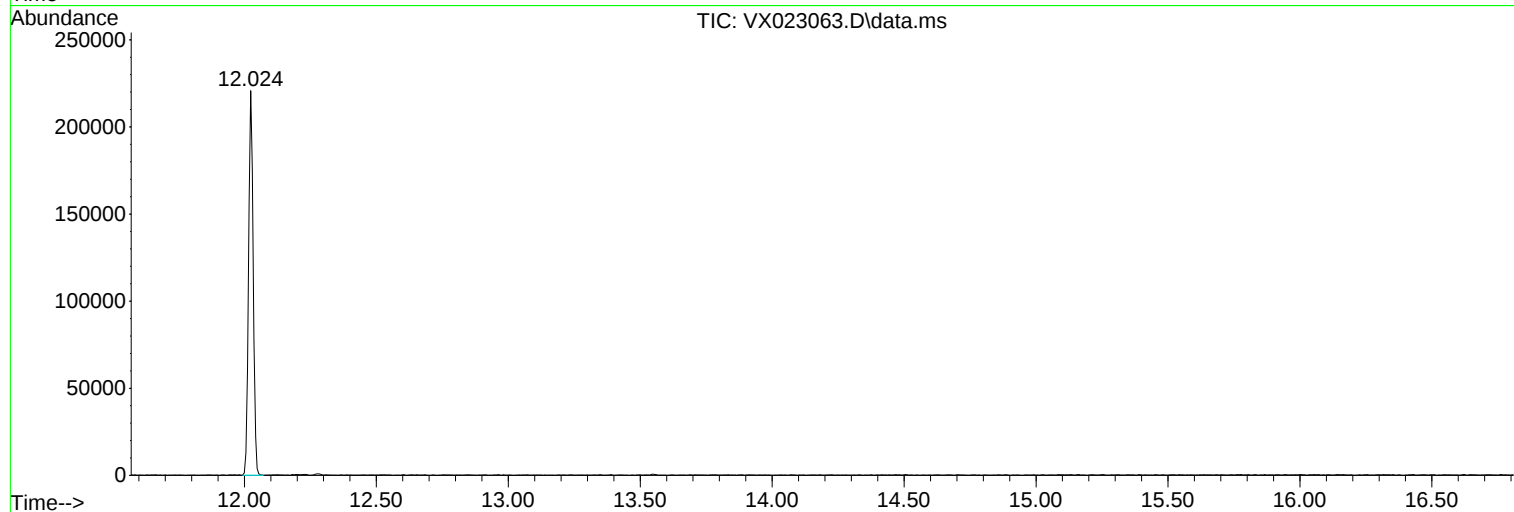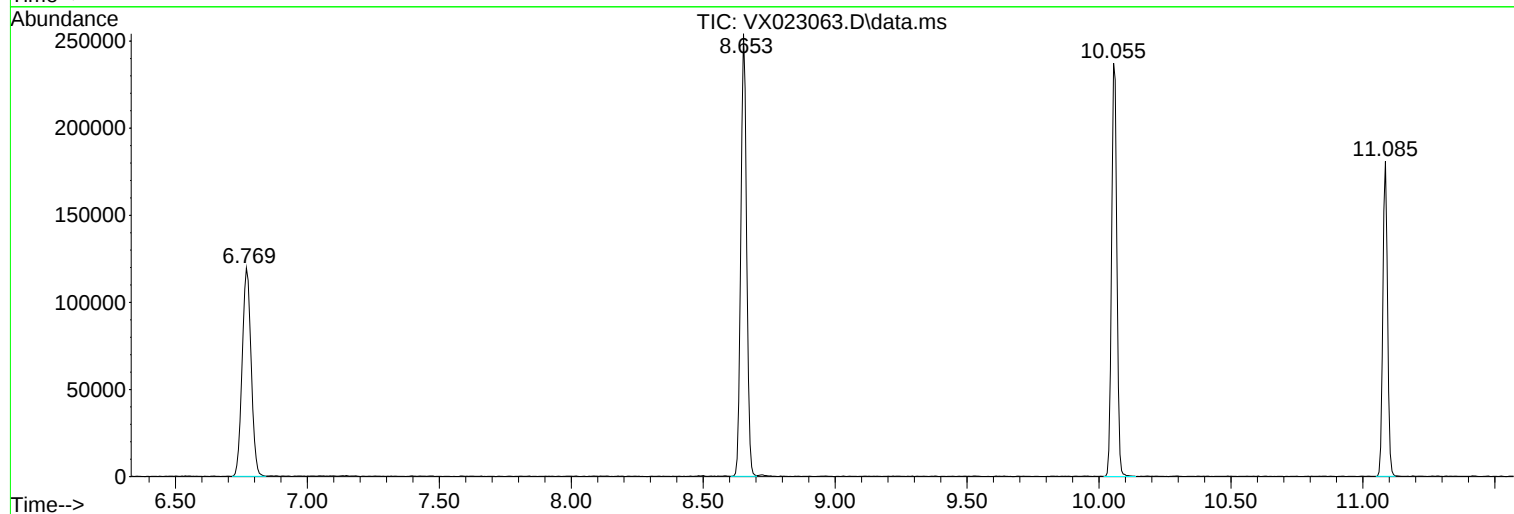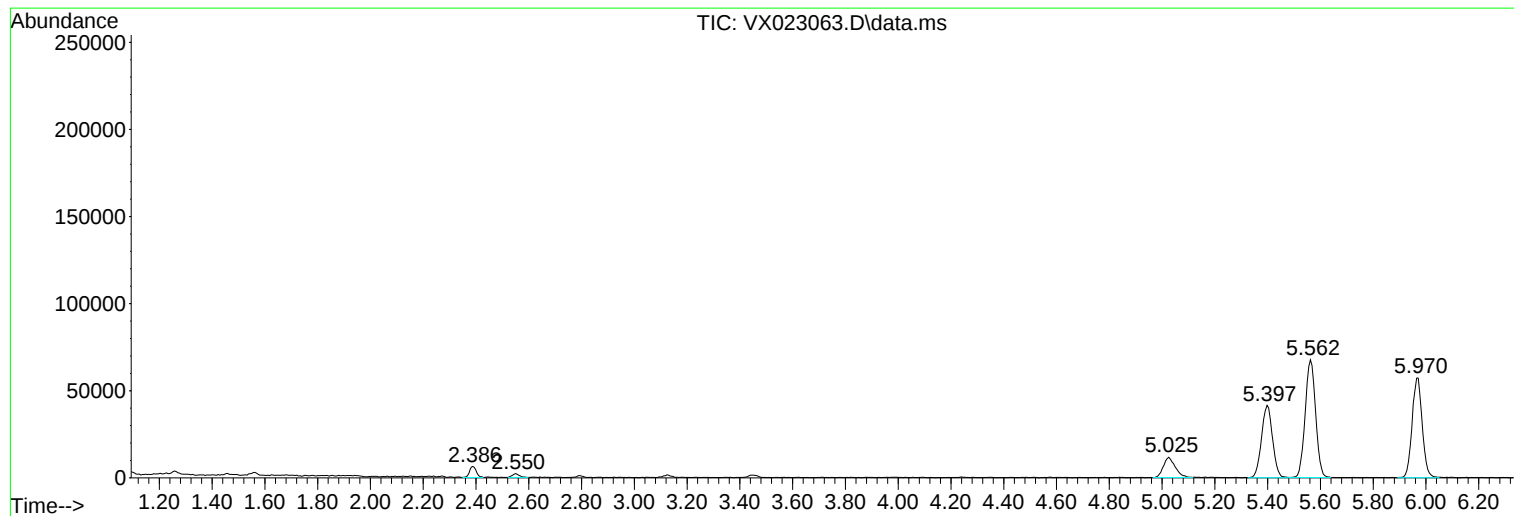

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023063.D
Acq On : 01 Jul 2021 03:53
Operator : JC/MD
Sample : M2845-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063021\
Data File : VX023063.D
Acq On : 01 Jul 2021 03:53
Operator : JC/MD
Sample : M2845-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
