

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063022\
Data File : VX029903.D
Acq On : 30 Jun 2022 11:47
Operator : JC/MD
Sample : VX0630WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0630WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M

Title : SW846 8260

Signal : TIC: VX029903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	24	28	38	rBV2	10343	27973	2.55%	0.498%
2	2.947	296	305	317	rBV	8841	20961	1.91%	0.373%
3	4.587	564	574	585	rBV	6101	19533	1.78%	0.348%
4	5.391	695	706	721	rBV	118607	343582	31.37%	6.117%
5	5.556	721	733	748	rVB2	215590	610862	55.77%	10.876%
6	5.964	789	800	817	rBV	131851	353655	32.29%	6.297%
7	6.763	921	931	952	rBV	345459	824020	75.22%	14.671%
8	8.653	1234	1241	1252	rBV	694164	1095413	100.00%	19.503%
9	10.055	1464	1471	1480	rBV	674575	908728	82.96%	16.179%
10	11.085	1632	1640	1653	rBV	486326	632072	57.70%	11.254%
11	12.024	1788	1794	1806	rBV	638331	779789	71.19%	13.884%




Sum of corrected areas: 5616588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063022\
Data File : VX029903.D
Acq On : 30 Jun 2022 11:47
Operator : JC/MD
Sample : VX0630WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0630WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

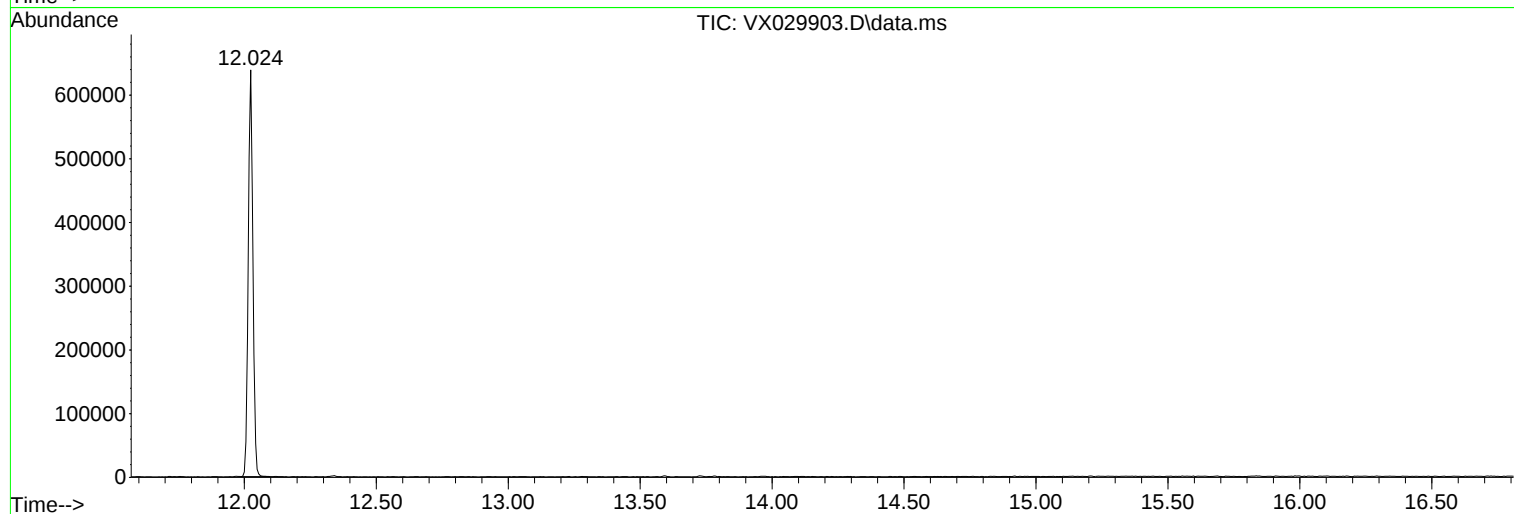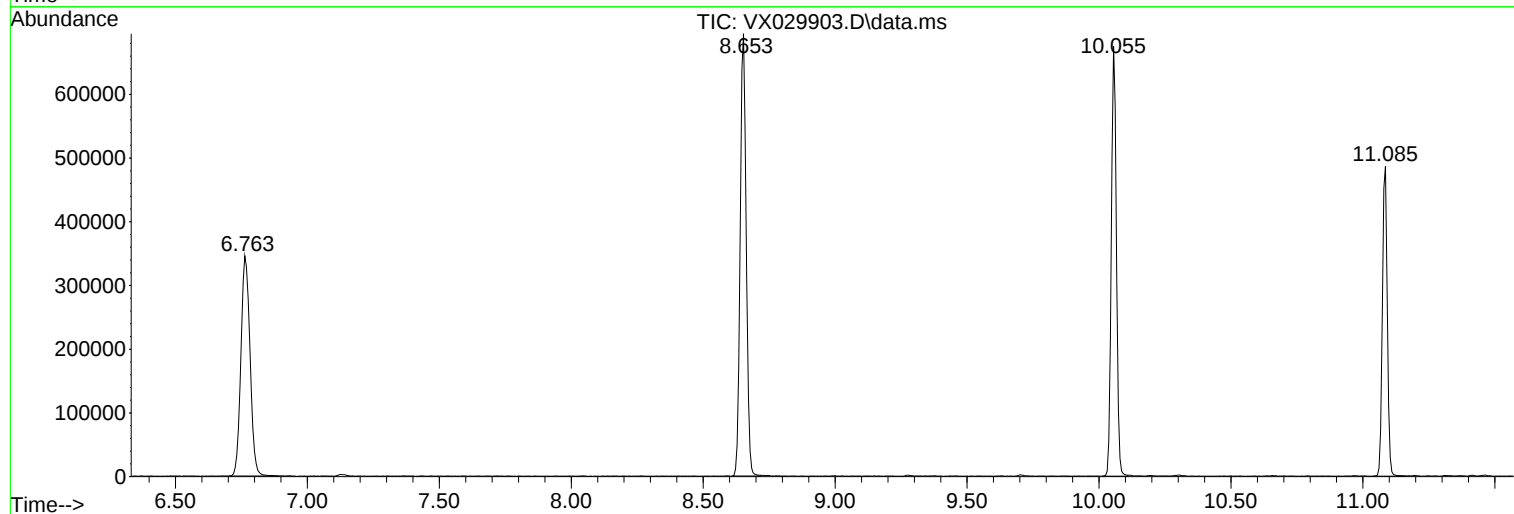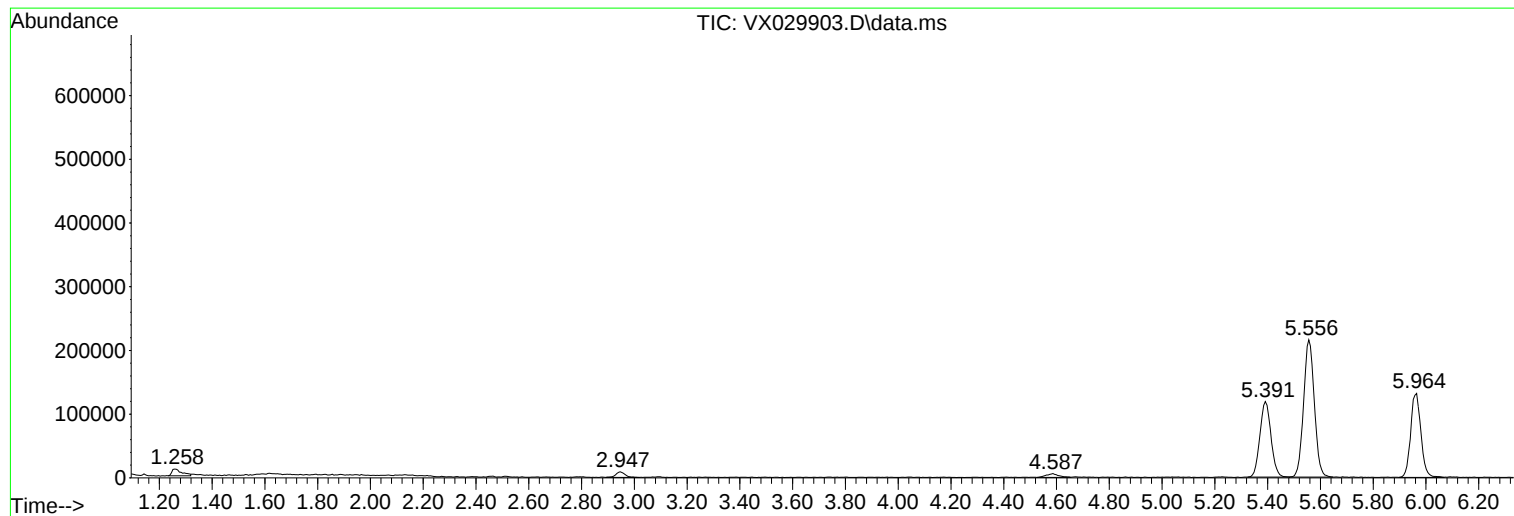

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063022\
Data File : VX029903.D
Acq On : 30 Jun 2022 11:47
Operator : JC/MD
Sample : VX0630WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0630WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063022\
Data File : VX029903.D
Acq On : 30 Jun 2022 11:47
Operator : JC/MD
Sample : VX0630WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0630WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc