


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063022\
 Data File : VX029901.D
 Acq On : 30 Jun 2022 09:10
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Title : SW846 8260
 Last Update : Wed Jun 29 05:54:51 2022

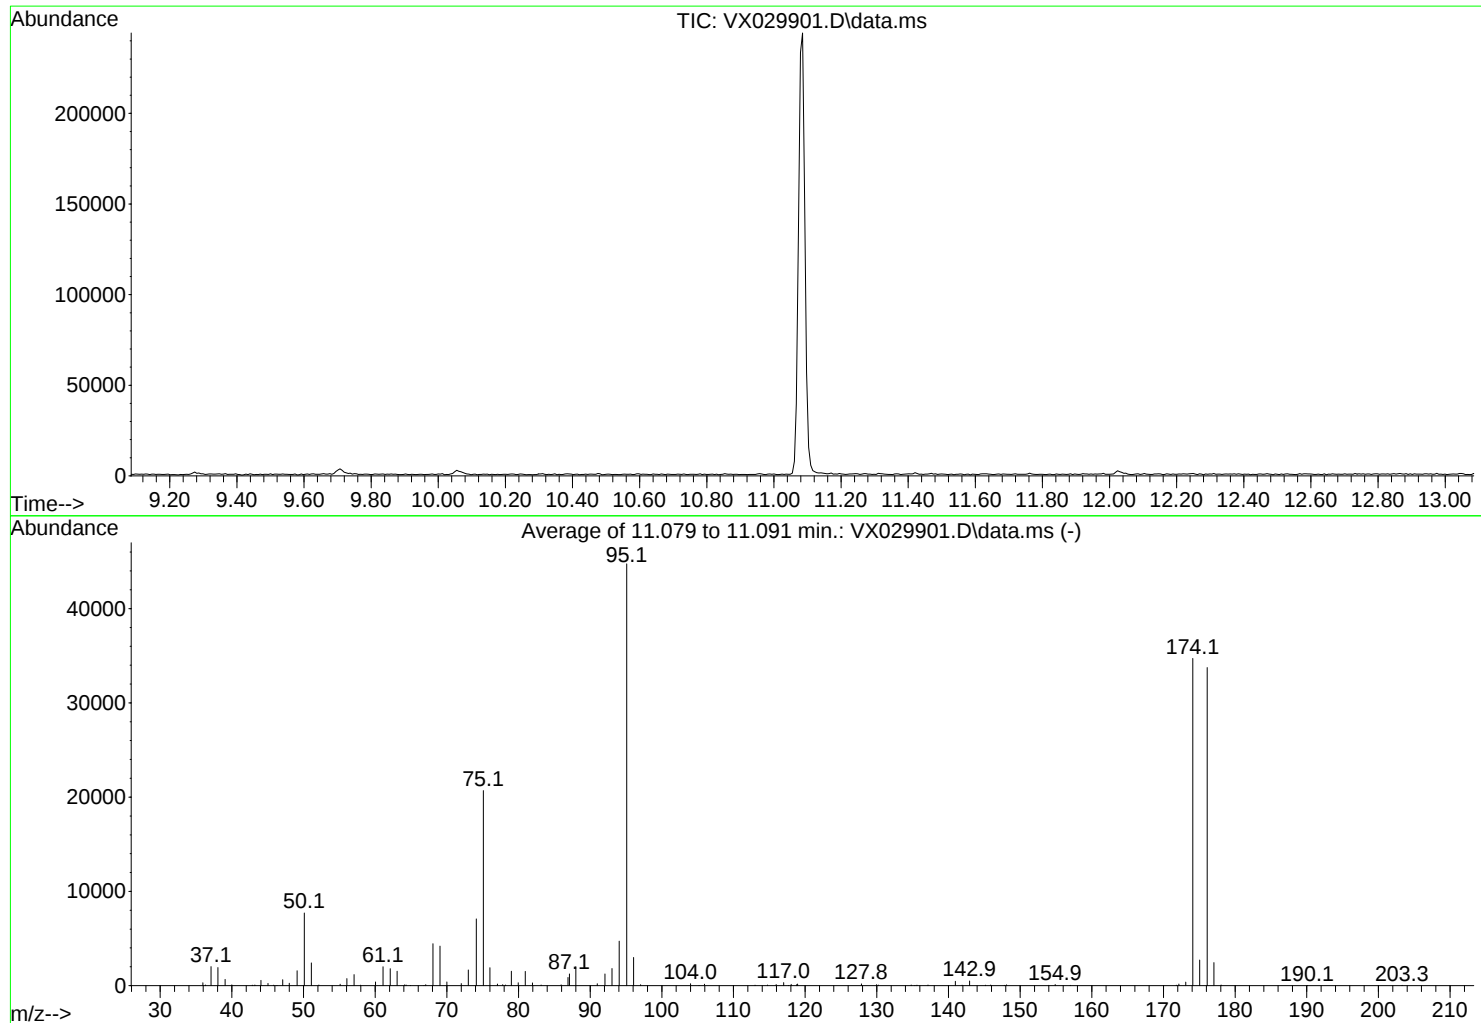

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	7707	PASS
75	95	30	60	46.2	20689	PASS
95	95	100	100	100.0	44752	PASS
96	95	5	9	6.7	2997	PASS
173	174	0.00	2	1.1	377	PASS
174	95	50	100	77.6	34712	PASS
175	174	5	9	7.8	2724	PASS
176	174	95	101	97.2	33752	PASS
177	176	5	9	7.3	2450	PASS