

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063023\
Data File : VX036391.D
Acq On : 30 Jun 2023 13:50
Operator : JC/MD
Sample : 03494-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M

Title : SW846 8260

Signal : TIC: VX036391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	720	rBV2	105877	306404	33.23%	6.265%
2	5.550	720	732	747	rVV	188819	529045	57.38%	10.818%
3	5.958	788	799	814	rBV	116599	313431	33.99%	6.409%
4	6.763	920	931	943	rBV	294271	688808	74.70%	14.085%
5	8.647	1233	1240	1249	rBV	592082	922049	100.00%	18.854%
6	10.055	1465	1471	1480	rBV	603366	804019	87.20%	16.441%
7	11.079	1634	1639	1653	rVB	482531	602972	65.39%	12.330%
8	12.018	1788	1793	1803	rBV	553453	723627	78.48%	14.797%




Sum of corrected areas: 4890355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063023\
Data File : VX036391.D
Acq On : 30 Jun 2023 13:50
Operator : JC/MD
Sample : 03494-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

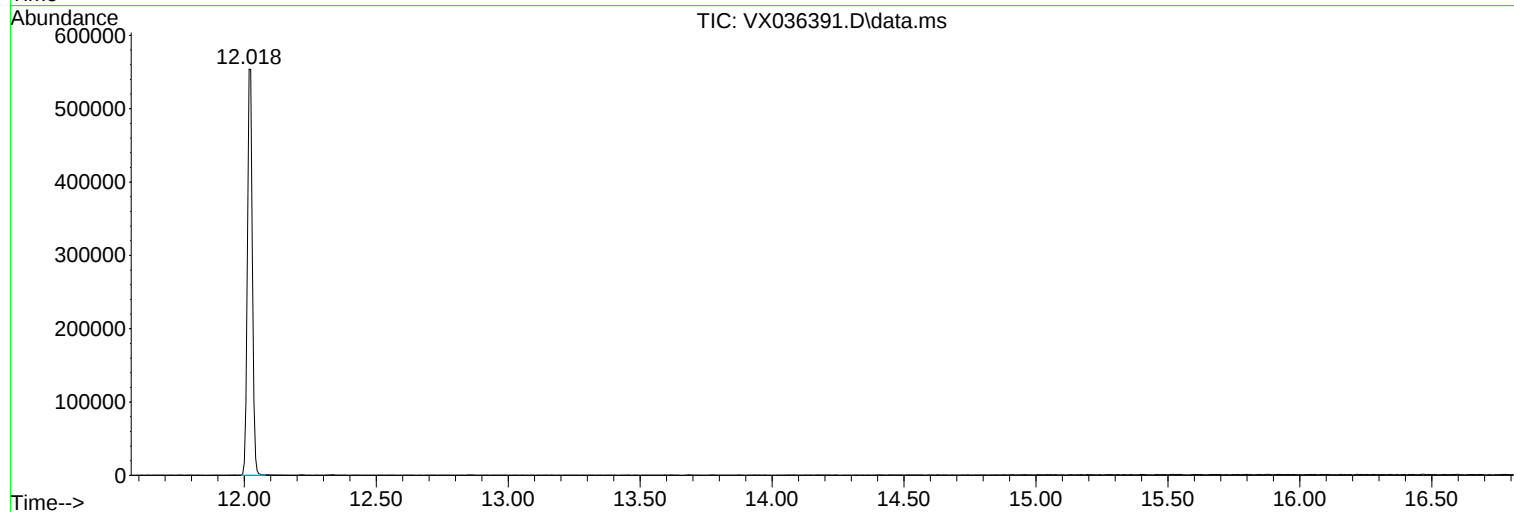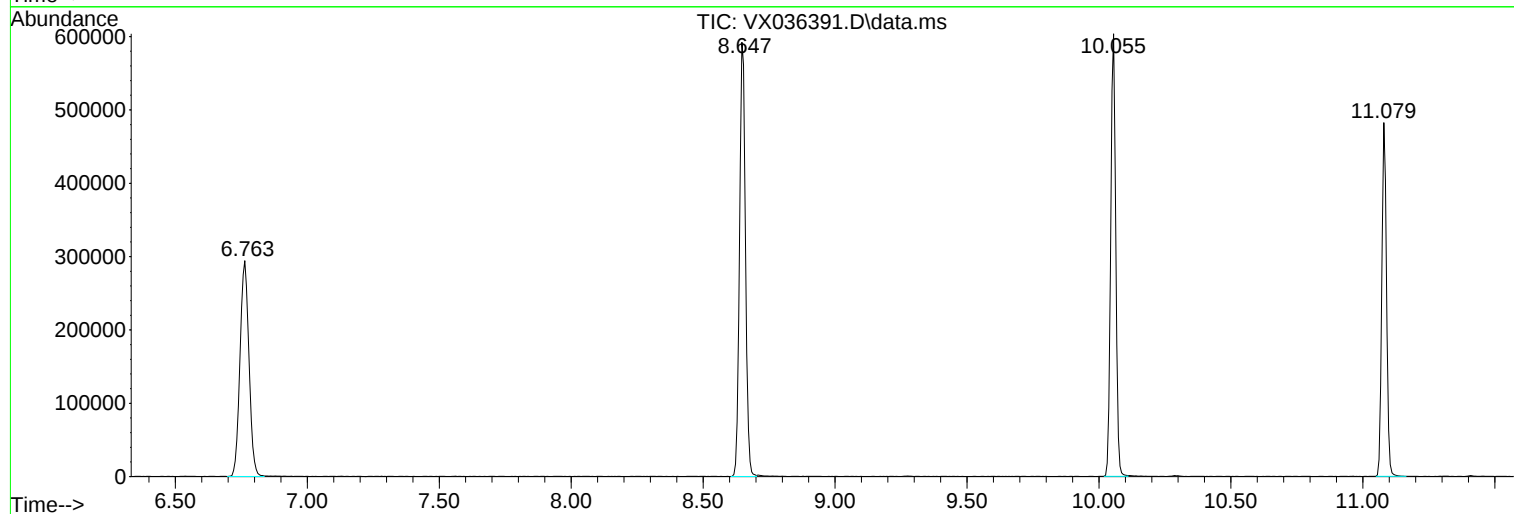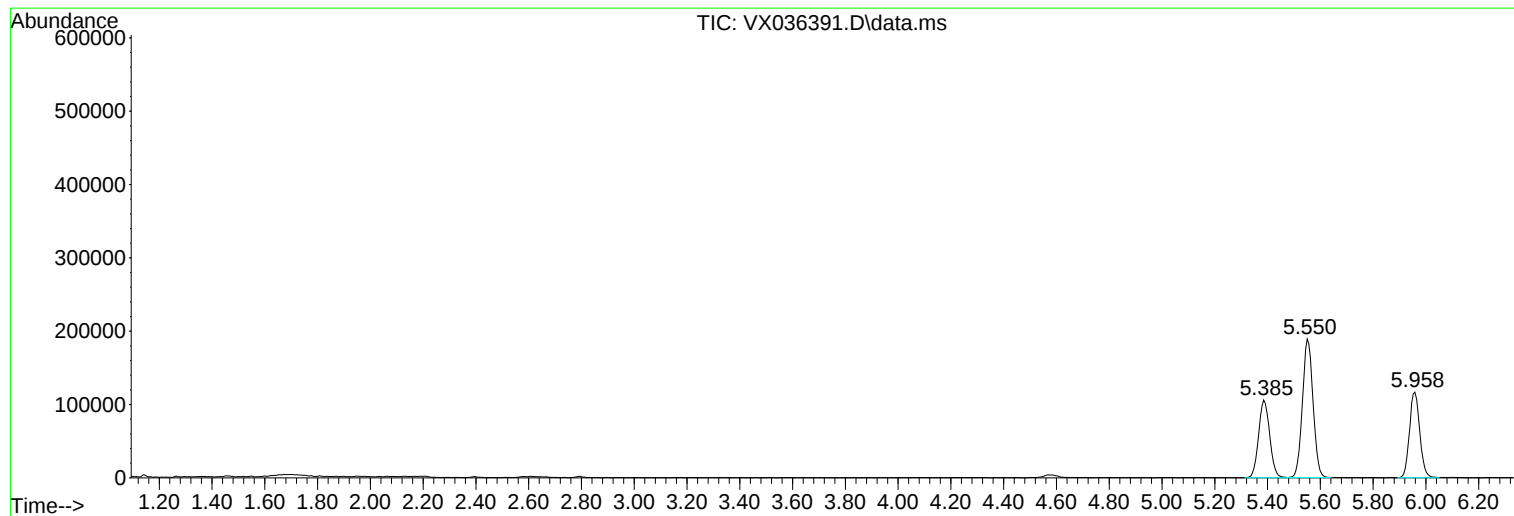

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063023\
Data File : VX036391.D
Acq On : 30 Jun 2023 13:50
Operator : JC/MD
Sample : 03494-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063023\
Data File : VX036391.D
Acq On : 30 Jun 2023 13:50
Operator : JC/MD
Sample : 03494-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc