



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063023\
Data File : VX036380.D
Acq On : 30 Jun 2023 08:21
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Title : SW846 8260
Last Update : Fri Jun 23 15:03:28 2023

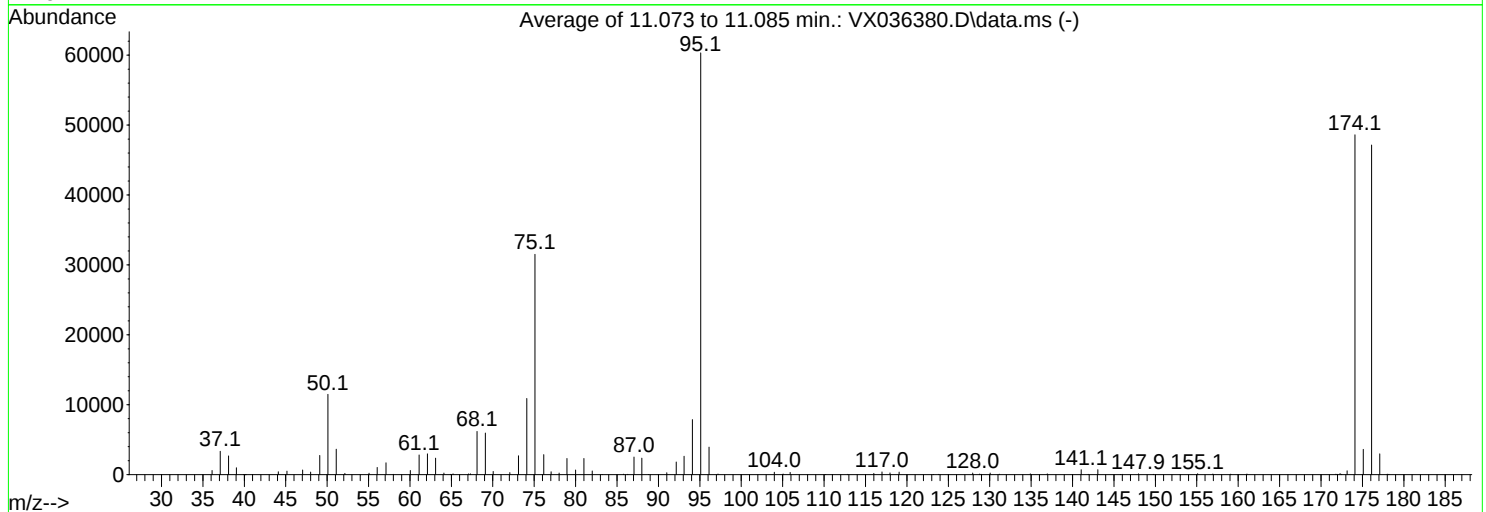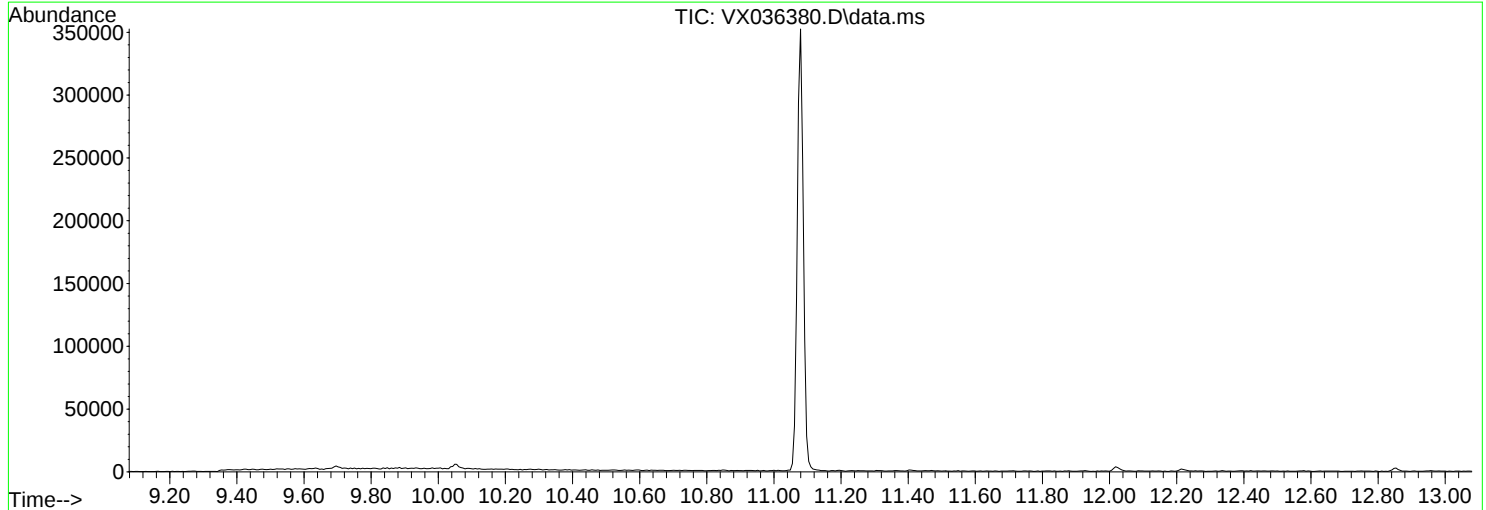

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	11489	PASS
75	95	30	60	52.2	31520	PASS
95	95	100	100	100.0	60331	PASS
96	95	5	9	6.5	3934	PASS
173	174	0.00	2	1.2	560	PASS
174	95	50	100	80.6	48613	PASS
175	174	5	9	7.5	3627	PASS
176	174	95	101	97.0	47147	PASS
177	176	5	9	6.3	2983	PASS