
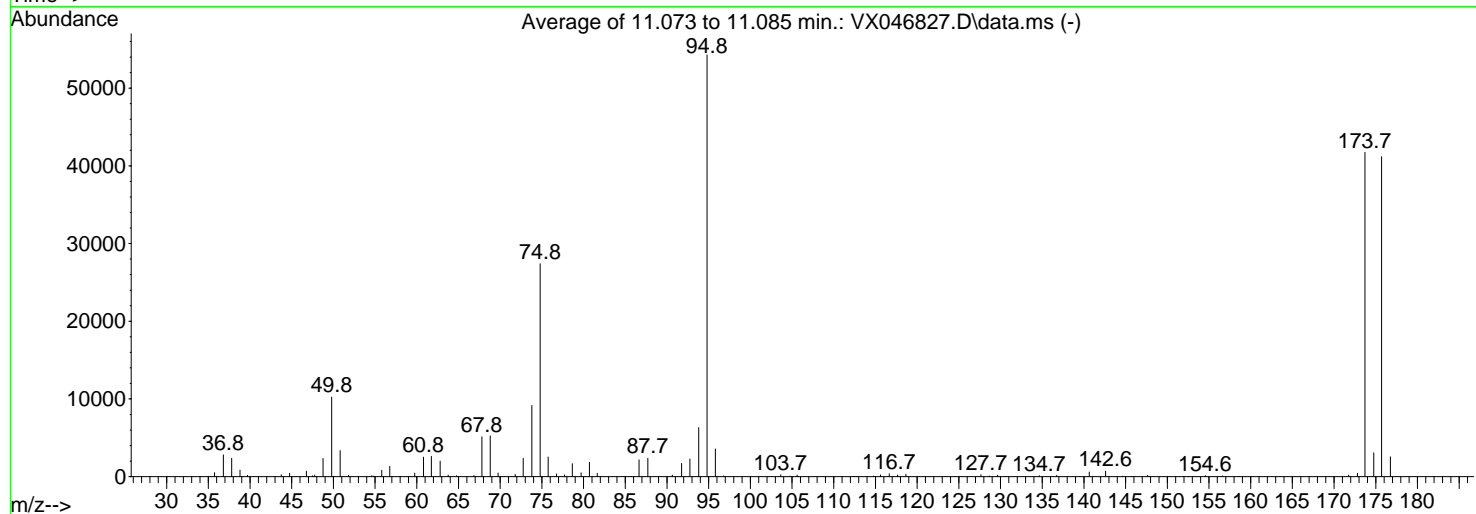


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX063025\
 Data File : VX046827.D
 Acq On : 30 Jun 2025 08:37
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061725W.M
 Title : SW846 8260
 Last Update : Wed Jun 18 03:09:16 2025

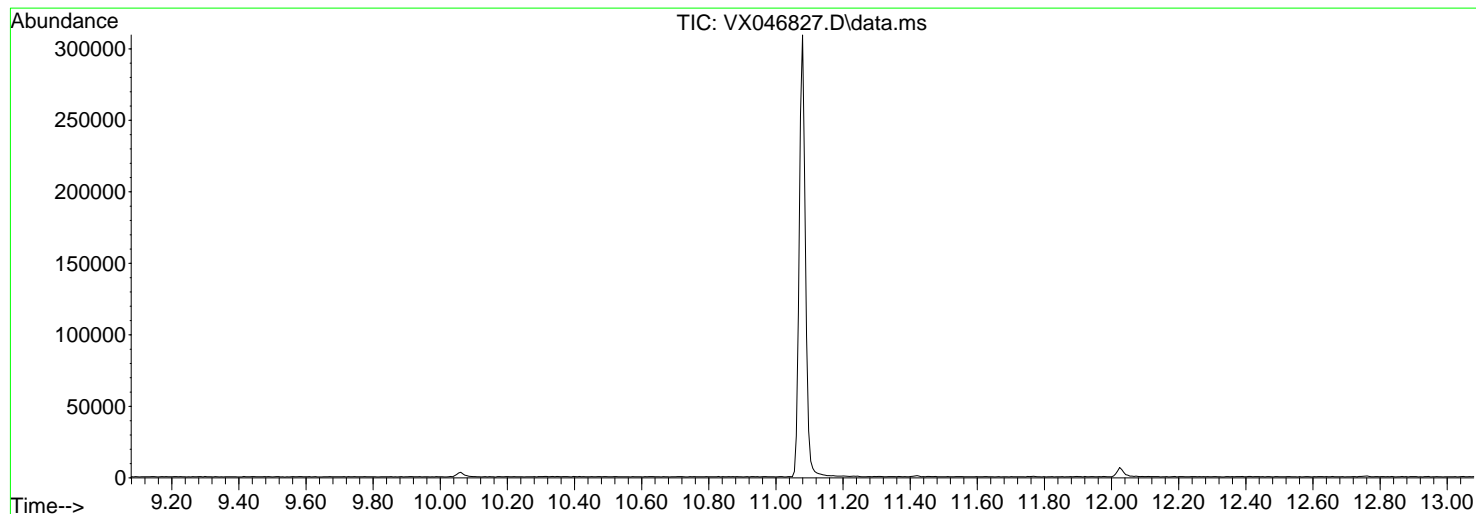

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	10245	PASS
75	95	30	60	50.5	27416	PASS
95	95	100	100	100.0	54285	PASS
96	95	5	9	6.6	3558	PASS
173	174	0.00	2	1.0	424	PASS
174	95	50	100	76.9	41731	PASS
175	174	5	9	7.4	3076	PASS
176	174	95	101	98.7	41184	PASS
177	176	5	9	6.2	2565	PASS