

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070119\
 Data File : VX010582.D
 Acq On : 01 Jul 2019 11:50
 Operator : JC/SP
 Sample : K3565-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0572

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.605	233	238	251	rVB	23387	41460	3.44%	0.549%
2	3.019	298	306	315	rVB	7033	17732	1.47%	0.235%
3	4.403	525	533	543	rVB4	4498	13122	1.09%	0.174%
4	4.696	569	581	589	rBV2	8678	28243	2.35%	0.374%
5	5.501	700	713	722	rBV	144703	419877	34.88%	5.555%
6	5.659	730	739	760	rVB	250107	716900	59.56%	9.485%
7	5.934	776	784	794	rBV6	5666	18715	1.55%	0.248%
8	6.062	796	805	816	rBV	135447	360058	29.91%	4.764%
9	6.263	830	838	846	rBV9	4062	12199	1.01%	0.161%
10	6.452	862	869	879	rVB6	5675	16261	1.35%	0.215%
11	6.860	926	936	953	rBV	363286	858254	71.30%	11.355%
12	7.464	1022	1035	1044	rBV	38524	95411	7.93%	1.262%
13	7.848	1091	1098	1105	rVB4	7246	14867	1.24%	0.197%
14	8.031	1121	1128	1136	rBV4	7154	17341	1.44%	0.229%
15	8.342	1174	1179	1183	rBV2	7577	14487	1.20%	0.192%
16	8.384	1183	1186	1191	rVB5	7200	12727	1.06%	0.168%
17	8.500	1200	1205	1209	rBV4	7157	12037	1.00%	0.159%
18	8.665	1225	1232	1235	rBV2	24248	44943	3.73%	0.595%
19	8.714	1235	1240	1248	rVB	785340	1203673	100.00%	15.925%
20	8.842	1255	1261	1265	rBV3	12513	21625	1.80%	0.286%
21	8.915	1269	1273	1277	rVB2	8365	13098	1.09%	0.173%
22	9.043	1288	1294	1302	rVB	25737	45995	3.82%	0.609%
23	9.165	1306	1314	1319	rBV3	13499	23155	1.92%	0.306%
24	9.573	1375	1381	1385	rBV4	11722	22589	1.88%	0.299%
25	9.622	1385	1389	1393	rVB	24351	33079	2.75%	0.438%
26	9.677	1393	1398	1403	rBV	45003	66893	5.56%	0.885%
27	9.884	1426	1432	1439	rBV4	8335	17821	1.48%	0.236%
28	10.110	1464	1469	1476	rVV	764141	1020189	84.76%	13.497%
29	10.250	1485	1492	1498	rVB	48504	69945	5.81%	0.925%
30	10.360	1501	1510	1516	rBV	93753	149723	12.44%	1.981%
31	10.640	1549	1556	1564	rBV5	9706	24149	2.01%	0.319%
32	10.835	1585	1588	1593	rVB4	10337	13857	1.15%	0.183%
33	10.908	1596	1600	1609	rVB7	9851	17842	1.48%	0.236%
34	11.018	1613	1618	1623	rBV	10378	14909	1.24%	0.197%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070119\
Data File : VX010582.D
Acq On : 01 Jul 2019 11:50
Operator : JC/SP
Sample : K3565-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0572

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260

35	11.134	1629	1637	1643	rBV	627774	816903	67.87%	10.808%
36	11.274	1652	1660	1666	rVB4	11100	18792	1.56%	0.249%
37	11.359	1670	1674	1678	rBV	11453	16220	1.35%	0.215%
38	11.433	1681	1686	1694	rVV	25769	55417	4.60%	0.733%
39	11.506	1694	1698	1706	rVB	20695	30095	2.50%	0.398%
40	11.664	1719	1724	1733	rBV	18478	26874	2.23%	0.356%
41	11.804	1743	1747	1753	rVB	40160	50772	4.22%	0.672%
42	12.079	1786	1792	1798	rVV	756104	971492	80.71%	12.853%
43	12.140	1798	1802	1807	rVB	16455	20413	1.70%	0.270%
44	12.371	1836	1840	1847	rVB7	11764	22784	1.89%	0.301%
45	12.768	1899	1905	1912	rBV7	5879	15281	1.27%	0.202%
46	13.347	1995	2000	2004	rBV2	9309	14462	1.20%	0.191%
47	13.646	2044	2049	2054	rBV6	6623	12493	1.04%	0.165%
48	13.835	2076	2080	2086	rVB	8349	13399	1.11%	0.177%


Sum of corrected areas: 7558573

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070119\
Data File : VX010582.D
Acq On : 01 Jul 2019 11:50
Operator : JC/SP
Sample : K3565-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0572

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

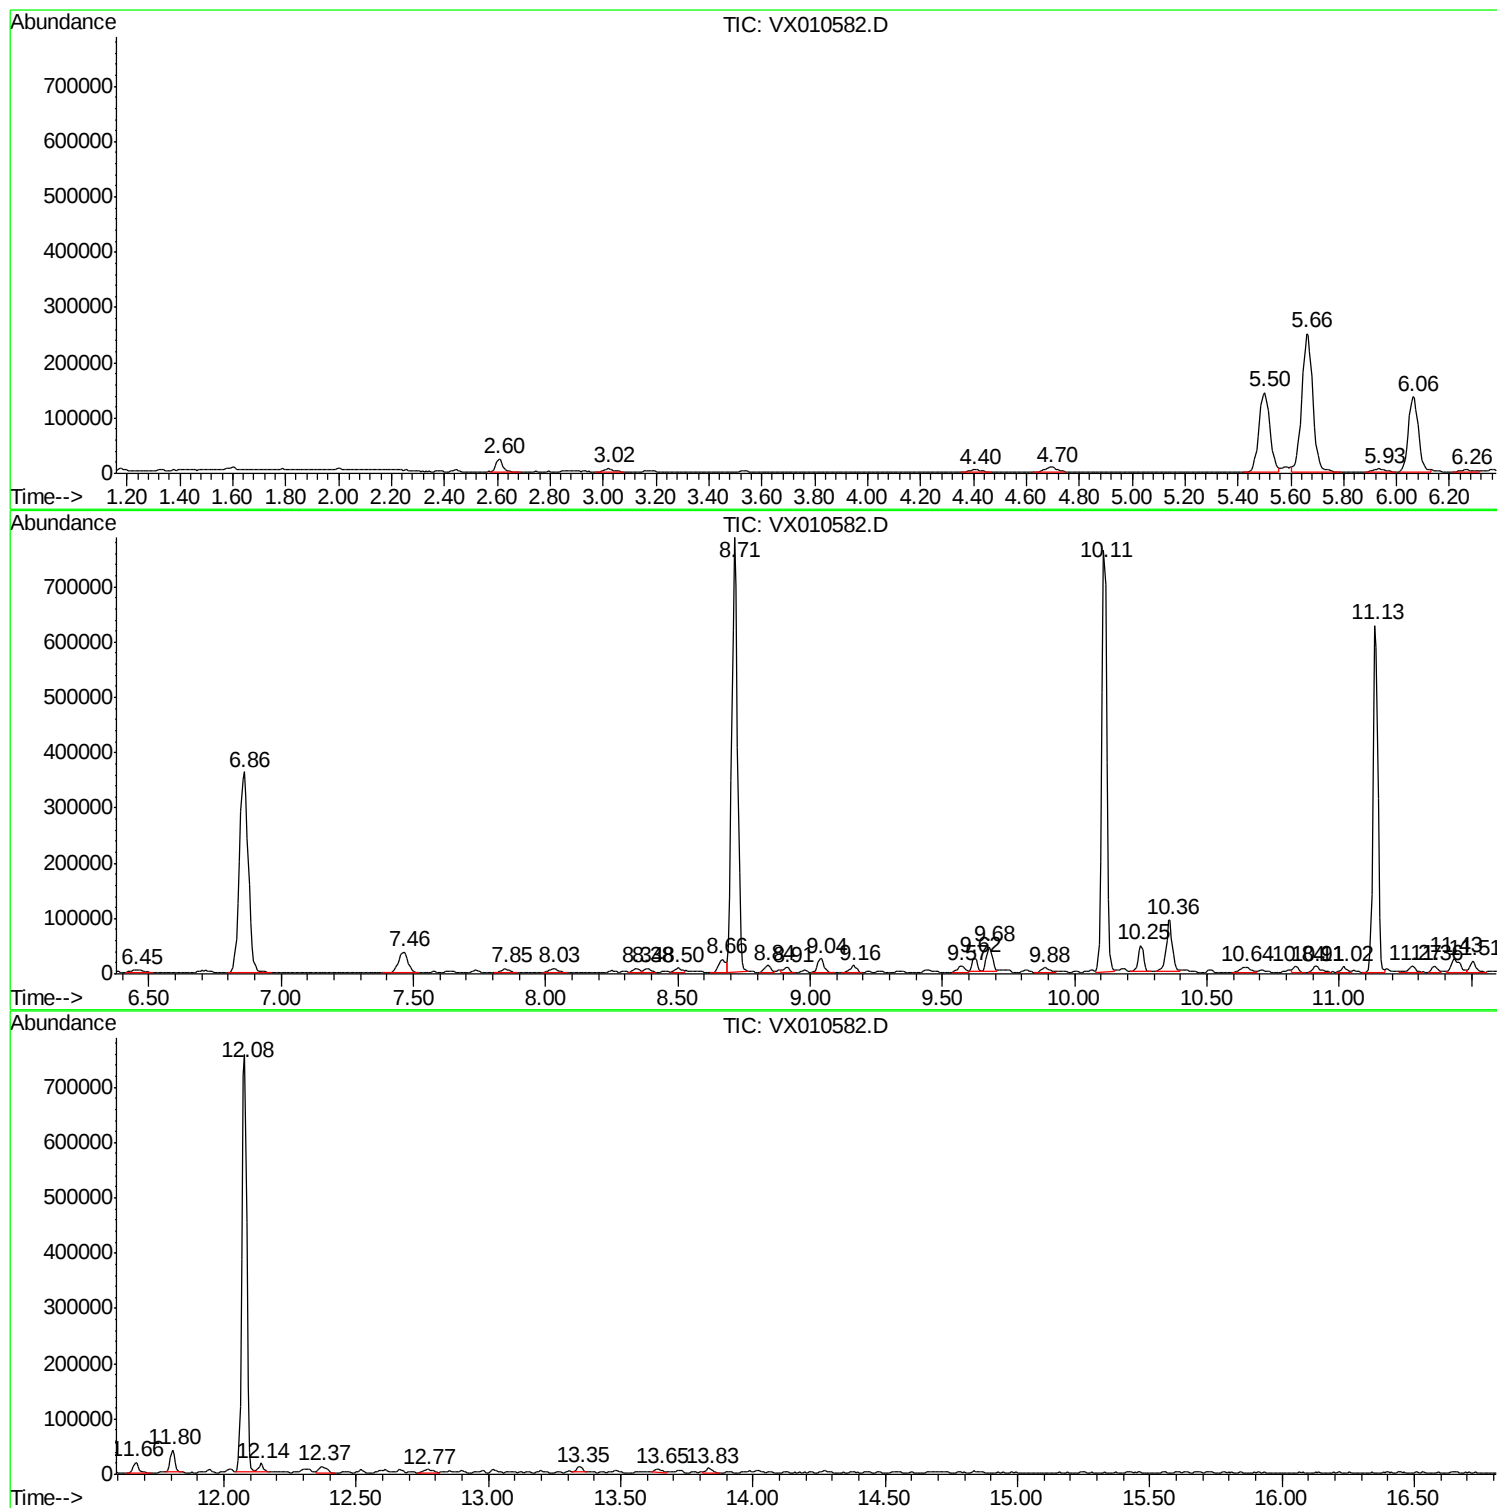

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070119\
Data File : VX010582.D
Acq On : 01 Jul 2019 11:50
Operator : JC/SP
Sample : K3565-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0572

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070119\
Data File : VX010582.D
Acq On : 01 Jul 2019 11:50
Operator : JC/SP
Sample : K3565-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0572

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc