

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070119\
 Data File : VX010583.D
 Acq On : 01 Jul 2019 12:14
 Operator : JC/SP
 Sample : K3565-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0575

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.611	232	239	246	rBV	14466	25848	2.15%	0.382%
2	5.500	700	713	724	rBV	144804	417362	34.76%	6.170%
3	5.659	730	739	760	rVB	246810	704758	58.70%	10.419%
4	6.067	794	806	819	rBV	137713	363004	30.24%	5.367%
5	6.860	926	936	950	rBV	370888	867608	72.27%	12.827%
6	7.463	1026	1035	1043	rVB4	17521	41409	3.45%	0.612%
7	8.713	1226	1240	1255	rBV	762618	1200533	100.00%	17.749%
8	10.109	1463	1469	1478	rBV	726494	1015279	84.57%	15.010%
9	10.249	1488	1492	1498	rBV	11593	16062	1.34%	0.237%
10	10.359	1502	1510	1516	rBV	20739	32042	2.67%	0.474%
11	11.018	1613	1618	1623	rVB	18163	23986	2.00%	0.355%
12	11.133	1630	1637	1653	rBV	620094	813704	67.78%	12.030%
13	11.359	1670	1674	1678	rBV	11731	15380	1.28%	0.227%
14	11.450	1683	1689	1695	rBV	10786	16918	1.41%	0.250%
15	11.670	1720	1725	1730	rBV	34515	47077	3.92%	0.696%
16	11.804	1743	1747	1756	rVB	62751	81625	6.80%	1.207%
17	12.078	1786	1792	1798	rBV	741052	955535	79.59%	14.127%
18	12.139	1798	1802	1809	rVB	37644	50012	4.17%	0.739%
19	12.298	1824	1828	1833	rVB2	14036	19965	1.66%	0.295%
20	12.755	1898	1903	1909	rBV3	7584	13005	1.08%	0.192%
21	13.340	1995	1999	2006	rVB3	13950	22260	1.85%	0.329%
22	13.834	2076	2080	2085	rVB	15718	20747	1.73%	0.307%


Sum of corrected areas: 6764119

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070119\
Data File : VX010583.D
Acq On : 01 Jul 2019 12:14
Operator : JC/SP
Sample : K3565-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0575

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

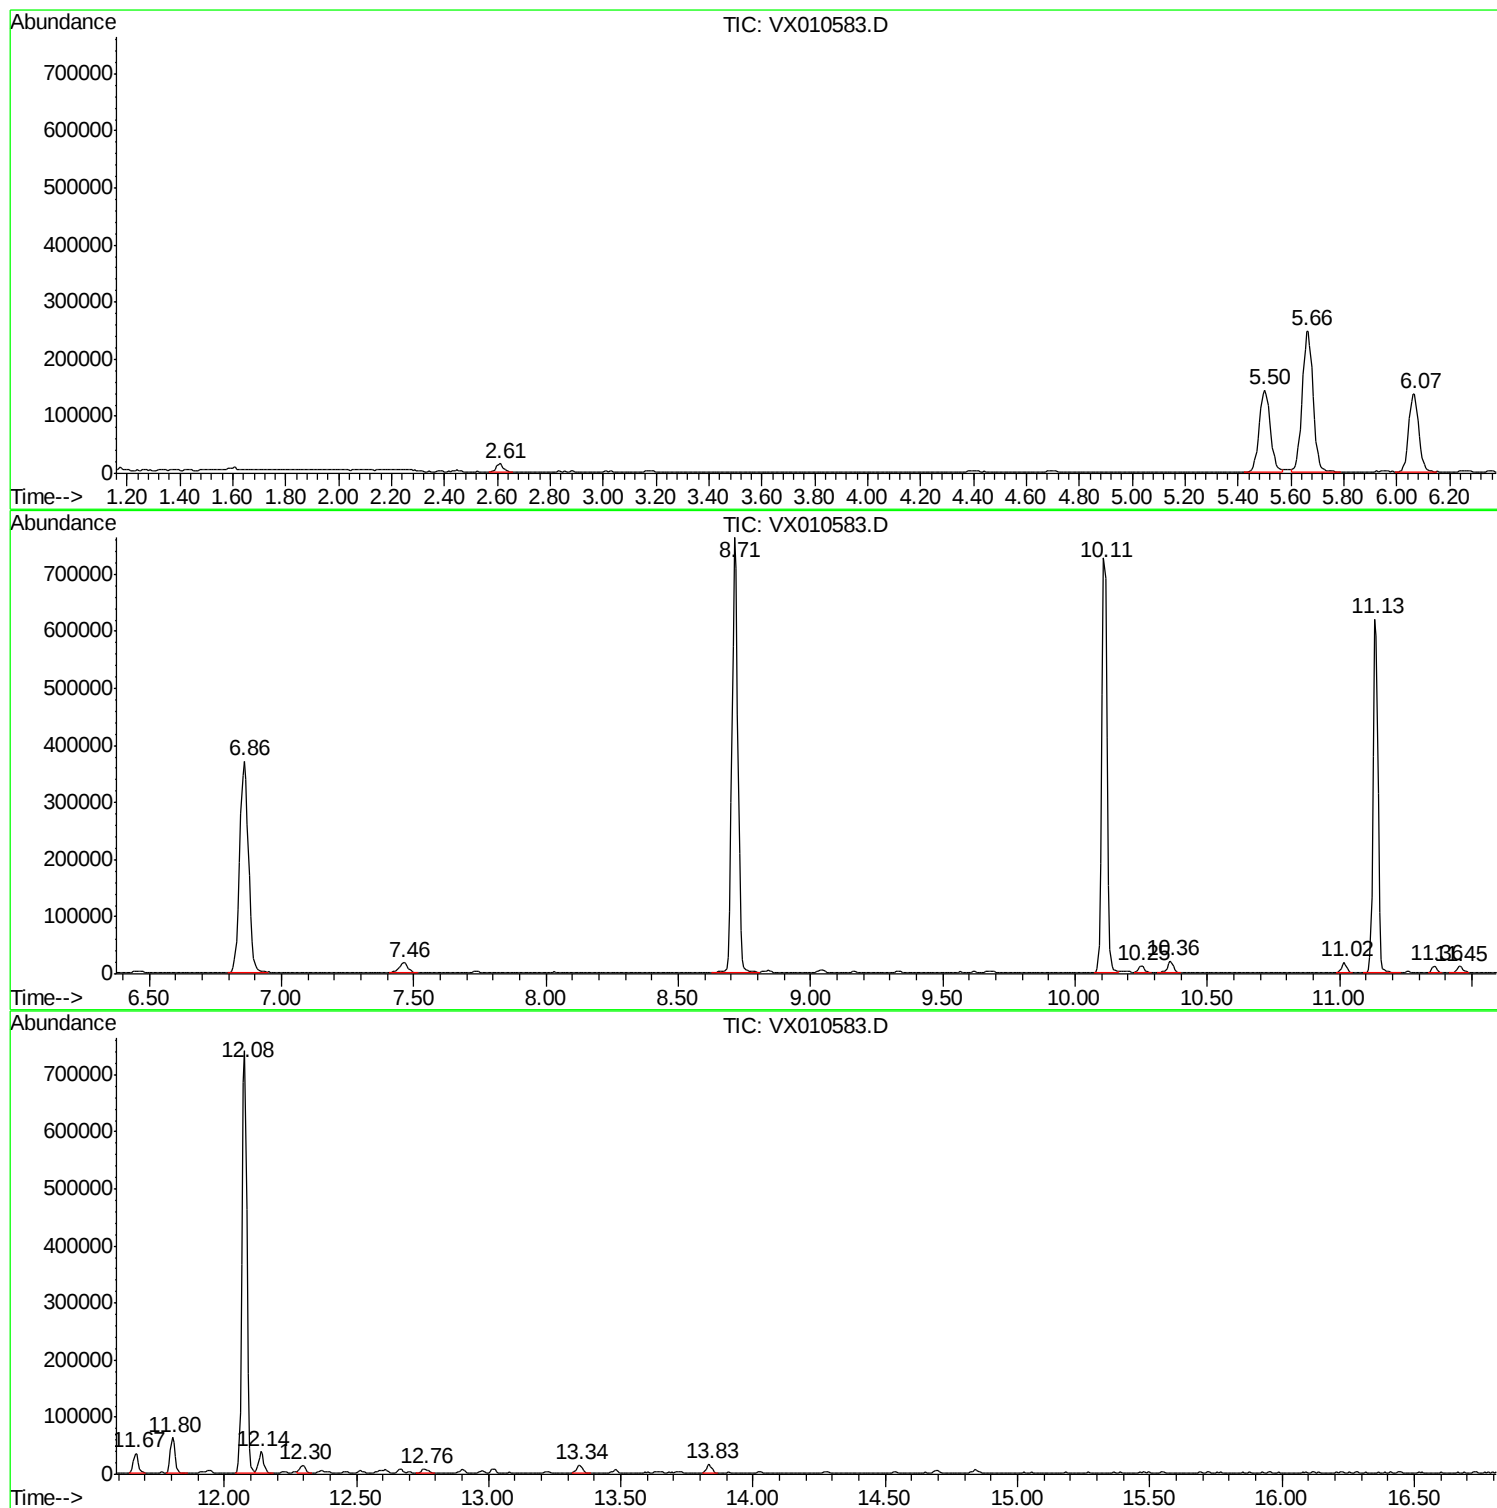

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070119\
Data File : VX010583.D
Acq On : 01 Jul 2019 12:14
Operator : JC/SP
Sample : K3565-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0575

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX070119\
Data File : VX010583.D
Acq On : 01 Jul 2019 12:14
Operator : JC/SP
Sample : K3565-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0575

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc