

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070120\
 Data File : VX017109.D
 Acq On : 01 Jul 2020 19:25
 Operator : JC/SP
 Sample : L3159-02 100X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 65BR-20200629

Quant Time: Jul 02 03:29:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 29 17:10:38 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	229546	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	391557	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	403197	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	218116	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	151071	53.38	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.76%	
35) Dibromofluoromethane	5.46	113	128502	51.88	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.76%	
50) Toluene-d8	8.70	98	470829	51.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.82%	
62) 4-Bromofluorobenzene	11.12	95	197416	55.14	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.28%	
Target Compounds						
27) cis-1,2-Dichloroethene	4.57	96	1065	0.373	ug/l	Qvalue 41

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070120\
Data File : VX017109.D
Acq On : 01 Jul 2020 19:25
Operator : JC/SP
Sample : L3159-02 100X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
65BR-20200629

Quant Time: Jul 02 03:29:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 29 17:10:38 2020
Response via : Initial Calibration

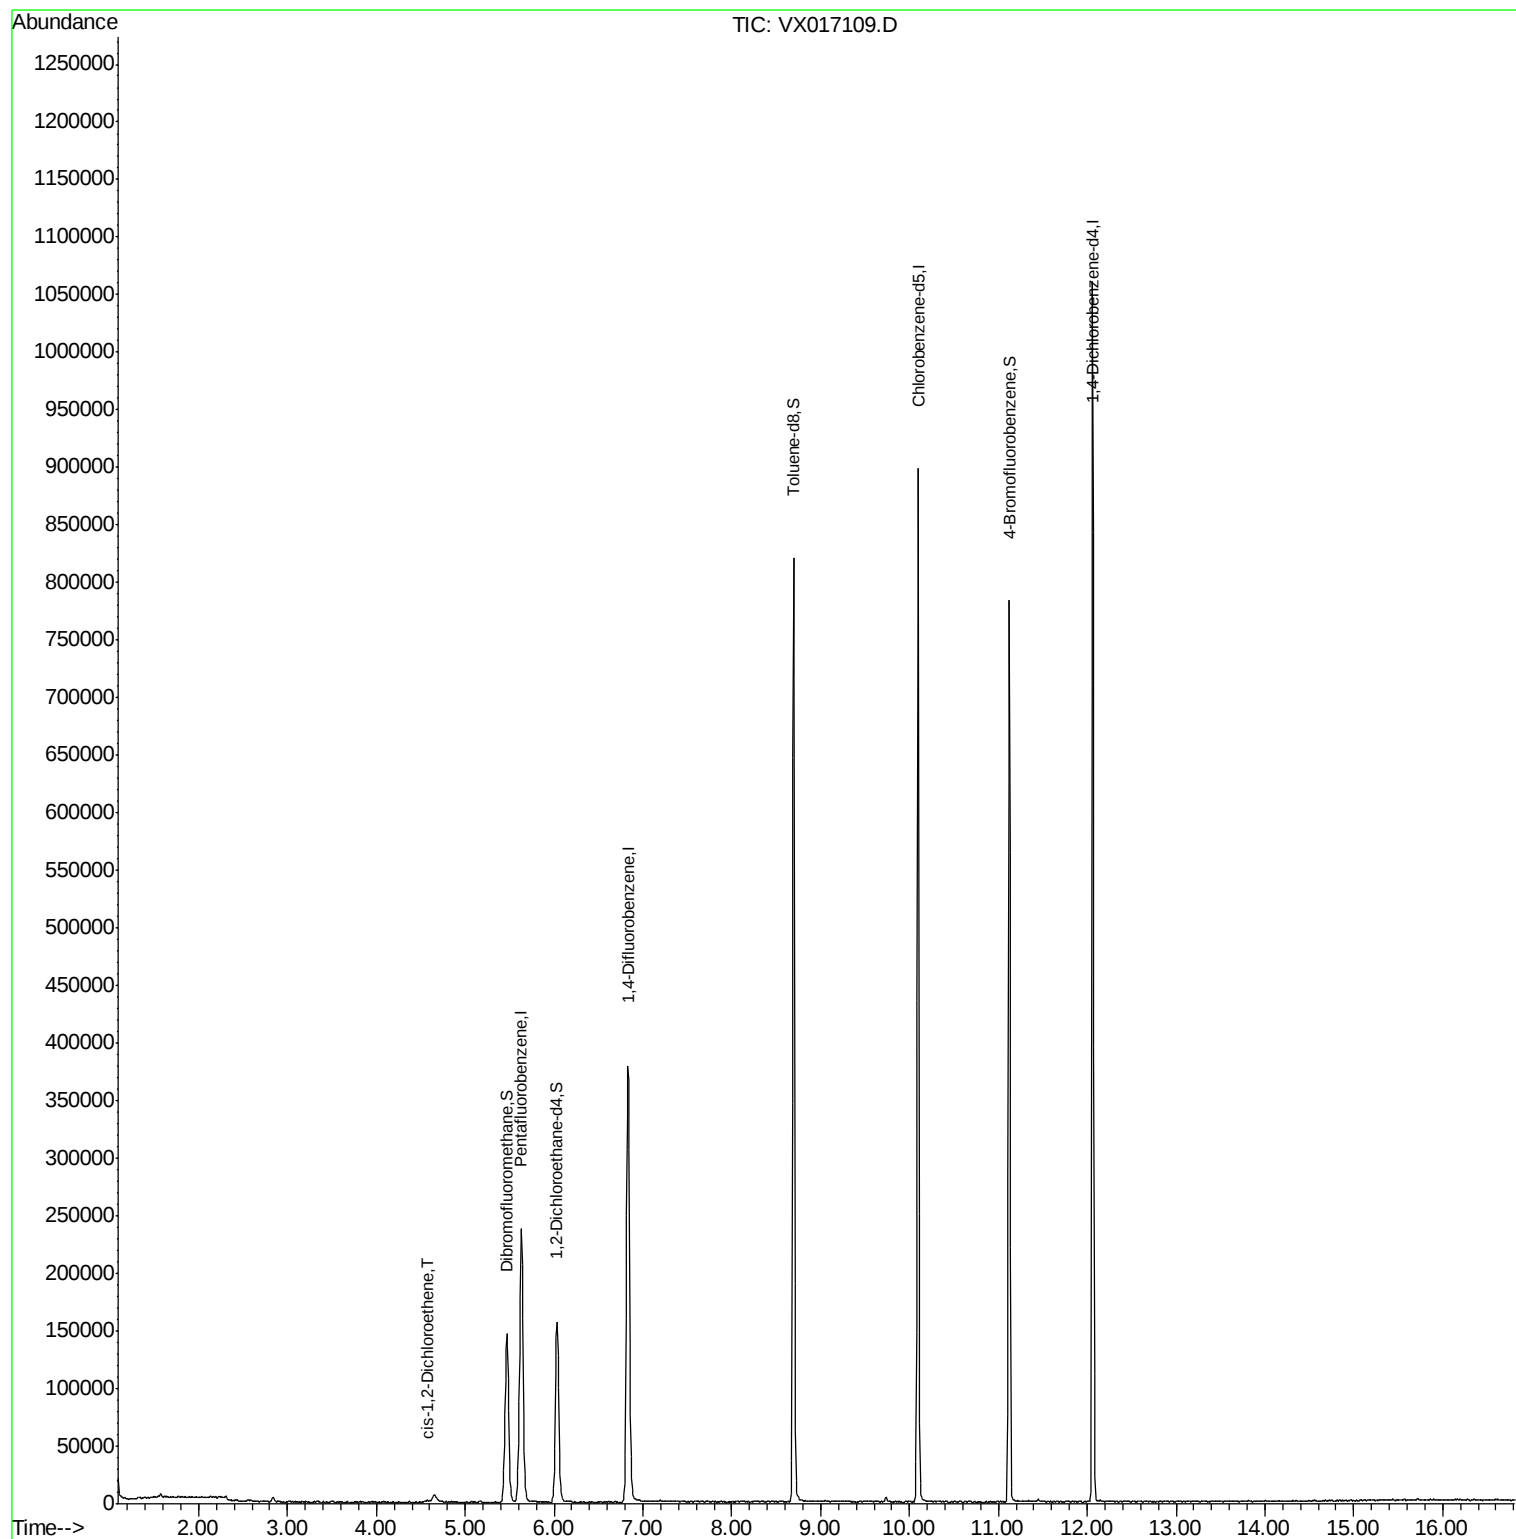



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017109.D

Acq: 01 Jul 2020 19:25

Instrument :

MSVOA_X

ClientSampleId :


65BR-20200629

Tot Ion:168 Resp: 229546

Ion Ratio Lower Upper




168 100

99 54.6 42.6 64.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

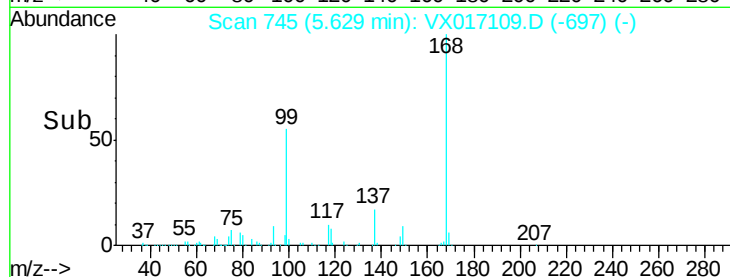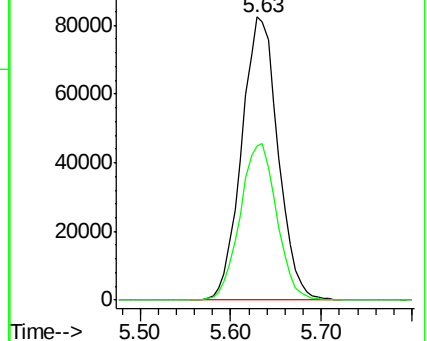

#27

cis-1,2-Dichloroethene

Concen: 0.373 ug/l

RT: 4.57 min Scan# 572

Delta R.T. 0.01 min

Lab File: VX017109.D

Acq: 01 Jul 2020 19:25


Tgt Ion: 96 Resp: 1065

Ion Ratio Lower Upper

96 100

61 45.5 0.0 282.8



98 50.4 0.0 127.6




Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

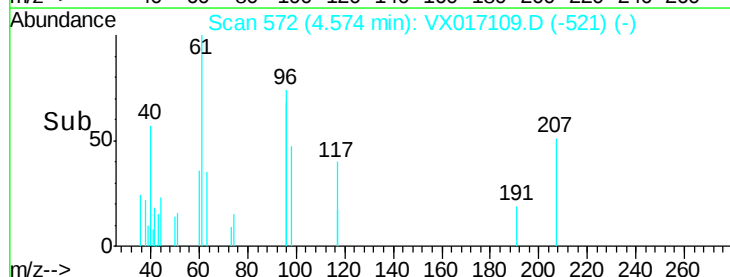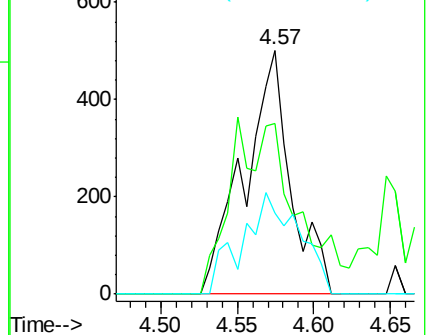

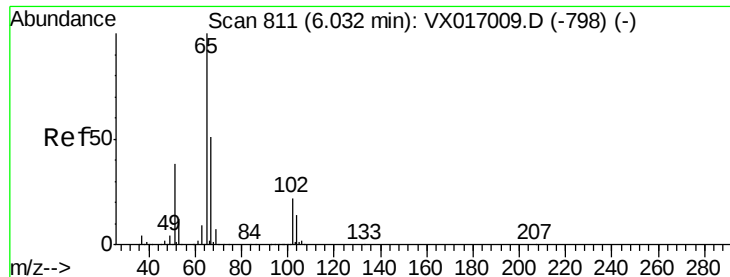

#33

1,2-Dichloroethane-d4

Concen: 53.385 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX017109.D

Acq: 01 Jul 2020 19:25

Instrument :

MSVOA_X

ClientSampleId :


65BR-20200629

Tot Ion: 65 Resp: 151071

Ion Ratio Lower Upper




65 100

67 50.8 0.0 103.8



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

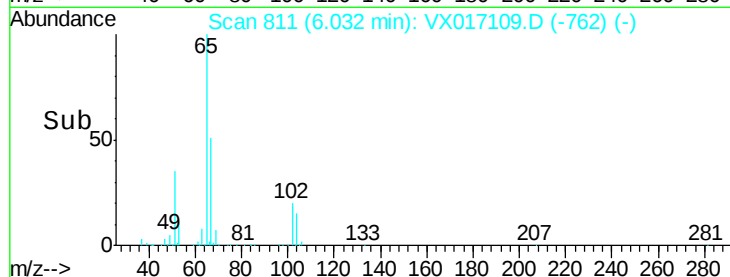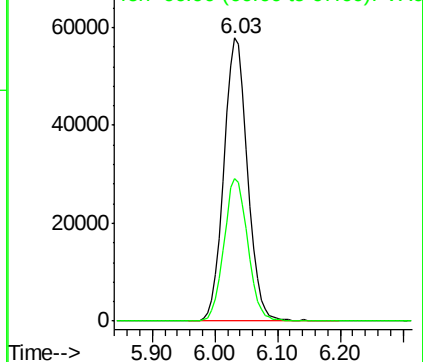

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017109.D

Acq: 01 Jul 2020 19:25


Tgt Ion: 114 Resp: 391557

Ion Ratio Lower Upper

114 100

63 20.5 0.0 41.4



88 15.8 0.0 32.4




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



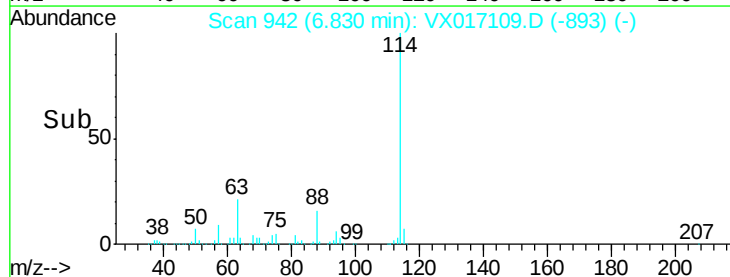
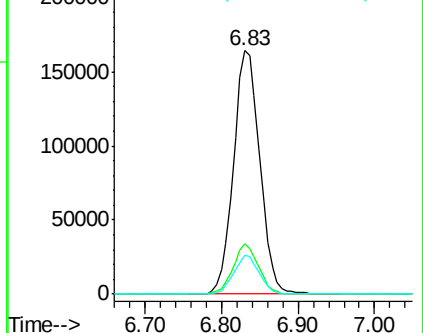


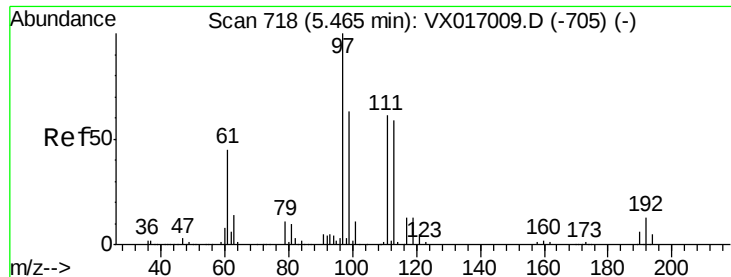

#35
 Dibromofluoromethane
 Concen: 51.881 ug/l
 RT: 5.46 min Scan# 718
 Delta R.T. -0.00 min
 Lab File: VX017109.D
 Acq: 01 Jul 2020 19:25




Instrument :
 MSVOA_X
 ClientSampleId :
 65BR-20200629


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.0	81.9	122.9
192	21.2	16.7	25.1

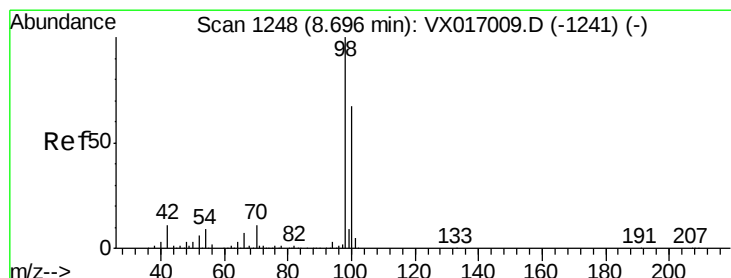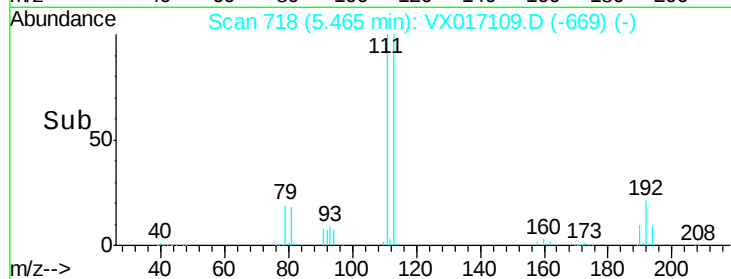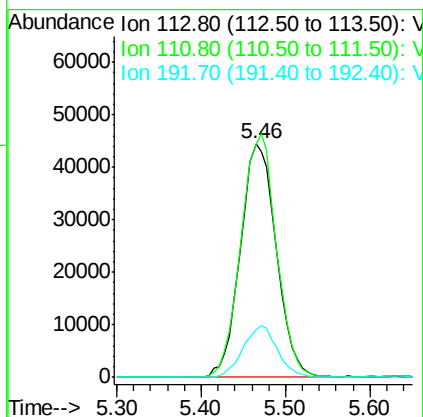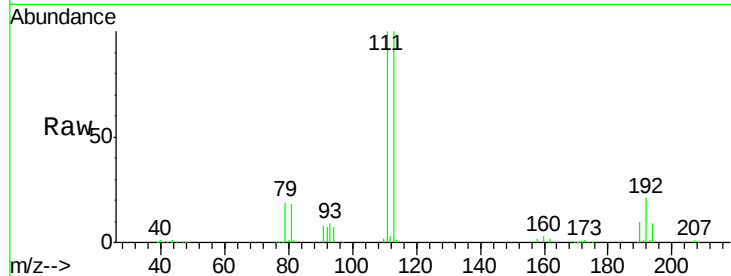

#50
 Toluene-d8
 Concen: 51.406 ug/l
 RT: 8.70 min Scan# 1248
 Delta R.T. -0.00 min
 Lab File: VX017109.D
 Acq: 01 Jul 2020 19:25

Tgt Ion	Ratio	Lower	Upper
98	100		
100	66.2	53.8	80.6

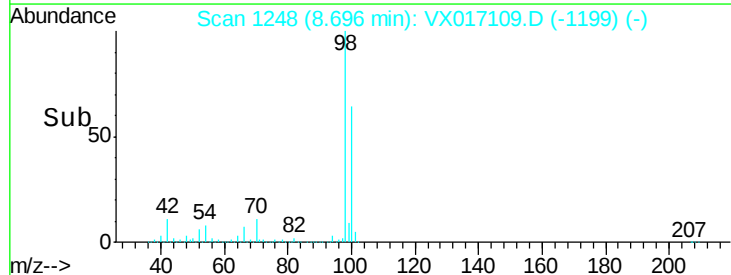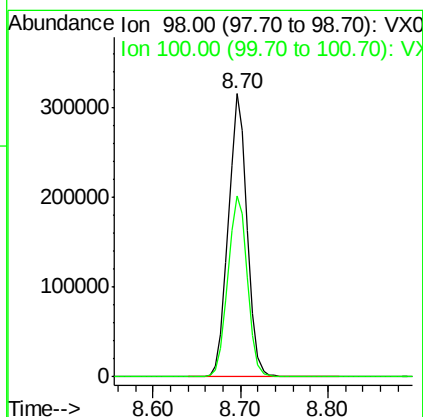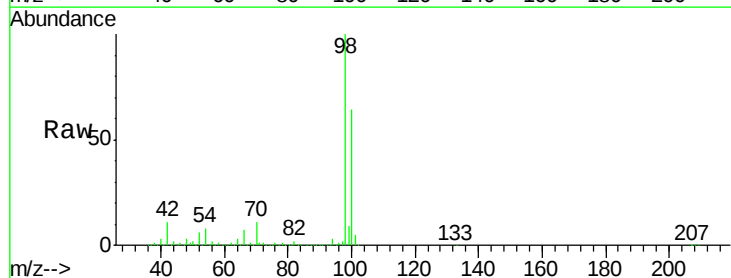

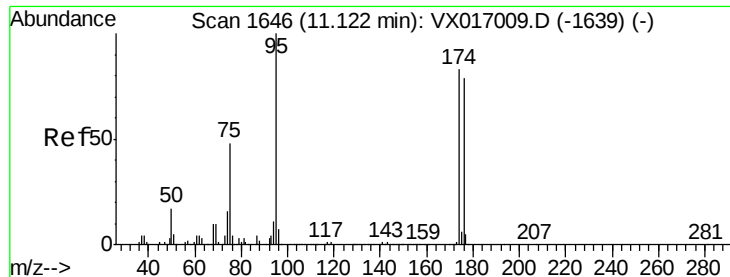

#62

4-Bromofluorobenzene

Concen: 55.139 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX017109.D

Acq: 01 Jul 2020 19:25

Instrument :

MSVOA_X

ClientSampleId :

65BR-20200629


Tot Ion: 95 Resp: 197416

Ion Ratio Lower Upper

95 100

174 83.0 0.0 164.0




176 80.3 0.0 157.6



Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

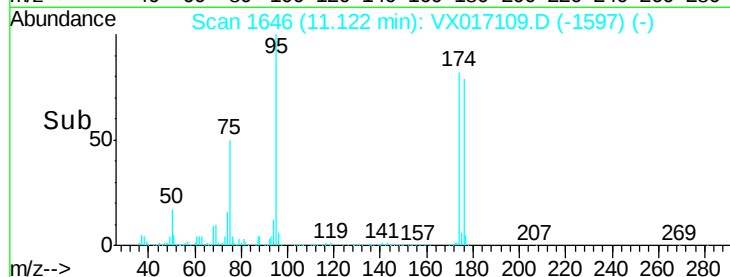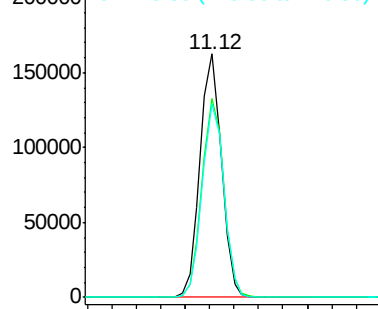

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX017109.D

Acq: 01 Jul 2020 19:25


Tgt Ion: 117 Resp: 403197

Ion Ratio Lower Upper

117 100

82 52.5 42.6 63.8



119 31.7 25.4 38.2




Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

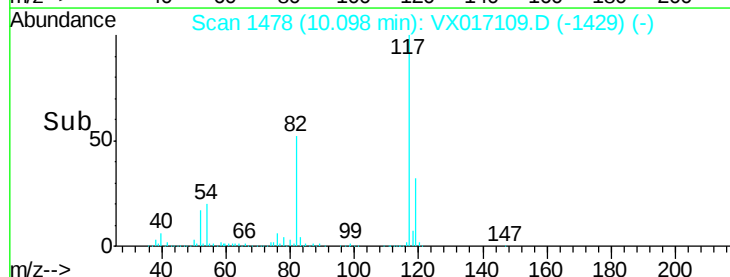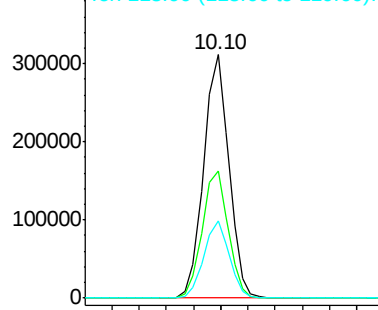

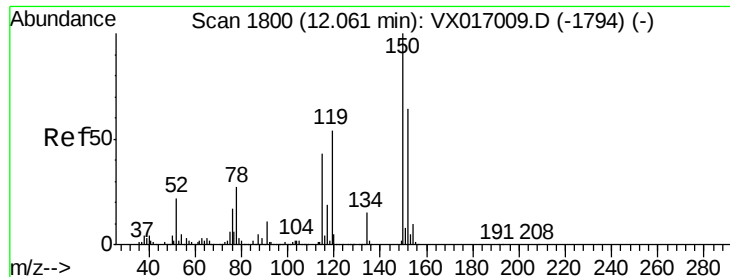

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX017109.D

Acq: 01 Jul 2020 19:25

Instrument :

MSVOA_X

ClientSampleId :

65BR-20200629


Tot Ion:152 Resp: 218116

Ion Ratio Lower Upper

152 100

115 56.2 40.9 122.7

150 150.7 0.0 351.6



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

