

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070120\
 Data File : VX017097.D
 Acq On : 01 Jul 2020 14:52
 Operator : JC/SP
 Sample : L3163-03 20X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 I-LDC-3

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.178	10	15	20	rVB	22042	22628	1.68%	0.233%
2	2.416	213	218	227	rBV	35425	58630	4.36%	0.603%
3	2.550	233	240	254	rBV	661732	1091495	81.14%	11.234%
4	4.647	575	584	594	rBV3	9112	29848	2.22%	0.307%
5	5.470	707	719	732	rBV	147587	425703	31.65%	4.382%
6	5.635	735	746	764	rVB	228459	656055	48.77%	6.753%
7	6.031	800	811	821	rBV	156050	414372	30.81%	4.265%
8	6.117	821	825	836	rVB2	11734	28722	2.14%	0.296%
9	6.830	931	942	953	rBV	374449	886121	65.88%	9.121%
10	8.464	1204	1210	1215	rBV2	11940	20725	1.54%	0.213%
11	8.695	1241	1248	1255	rBV	802482	1235865	91.88%	12.720%
12	8.762	1257	1259	1266	rVB2	9875	15167	1.13%	0.156%
13	8.890	1274	1280	1287	rVB	16424	25152	1.87%	0.259%
14	10.098	1471	1478	1493	rBV	853855	1158480	86.12%	11.924%
15	10.341	1515	1518	1526	rVB4	17984	29595	2.20%	0.305%
16	11.122	1640	1646	1653	rBV	743366	933194	69.38%	9.605%
17	12.061	1794	1800	1807	rBV	1031129	1239731	92.17%	12.760%
18	13.816	2082	2088	2098	rBV	1153003	1345121	100.00%	13.845%
19	13.908	2098	2103	2113	rVB	42035	57356	4.26%	0.590%
20	14.676	2225	2229	2235	rVB	19332	26350	1.96%	0.271%
21	14.822	2248	2253	2260	rVB	11047	15265	1.13%	0.157%


Sum of corrected areas: 9715575

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070120\
Data File : VX017097.D
Acq On : 01 Jul 2020 14:52
Operator : JC/SP
Sample : L3163-03 20X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-LDC-3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

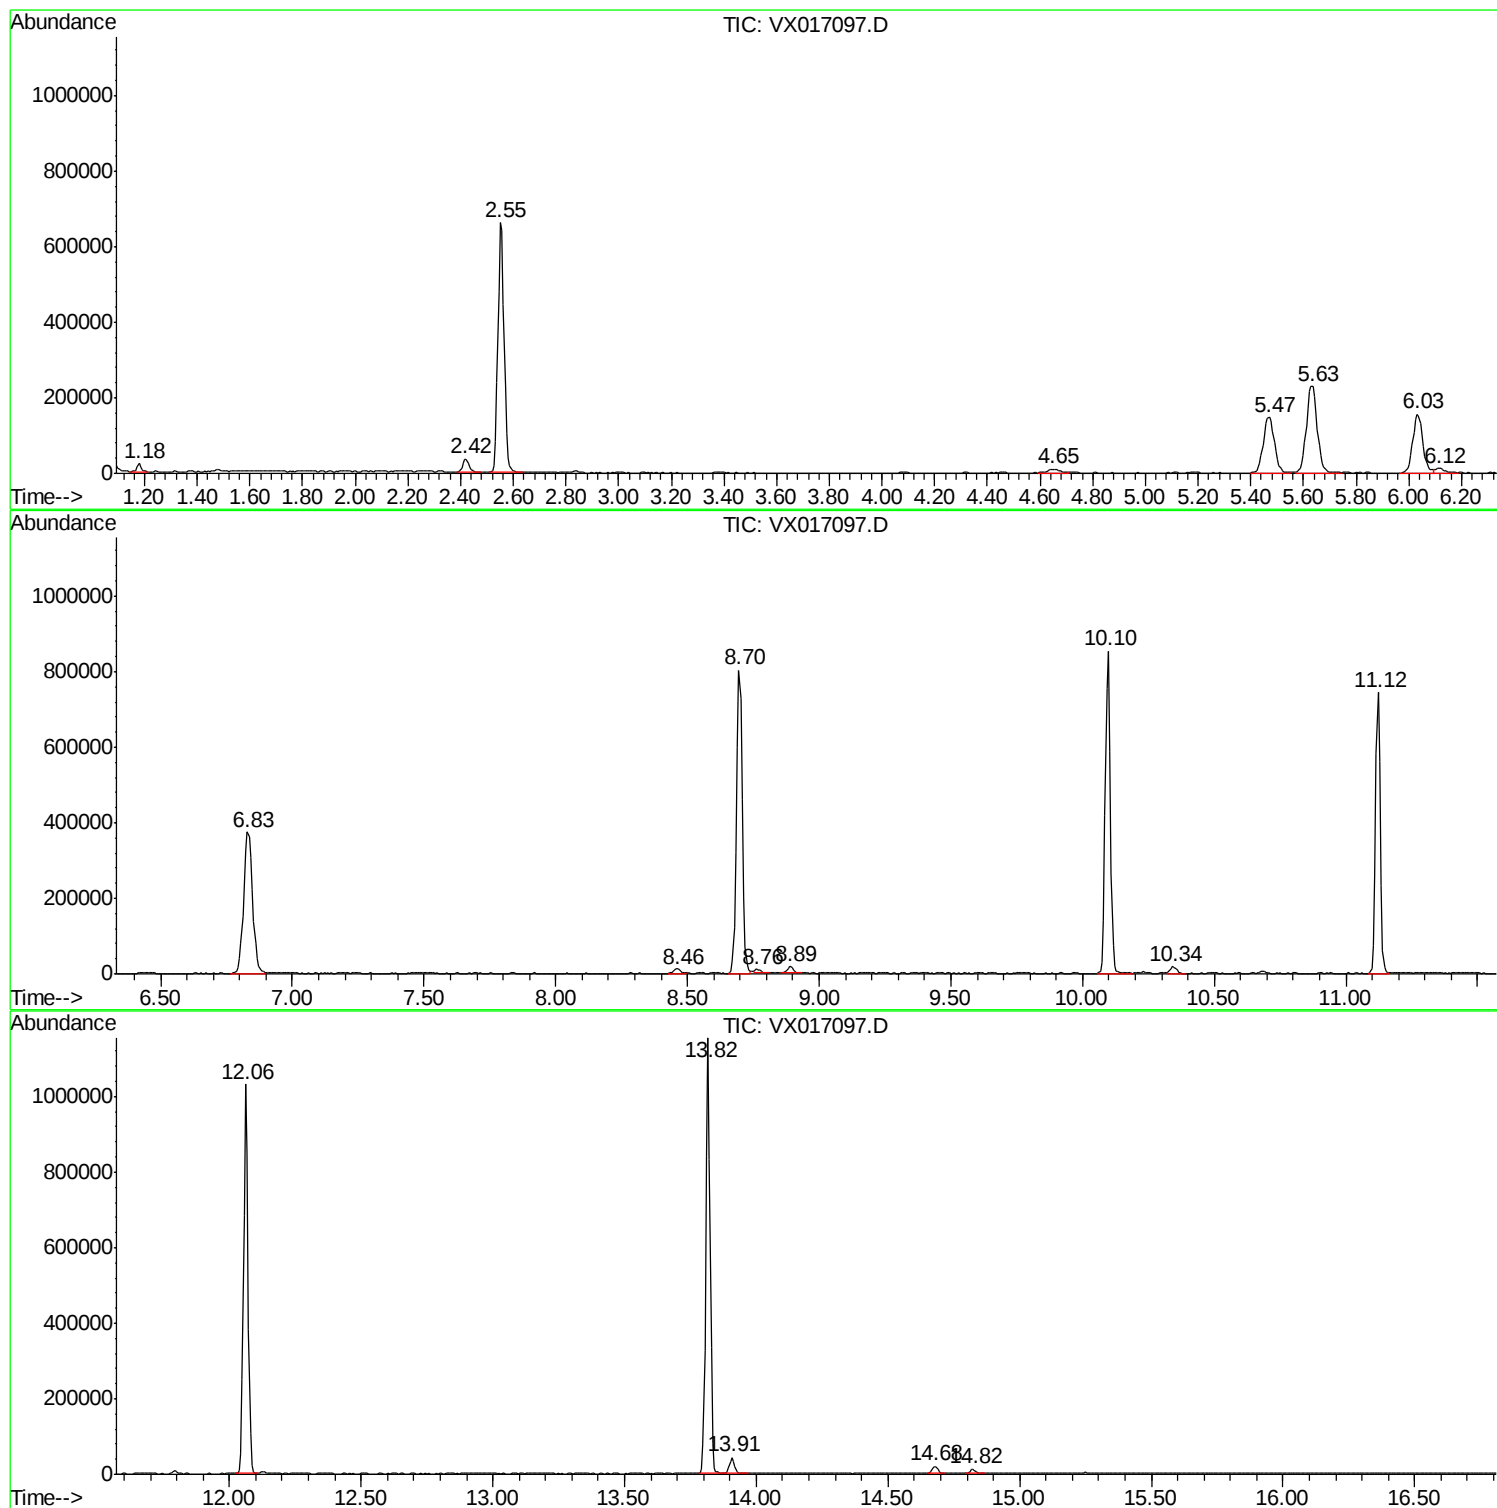

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070120\
Data File : VX017097.D
Acq On : 01 Jul 2020 14:52
Operator : JC/SP
Sample : L3163-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-LDC-3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX070120\
Data File : VX017097.D
Acq On : 01 Jul 2020 14:52
Operator : JC/SP
Sample : L3163-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-LDC-3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc