

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX070120\  
Data File : VX017111.D  
Acq On : 01 Jul 2020 20:11  
Operator : JC/SP  
Sample : L3159-04 100X  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
40S-20200629

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X062920W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.470       | 707           | 719         | 731          | rBV      | 142732         | 418791        | 33.14%          | 5.999%        |
| 2         | 5.629       | 734           | 745         | 762          | rVB      | 234709         | 657950        | 52.06%          | 9.424%        |
| 3         | 6.031       | 801           | 811         | 827          | rBV      | 154126         | 407587        | 32.25%          | 5.838%        |
| 4         | 6.830       | 932           | 942         | 962          | rBV      | 374136         | 894148        | 70.75%          | 12.807%       |
| 5         | 8.695       | 1239          | 1248        | 1261         | rBV      | 802076         | 1237484       | 97.92%          | 17.725%       |
| 6         | 10.098      | 1472          | 1478        | 1488         | rBV      | 875051         | 1157468       | 91.59%          | 16.579%       |
| 7         | 11.122      | 1639          | 1646        | 1659         | rBV      | 762299         | 944414        | 74.73%          | 13.527%       |
| 8         | 12.061      | 1794          | 1800        | 1810         | rBV      | 1024701        | 1263739       | 100.00%         | 18.101%       |


Sum of corrected areas: 6981581

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX070120\  
Data File : VX017111.D  
Acq On : 01 Jul 2020 20:11  
Operator : JC/SP  
Sample : L3159-04 100X  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
40S-20200629

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X062920W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

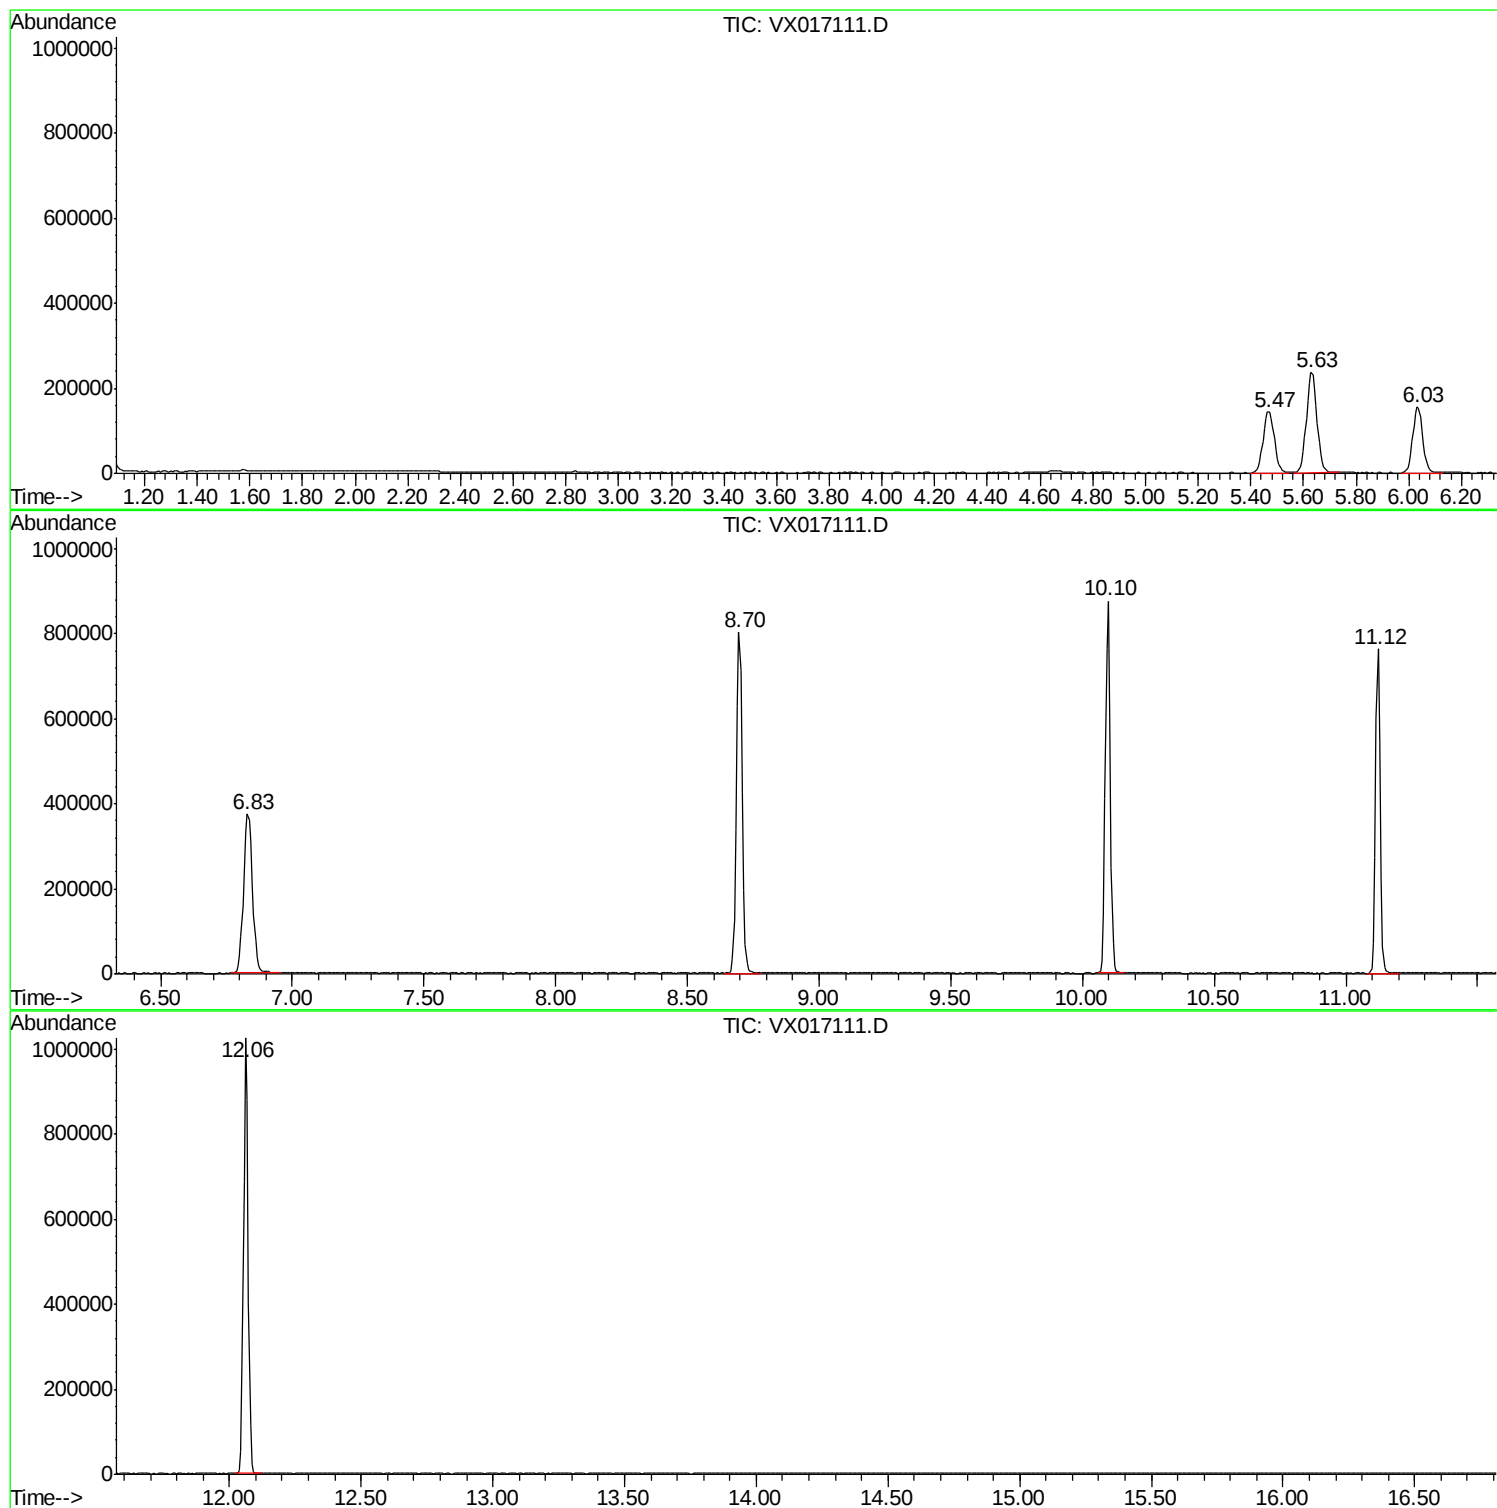

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX070120\  
Data File : VX017111.D  
Acq On : 01 Jul 2020 20:11  
Operator : JC/SP  
Sample : L3159-04 100X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
40S-20200629

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X062920W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX070120\  
Data File : VX017111.D  
Acq On : 01 Jul 2020 20:11  
Operator : JC/SP  
Sample : L3159-04 100X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
40S-20200629

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X062920W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |