


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX070120\
Data File : VX017113.D
Acq On : 01 Jul 2020 21:19
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Title : SW846 8260
Last Update : Mon Jun 29 17:10:38 2020

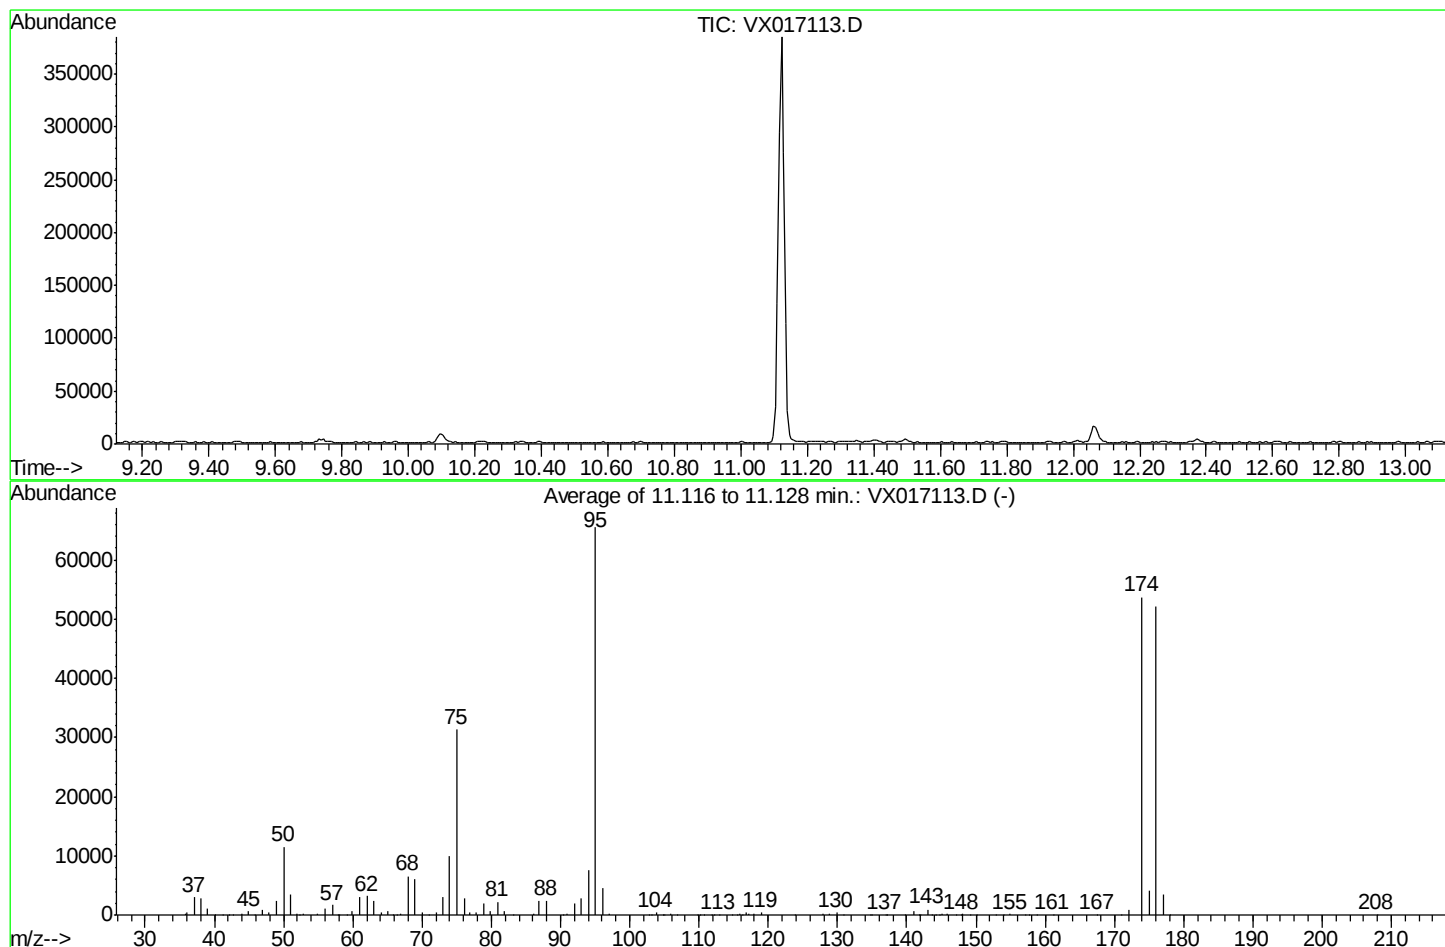

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	11474	PASS
75	95	30	60	47.8	31300	PASS
95	95	100	100	100.0	65512	PASS
96	95	5	9	6.8	4487	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.0	53741	PASS
175	174	5	9	7.6	4089	PASS
176	174	95	101	97.0	52112	PASS
177	176	5	9	6.8	3566	PASS