

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
 Data File : VX023085.D
 Acq On : 01 Jul 2021 15:16
 Operator : JC/MD
 Sample : M2882-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DRIP-COMP-AUD-1121-1122DL

Quant Time: Jul 01 16:06:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 23 19:12:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	55682	50.00	ug/l	# 0.01
34) 1,4-Difluorobenzene	6.769	114	111726	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	101679	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	37561	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	58994	58.38	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 116.76%	
35) Dibromofluoromethane	5.391	113	36344	51.23	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.46%	
50) Toluene-d8	8.653	98	139941	50.33	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 100.66%	
62) 4-Bromofluorobenzene	11.085	95	50231	48.40	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 96.80%	


Target Compounds				Qvalue		
3) Chloromethane	1.294	50	202	0.23	ug/l	91
5) Bromomethane	1.611	94	190	0.43	ug/l	89
10) Methyl Iodide	2.459	142	130	4.02	ug/l #	60
11) Tert butyl alcohol	2.977	59	5075	24.10	ug/l #	82
13) Acrolein	2.251	56	4852	37.04	ug/l #	14
14) Allyl chloride	2.648	41	723	0.53	ug/l #	37
16) Acetone	2.386	43	21084	47.06	ug/l #	33
17) Carbon Disulfide	2.507	76	491	3.75	ug/l #	75
18) Methyl Acetate	2.709	43	694	0.63	ug/l #	47
20) Methylene Chloride	2.794	84	1092	1.59	ug/l #	73
22) Diisopropyl ether	3.885	45	37491	13.13	ug/l #	1
23) Vinyl Acetate	3.885	43	100081	41.79	ug/l #	68
25) 2-Butanone	4.568	43	207382	297.69	ug/l #	89
29) Tetrahydrofuran	5.044	42	383	0.85	ug/l #	37
31) Cyclohexane	5.568	56	2031	1.42	ug/l #	35
36) 1,1-Dichloropropene	5.562	75	6967	5.87	ug/l #	48
37) Ethyl Acetate	4.568	43	207382	150.86	ug/l #	65
38) Carbon Tetrachloride	5.556	117	7287	7.32	ug/l #	12
40) Benzene	6.043	78	1747	0.51	ug/l	99
44) Trichloroethene	7.141	130	271	0.33	ug/l	48
51) 4-Methyl-2-Pentanone	8.580	43	696	0.51	ug/l #	72
52) Toluene	8.726	92	3484	1.68	ug/l	98
53) t-1,3-Dichloropropene	9.000	75	20	3.68	ug/l #	44
56) Ethyl methacrylate	9.000	69	153	2.67	ug/l #	1
59) 2-Hexanone	9.165	43	1042	1.00	ug/l	76
68) m/p-Xylenes	10.299	106	713	0.49	ug/l	86
74) N-amyl acetate	10.847	43	472	2.31	ug/l #	38
75) 1,1,2,2-Tetrachloroethane	11.152	83	682	0.62	ug/l #	26
76) 1,2,3-Trichloropropane	11.085	75	30991	31.24	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	30991	79.90	ug/l #	12
93) 1,2,4-Trichlorobenzene	13.597	180	165	0.24	ug/l #	56
95) Naphthalene	13.780	128	1799	2.49	ug/l #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
Data File : VX023085.D
Acq On : 01 Jul 2021 15:16
Operator : JC/MD
Sample : M2882-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL

Quant Time: Jul 01 16:06:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 19:12:26 2021
Response via : Initial Calibration




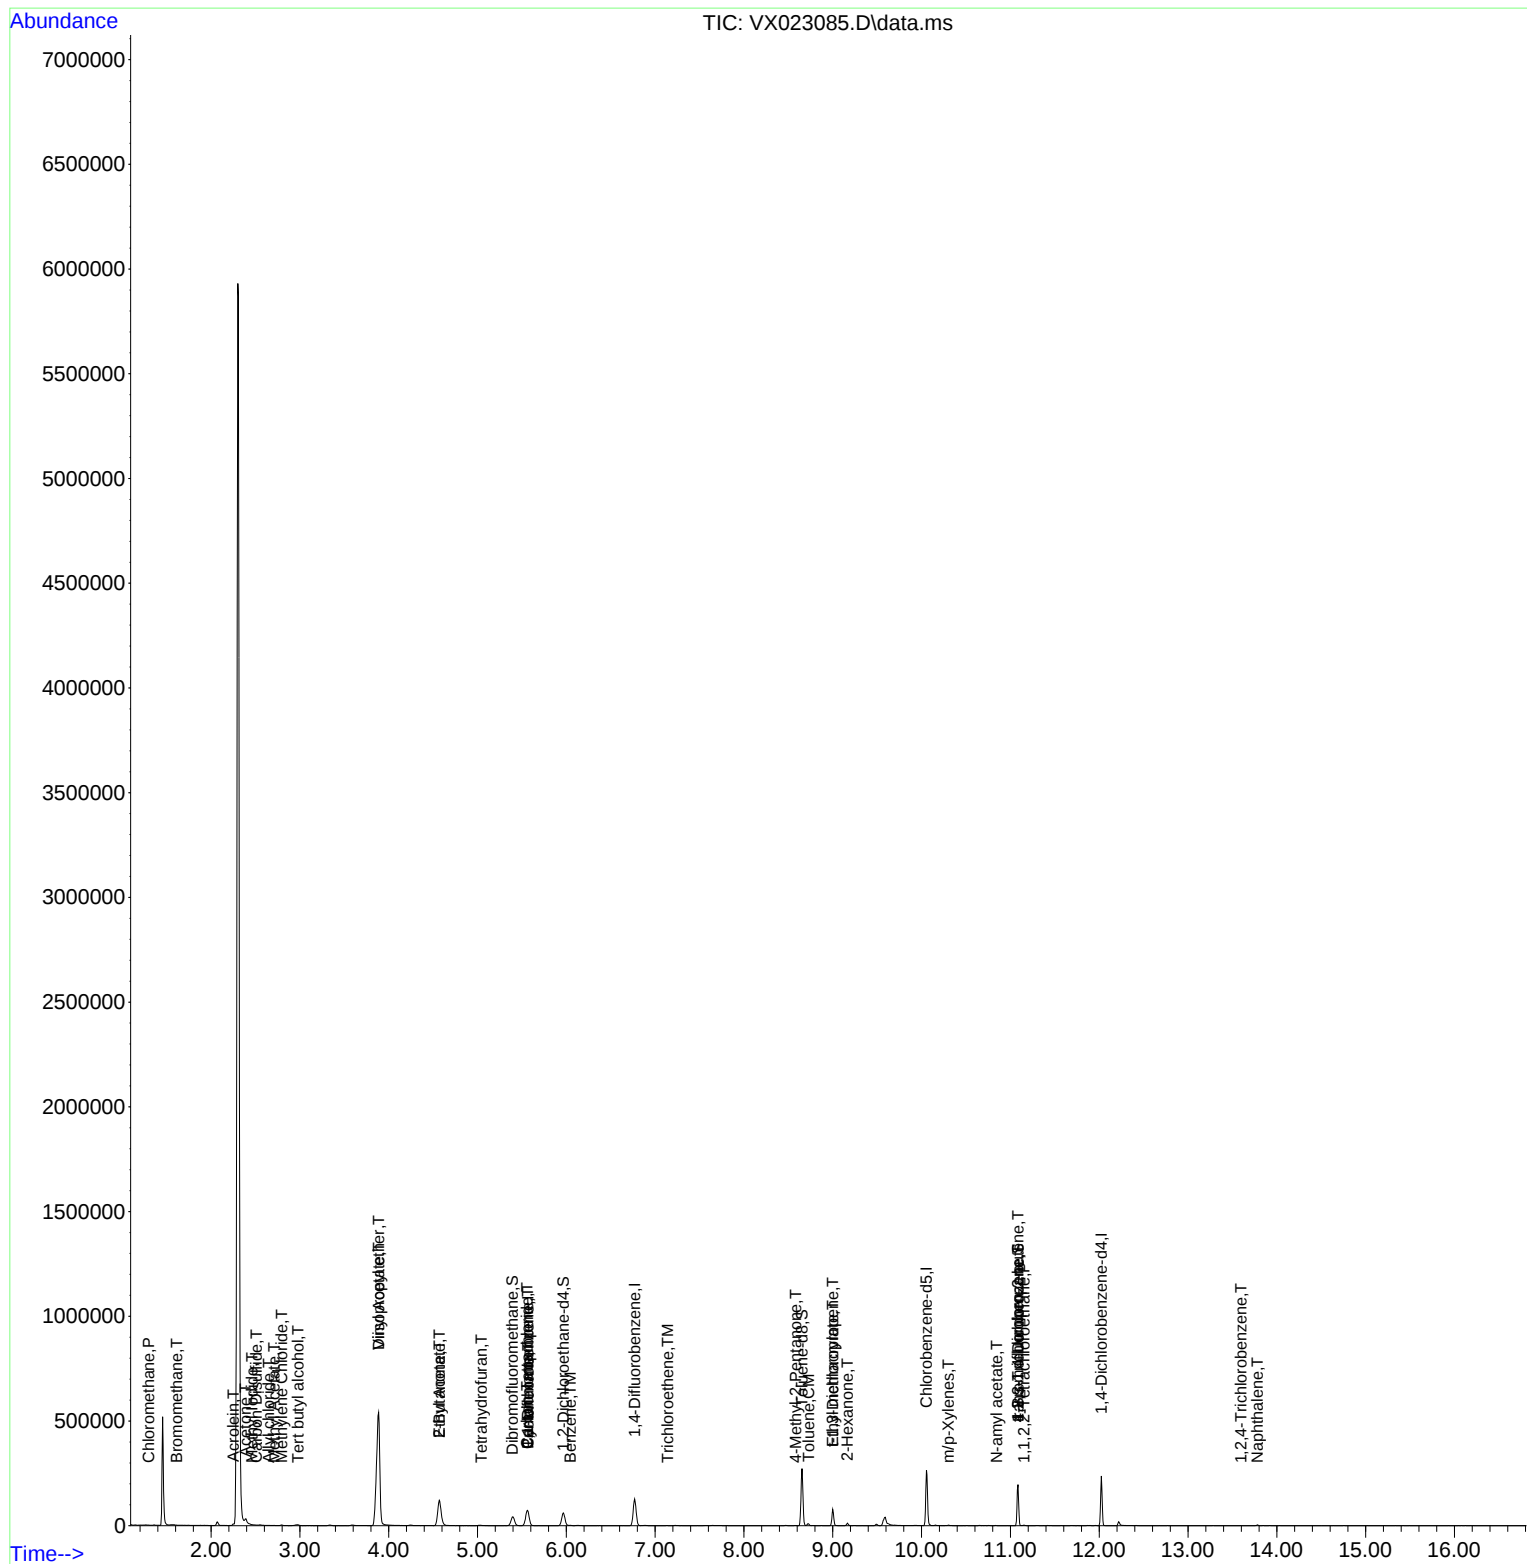




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.012 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion:168 Resp: 55682
Ion Ratio Lower Upper
168 100
99 74.9 45.8 68.6#

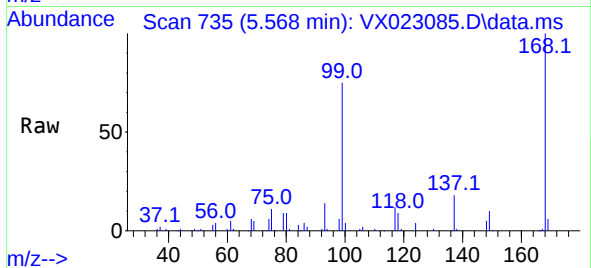

#3
Chloromethane
Concen: 0.23 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 50 Resp: 202
Ion Ratio Lower Upper
50 100
52 37.8 26.4 39.6


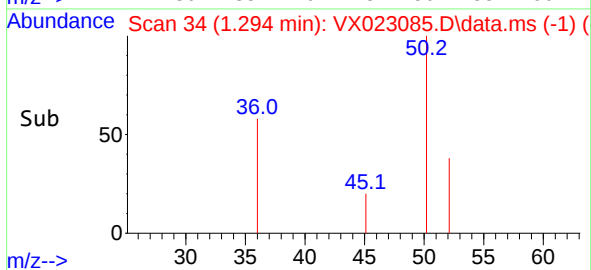




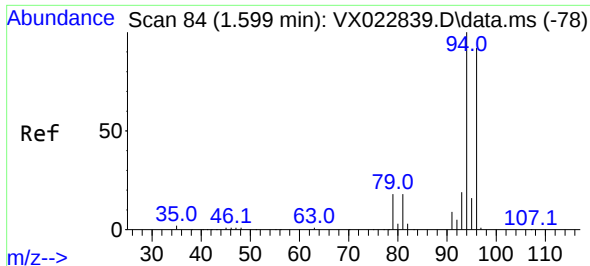

#5
Bromomethane
Concen: 0.43 ug/l
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 94 Resp: 190
Ion Ratio Lower Upper
94 100
96 106.0 76.4 114.6

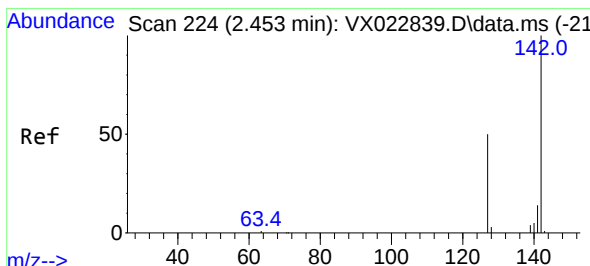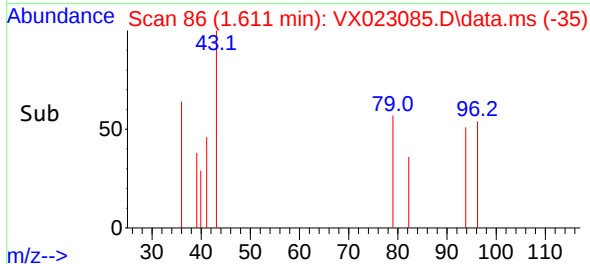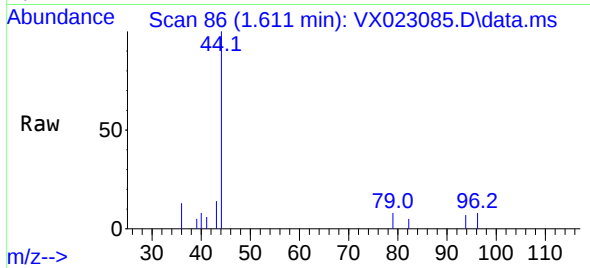

#10
Methyl Iodide
Concen: 4.02 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 142 Resp: 130
Ion Ratio Lower Upper
142 100
127 15.4 33.3 49.9#
141 0.0 11.4 17.0#

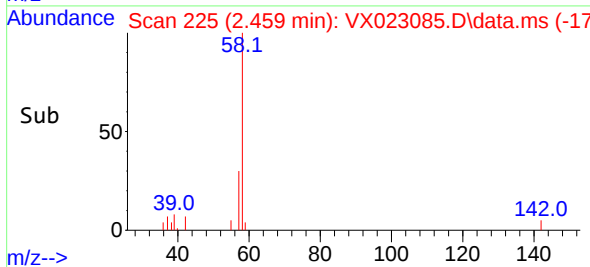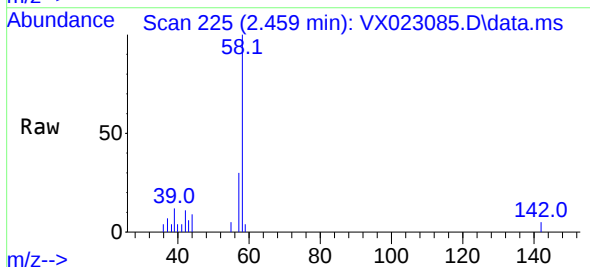







#11

Tert butyl alcohol
Concen: 24.10 ug/l
RT: 2.977 min Scan# 310
Delta R.T. -0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL




Tgt Ion: 59 Resp: 5075
Ion Ratio Lower Upper
59 100
57 16.3 7.8 11.8#




#13

Acrolein
Concen: 37.04 ug/l
RT: 2.251 min Scan# 191
Delta R.T. 0.006 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 56 Resp: 4852
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#









#14
 Allyl chloride
 Concen: 0.53 ug/l
 RT: 2.648 min Scan# 256
 Delta R.T. -0.018 min
 Lab File: VX023085.D
 Acq: 01 Jul 2021 15:16

Instrument :
 MSVOA_X
 ClientSampleId :
 DRIP-COMP-AUD-1121-1122DL

Tgt Ion: 41 Resp: 723




Ion	Ratio	Lower	Upper
41	100		
39	15.5	51.6	77.4#
76	0.0	30.5	45.7#

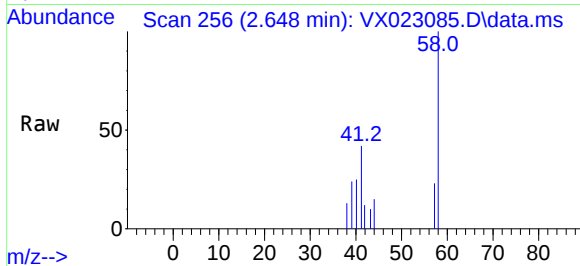


#16
 Acetone
 Concen: 47.06 ug/l
 RT: 2.386 min Scan# 213
 Delta R.T. -0.006 min
 Lab File: VX023085.D
 Acq: 01 Jul 2021 15:16

Tgt Ion: 43 Resp: 21084

Ion	Ratio	Lower	Upper
43	100		
58	73.7	27.8	41.8#


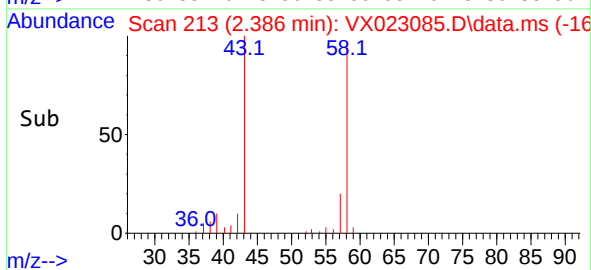

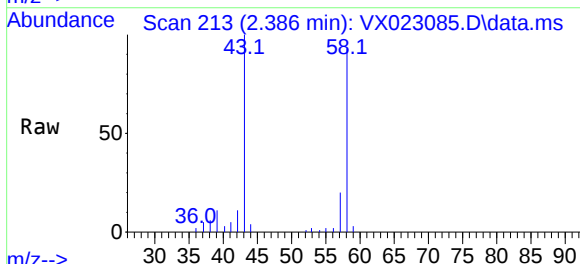




#17
Carbon Disulfide
Concen: 3.75 ug/l
RT: 2.507 min Scan# 233
Delta R.T. -0.007 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 76 Resp: 491
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#



#18
Methyl Acetate
Concen: 0.63 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 43 Resp: 694
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

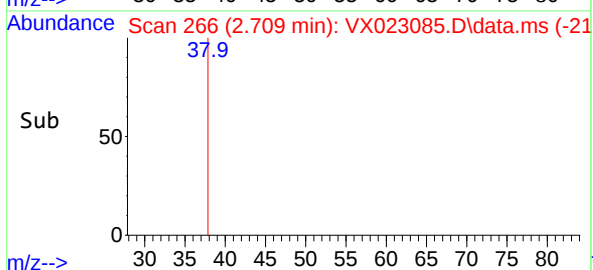



#20

Methylene Chloride

Concen: 1.59 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.000 min

Lab File: VX023085.D

Acq: 01 Jul 2021 15:16

Instrument :

MSVOA_X

ClientSampleId :

DRIP-COMP-AUD-1121-1122DL

Tgt Ion: 84 Resp: 1092





Ion Ratio Lower Upper

84 100

49 152.0 88.6 132.8#

51 45.6 27.0 40.6#

86 69.0 50.3 75.5

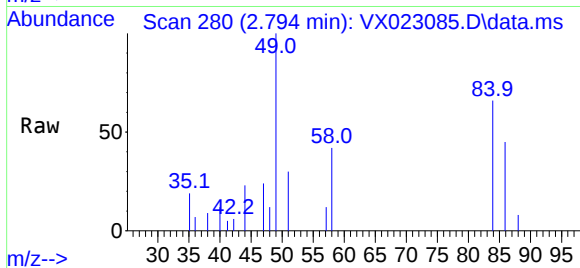

#22

Diisopropyl ether

Concen: 13.13 ug/l

RT: 3.885 min Scan# 459

Delta R.T. 0.116 min

Lab File: VX023085.D

Acq: 01 Jul 2021 15:16

Tgt Ion: 45 Resp: 37491




Ion Ratio Lower Upper


45 100

43 272.0 58.0 87.0#

87 0.0 25.4 38.0#

59 817.0 10.2 15.2#


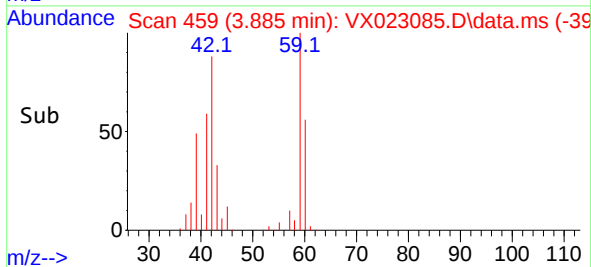
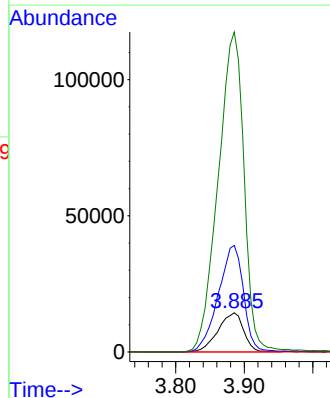
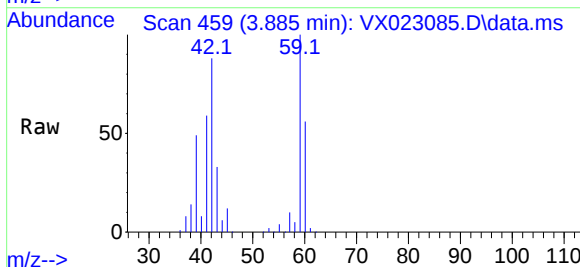




#23
 Vinyl Acetate
 Concen: 41.79 ug/l
 RT: 3.885 min Scan# 459
 Delta R.T. 0.152 min
 Lab File: VX023085.D
 Acq: 01 Jul 2021 15:16




Instrument :
 MSVOA_X
 ClientSampleId :
 DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 43 Resp: 100081
 Ion Ratio Lower Upper
 43 100
 86 0.0 9.9 14.9#



#25
 2-Butanone
 Concen: 297.69 ug/l
 RT: 4.568 min Scan# 571
 Delta R.T. 0.000 min
 Lab File: VX023085.D
 Acq: 01 Jul 2021 15:16

Tgt Ion: 43 Resp: 207382
 Ion Ratio Lower Upper
 43 100
 72 23.6 23.7 35.5#

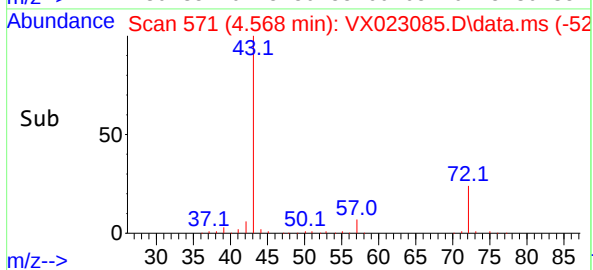




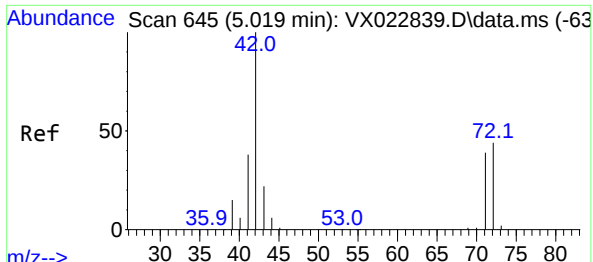


#29
Tetrahydrofuran
Concen: 0.85 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.025 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL

Tgt Ion: 42 Resp: 383




Ion	Ratio	Lower	Upper
42	100		
72	12.5	41.7	62.5#
71	0.0	38.4	57.6#

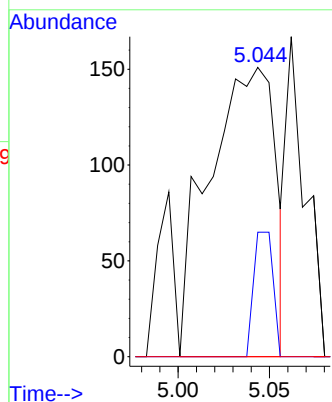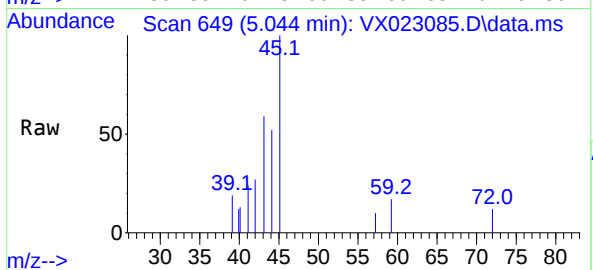


#31
Cyclohexane
Concen: 1.42 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.092 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 56 Resp: 2031

Ion	Ratio	Lower	Upper
56	100		
69	140.4	25.3	37.9#
84	107.0	71.4	107.0


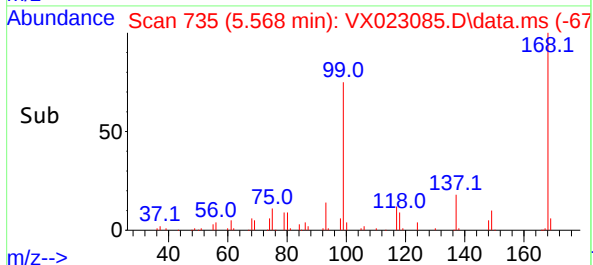

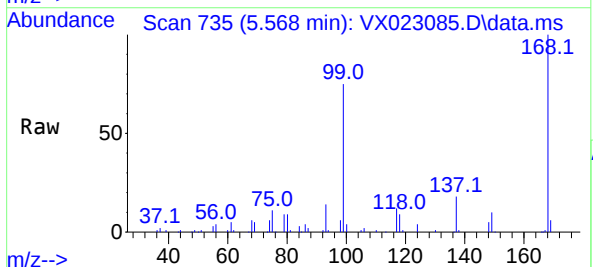




#33
1,2-Dichloroethane-d4
Concen: 58.38 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 65 Resp: 58994
Ion Ratio Lower Upper
65 100
67 49.9 0.0 105.4

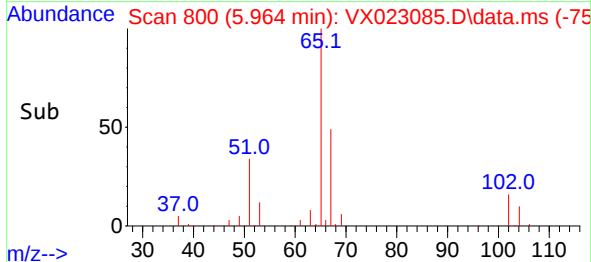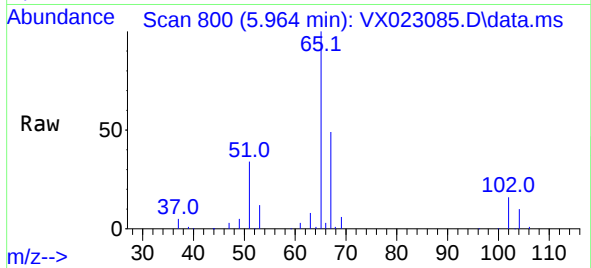

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 114 Resp: 111726
Ion Ratio Lower Upper
114 100
63 25.3 0.0 40.8
88 18.0 0.0 32.8


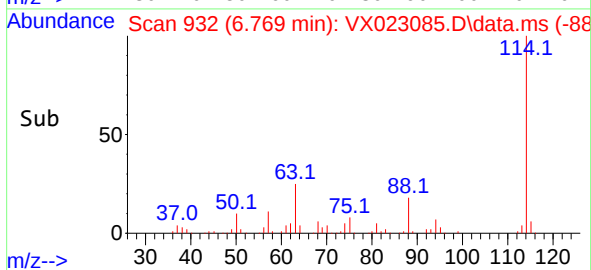




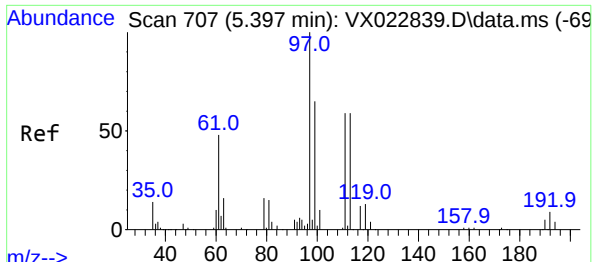

#35
Dibromofluoromethane
Concen: 51.23 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion:113 Resp: 36344
Ion Ratio Lower Upper
113 100
111 100.9 81.9 122.9
192 14.5 16.7 25.1#

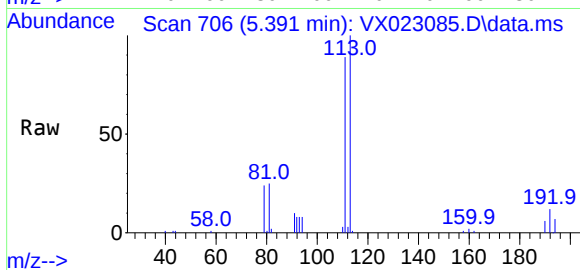

#36
1,1-Dichloropropene
Concen: 5.87 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 75 Resp: 6967
Ion Ratio Lower Upper
75 100
110 7.8 18.1 54.4#
77 0.0 25.3 37.9#

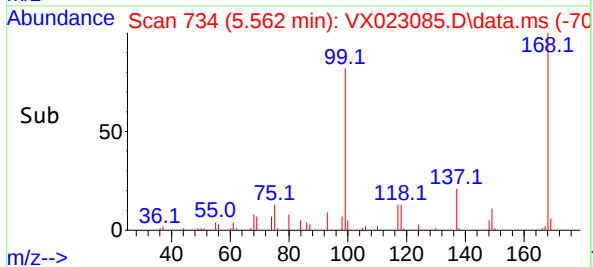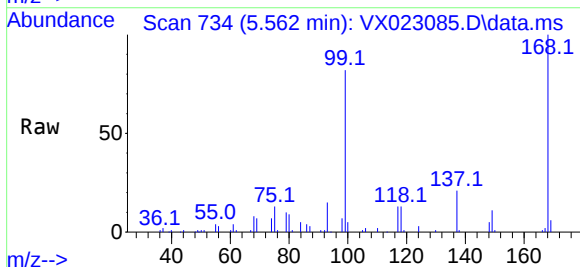



#37

Ethyl Acetate

Concen: 150.86 ug/l

RT: 4.568 min Scan# 571

Delta R.T. -0.159 min

Lab File: VX023085.D


Acq: 01 Jul 2021 15:16

Instrument :

MSVOA_X




ClientSampleId :

DRIP-COMP-AUD-1121-1122DL



Tgt Ion: 43 Resp: 207382

Ion	Ratio	Lower	Upper
43	100		
61	0.1	12.8	19.2#
70	0.0	10.5	15.7#



#38

Carbon Tetrachloride

Concen: 7.32 ug/l

RT: 5.556 min Scan# 733




Delta R.T. -0.134 min


Lab File: VX023085.D

Acq: 01 Jul 2021 15:16

Tgt Ion: 117 Resp: 7287

Ion	Ratio	Lower	Upper
117	100		
119	0.0	76.2	114.2#
121	0.0	24.8	37.2#


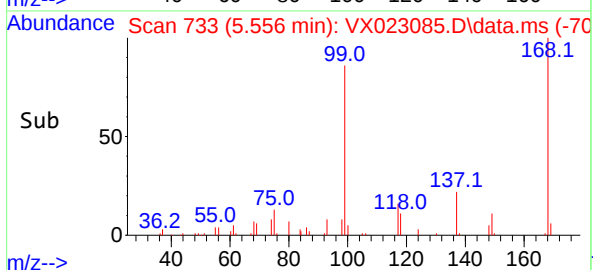






#40
Benzene
Concen: 0.51 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.007 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 78 Resp: 1747
Ion Ratio Lower Upper
78 100
77 22.9 18.9 28.3

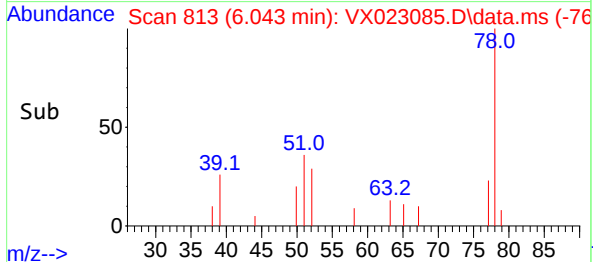

#44
Trichloroethene
Concen: 0.33 ug/l
RT: 7.141 min Scan# 993
Delta R.T. 0.012 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion:130 Resp: 271
Ion Ratio Lower Upper
130 100
95 47.1 0.0 198.0


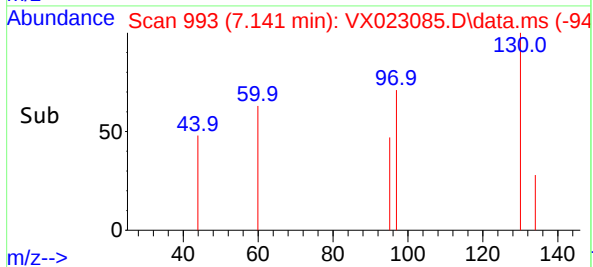

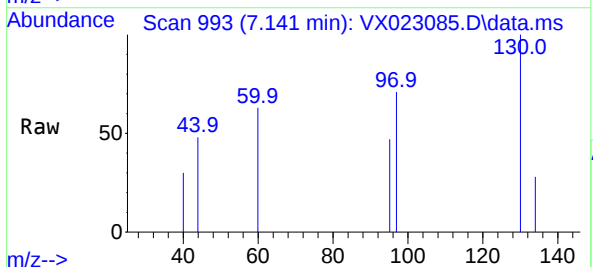




#50
Toluene-d8
Concen: 50.33 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 98 Resp: 139941
Ion Ratio Lower Upper
98 100
100 64.6 51.9 77.9

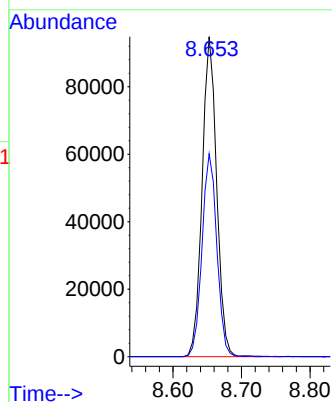

#51
4-Methyl-2-Pentanone
Concen: 0.51 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. -0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 43 Resp: 696
Ion Ratio Lower Upper
43 100
58 26.1 35.4 53.0#

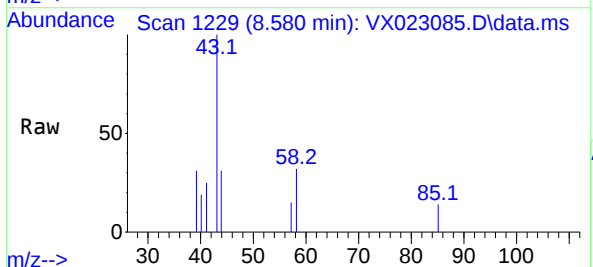



#52

Toluene

Concen: 1.68 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. 0.006 min

Lab File: VX023085.D





Acq: 01 Jul 2021 15:16

Tgt Ion: 92 Resp: 3484

Ion Ratio Lower Upper

92 100

91 168.1 137.1 205.7



#53

t-1,3-Dichloropropene

Concen: 3.68 ug/l

RT: 9.000 min Scan# 1298

Delta R.T. 0.018 min

Lab File: VX023085.D




Acq: 01 Jul 2021 15:16


Tgt Ion: 75 Resp: 20

Ion Ratio Lower Upper

75 100

77 0.0 24.9 37.3#



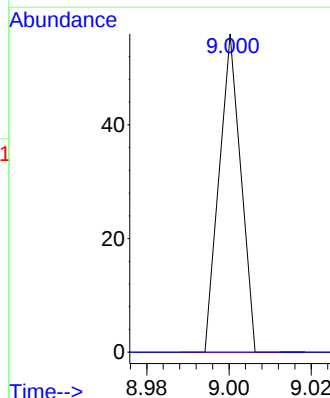





#56
Ethyl methacrylate
Concen: 2.67 ug/l
RT: 9.000 min Scan# 1298
Delta R.T. -0.122 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 69 Resp: 153
Ion Ratio Lower Upper
69 100
41 8175.2 46.8 70.2#
39 3052.3 24.7 37.1#

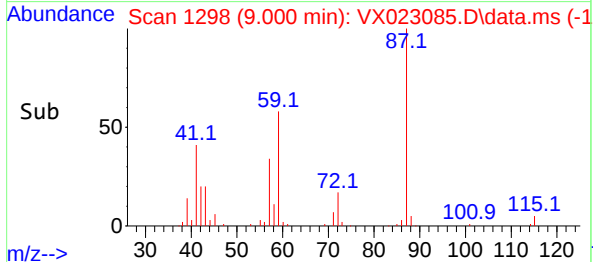

#59
2-Hexanone
Concen: 1.00 ug/l
RT: 9.165 min Scan# 1325
Delta R.T. -0.268 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 43 Resp: 1042
Ion Ratio Lower Upper
43 100
58 43.2 30.9 92.8


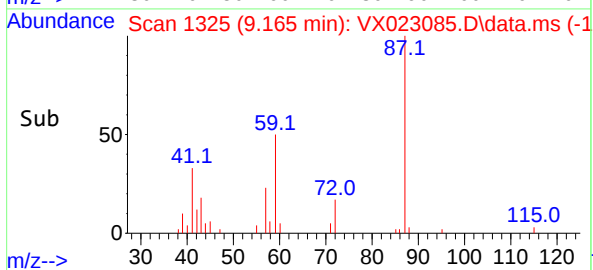






#62
4-Bromofluorobenzene
Concen: 48.40 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 95 Resp: 50231
Ion Ratio Lower Upper
95 100
174 57.2 0.0 154.6
176 56.1 0.0 155.8

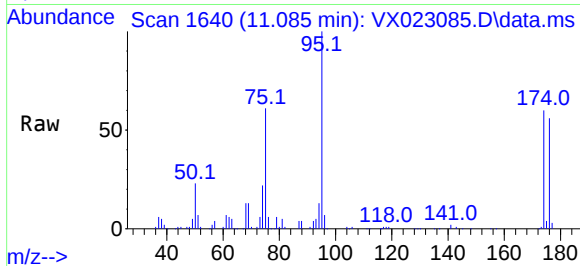

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 117 Resp: 101679
Ion Ratio Lower Upper
117 100
82 65.0 47.4 71.2
119 30.4 26.6 39.8


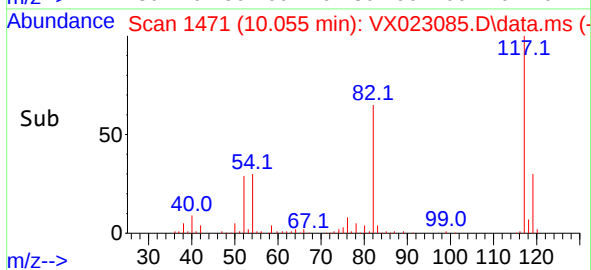

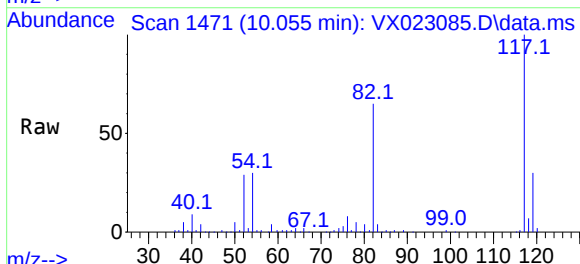




#68
m/p-Xylenes
Concen: 0.49 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion:106 Resp: 713
Ion Ratio Lower Upper
106 100
91 181.9 162.8 244.2

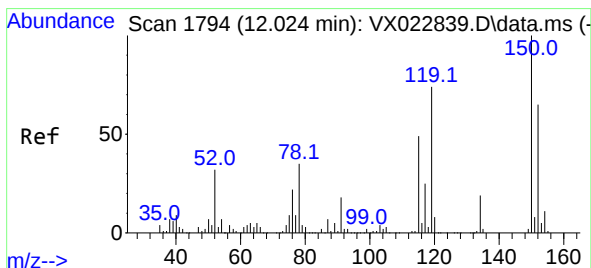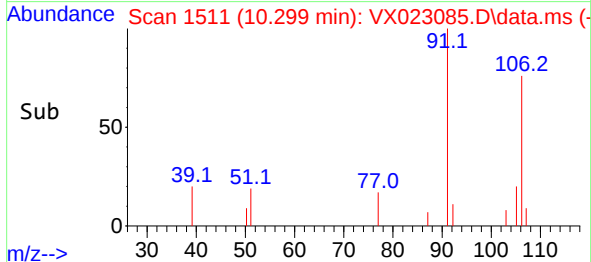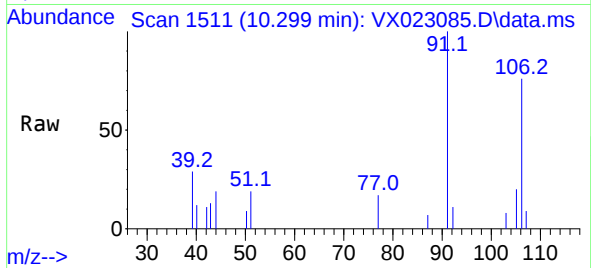

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion:152 Resp: 37561
Ion Ratio Lower Upper
152 100
115 71.7 41.1 123.3
150 160.3 0.0 349.0

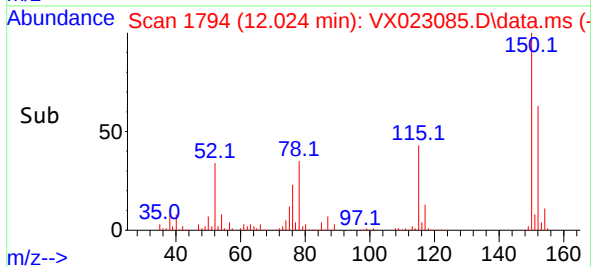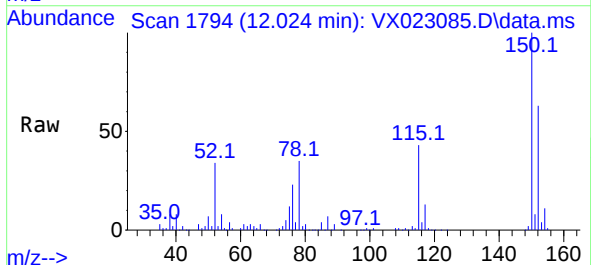







#74
N-amy1 acetate
Concen: 2.31 ug/l
RT: 10.847 min Scan# 1601
Delta R.T. 0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL

Tgt Ion: 43 Resp: 472




Ion	Ratio	Lower	Upper
43	100		
70	0.0	39.0	58.6#
55	0.0	21.5	32.3#
61	0.0	22.1	33.1#

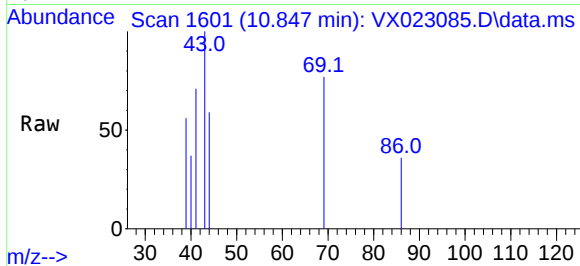


#75
1,1,2,2-Tetrachloroethane
Concen: 0.62 ug/l
RT: 11.152 min Scan# 1651
Delta R.T. -0.061 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 83 Resp: 682

Ion	Ratio	Lower	Upper
83	100		
131	0.0	5.1	15.2#
85	0.0	31.8	95.4#


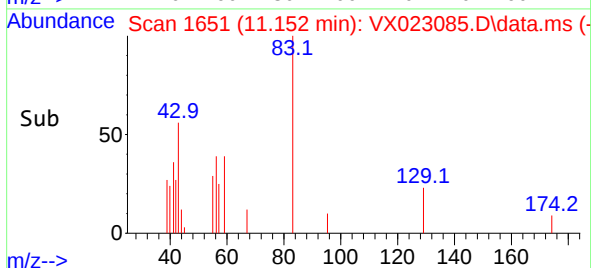
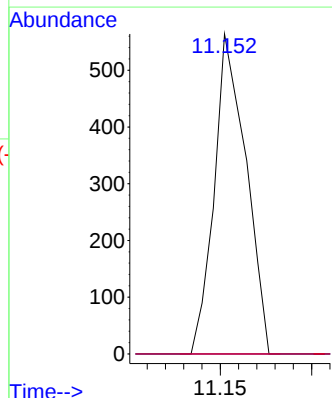
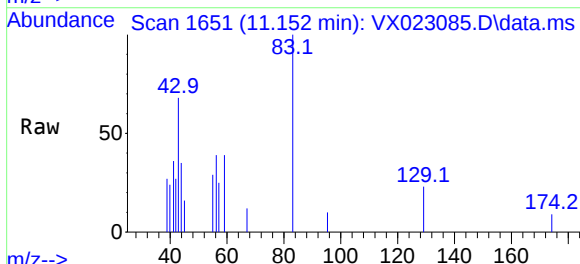




#76
1,2,3-Trichloropropane
Concen: 31.24 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16




Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL


Tgt Ion: 75 Resp: 30991
Ion Ratio Lower Upper
75 100
77 0.8 19.1 57.5#

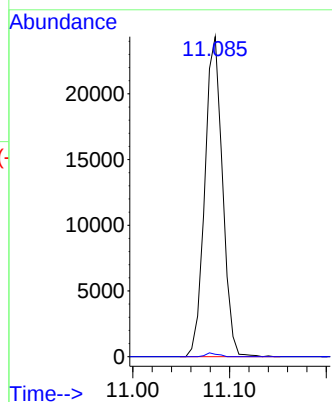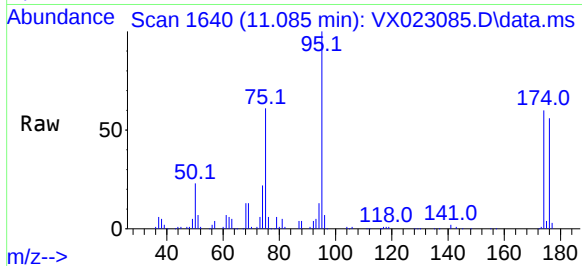

#81
trans-1,4-Dichloro-2-butene
Concen: 79.90 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion: 75 Resp: 30991
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


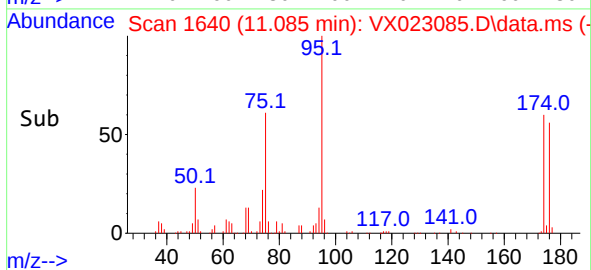

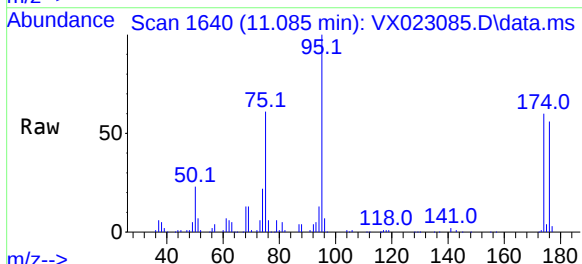




#93
1,2,4-Trichlorobenzene
Concen: 0.24 ug/l
RT: 13.597 min Scan# 2052
Delta R.T. 0.006 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Instrument :
MSVOA_X
ClientSampleId :
DRIP-COMP-AUD-1121-1122DL

Tgt Ion:180 Resp: 165
Ion Ratio Lower Upper
180 100
182 56.4 47.7 143.1
145 0.0 15.0 45.0#

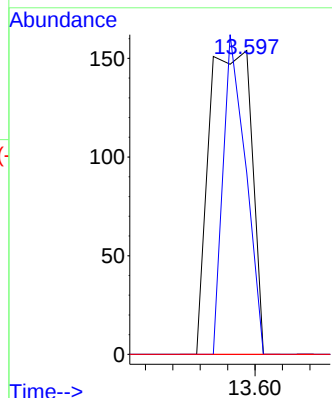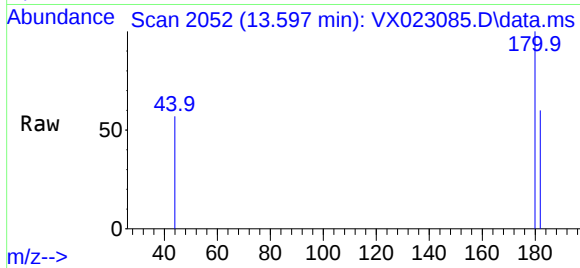

#95
Naphthalene
Concen: 2.49 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX023085.D
Acq: 01 Jul 2021 15:16

Tgt Ion:128 Resp: 1799
Ion Ratio Lower Upper
128 100
127 11.0 10.3 15.5
129 6.8 8.8 13.2#

