

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
 Data File : VX023094.D
 Acq On : 01 Jul 2021 18:48
 Operator : JC/MD
 Sample : M2908-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-CROPSEY-SOLIDS

Quant Time: Jul 02 04:32:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 23 19:12:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	54680	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	113914	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	100326	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	34052	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	64203	64.699	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 129.400%			#
35) Dibromofluoromethane	5.397	113	37895	52.386	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 104.780%			
50) Toluene-d8	8.653	98	143356	50.565	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 101.140%			
62) 4-Bromofluorobenzene	11.085	95	51434	48.611	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 97.220%			
Target Compounds						Qvalue
10) Methyl Iodide	2.477	142	19	3.900	ug/l	# 42
11) Tert butyl alcohol	2.953	59	5419	26.202	ug/l	# 76
13) Acrolein	2.246	56	234	1.819	ug/l	# 77
16) Acetone	2.386	43	22154	50.358	ug/l	# 83
17) Carbon Disulfide	2.514	76	377	3.697	ug/l	# 75
18) Methyl Acetate	2.715	43	1464	1.352	ug/l	# 69
20) Methylene Chloride	2.794	84	7316	8.695	ug/l	94
25) 2-Butanone	4.580	43	4262	6.230	ug/l	92
26) 2,2-Dichloropropane	4.587	77	271	0.238	ug/l	# 52
29) Tetrahydrofuran	5.038	42	891	2.025	ug/l	# 48
31) Cyclohexane	5.556	56	2078	1.483	ug/l	# 47
36) 1,1-Dichloropropene	5.562	75	7019	5.801	ug/l	# 45
38) Carbon Tetrachloride	5.562	117	7478	7.369	ug/l	# 17
41) Methacrylonitrile	5.044	41	683	0.885	ug/l	# 44
43) Isopropyl Acetate	6.355	43	13258	5.884	ug/l	# 92
48) Methyl methacrylate	7.604	41	4365	4.186	ug/l	# 10
49) 1,4-Dioxane	7.806	88	33	1.470	ug/l	# 1
51) 4-Methyl-2-Pentanone	8.555	43	51064	36.412	ug/l	# 44
52) Toluene	8.720	92	6489	3.077	ug/l	98
53) t-1,3-Dichloropropene	8.726	75	45	3.696	ug/l	# 1
54) cis-1,3-Dichloropropene	8.555	75	19241	14.508	ug/l	# 71
56) Ethyl methacrylate	9.000	69	107	2.644	ug/l	# 29
57) 1,3-Dichloropropane	9.488	76	11230	7.301	ug/l	# 42
59) 2-Hexanone	9.378	43	5398	5.074	ug/l	# 19
67) Ethyl Benzene	10.201	91	787	0.202	ug/l	# 86
68) m/p-Xylenes	10.311	106	876	0.606	ug/l	90
69) o-Xylene	10.646	106	326	0.232	ug/l	34
74) N-amyl acetate	10.823	43	243	2.198	ug/l	# 38
76) 1,2,3-Trichloropropane	11.085	75	32060	35.644	ug/l	# 38
80) 1,3,5-Trimethylbenzene	11.451	105	661	0.279	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.085	75	32060	90.250	ug/l	# 12
84) 1,2,4-Trimethylbenzene	11.756	105	1176	0.494	ug/l	96
85) sec-Butylbenzene	11.756	105	1176	0.390	ug/l	# 57
92) 1,2-Dibromo-3-Chloropr...	13.146	75	25	4.071	ug/l	# 1
95) Naphthalene	13.780	128	2097	2.649	ug/l	# 93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
Data File : VX023094.D
Acq On : 01 Jul 2021 18:48
Operator : JC/MD
Sample : M2908-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Quant Time: Jul 02 04:32:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 19:12:26 2021
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Jul 02 04:32:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 19:12:26 2021
Response via : Initial Calibration








#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.006 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS







Tgt Ion:168 Resp: 54680
Ion Ratio Lower Upper
168 100
99 79.6 45.8 68.6#

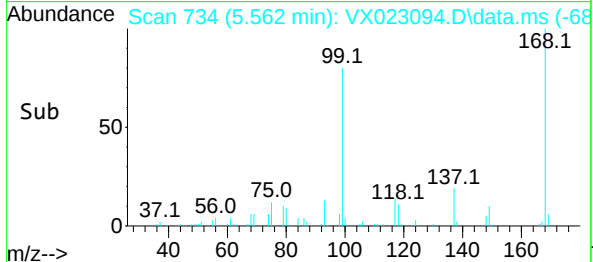

#10
Methyl Iodide
Concen: 3.900 ug/l
RT: 2.477 min Scan# 228
Delta R.T. 0.024 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion:142 Resp: 19
Ion Ratio Lower Upper
142 100
127 0.0 33.3 49.9#
141 0.0 11.4 17.0#

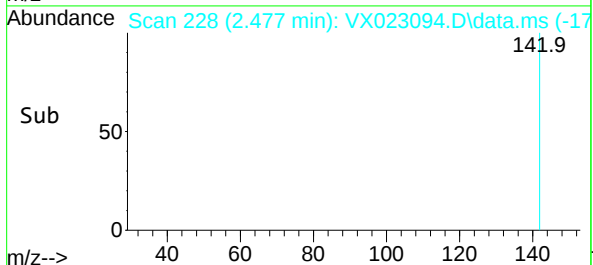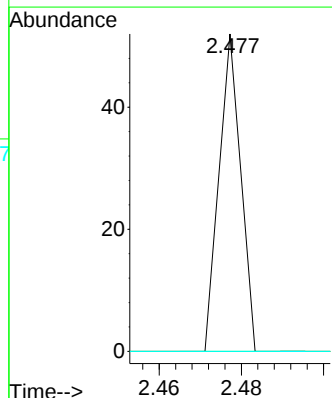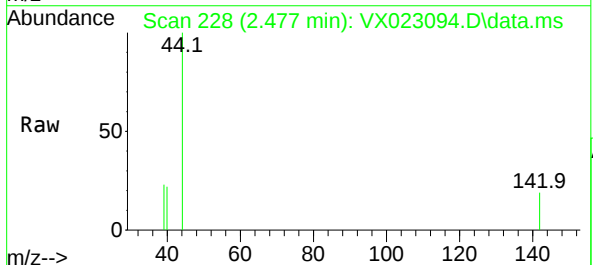







#11

Tert butyl alcohol
Concen: 26.202 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.024 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS




Tgt Ion: 59 Resp: 5419
Ion Ratio Lower Upper
59 100
57 1.0 7.8 11.8#

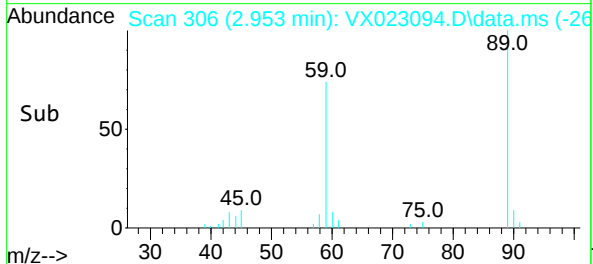


#13

Acrolein
Concen: 1.819 ug/l
RT: 2.246 min Scan# 190
Delta R.T. 0.001 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 56 Resp: 234
Ion Ratio Lower Upper
56 100
55 89.3 56.4 84.6#


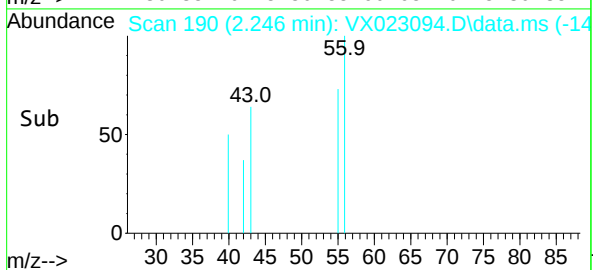






#16
Acetone
Concen: 50.358 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion: 43 Resp: 22154
Ion Ratio Lower Upper
43 100
58 25.1 27.8 41.8#

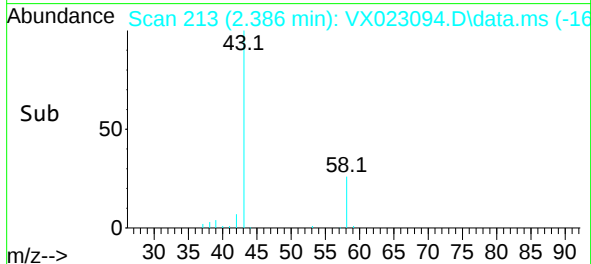

#17
Carbon Disulfide
Concen: 3.697 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 76 Resp: 377
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


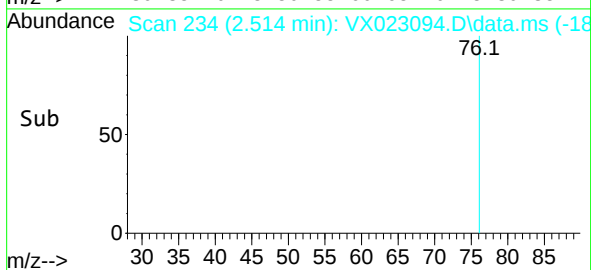

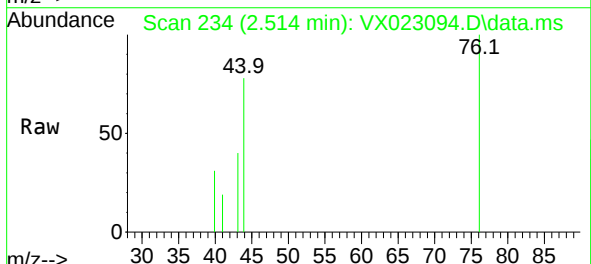




#18
Methyl Acetate
Concen: 1.352 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion: 43 Resp: 1464
Ion Ratio Lower Upper
43 100
74 11.4 21.9 32.9#

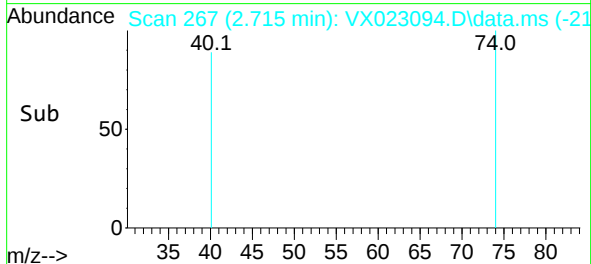

#20
Methylene Chloride
Concen: 8.695 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 84 Resp: 7316
Ion Ratio Lower Upper
84 100
49 118.4 88.6 132.8
51 39.4 27.0 40.6
86 62.7 50.3 75.5

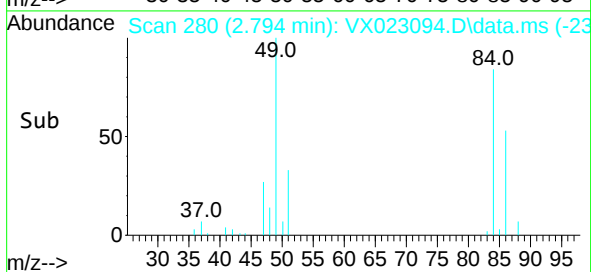



#25

2-Butanone

Concen: 6.230 ug/l

RT: 4.580 min Scan# 573

Delta R.T. 0.013 min

Lab File: VX023094.D





Acq: 01 Jul 2021 18:48

Tgt Ion: 43 Resp: 4262

Ion Ratio Lower Upper

43 100

72 25.4 23.7 35.5



#26

2,2-Dichloropropane

Concen: 0.238 ug/l

RT: 4.587 min Scan# 574

Delta R.T. 0.104 min

Lab File: VX023094.D




Acq: 01 Jul 2021 18:48


Tgt Ion: 77 Resp: 271

Ion Ratio Lower Upper

77 100

97 0.0 11.7 35.1#

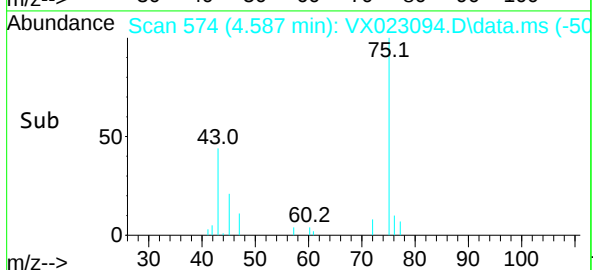



#29

Tetrahydrofuran

Concen: 2.025 ug/l

RT: 5.038 min Scan# 648





Delta R.T. 0.019 min

Lab File: VX023094.D

Acq: 01 Jul 2021 18:48

Tgt Ion:	42	Resp:	891
Ion	Ratio	Lower	Upper
42	100		
72	28.3	41.7	62.5#
71	0.0	38.4	57.6#

Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS



#31

Cyclohexane

Concen: 1.483 ug/l




RT: 5.556 min Scan# 733


Delta R.T. 0.080 min

Lab File: VX023094.D

Acq: 01 Jul 2021 18:48

Tgt Ion:	56	Resp:	2078
Ion	Ratio	Lower	Upper
56	100		
69	143.7	25.3	37.9#
84	89.6	71.4	107.0

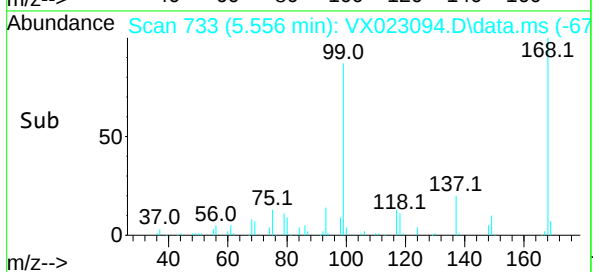







#33

1,2-Dichloroethane-d4
Concen: 64.699 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS




Tgt Ion: 65 Resp: 64203
Ion Ratio Lower Upper
65 100
67 48.2 0.0 105.4




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 114 Resp: 113914
Ion Ratio Lower Upper
114 100
63 26.4 0.0 40.8
88 18.2 0.0 32.8

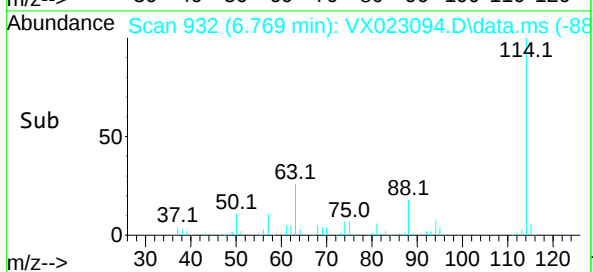



#35

Dibromofluoromethane

Concen: 52.386 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.000 min

Lab File: VX023094.D

Acq: 01 Jul 2021 18:48





Tgt Ion:113 Resp: 37895

Ion Ratio Lower Upper

113 100

111 103.0 81.9 122.9

192 13.0 16.7 25.1#

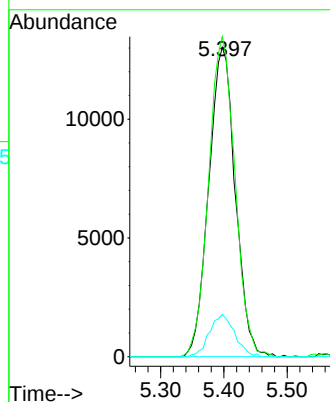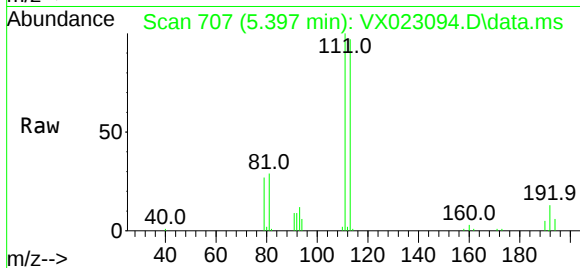

#36

1,1-Dichloropropene

Concen: 5.801 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.140 min

Lab File: VX023094.D

Acq: 01 Jul 2021 18:48




Tgt Ion: 75 Resp: 7019


Ion Ratio Lower Upper

75 100

110 4.7 18.1 54.4#


77 0.0 25.3 37.9#

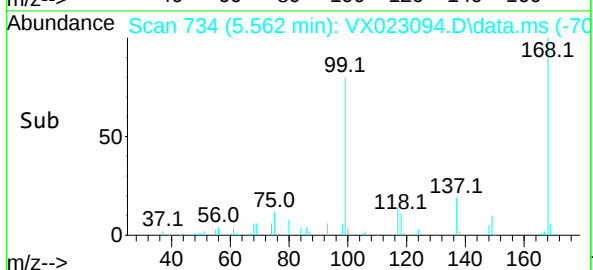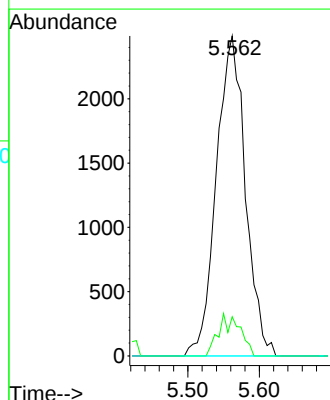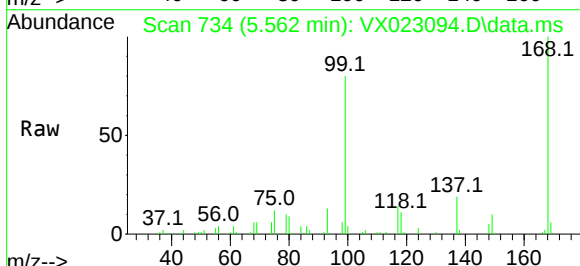






#38
Carbon Tetrachloride
Concen: 7.369 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48


Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS





Tgt Ion: 117 Resp: 7478
Ion Ratio Lower Upper
117 100
119 6.4 76.2 114.2#
121 0.0 24.8 37.2#




#41
Methacrylonitrile
Concen: 0.885 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.116 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

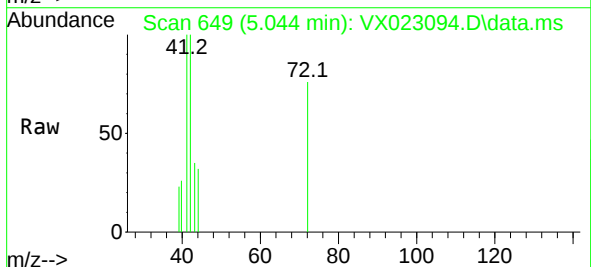

Tgt Ion: 41 Resp: 683
Ion Ratio Lower Upper
41 100
39 53.9 42.5 63.7
67 0.0 65.0 97.6#
52 0.0 25.3 37.9#



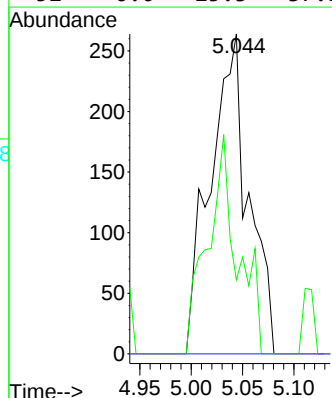





#43
Isopropyl Acetate
Concen: 5.884 ug/l
RT: 6.355 min Scan# 864
Delta R.T. 0.001 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion: 43 Resp: 13258
Ion Ratio Lower Upper
43 100
61 19.1 18.2 27.4
87 12.0 12.5 18.7#

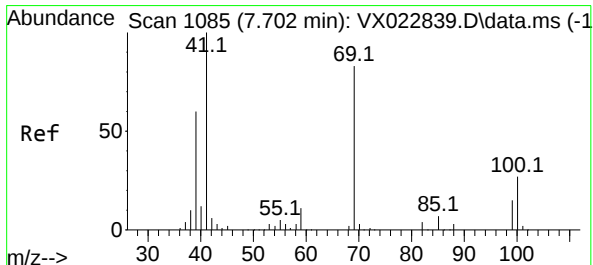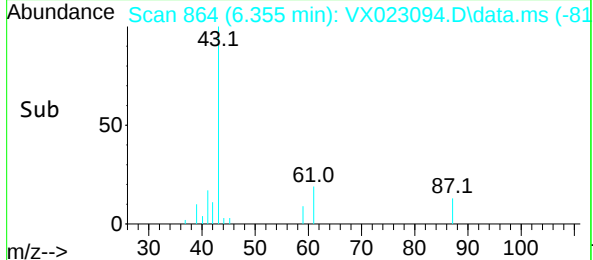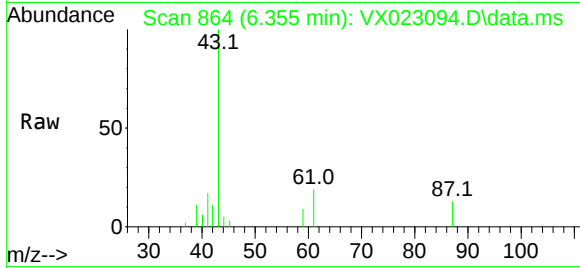

#48
Methyl methacrylate
Concen: 4.186 ug/l
RT: 7.604 min Scan# 1069
Delta R.T. -0.098 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 41 Resp: 4365
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 0.0 44.6 67.0#


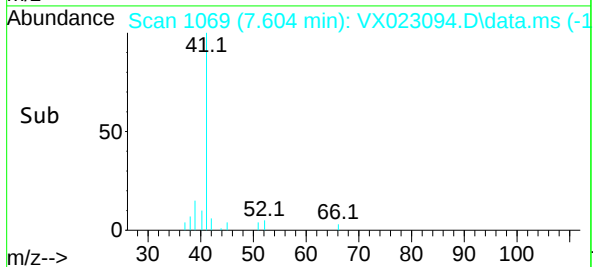

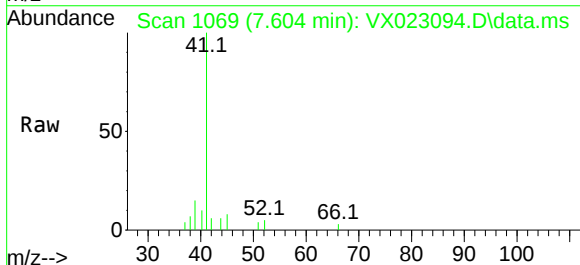




#49
1,4-Dioxane
Concen: 1.470 ug/l
RT: 7.806 min Scan# 1102
Delta R.T. 0.141 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion: 88 Resp: 33
Ion Ratio Lower Upper
88 100
43 2160548.5 23.2 34.8#
58 8593.9 55.0 82.4#

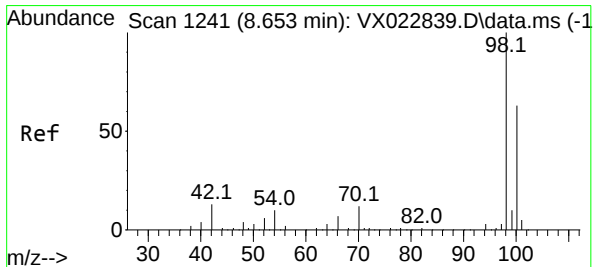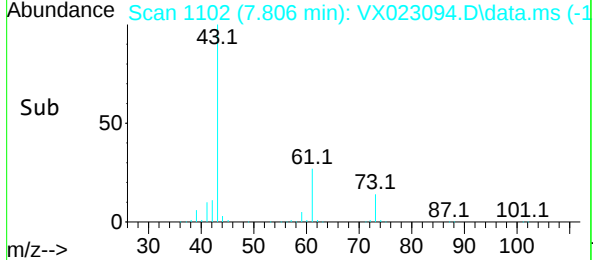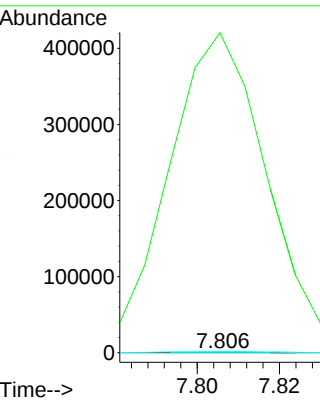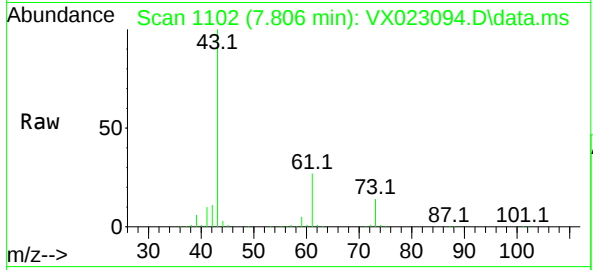

#50
Toluene-d8
Concen: 50.565 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 98 Resp: 143356
Ion Ratio Lower Upper
98 100
100 65.6 51.9 77.9


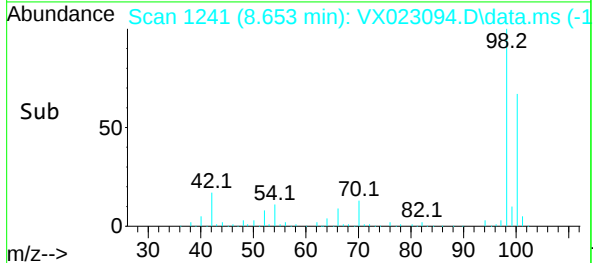
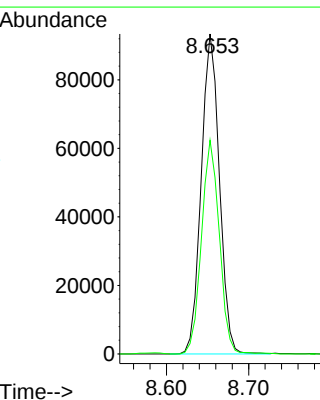
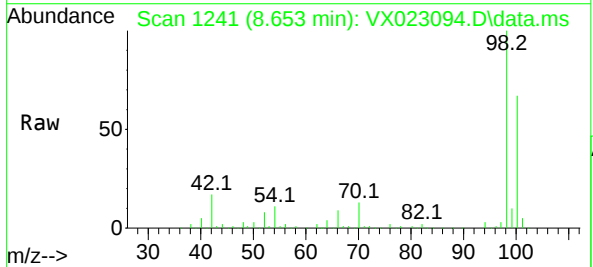




#51
4-Methyl-2-Pentanone
Concen: 36.412 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.025 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion: 43 Resp: 51064
Ion Ratio Lower Upper
43 100
58 7.9 35.4 53.0#

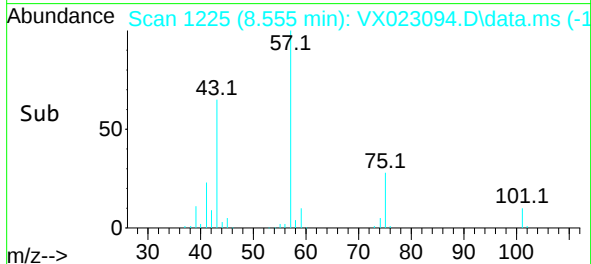

#52
Toluene
Concen: 3.077 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 92 Resp: 6489
Ion Ratio Lower Upper
92 100
91 168.9 137.1 205.7




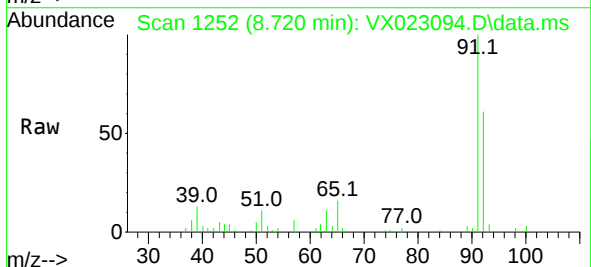




#53
t-1,3-Dichloropropene
Concen: 3.696 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. -0.256 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion: 75 Resp: 45
Ion Ratio Lower Upper
75 100
77 169.6 24.9 37.3#

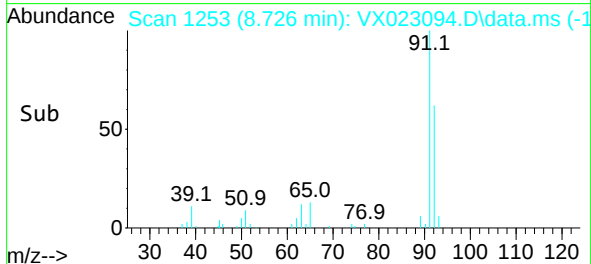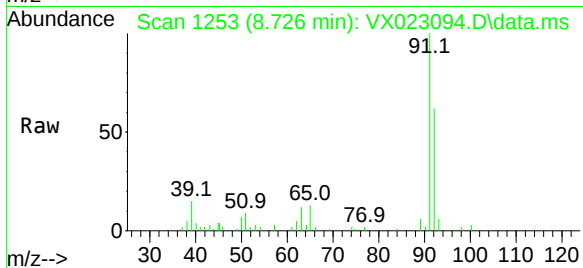

#54
cis-1,3-Dichloropropene
Concen: 14.508 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.183 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 75 Resp: 19241
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#
39 39.0 35.1 52.7

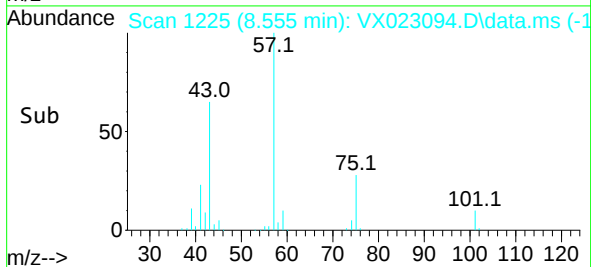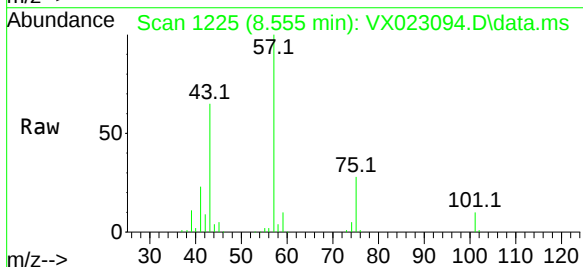



#56

Ethyl methacrylate

Concen: 2.644 ug/l

RT: 9.000 min Scan# 1298

Delta R.T. -0.122 min

Lab File: VX023094.D

Acq: 01 Jul 2021 18:48





Tgt Ion: 69 Resp: 107

Ion Ratio Lower Upper

69 100

41 0.0 46.8 70.2#

39 0.0 24.7 37.1#

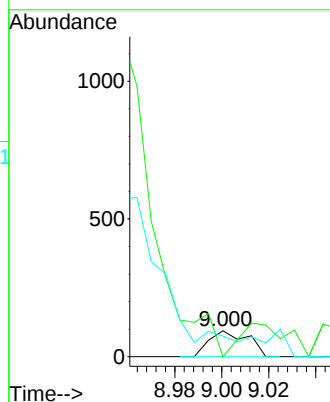

#57

1,3-Dichloropropane

Concen: 7.301 ug/l

RT: 9.488 min Scan# 1378

Delta R.T. 0.177 min

Lab File: VX023094.D




Acq: 01 Jul 2021 18:48


Tgt Ion: 76 Resp: 11230

Ion Ratio Lower Upper

76 100

78 0.0 26.2 39.2#


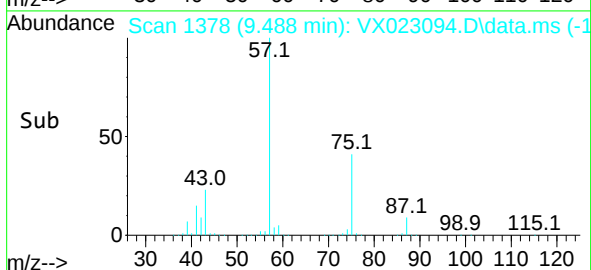
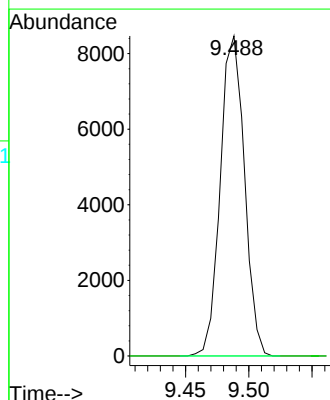





#59
2-Hexanone
Concen: 5.074 ug/l
RT: 9.378 min Scan# 1360
Delta R.T. -0.055 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion: 43 Resp: 5398
Ion Ratio Lower Upper
43 100
58 0.0 30.9 92.8#

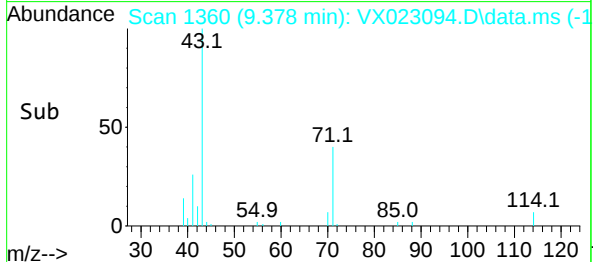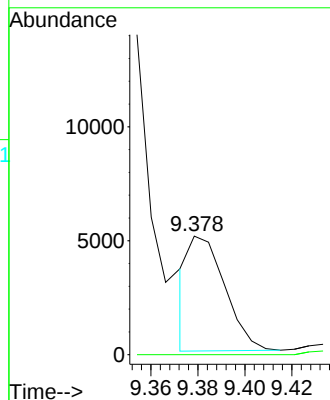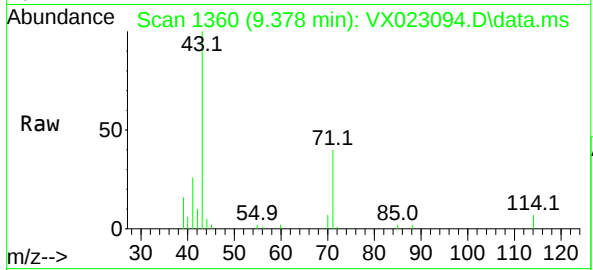

#62
4-Bromofluorobenzene
Concen: 48.611 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 95 Resp: 51434
Ion Ratio Lower Upper
95 100
174 55.9 0.0 154.6
176 52.5 0.0 155.8



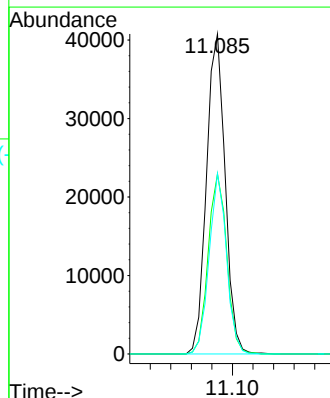
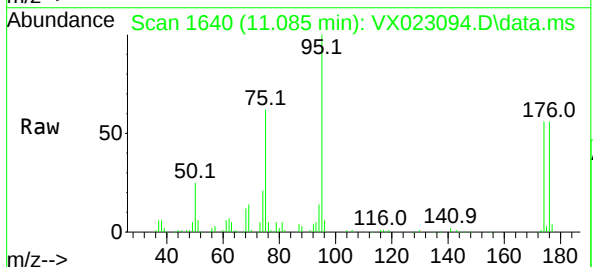




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion:117 Resp: 100326
Ion Ratio Lower Upper
117 100
82 67.8 47.4 71.2
119 31.9 26.6 39.8

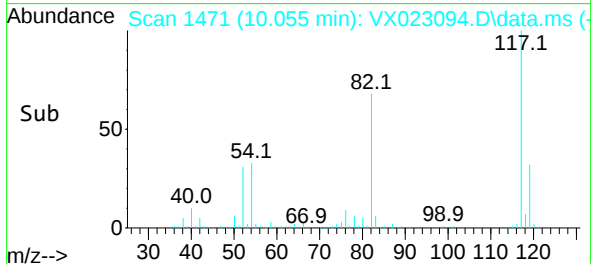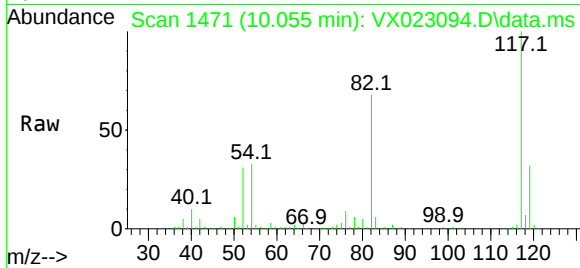

#67
Ethyl Benzene
Concen: 0.202 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 91 Resp: 787
Ion Ratio Lower Upper
91 100
106 23.2 24.6 37.0#


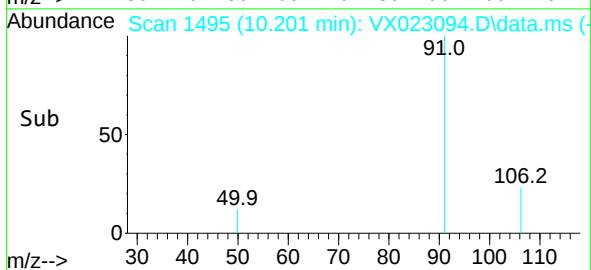

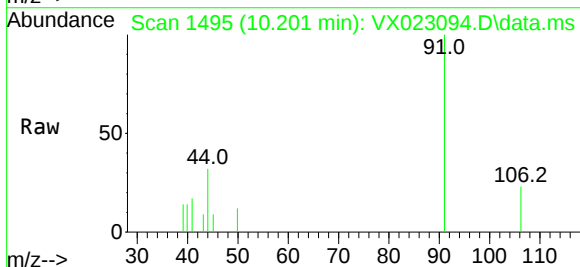




#68
m/p-Xylenes
Concen: 0.606 ug/l
RT: 10.311 min Scan# 1513
Delta R.T. 0.006 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion:106 Resp: 876
Ion Ratio Lower Upper
106 100
91 188.2 162.8 244.2

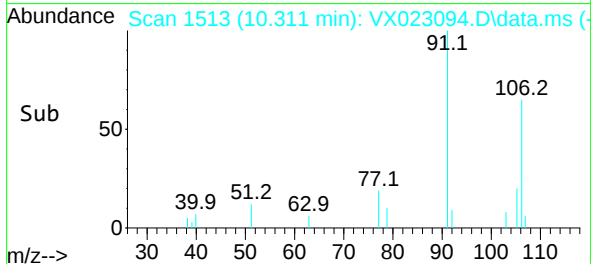

#69
o-Xylene
Concen: 0.232 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion:106 Resp: 326
Ion Ratio Lower Upper
106 100
91 321.2 108.1 324.2


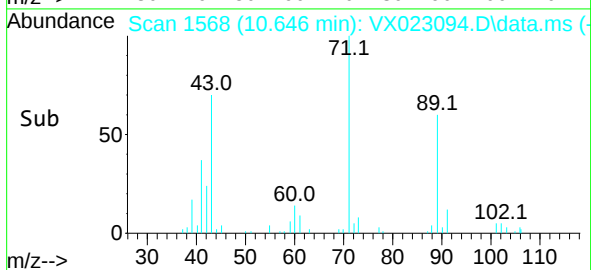

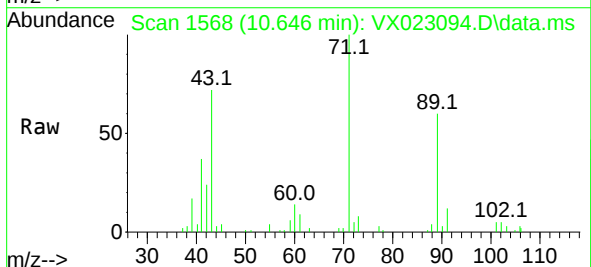




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion:152 Resp: 34052
Ion Ratio Lower Upper
152 100
115 74.6 41.1 123.3
150 160.7 0.0 349.0

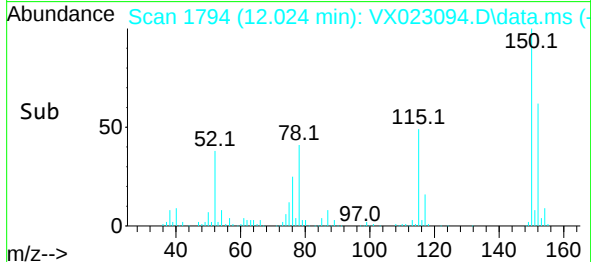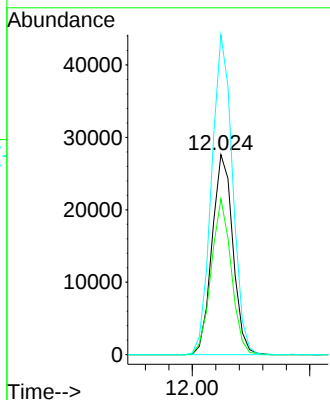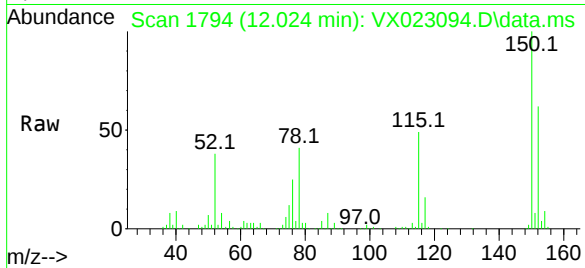

#74
N-ethyl acetate
Concen: 2.198 ug/l
RT: 10.823 min Scan# 1597
Delta R.T. -0.024 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 43 Resp: 243
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.6#
55 0.0 21.5 32.3#
61 0.0 22.1 33.1#


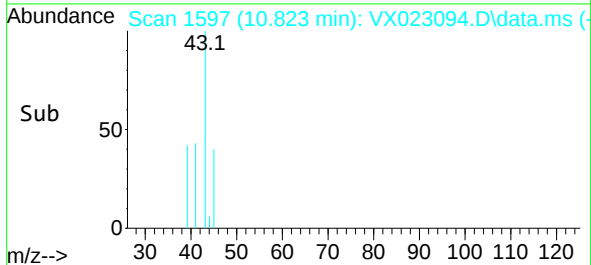
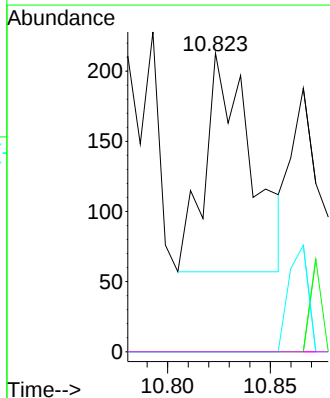
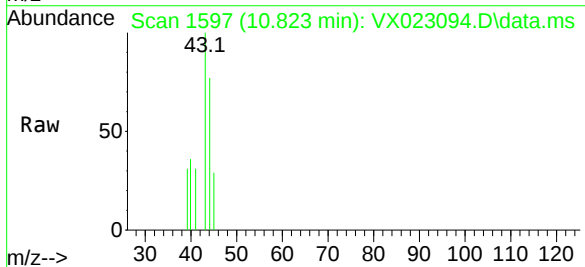




#76
1,2,3-Trichloropropane
Concen: 35.644 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48




Instrument :
MSVOA_X
ClientSampleId :
WC-CROPSEY-SOLIDS


Tgt Ion: 75 Resp: 32060
Ion Ratio Lower Upper
75 100
77 0.8 19.1 57.5#

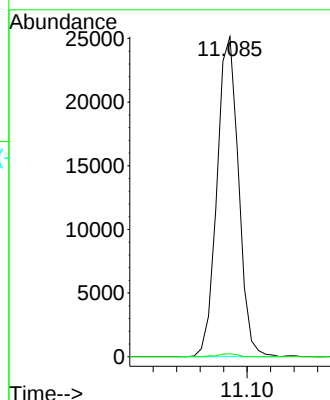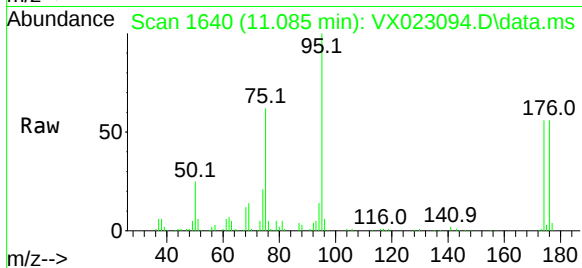

#80
1,3,5-Trimethylbenzene
Concen: 0.279 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX023094.D
Acq: 01 Jul 2021 18:48

Tgt Ion: 105 Resp: 661
Ion Ratio Lower Upper
105 100
120 44.2 23.8 71.5


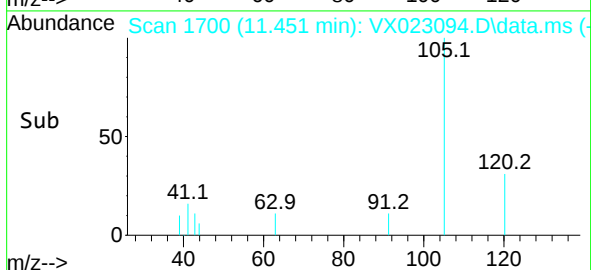
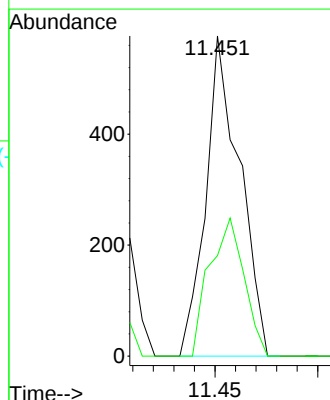
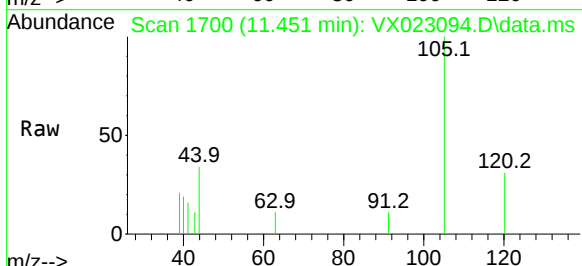




#81
 trans-1,4-Dichloro-2-butene
 Concen: 90.250 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. 0.061 min
 Lab File: VX023094.D
 Acq: 01 Jul 2021 18:48




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-CROPSEY-SOLIDS


Tgt Ion: 75 Resp: 32060
 Ion Ratio Lower Upper
 75 100
 53 0.0 74.5 111.7#
 89 0.0 37.9 56.9#

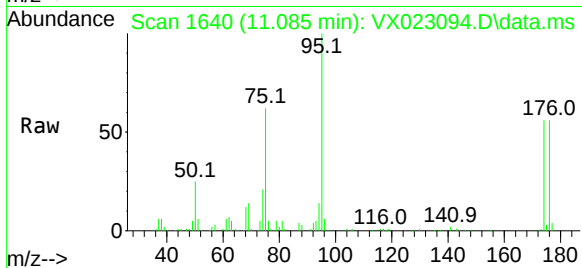

#84
 1,2,4-Trimethylbenzene
 Concen: 0.494 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.000 min
 Lab File: VX023094.D
 Acq: 01 Jul 2021 18:48

Tgt Ion: 105 Resp: 1176
 Ion Ratio Lower Upper
 105 100
 120 42.5 22.4 67.3


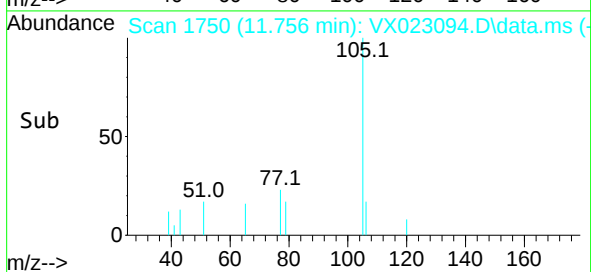

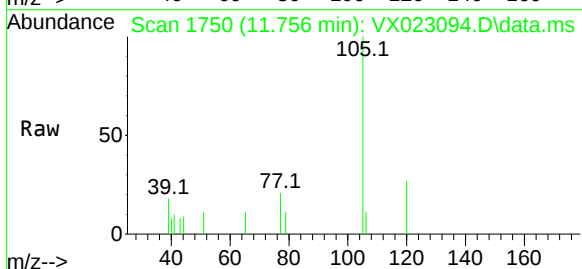




#85
 sec-Butylbenzene
 Concen: 0.390 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.140 min
 Lab File: VX023094.D
 Acq: 01 Jul 2021 18:48




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-CROPSEY-SOLIDS


Tgt Ion:105 Resp: 1176
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 29.8#

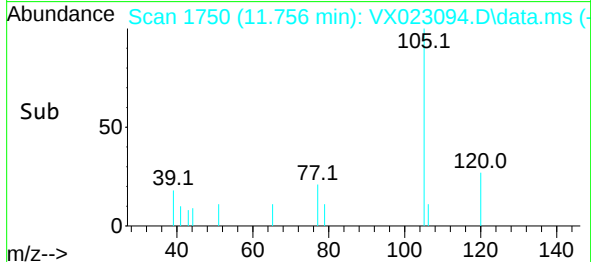

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 4.071 ug/l
 RT: 13.146 min Scan# 1978
 Delta R.T. 0.201 min
 Lab File: VX023094.D
 Acq: 01 Jul 2021 18:48

Tgt Ion: 75 Resp: 25
 Ion Ratio Lower Upper
 75 100
 155 0.0 45.3 135.9#
 157 0.0 57.7 173.1#

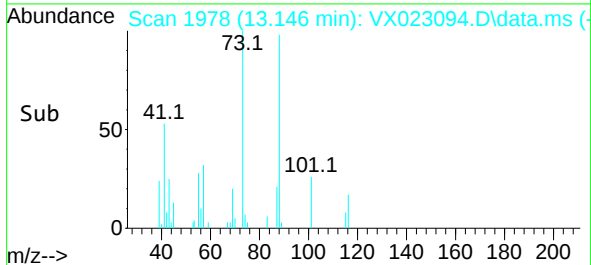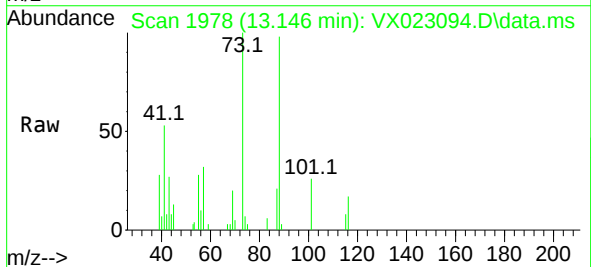

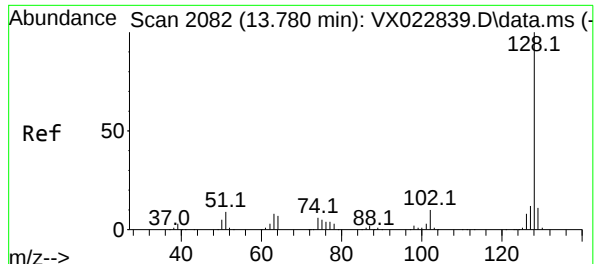

#95

Naphthalene

Concen: 2.649 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.000 min

Lab File: VX023094.D

Acq: 01 Jul 2021 18:48

Tgt Ion:128 Resp: 2097

Ion Ratio Lower Upper

128 100

127 9.9 10.3 15.5#

129 8.7 8.8 13.2#

