

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
 Data File : VX023095.D
 Acq On : 01 Jul 2021 19:12
 Operator : JC/MD
 Sample : M2896-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FS-01

Quant Time: Jul 02 04:32:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 23 19:12:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	56967	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	116348	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	106612	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	38915	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	65374	63.235	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 126.460%#	
35) Dibromofluoromethane	5.397	113	38026	51.467	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.940%	
50) Toluene-d8	8.653	98	148683	51.347	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 102.700%	
62) 4-Bromofluorobenzene	11.085	95	55129	51.013	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 102.020%	


Target Compounds				Qvalue		
11) Tert butyl alcohol	2.947	59	3164	14.685	ug/l	# 77
13) Acrolein	2.245	56	386	2.880	ug/l	# 41
16) Acetone	2.386	43	29261	63.843	ug/l	# 85
17) Carbon Disulfide	2.514	76	447	3.722	ug/l	# 75
18) Methyl Acetate	2.715	43	1616	1.433	ug/l	# 87
20) Methylene Chloride	2.794	84	6949	7.960	ug/l	# 81
25) 2-Butanone	4.574	43	8140	11.421	ug/l	# 88
29) Tetrahydrofuran	5.032	42	805	1.756	ug/l	# 59
31) Cyclohexane	5.568	56	2167	1.485	ug/l	# 51
36) 1,1-Dichloropropene	5.556	75	6915	5.596	ug/l	# 49
37) Ethyl Acetate	4.714	43	292	0.204	ug/l	# 64
38) Carbon Tetrachloride	5.562	117	8150	7.863	ug/l	# 18
41) Methacrylonitrile	5.013	41	725	0.919	ug/l	# 40
43) Isopropyl Acetate	6.354	43	11991	5.210	ug/l	# 88
48) Methyl methacrylate	7.604	41	3654	3.430	ug/l	# 10
49) 1,4-Dioxane	7.805	88	61	2.660	ug/l	# 1
51) 4-Methyl-2-Pentanone	8.555	43	44738	31.233	ug/l	# 45
52) Toluene	8.726	92	2485	1.154	ug/l	96
54) cis-1,3-Dichloropropene	8.555	75	17209	13.026	ug/l	# 68
56) Ethyl methacrylate	9.256	69	107	2.643	ug/l	# 1
57) 1,3-Dichloropropane	9.488	76	8872	5.647	ug/l	# 42
59) 2-Hexanone	9.378	43	4349	4.002	ug/l	# 19
68) m/p-Xylenes	10.305	106	752	0.490	ug/l	92
69) o-Xylene	10.640	106	536	0.359	ug/l	68
74) N-amyl acetate	10.896	43	329	2.225	ug/l	# 38
76) 1,2,3-Trichloropropane	11.085	75	34238	33.309	ug/l	# 38
81) trans-1,4-Dichloro-2-b...	11.085	75	34238	84.764	ug/l	# 12
84) 1,2,4-Trimethylbenzene	11.756	105	703	0.258	ug/l	90
85) sec-Butylbenzene	11.756	105	703	0.204	ug/l	# 57
90) Hexachloroethane	12.695	117	623	4.850	ug/l	# 9
92) 1,2-Dibromo-3-Chloropr...	12.951	75	19	4.038	ug/l	# 1
95) Naphthalene	13.780	128	1434	2.357	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
Data File : VX023095.D
Acq On : 01 Jul 2021 19:12
Operator : JC/MD
Sample : M2896-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FS-01


Quant Time: Jul 02 04:32:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 23 19:12:26 2021
Response via : Initial Calibration

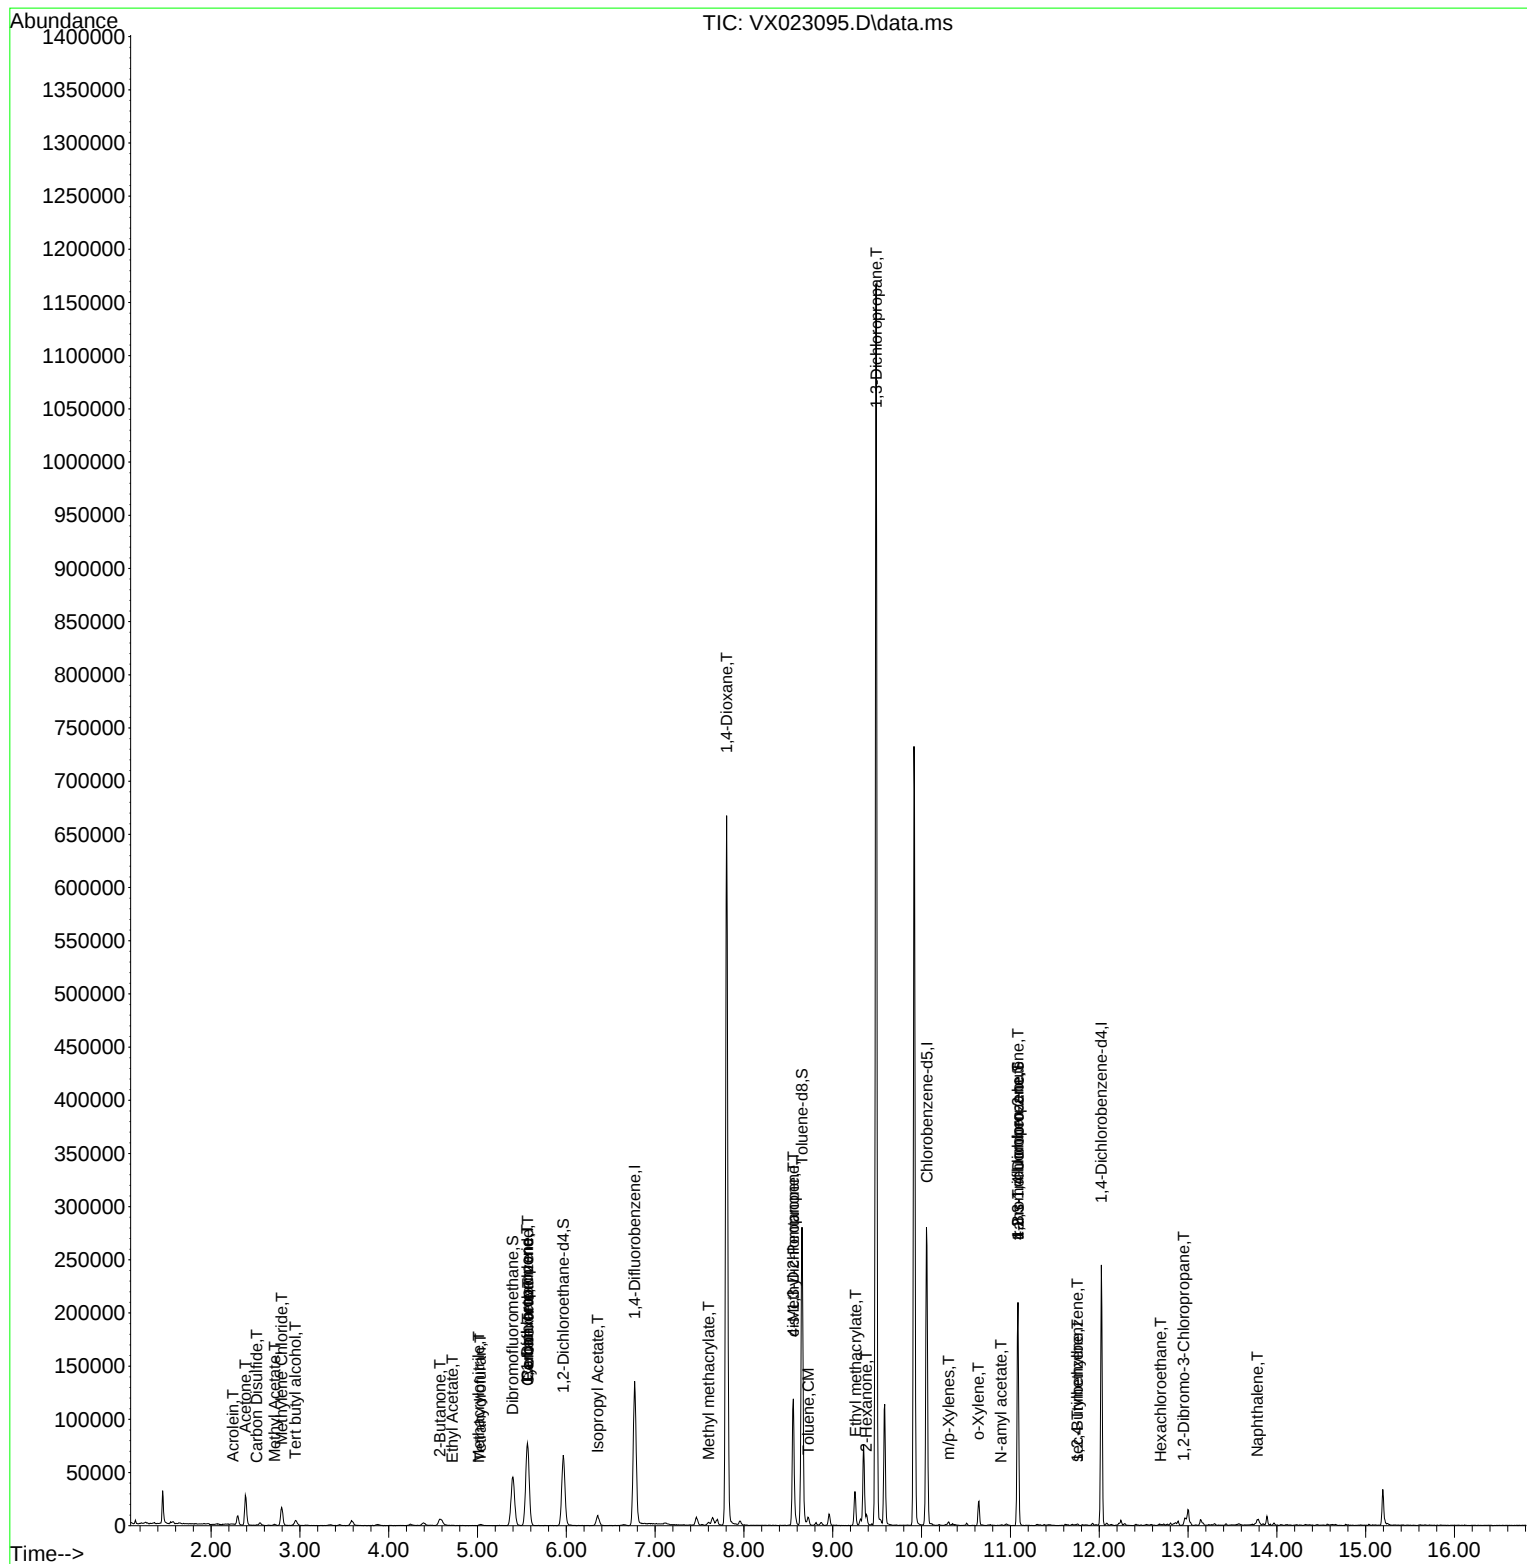






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.006 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Instrument :
MSVOA_X
ClientSampleId :
FS-01



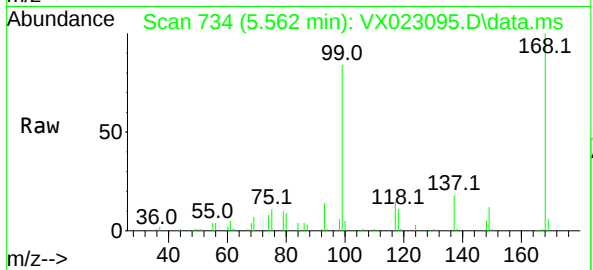



Tgt Ion:168 Resp: 56967
Ion Ratio Lower Upper
168 100
99 84.2 45.8 68.6#

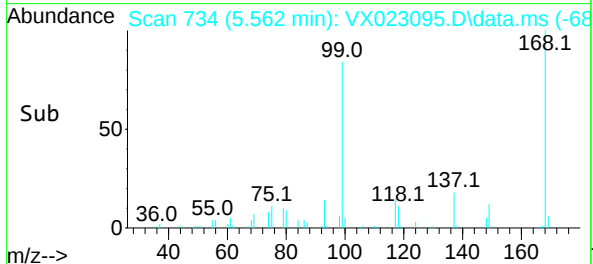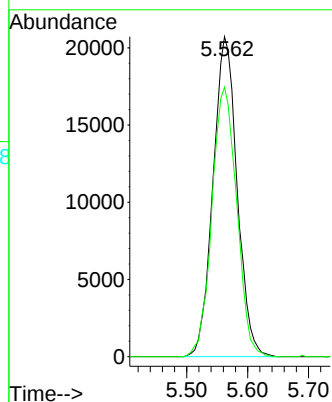

#11
Tert butyl alcohol
Concen: 14.685 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.030 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 59 Resp: 3164
Ion Ratio Lower Upper
59 100
57 1.4 7.8 11.8#


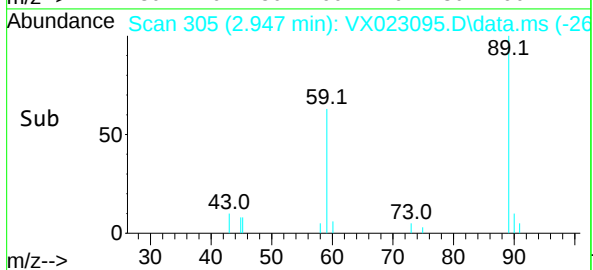
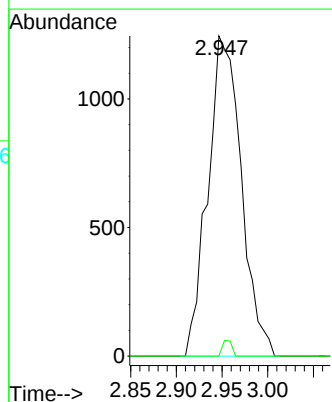
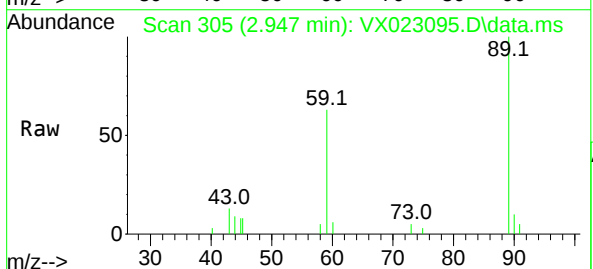




#13
Acrolein
Concen: 2.880 ug/l
RT: 2.245 min Scan# 190
Delta R.T. 0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion: 56 Resp: 386
Ion Ratio Lower Upper
56 100
55 119.4 56.4 84.6#

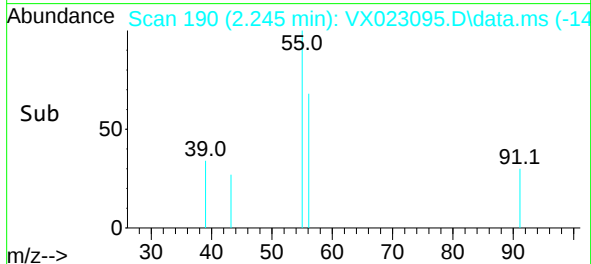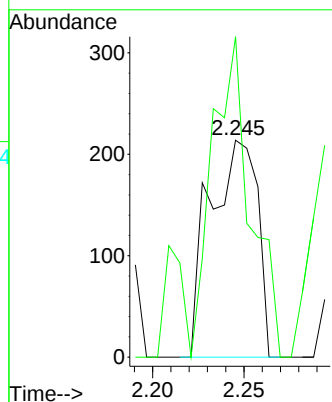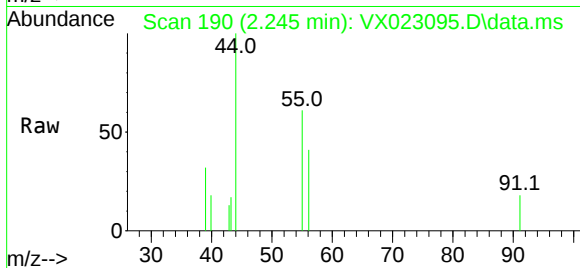

#16
Acetone
Concen: 63.843 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12


Tgt Ion: 43 Resp: 29261
Ion Ratio Lower Upper
43 100
58 26.0 27.8 41.8#

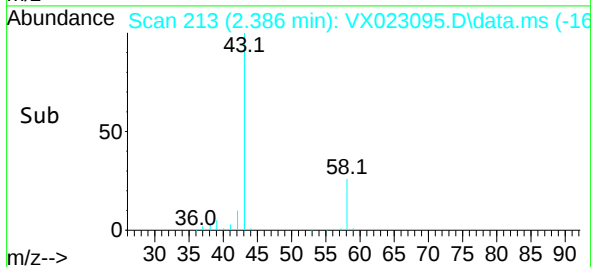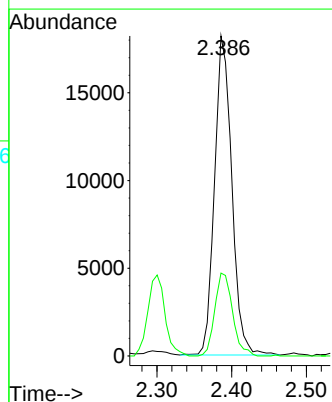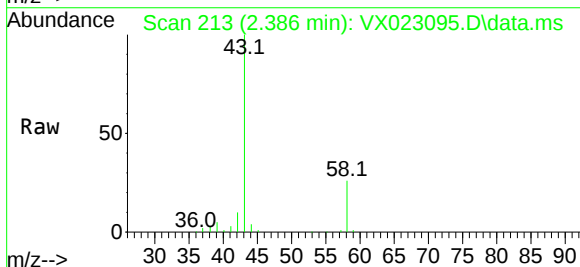






#17
Carbon Disulfide
Concen: 3.722 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12


Instrument :
MSVOA_X
ClientSampleId :
FS-01





Tgt Ion: 76 Resp: 447
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

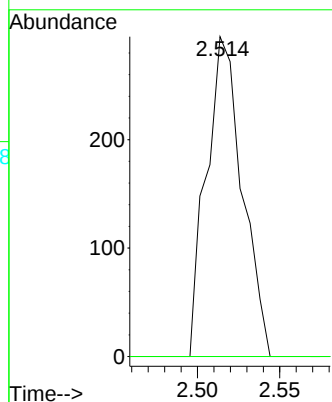


#18
Methyl Acetate
Concen: 1.433 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12



Tgt Ion: 43 Resp: 1616
Ion Ratio Lower Upper
43 100
74 20.4 21.9 32.9#




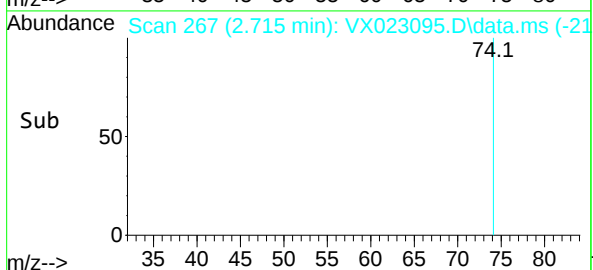




#20
Methylene Chloride
Concen: 7.960 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion:	84	Resp:	6949
Ion	Ratio	Lower	Upper
84	100		
49	141.4	88.6	132.8#
51	44.2	27.0	40.6#
86	62.7	50.3	75.5

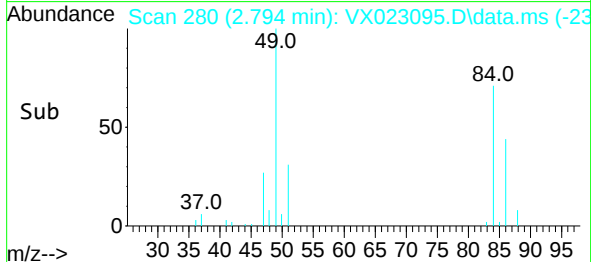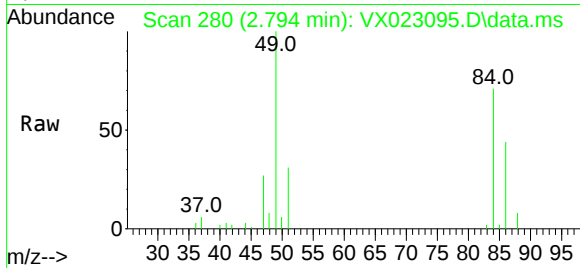

#25
2-Butanone
Concen: 11.421 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion:	43	Resp:	8140
Ion	Ratio	Lower	Upper
43	100		
72	22.9	23.7	35.5#

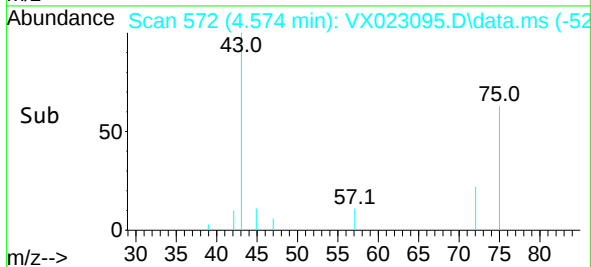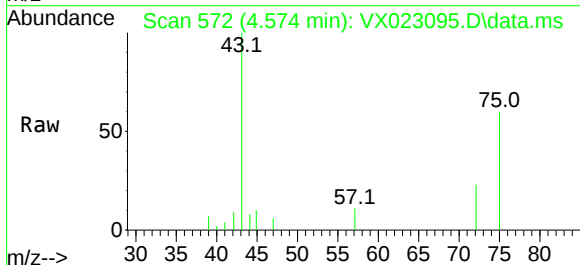



#29

Tetrahydrofuran

Concen: 1.756 ug/l

RT: 5.032 min Scan# 647

Delta R.T. 0.013 min

Lab File: VX023095.D

Acq: 01 Jul 2021 19:12





Instrument :

MSVOA_X

ClientSampleId :

FS-01

Tgt Ion:	42	Resp:	805
Ion	Ratio	Lower	Upper
42	100		
72	8.8	41.7	62.5#
71	36.0	38.4	57.6#

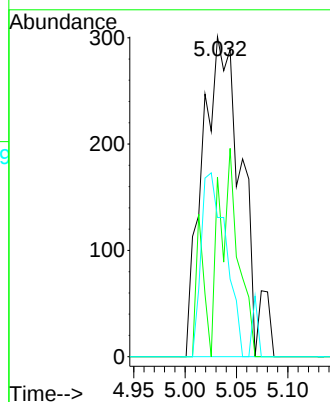

#31

Cyclohexane

Concen: 1.485 ug/l




RT: 5.568 min Scan# 735


Delta R.T. 0.092 min

Lab File: VX023095.D

Acq: 01 Jul 2021 19:12

Tgt Ion:	56	Resp:	2167
Ion	Ratio	Lower	Upper
56	100		
69	134.1	25.3	37.9#
84	88.0	71.4	107.0

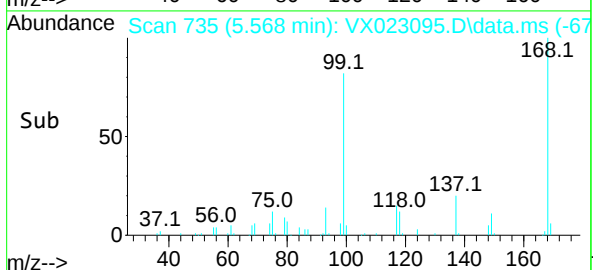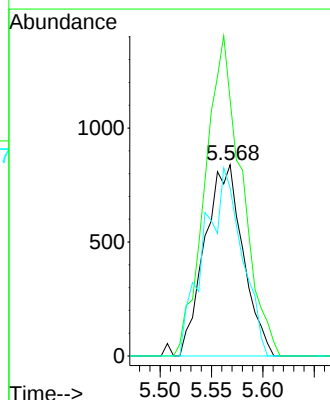







#33

1,2-Dichloroethane-d4
Concen: 63.235 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Instrument :
MSVOA_X
ClientSampled :
FS-01




Tgt Ion: 65 Resp: 65374
Ion Ratio Lower Upper
65 100
67 48.1 0.0 105.4

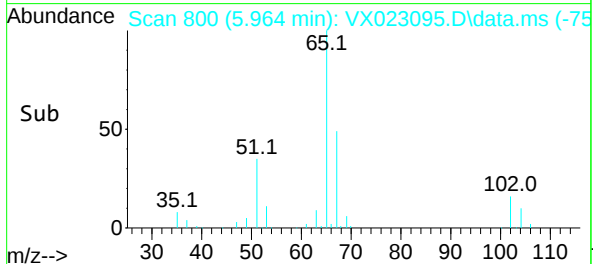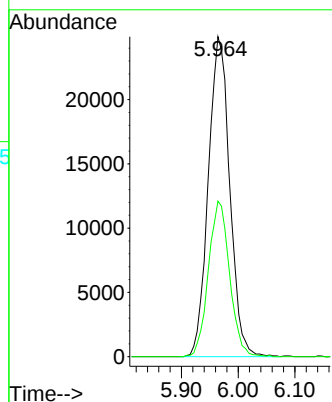


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 114 Resp: 116348
Ion Ratio Lower Upper
114 100
63 26.5 0.0 40.8
88 19.0 0.0 32.8

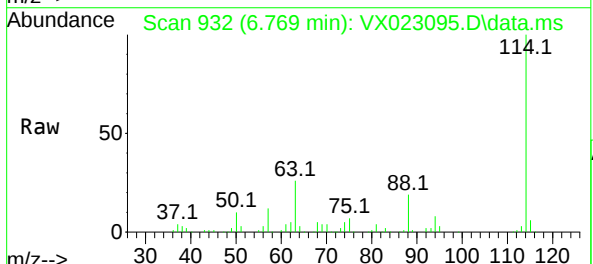



#35

Dibromofluoromethane

Concen: 51.467 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.000 min

Lab File: VX023095.D

Acq: 01 Jul 2021 19:12





Tgt Ion:113 Resp: 38026

Ion Ratio Lower Upper

113 100

111 104.5 81.9 122.9

192 14.3 16.7 25.1#

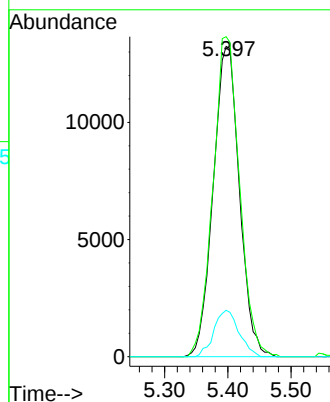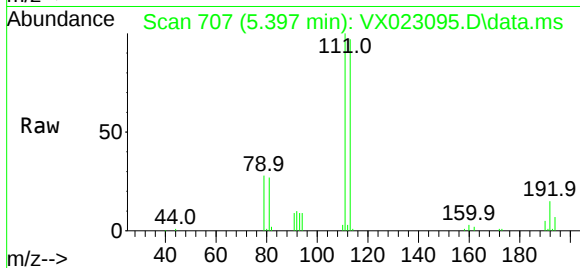

#36

1,1-Dichloropropene

Concen: 5.596 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.146 min

Lab File: VX023095.D

Acq: 01 Jul 2021 19:12




Tgt Ion: 75 Resp: 6915


Ion Ratio Lower Upper

75 100

110 8.8 18.1 54.4#

77 0.0 25.3 37.9#

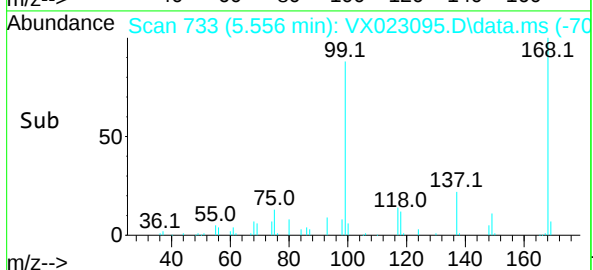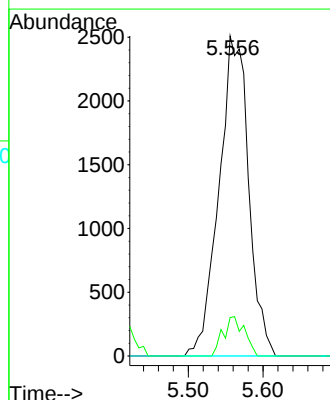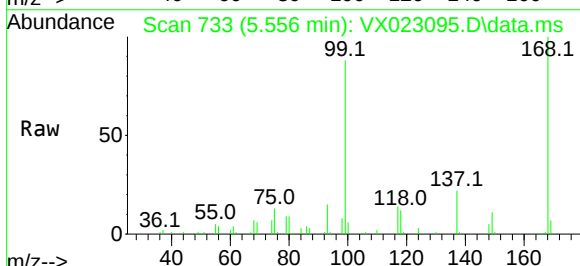



#37

Ethyl Acetate

Concen: 0.204 ug/l

RT: 4.714 min Scan# 595





Delta R.T. -0.013 min

Lab File: VX023095.D

Acq: 01 Jul 2021 19:12

Instrument :
MSVOA_X
ClientSampled :
FS-01

Tgt Ion: 43	Resp: 292
Ion Ratio	Lower Upper
43 100	
61 0.0	12.8 19.2#
70 0.0	10.5 15.7#

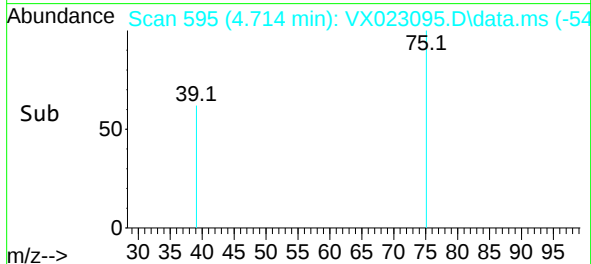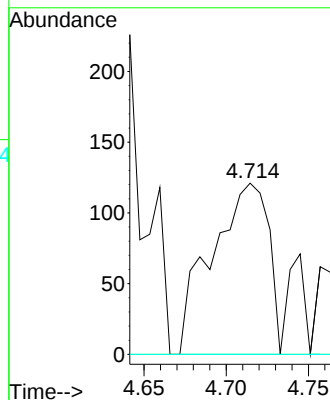

#38

Carbon Tetrachloride

Concen: 7.863 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.128 min

Lab File: VX023095.D

Acq: 01 Jul 2021 19:12

Tgt Ion: 117	Resp: 8150
Ion Ratio	Lower Upper
117 100	
119 7.1	76.2 114.2#
121 0.0	24.8 37.2#



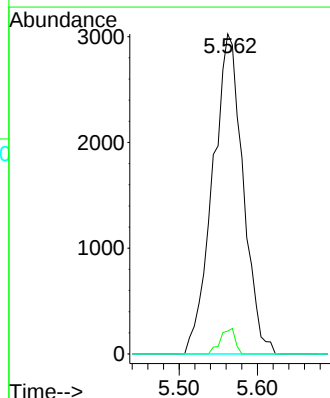
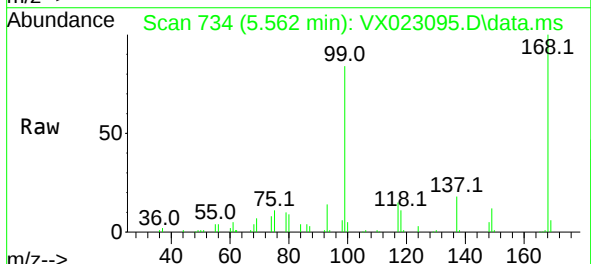




#41
Methacrylonitrile
Concen: 0.919 ug/l
RT: 5.013 min Scan# 644
Delta R.T. 0.085 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion:	41	Resp:	725
Ion	Ratio	Lower	Upper
41	100		
39	43.9	42.5	63.7
67	0.0	65.0	97.6#
52	0.0	25.3	37.9#

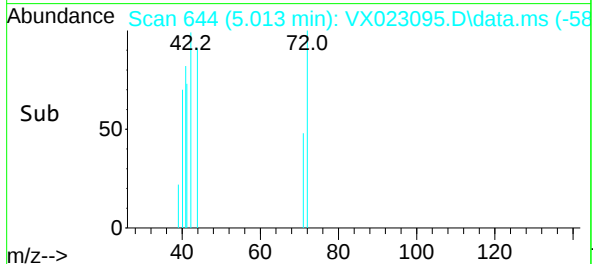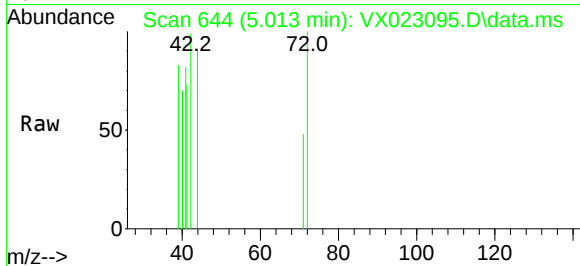

#43
Isopropyl Acetate
Concen: 5.210 ug/l
RT: 6.354 min Scan# 864
Delta R.T. 0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion:	43	Resp:	11991
Ion	Ratio	Lower	Upper
43	100		
61	17.0	18.2	27.4#
87	10.4	12.5	18.7#


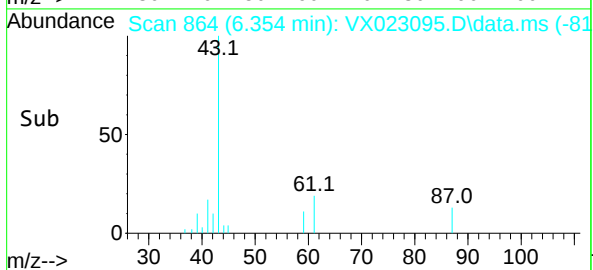

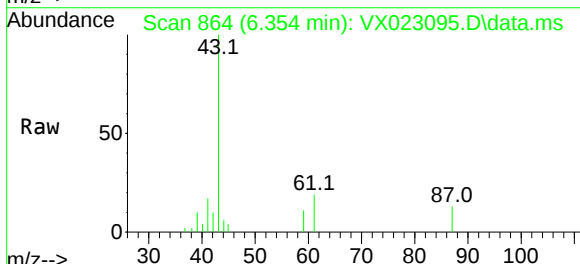




#48
Methyl methacrylate
Concen: 3.430 ug/l
RT: 7.604 min Scan# 1069
Delta R.T. -0.098 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion: 41 Resp: 3654
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 0.0 44.6 67.0#

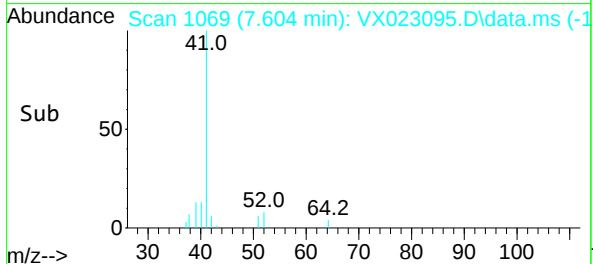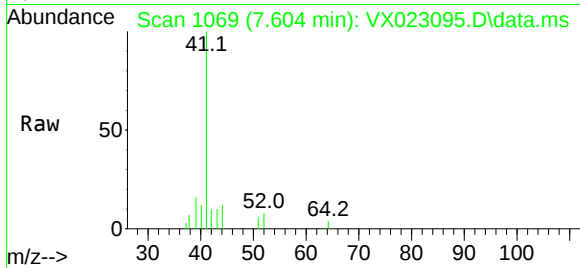

#49
1,4-Dioxane
Concen: 2.660 ug/l
RT: 7.805 min Scan# 1102
Delta R.T. 0.140 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 88 Resp: 61
Ion Ratio Lower Upper
88 100
43 999982.0 23.2 34.8#
58 4373.8 55.0 82.4#

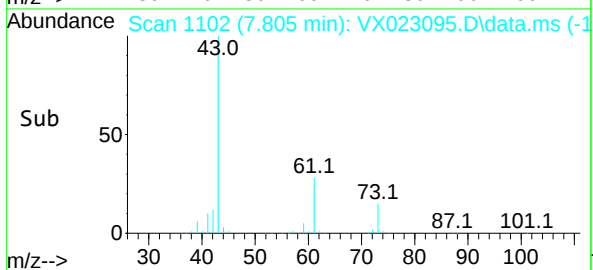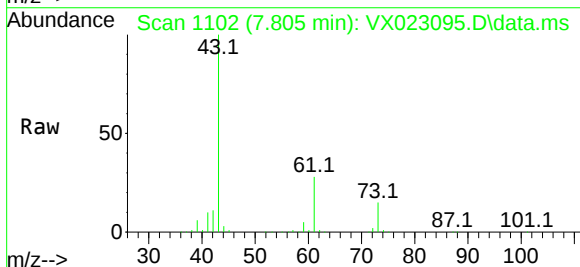



#50

Toluene-d8

Concen: 51.347 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX023095.D





Acq: 01 Jul 2021 19:12

Tgt Ion: 98 Resp: 148683

Ion Ratio Lower Upper

98 100

100 65.1 51.9 77.9

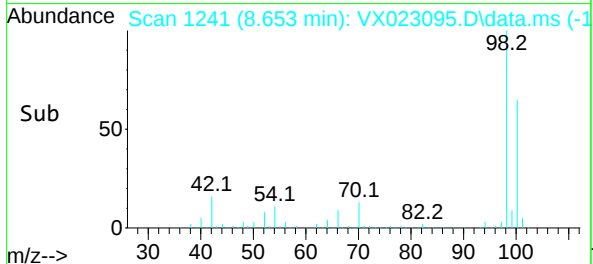

#51

4-Methyl-2-Pentanone

Concen: 31.233 ug/l

RT: 8.555 min Scan# 1225

Delta R.T. -0.025 min

Lab File: VX023095.D




Acq: 01 Jul 2021 19:12


Tgt Ion: 43 Resp: 44738

Ion Ratio Lower Upper

43 100

58 8.3 35.4 53.0#


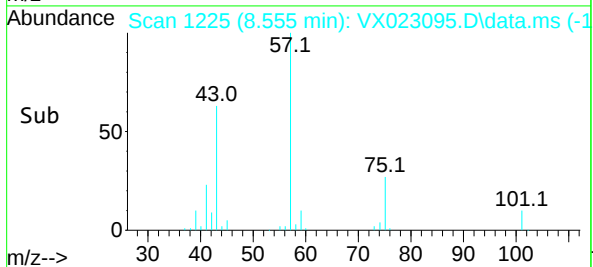

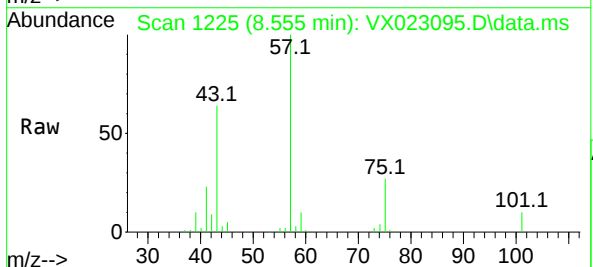




#52
Toluene
Concen: 1.154 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion: 92 Resp: 2485
Ion Ratio Lower Upper
92 100
91 166.3 137.1 205.7

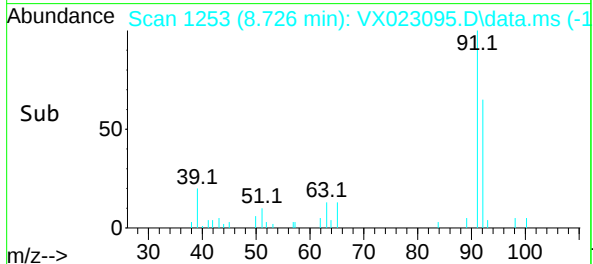

#54
cis-1,3-Dichloropropene
Concen: 13.026 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.183 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 75 Resp: 17209
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#
39 35.8 35.1 52.7


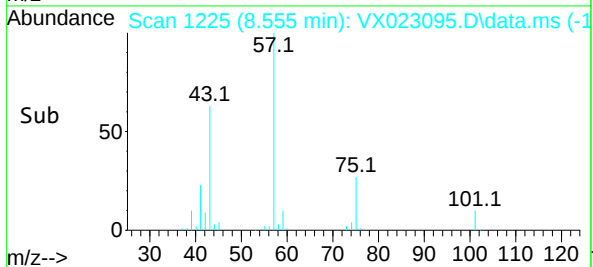

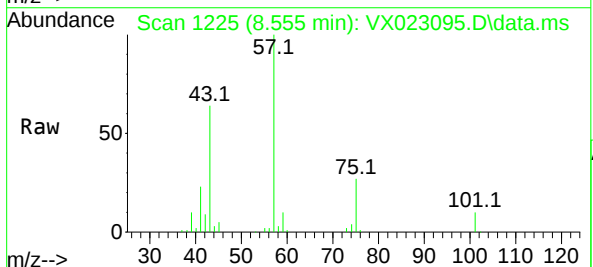




#56
Ethyl methacrylate
Concen: 2.643 ug/l
RT: 9.256 min Scan# 1340
Delta R.T. 0.134 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion: 69 Resp: 107
Ion Ratio Lower Upper
69 100
41 4949.5 46.8 70.2#
39 2512.1 24.7 37.1#

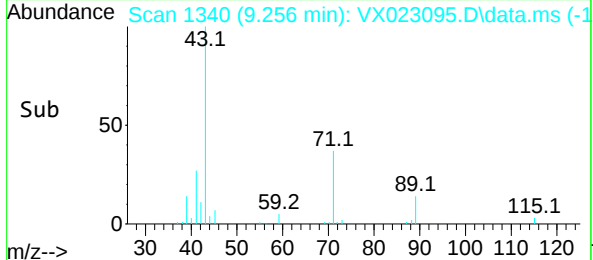

#57
1,3-Dichloropropane
Concen: 5.647 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.177 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 76 Resp: 8872
Ion Ratio Lower Upper
76 100
78 0.0 26.2 39.2#


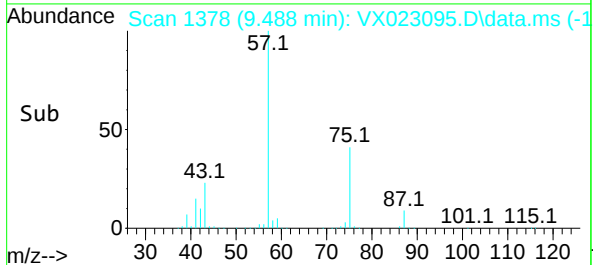

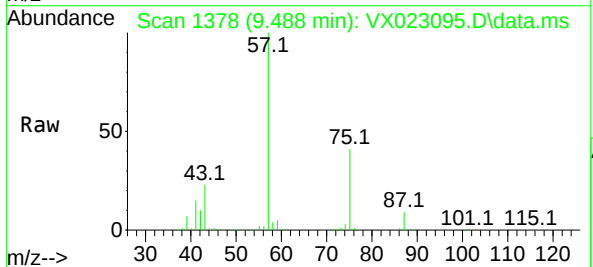




#59
2-Hexanone
Concen: 4.002 ug/l
RT: 9.378 min Scan# 1360
Delta R.T. -0.055 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion: 43 Resp: 4349
Ion Ratio Lower Upper
43 100
58 0.0 30.9 92.8#

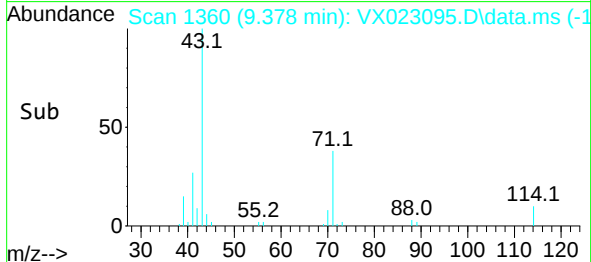

#62
4-Bromofluorobenzene
Concen: 51.013 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 95 Resp: 55129
Ion Ratio Lower Upper
95 100
174 54.9 0.0 154.6
176 51.5 0.0 155.8


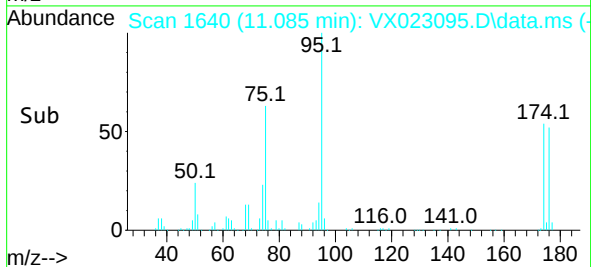

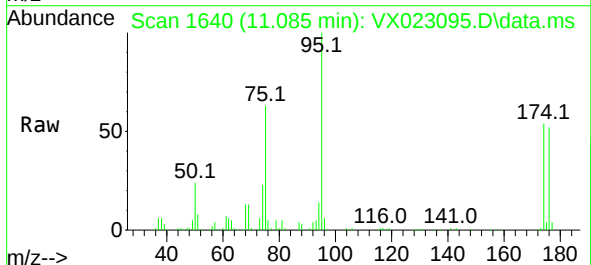




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.006 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion:117 Resp: 106612
Ion Ratio Lower Upper
117 100
82 63.8 47.4 71.2
119 31.1 26.6 39.8

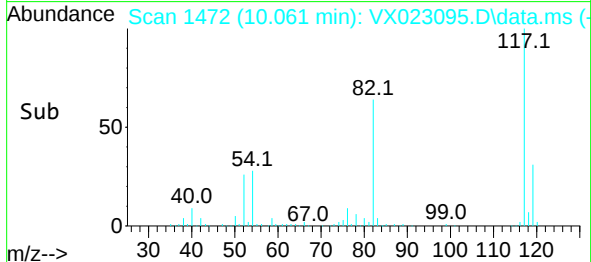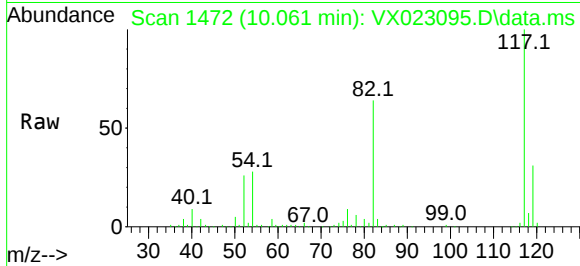

#68
m/p-Xylenes
Concen: 0.490 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion:106 Resp: 752
Ion Ratio Lower Upper
106 100
91 215.3 162.8 244.2


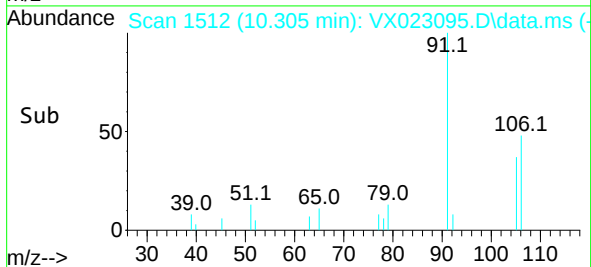

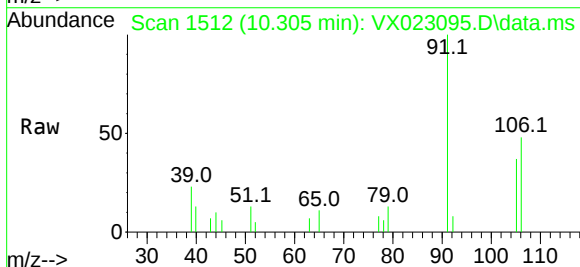


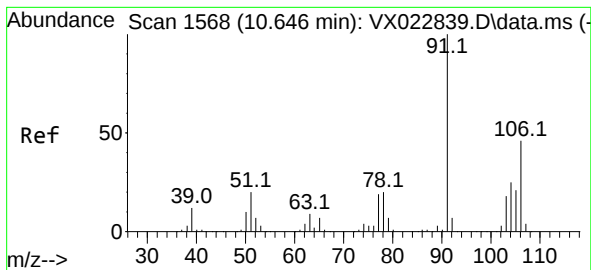

#69
o-Xylene
Concen: 0.359 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion:106 Resp: 536
Ion Ratio Lower Upper
106 100
91 267.0 108.1 324.2

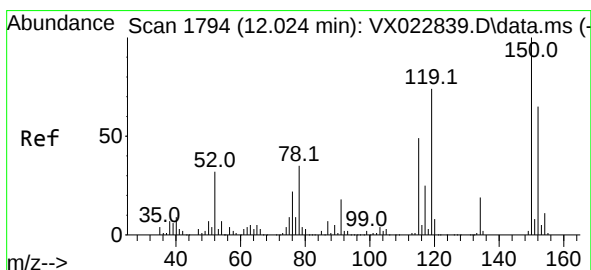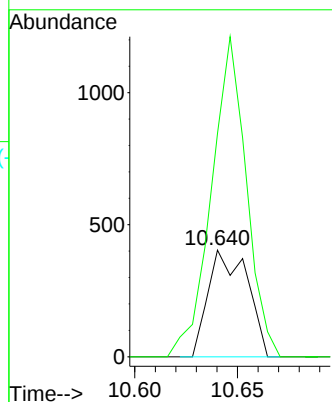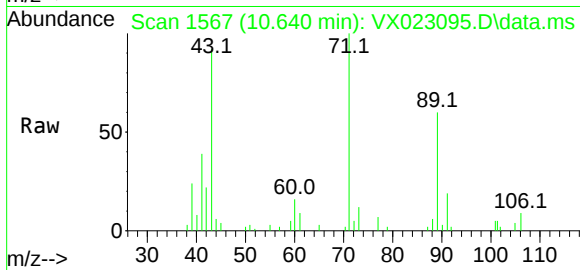

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion:152 Resp: 38915
Ion Ratio Lower Upper
152 100
115 74.3 41.1 123.3
150 163.1 0.0 349.0

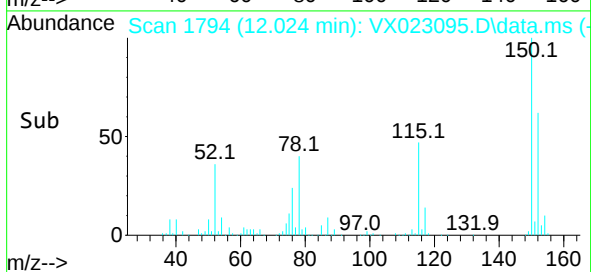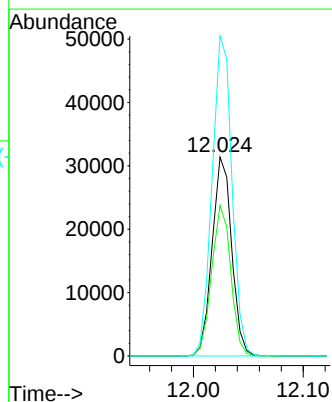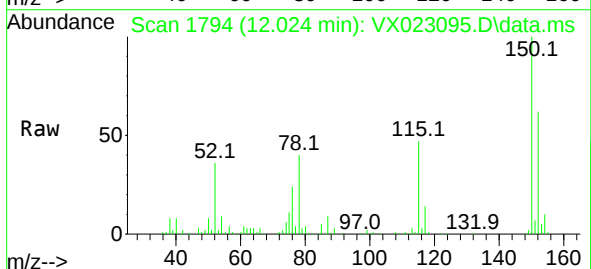







#74
N-amy1 acetate
Concen: 2.225 ug/l
RT: 10.896 min Scan# 1609
Delta R.T. 0.049 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Instrument :
MSVOA_X
ClientSampled :
FS-01

Tgt Ion: 43 Resp: 329




Ion	Ratio	Lower	Upper
43	100		
70	0.0	39.0	58.6#
55	0.0	21.5	32.3#
61	0.0	22.1	33.1#

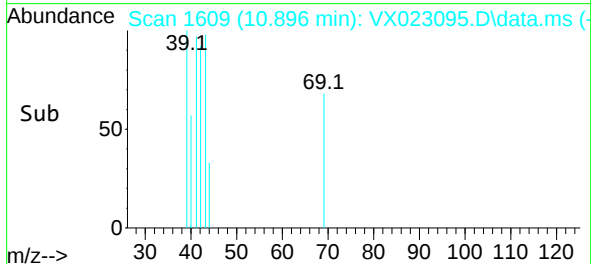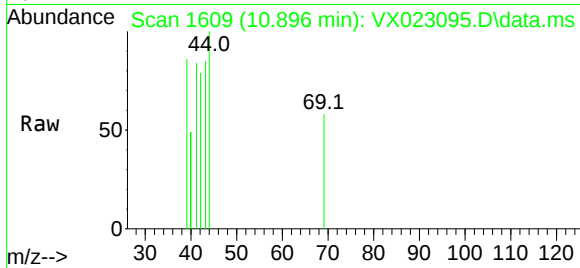


#76
1,2,3-Trichloropropane
Concen: 33.309 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 75 Resp: 34238

Ion	Ratio	Lower	Upper
75	100		
77	0.9	19.1	57.5#


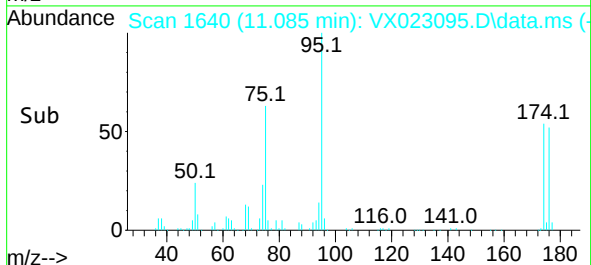

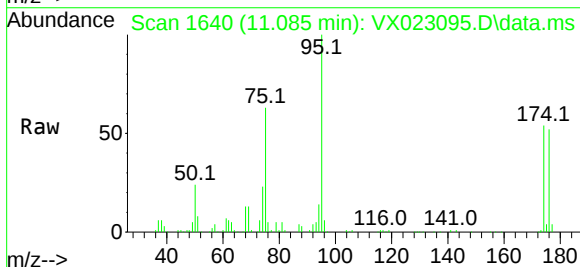




#81
trans-1,4-Dichloro-2-butene
Concen: 84.764 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12




Instrument :
MSVOA_X
ClientSampled :
FS-01


Tgt Ion: 75 Resp: 34238
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.2 37.9 56.9#

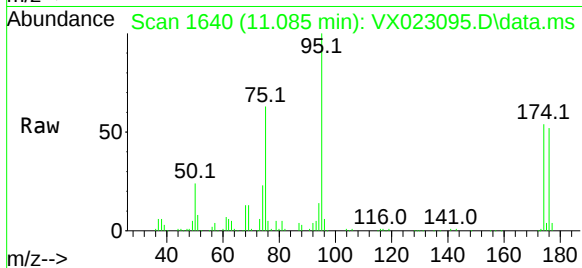

#84
1,2,4-Trimethylbenzene
Concen: 0.258 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 105 Resp: 703
Ion Ratio Lower Upper
105 100
120 38.4 22.4 67.3


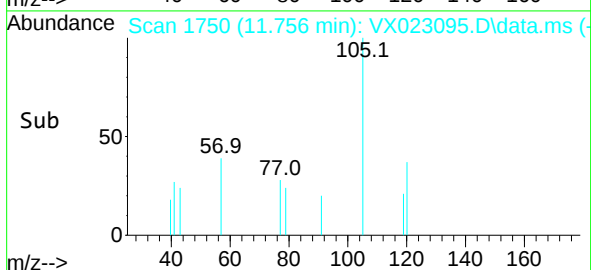

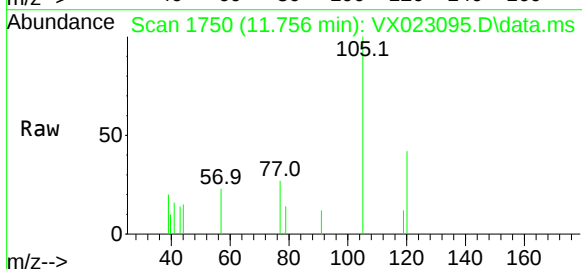




#85
 sec-Butylbenzene
 Concen: 0.204 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.140 min
 Lab File: VX023095.D
 Acq: 01 Jul 2021 19:12




Instrument :
 MSVOA_X
 ClientSampled :
 FS-01


Tgt Ion:105 Resp: 703
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 29.8#

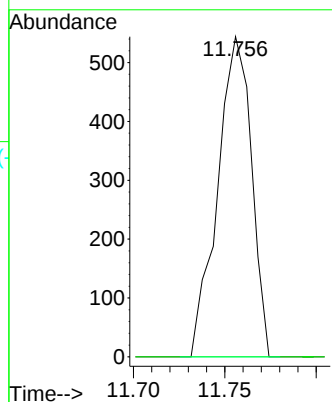

#90
 Hexachloroethane
 Concen: 4.850 ug/l
 RT: 12.695 min Scan# 1904
 Delta R.T. 0.153 min
 Lab File: VX023095.D
 Acq: 01 Jul 2021 19:12


Tgt Ion:117 Resp: 623
 Ion Ratio Lower Upper
 117 100
 201 0.0 40.4 121.2#

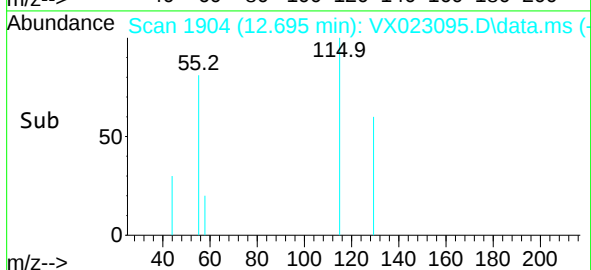






#92
1,2-Dibromo-3-Chloropropane
Concen: 4.038 ug/l
RT: 12.951 min Scan# 1946
Delta R.T. 0.006 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Instrument :
MSVOA_X
ClientSampled :
FS-01

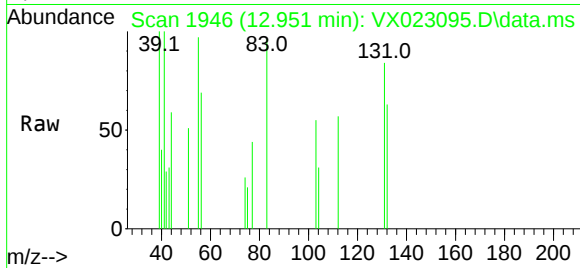

Tgt Ion: 75 Resp: 19
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

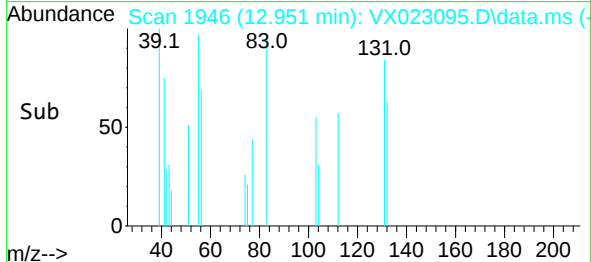

#95
Naphthalene
Concen: 2.357 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX023095.D
Acq: 01 Jul 2021 19:12

Tgt Ion: 128 Resp: 1434
Ion Ratio Lower Upper
128 100
127 14.6 10.3 15.5
129 12.5 8.8 13.2

