

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
 Data File : VX023087.D
 Acq On : 01 Jul 2021 16:03
 Operator : JC/MD
 Sample : M2892-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M

Title : SW846 8260

Signal : TIC: VX023087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	231	240	246	rBV	5286	10686	2.67%	0.474%
2	3.123	326	334	344	rVB2	24503	55188	13.78%	2.449%
3	5.397	695	707	719	rBV2	43933	123969	30.95%	5.500%
4	5.562	723	734	747	rVB3	69482	198660	49.60%	8.814%
5	5.964	790	800	814	rBV	63275	159813	39.90%	7.091%
6	6.251	836	847	858	rBV2	17089	50074	12.50%	2.222%
7	6.769	922	932	943	rBV	125308	295857	73.87%	13.127%
8	7.988	1125	1132	1139	rBV2	13007	25357	6.33%	1.125%
9	8.110	1146	1152	1158	rVB4	3656	7319	1.83%	0.325%
10	8.653	1232	1241	1253	rBV	262405	400493	100.00%	17.769%
11	9.579	1387	1393	1399	rBV2	18738	41699	10.41%	1.850%
12	10.055	1466	1471	1480	rVB	257870	354083	88.41%	15.710%
13	11.085	1634	1640	1649	rVB	197012	247385	61.77%	10.976%
14	12.024	1789	1794	1802	rVB	230335	283274	70.73%	12.568%




Sum of corrected areas: 2253857

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
Data File : VX023087.D
Acq On : 01 Jul 2021 16:03
Operator : JC/MD
Sample : M2892-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

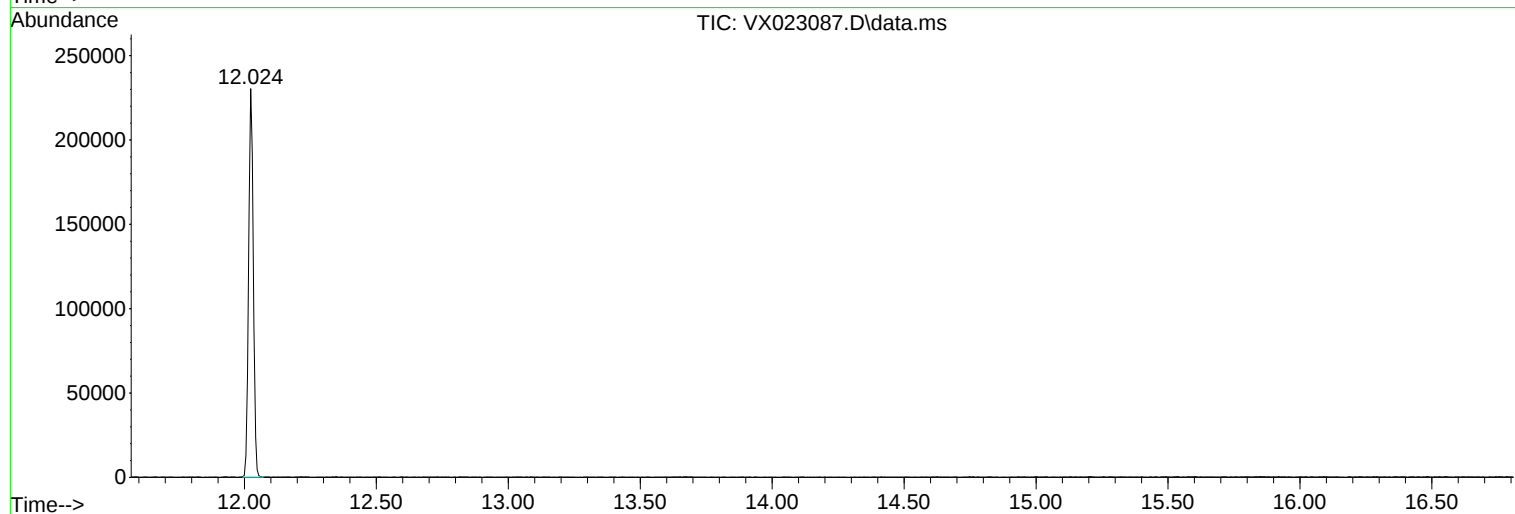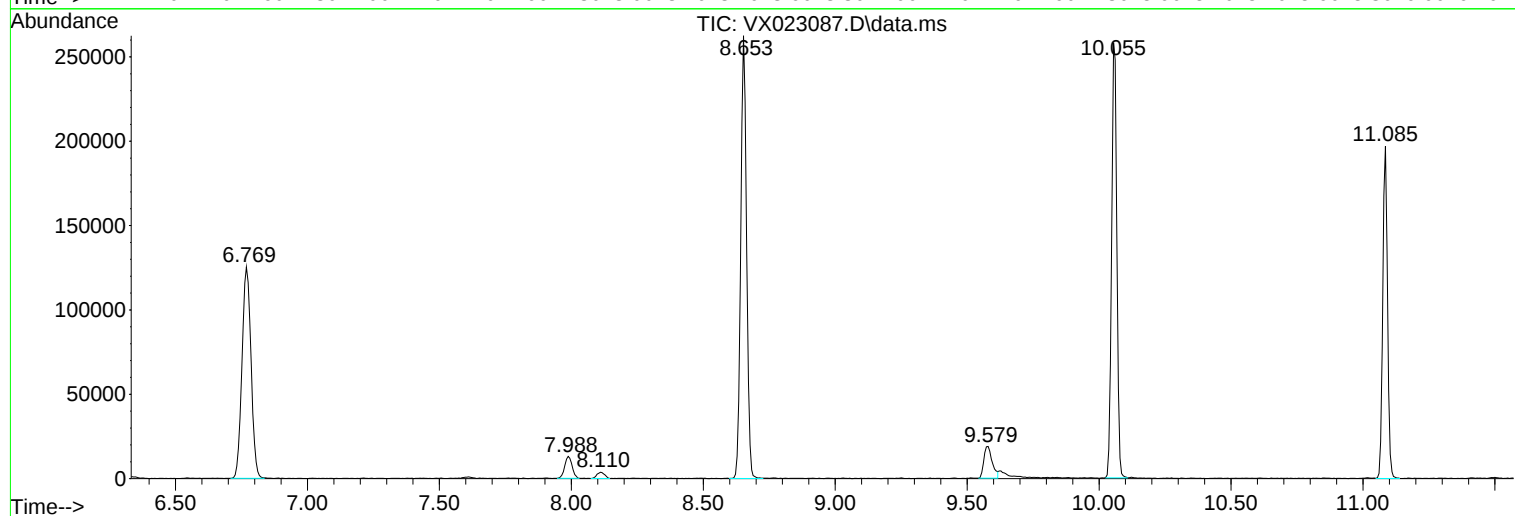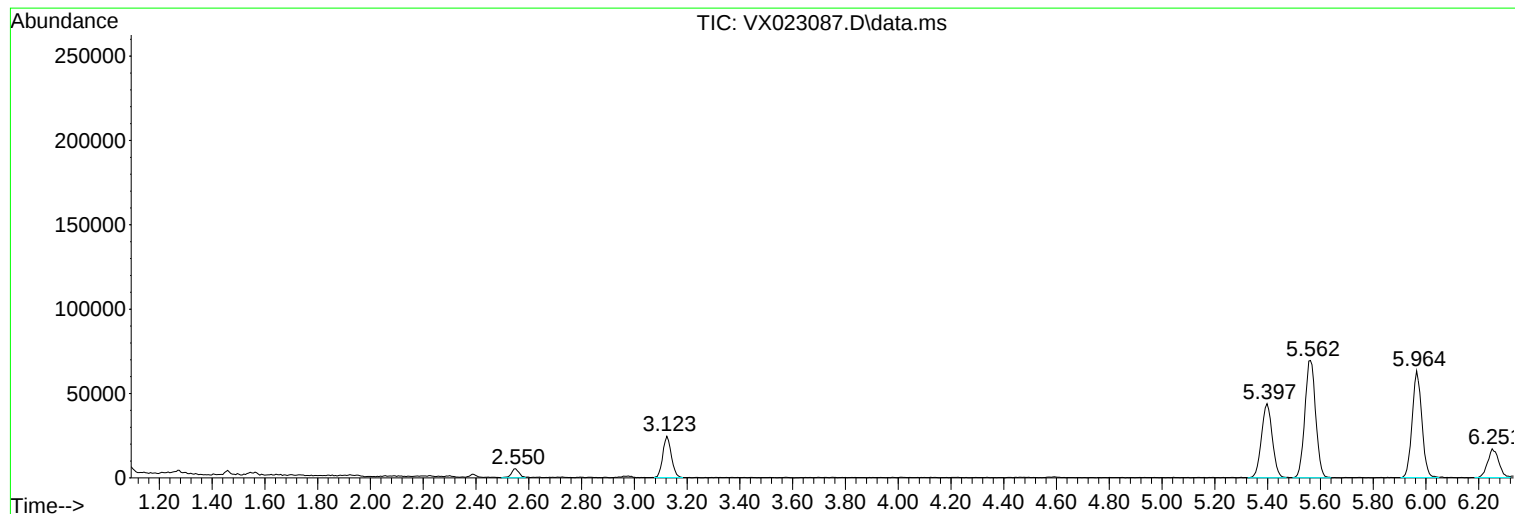

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
Data File : VX023087.D
Acq On : 01 Jul 2021 16:03
Operator : JC/MD
Sample : M2892-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexane, 2,2-dimethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.251	8.46 ug/l	50074	1,4-Difluorobenzene	6.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexane, 2,2-dimethyl-	114	C8H18	000590-73-8	72
2			Butane, 2,2,3,3-tetramethyl-	114	C8H18	000594-82-1	64
3			Pentane, 2,2,4-trimethyl-	114	C8H18	000540-84-1	64
4			Pentane, 2,2,4,4-tetramethyl-	128	C9H20	001070-87-7	64
5			Hexane, 2,2,5,5-tetramethyl-	142	C10H22	001071-81-4	50

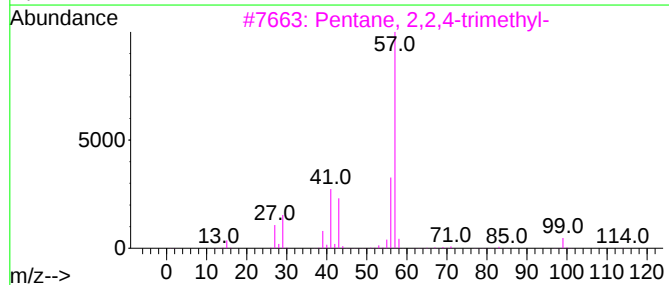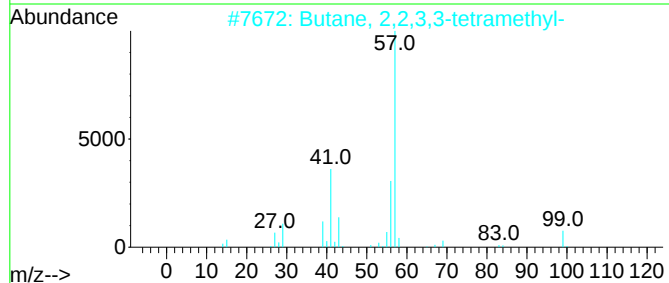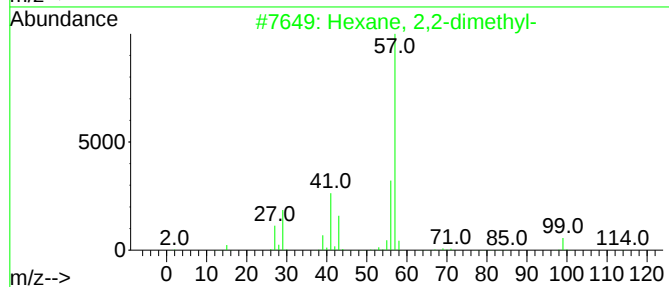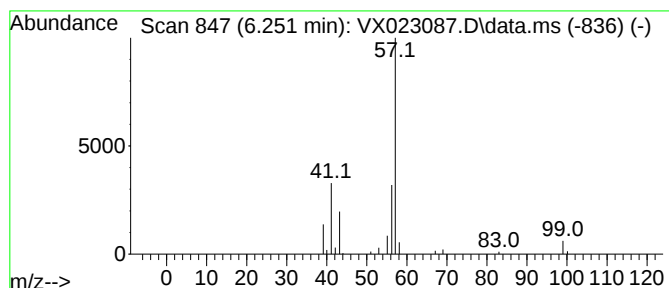

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
Data File : VX023087.D
Acq On : 01 Jul 2021 16:03
Operator : JC/MD
Sample : M2892-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.579	5.89 ug/l	41699	Chlorobenzene-d5	10.061

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
2			R-(-)-1,2-propanediol	76	C3H8O2	004254-14-2	9
3			Propylene Glycol	76	C3H8O2	000057-55-6	9
4			2-Butanol	74	C4H10O	000078-92-2	9
5			Methane, nitroso-	45	CH3NO	000865-40-7	4

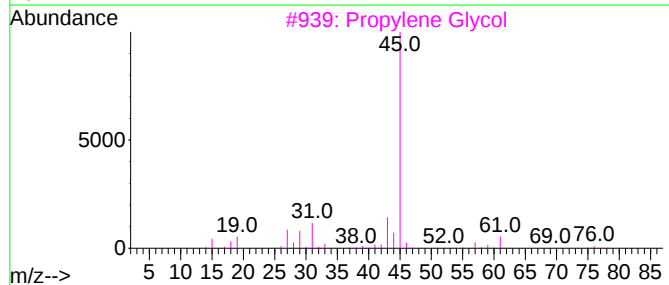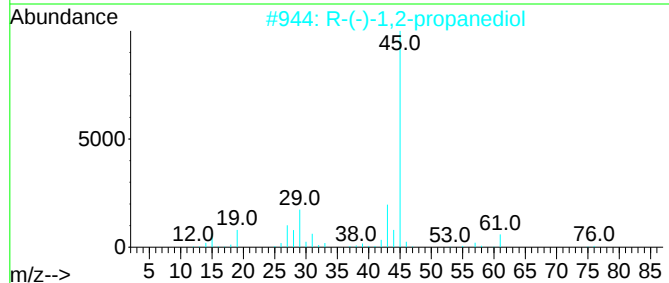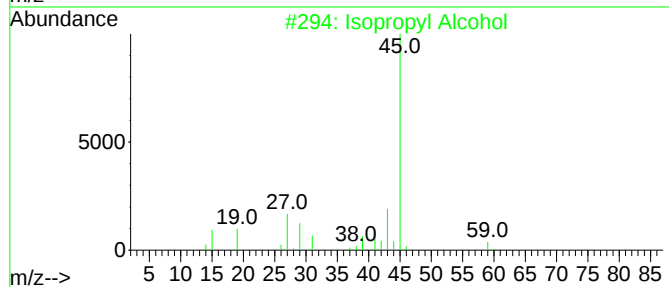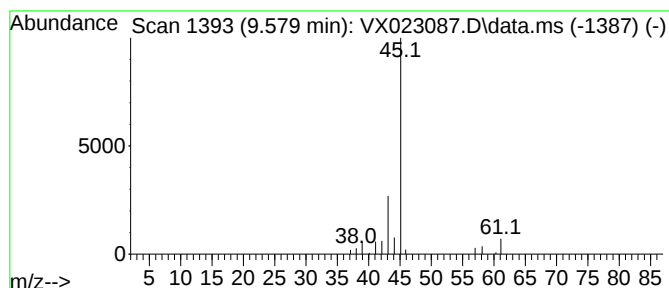

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070121\
Data File : VX023087.D
Acq On : 01 Jul 2021 16:03
Operator : JC/MD
Sample : M2892-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062321W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexane, 2,2-dim...	6.251	8.5	ug/l	50074	2	6.769	295857	50.0
Isopropyl Alcohol	9.579	5.9	ug/l	41699	3	10.061	354083	50.0