

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070124\
 Data File : VX042108.D
 Acq On : 01 Jul 2024 12:49
 Operator : JC/MD
 Sample : P3073-02DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW12-20240625DL

Quant Time: Jul 02 02:03:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 23:51:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	142619	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	220316	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	224889	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	121303	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	70230	42.704	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	85.400%
35) Dibromofluoromethane	5.385	113	68614	43.892	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	87.780%
50) Toluene-d8	8.647	98	260861	47.500	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.000%
62) 4-Bromofluorobenzene	11.079	95	104219	51.481	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.960%
Target Compounds						
						Qvalue
5) Bromomethane	1.605	94	290	0.430	ug/l	# 63
6) Chloroethane	1.660	64	317	Below Cal		93
11) Tert butyl alcohol	2.941	59	4197	13.447	ug/l	# 78
16) Acetone	2.392	43	1616	2.238	ug/l	95
20) Methylene Chloride	2.788	84	889	0.562	ug/l	# 83
36) 1,1-Dichloropropene	5.550	75	8123	4.893	ug/l	# 51
38) Carbon Tetrachloride	5.550	117	11770	6.417	ug/l	# 15
39) Methylcyclohexane	7.379	83	8346	3.975	ug/l	95
40) Benzene	6.038	78	4205	0.751	ug/l	# 86
52) Toluene	8.726	92	1288	0.361	ug/l	98
55) 1,1,2-Trichloroethane	9.104	97	1304	0.878	ug/l	# 20
67) Ethyl Benzene	10.195	91	352744	48.125	ug/l	97
68) m/p-Xylenes	10.305	106	11849	4.005	ug/l	93
69) o-Xylene	10.640	106	10282	3.510	ug/l	94
70) Styrene	10.647	104	1032	0.210	ug/l	# 1
73) Isopropylbenzene	10.964	105	119878	16.253	ug/l	97
76) 1,2,3-Trichloropropane	11.079	75	47140	21.406	ug/l	# 39
78) n-propylbenzene	11.305	91	132286	16.530	ug/l	97
79) 2-Chlorotoluene	11.396	91	6985	1.355	ug/l	# 48
80) 1,3,5-Trimethylbenzene	11.451	105	44939	7.315	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.079	75	47140	60.792	ug/l	# 5
82) 4-Chlorotoluene	11.451	91	4968	0.872	ug/l	# 46
83) tert-Butylbenzene	11.750	119	46125	6.843	ug/l	# 71
84) 1,2,4-Trimethylbenzene	11.750	105	357259	57.964	ug/l	91
85) sec-Butylbenzene	11.750	105	357259	46.856	ug/l	# 57
86) p-Isopropyltoluene	11.969	119	29732	4.464	ug/l	92
89) n-Butylbenzene	12.317	91	13820	2.696	ug/l	# 16
90) Hexachloroethane	12.695	117	325189	286.780	ug/l	# 17
92) 1,2-Dibromo-3-Chloropr...	12.963	75	756	1.391	ug/l	# 9
95) Naphthalene	13.774	128	2481514	281.813	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070124\
Data File : VX042108.D
Acq On : 01 Jul 2024 12:49
Operator : JC/MD
Sample : P3073-02DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL


Quant Time: Jul 02 02:03:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration

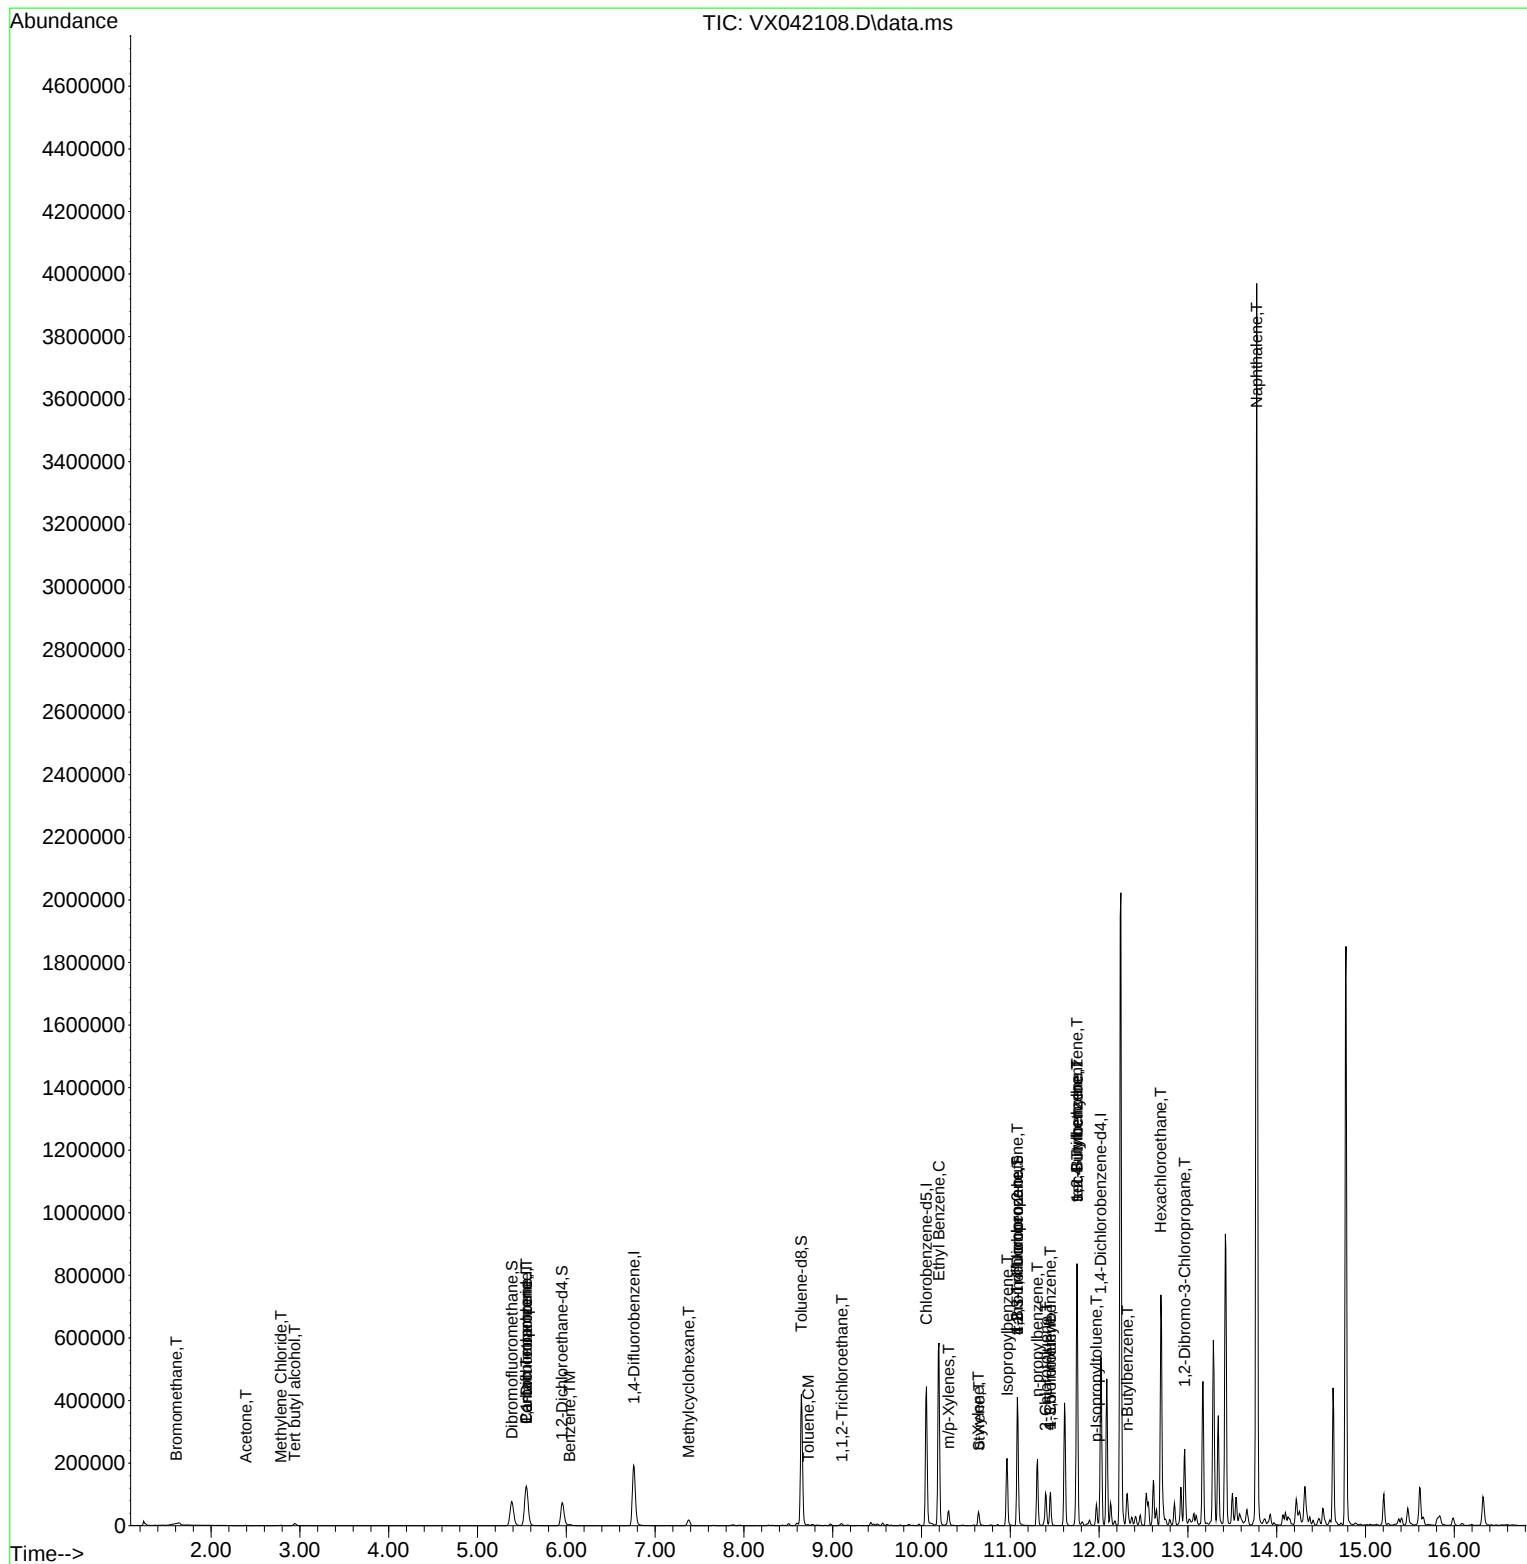






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 74
Delta R.T. -0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49


Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL





Tgt Ion:168 Resp: 142619
Ion Ratio Lower Upper
168 100
99 45.3 56.6 85.0#

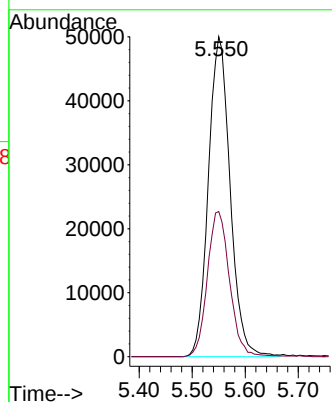


#5
Bromomethane
Concen: 0.430 ug/l
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49




Tgt Ion: 94 Resp: 290
Ion Ratio Lower Upper
94 100
96 58.1 74.6 111.8#

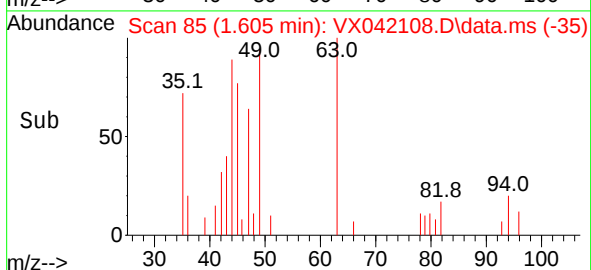



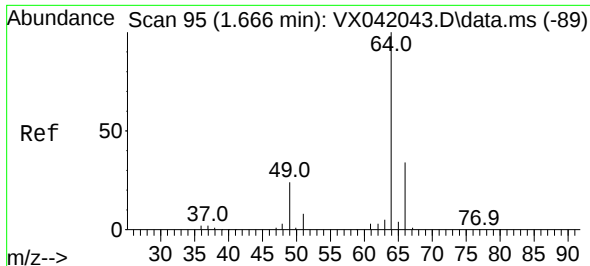


#6
Chloroethane
Concen: Below Cal
RT: 1.660 min Scan# 94
Delta R.T. 0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL



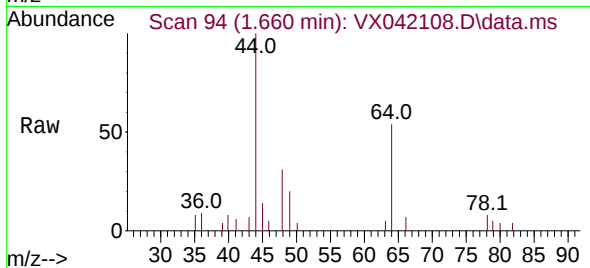



Tgt Ion: 64 Resp: 317
Ion Ratio Lower Upper
64 100
66 35.5 25.1 37.7

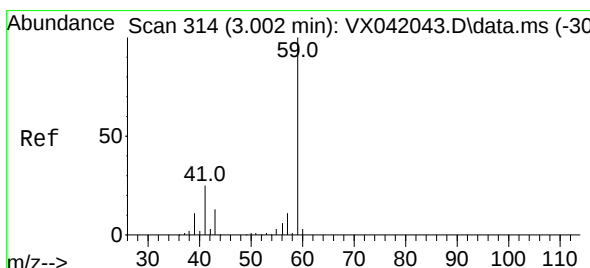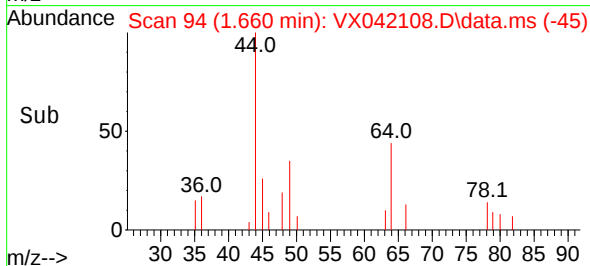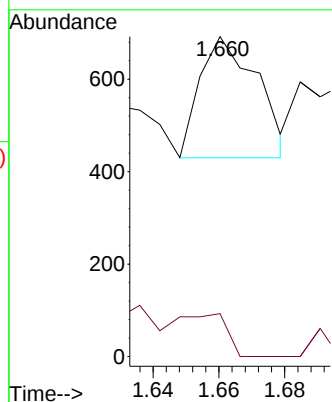

#11
Tert butyl alcohol
Concen: 13.447 ug/l
RT: 2.941 min Scan# 304
Delta R.T. -0.067 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Tgt Ion: 59 Resp: 4197
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#


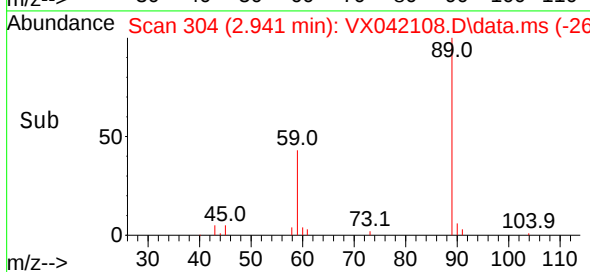
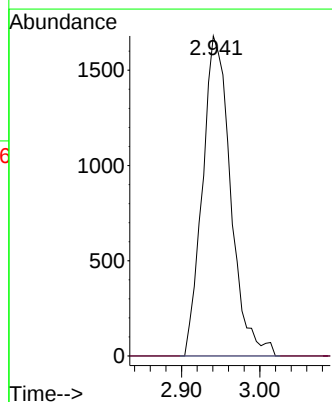
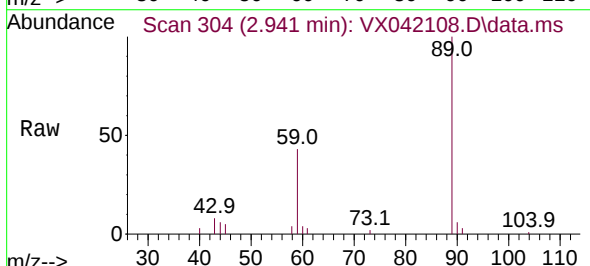




#16
Acetone
Concen: 2.238 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49




Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL


Tgt Ion: 43 Resp: 1616
Ion Ratio Lower Upper
43 100
58 29.9 21.9 32.9

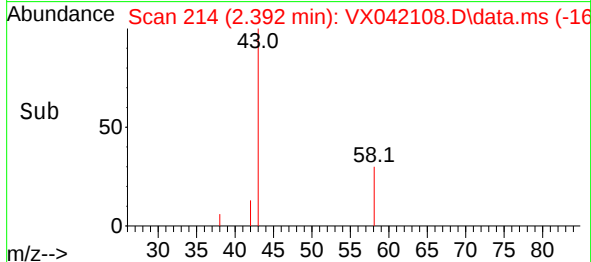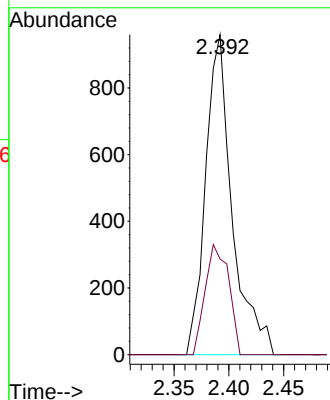

#20
Methylene Chloride
Concen: 0.562 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Tgt Ion: 84 Resp: 889
Ion Ratio Lower Upper
84 100
49 109.4 103.6 155.4
51 25.0 33.8 50.6#
86 69.2 49.4 74.0

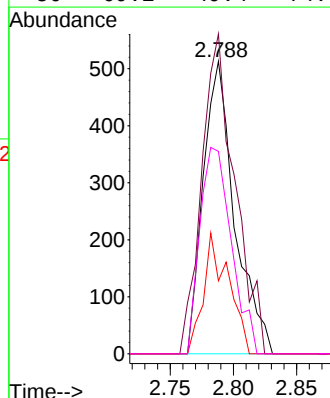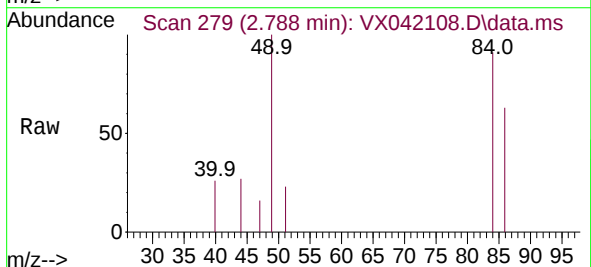



#33

1,2-Dichloroethane-d4

Concen: 42.704 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :





MW12-20240625DL

Tgt Ion: 65 Resp: 70230

Ion Ratio Lower Upper

65 100

67 53.9 0.0 100.2

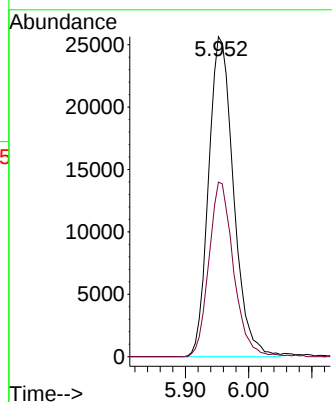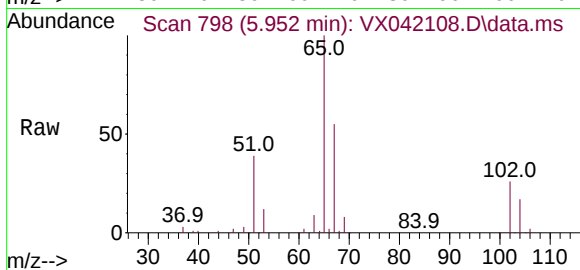

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49




Tgt Ion: 114 Resp: 220316


Ion Ratio Lower Upper

114 100

63 16.4 0.0 45.0

88 14.9 0.0 36.6

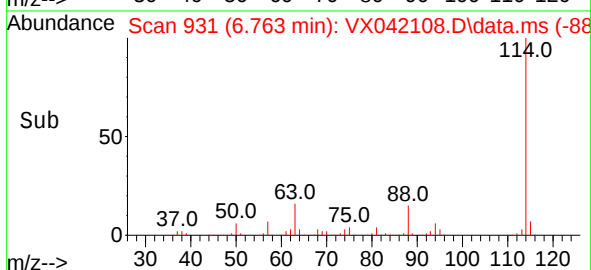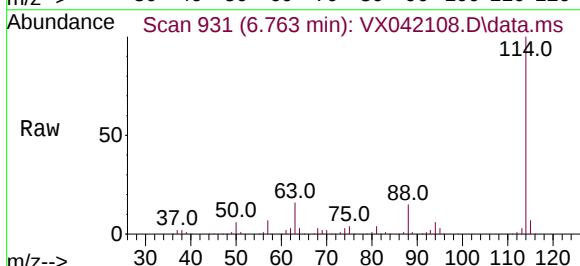



#35

Dibromofluoromethane

Concen: 43.892 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.006 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :

MW12-20240625DL





Tgt Ion:113 Resp: 68614

Ion Ratio Lower Upper

113 100

111 103.0 82.9 124.3

192 25.8 13.3 19.9#

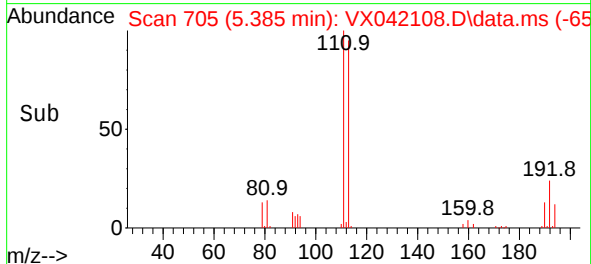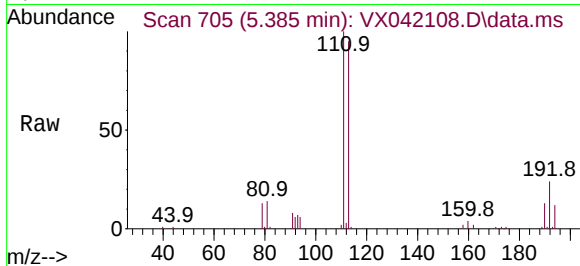

#36

1,1-Dichloropropene

Concen: 4.893 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.140 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49




Tgt Ion: 75 Resp: 8123


Ion Ratio Lower Upper

75 100

110 9.6 17.0 50.9#

77 0.0 24.7 37.1#

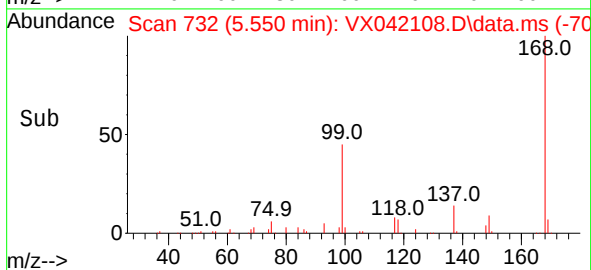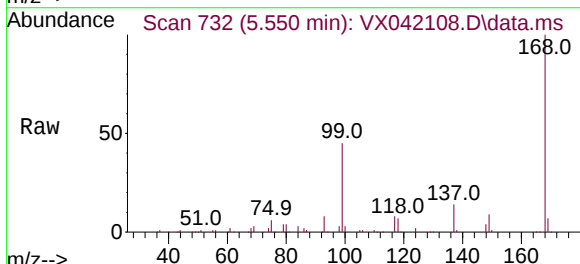



#38

Carbon Tetrachloride

Concen: 6.417 ug/l

RT: 5.550 min Scan# 753

Delta R.T. -0.128 min

Lab File: VX042108.D


Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :

MW12-20240625DL






Tgt Ion:117 Resp: 11770

Ion Ratio Lower Upper

117 100

119 5.3 78.2 117.2#

121 0.0 24.4 36.6#

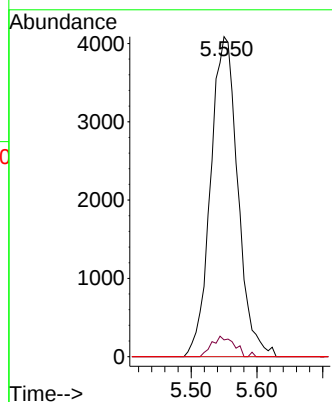

#39

Methylcyclohexane

Concen: 3.975 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. 0.000 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49




Tgt Ion: 83 Resp: 8346


Ion Ratio Lower Upper

83 100

55 75.6 64.6 97.0

98 48.3 36.7 55.1


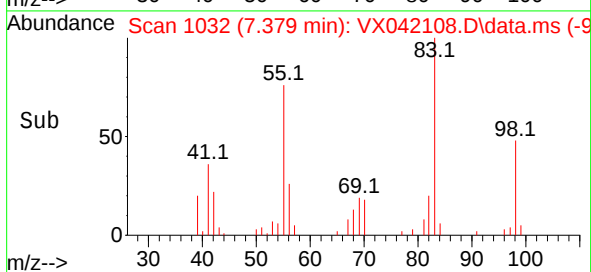

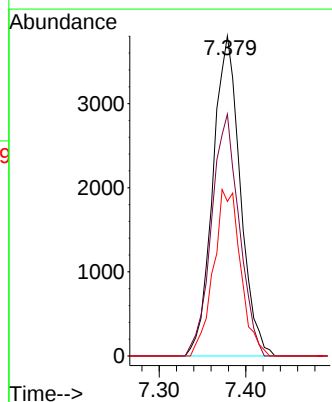




#40
Benzene
Concen: 0.751 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49




Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL


Tgt Ion: 78 Resp: 4205
Ion Ratio Lower Upper
78 100
77 30.9 19.3 28.9#

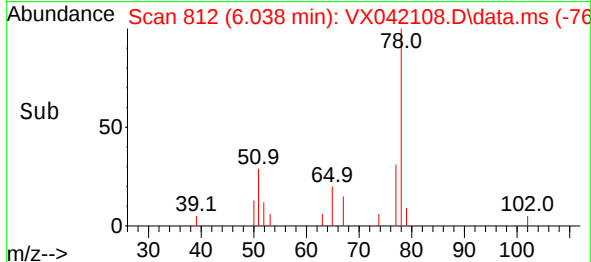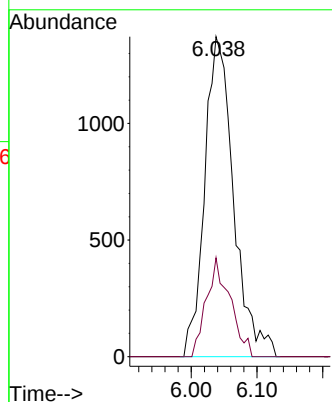

#50
Toluene-d8
Concen: 47.500 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Tgt Ion: 98 Resp: 260861
Ion Ratio Lower Upper
98 100
100 66.7 53.1 79.7

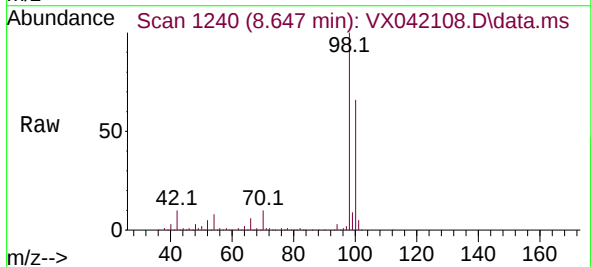



#52

Toluene

Concen: 0.361 ug/l

RT: 8.726 min Scan# 1315

Delta R.T. 0.006 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :





MW12-20240625DL

Tgt Ion: 92 Resp: 1288

Ion Ratio Lower Upper

92 100

91 170.2 134.2 201.2

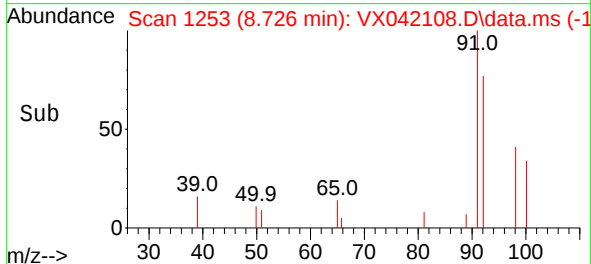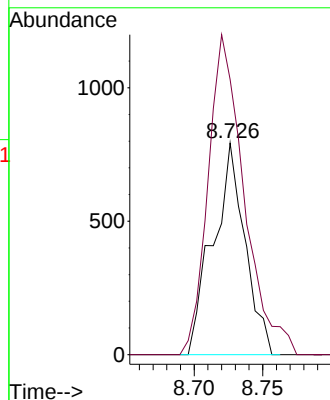

#55

1,1,2-Trichloroethane

Concen: 0.878 ug/l

RT: 9.104 min Scan# 1315

Delta R.T. -0.049 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Tgt Ion: 97 Resp: 1304




Ion Ratio Lower Upper


97 100

83 7.5 65.8 98.8#

85 0.0 41.6 62.4#


99 0.0 47.8 71.8#

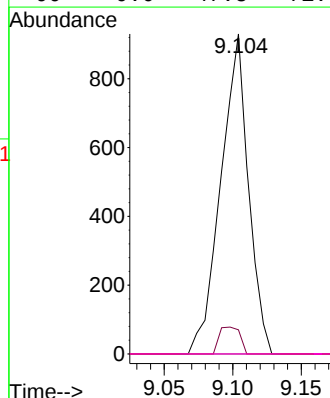






#62
4-Bromofluorobenzene
Concen: 51.481 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL







Tgt Ion: 95 Resp: 104219
Ion Ratio Lower Upper
95 100
174 98.2 0.0 135.6
176 95.0 0.0 131.0

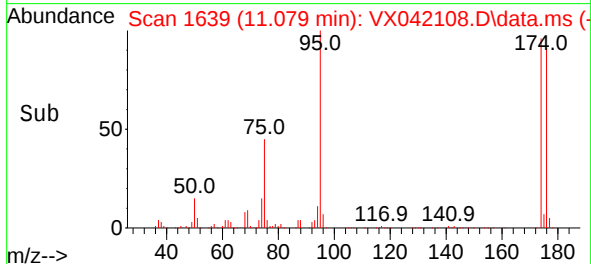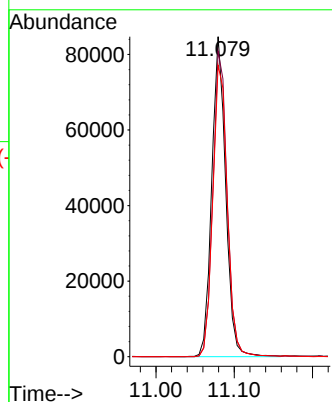

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Tgt Ion: 117 Resp: 224889
Ion Ratio Lower Upper
117 100
82 50.8 46.2 69.4
119 33.5 25.5 38.3


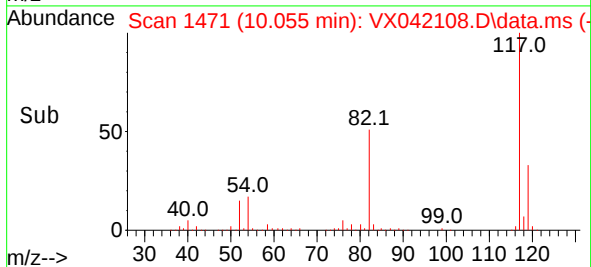






#67
Ethyl Benzene
Concen: 48.125 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49




Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL


Tgt Ion: 91 Resp: 352744
Ion Ratio Lower Upper
91 100
106 32.5 24.9 37.3

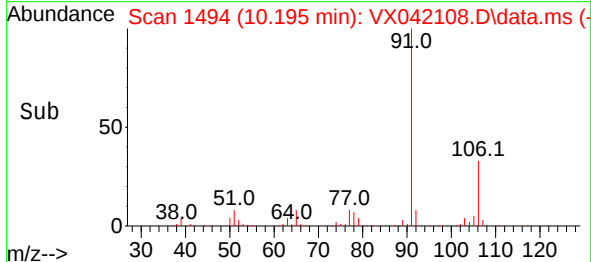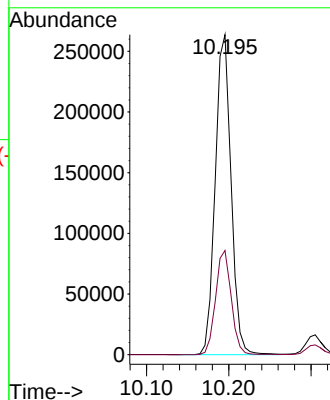

#68
m/p-Xylenes
Concen: 4.005 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Tgt Ion: 106 Resp: 11849
Ion Ratio Lower Upper
106 100
91 196.4 165.5 248.3



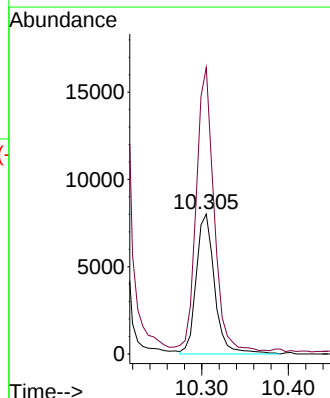





#69
o-Xylene
Concen: 3.510 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49




Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL


Tgt Ion:106 Resp: 10282
Ion Ratio Lower Upper
106 100
91 207.6 108.9 326.8

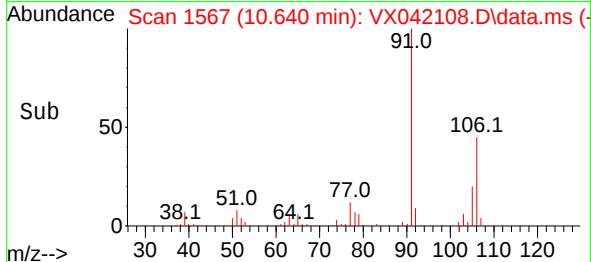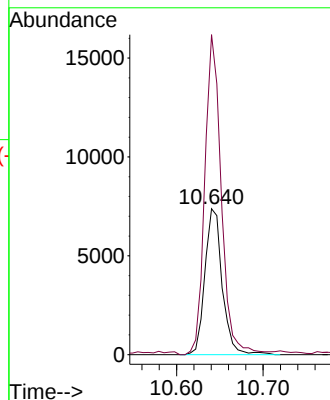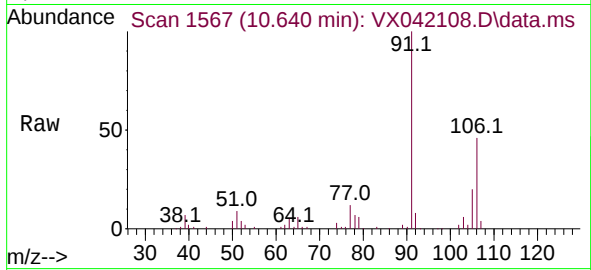

#70
Styrene
Concen: 0.210 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. -0.012 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Tgt Ion:104 Resp: 1032
Ion Ratio Lower Upper
104 100
78 166.6 43.6 65.4#
103 155.6 43.6 65.4#

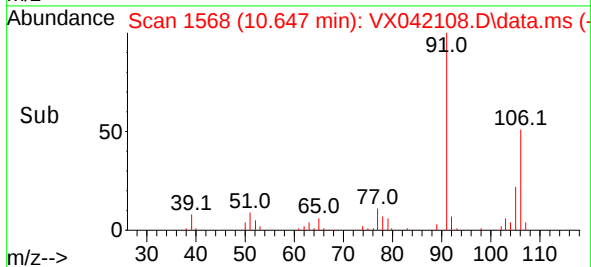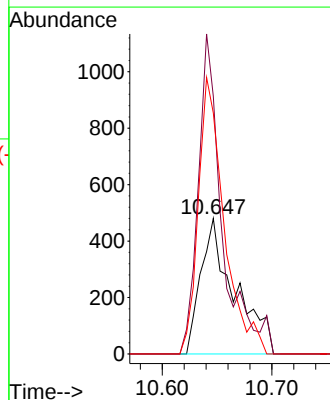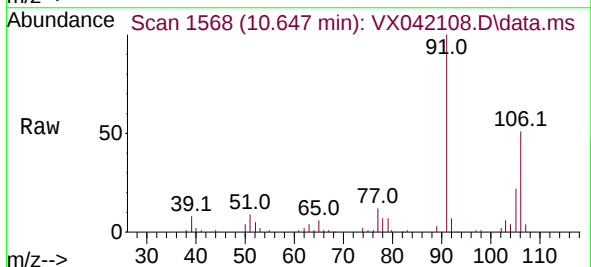



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :

MW12-20240625DL


Tgt Ion:152 Resp: 121303

Ion Ratio Lower Upper




152 100

115 54.4 43.3 129.9

150 158.7 0.0 345.0

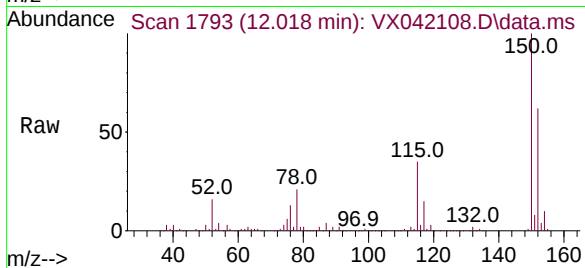

Abundance

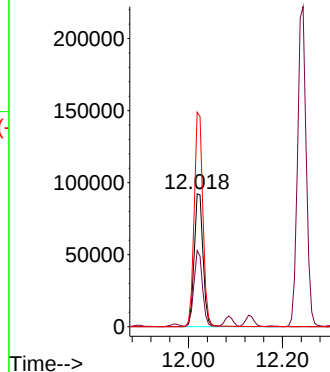

#73

Isopropylbenzene

Concen: 16.253 ug/l

RT: 10.964 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX042108.D


Acq: 01 Jul 2024 12:49

Tgt Ion:105 Resp: 119878



Ion Ratio Lower Upper


105 100

120 27.4 12.9 38.6

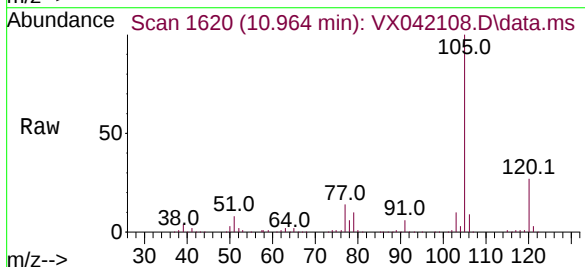

Abundance

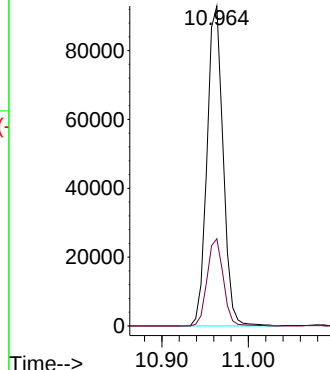



#76

1,2,3-Trichloropropane

Concen: 21.406 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :





MW12-20240625DL

Tgt Ion: 75 Resp: 47140

Ion Ratio Lower Upper

75 100

77 1.6 19.1 57.5#

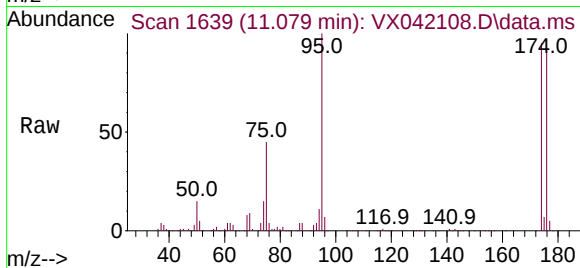

#78

n-propylbenzene

Concen: 16.530 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX042108.D




Acq: 01 Jul 2024 12:49


Tgt Ion: 91 Resp: 132286

Ion Ratio Lower Upper

91 100

120 24.4 11.5 34.4

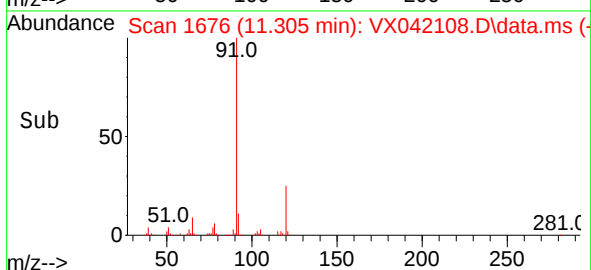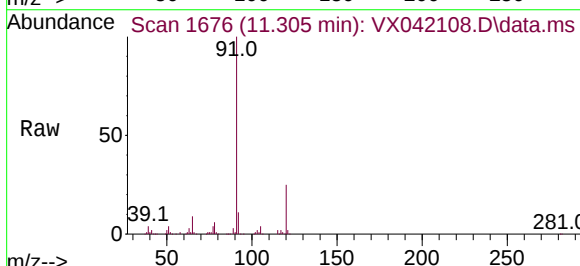



#79

2-Chlorotoluene

Concen: 1.355 ug/l

RT: 11.396 min Scan# 1

Delta R.T. 0.031 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :





MW12-20240625DL

Tgt Ion: 91 Resp: 6985

Ion Ratio Lower Upper

91 100

126 3.3 16.3 48.8#

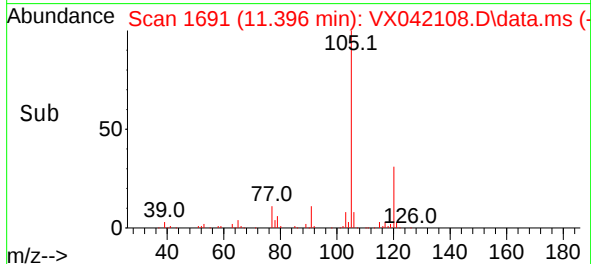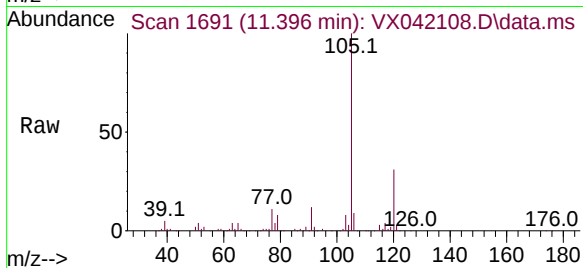

#80

1,3,5-Trimethylbenzene

Concen: 7.315 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX042108.D




Acq: 01 Jul 2024 12:49


Tgt Ion:105 Resp: 44939

Ion Ratio Lower Upper

105 100

120 52.4 24.1 72.3



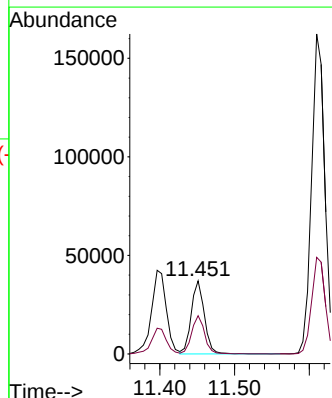
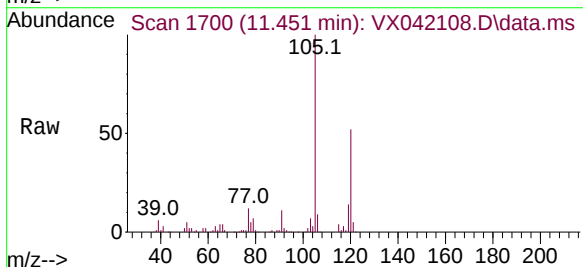




#81
trans-1,4-Dichloro-2-butene
Concen: 60.792 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49




Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL


Tgt Ion: 75 Resp: 47140
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

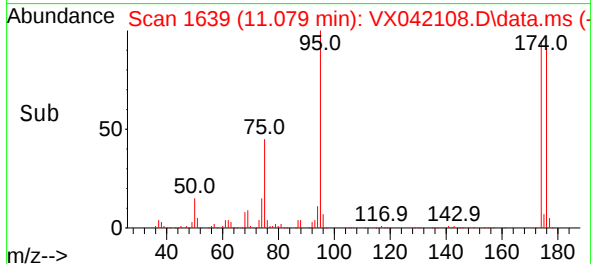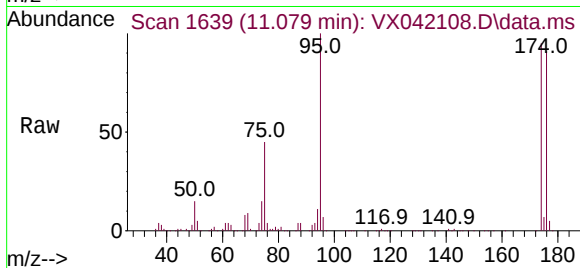

#82
4-Chlorotoluene
Concen: 0.872 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Tgt Ion: 91 Resp: 4968
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6#

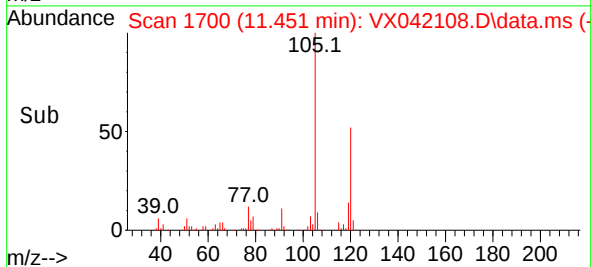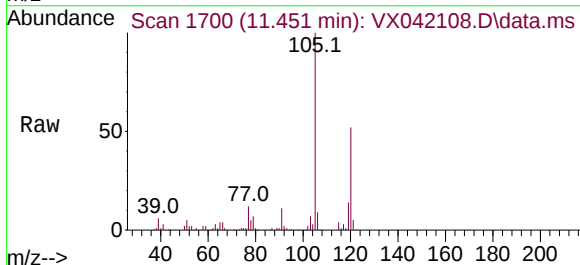



#83

tert-Butylbenzene

Concen: 6.843 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.037 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :

MW12-20240625DL





Tgt Ion:119 Resp: 46125

Ion Ratio Lower Upper

119 100

91 79.3 31.2 93.6

134 0.0 11.7 35.0#

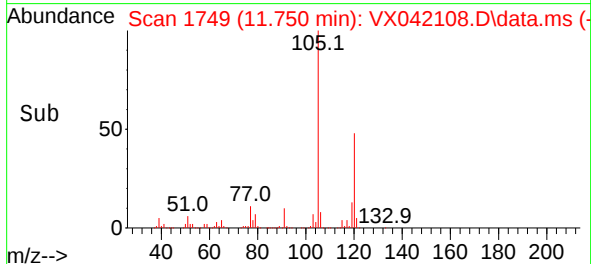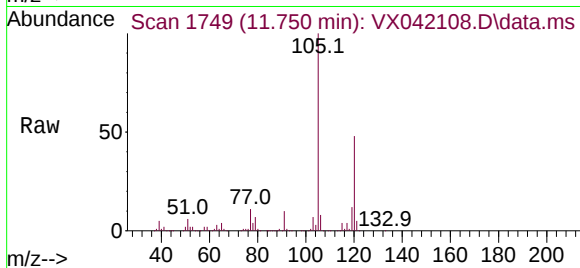

#84

1,2,4-Trimethylbenzene

Concen: 57.964 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.000 min

Lab File: VX042108.D




Acq: 01 Jul 2024 12:49


Tgt Ion:105 Resp: 357259

Ion Ratio Lower Upper

105 100

120 47.9 21.2 63.6

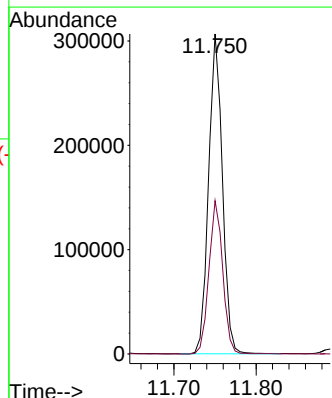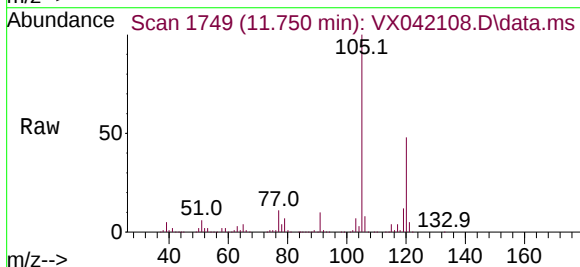



#85

sec-Butylbenzene

Concen: 46.856 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :





MW12-20240625DL

Tgt Ion:105 Resp: 357259

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.4#

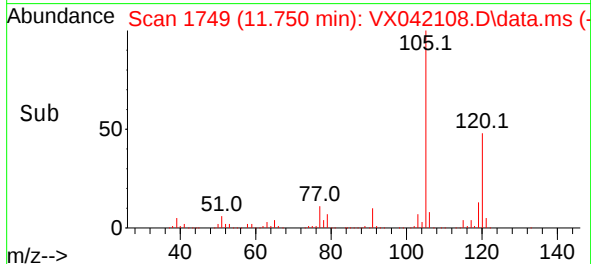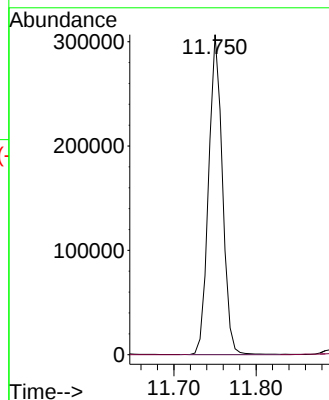

#86

p-Isopropyltoluene

Concen: 4.464 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. -0.036 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49




Tgt Ion:119 Resp: 29732


Ion Ratio Lower Upper

119 100

134 28.3 12.8 38.3

91 21.0 13.1 39.3

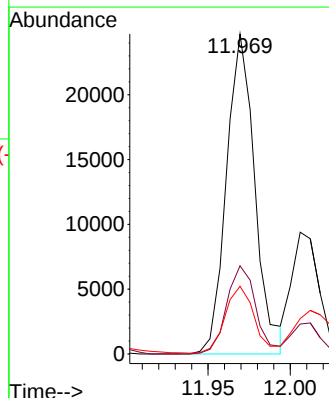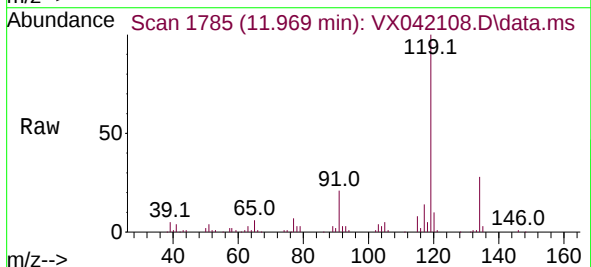



#89

n-Butylbenzene

Concen: 2.696 ug/l

RT: 12.317 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX042108.D

Acq: 01 Jul 2024 12:49

Instrument :

MSVOA_X

ClientSampleId :

MW12-20240625DL





Tgt Ion: 91 Resp: 13820

Ion Ratio Lower Upper

91 100

92 36.0 27.4 82.0

134 131.5 12.6 37.8#

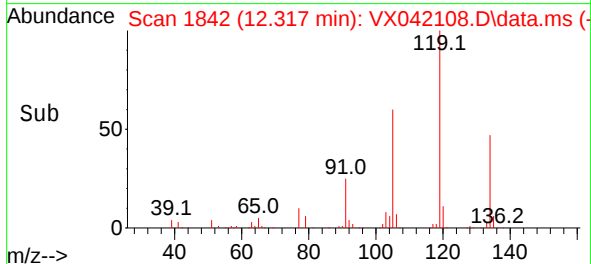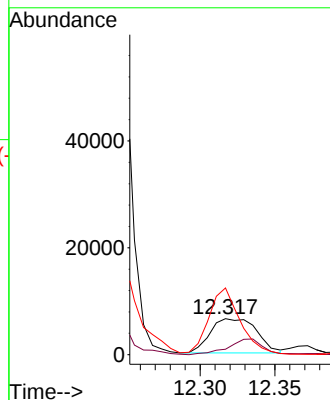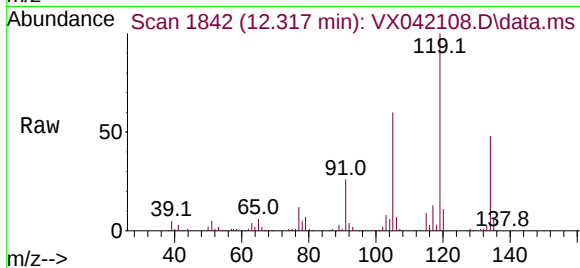

#90

Hexachloroethane

Concen: 286.780 ug/l

RT: 12.695 min Scan# 1904

Delta R.T. 0.159 min

Lab File: VX042108.D




Acq: 01 Jul 2024 12:49


Tgt Ion:117 Resp: 325189

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#



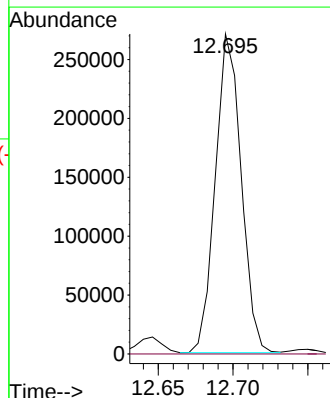
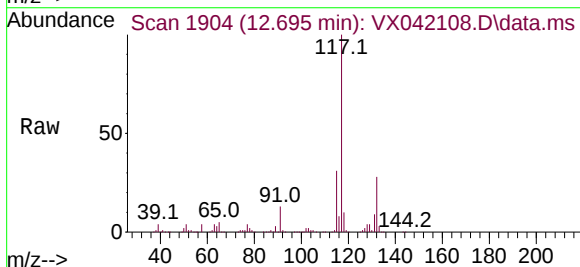


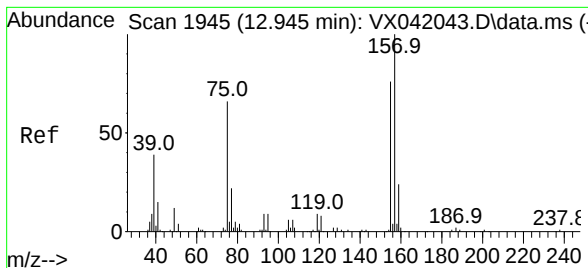

#92
1,2-Dibromo-3-Chloropropane
Concen: 1.391 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.018 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Instrument :
MSVOA_X
ClientSampleId :
MW12-20240625DL

Tgt Ion: 75 Resp: 756
Ion Ratio Lower Upper
75 100
155 0.0 36.1 108.5#
157 0.0 44.9 134.7#

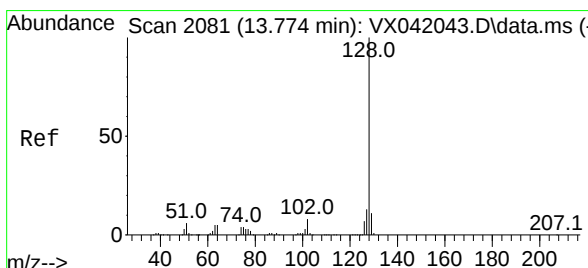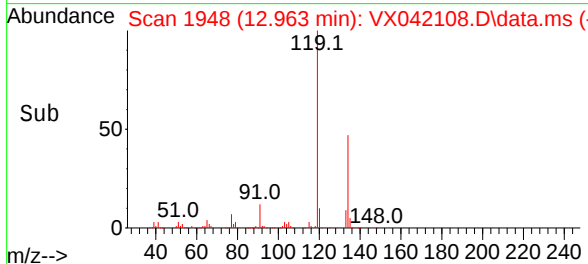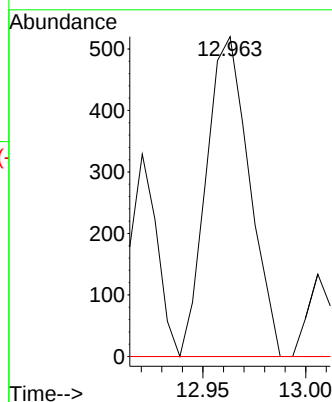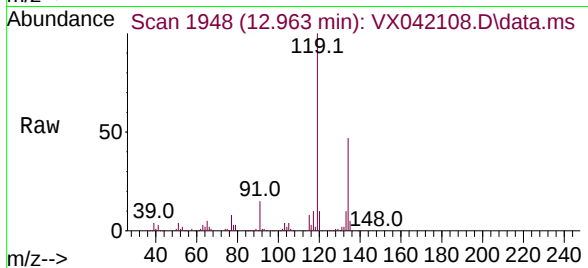

#95
Naphthalene
Concen: 281.813 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX042108.D
Acq: 01 Jul 2024 12:49

Tgt Ion:128 Resp: 2481514
Ion Ratio Lower Upper
128 100
127 13.5 10.3 15.5
129 11.7 8.8 13.2

