

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070124\
 Data File : VX042121.D
 Acq On : 01 Jul 2024 17:52
 Operator : JC/MD
 Sample : P3135-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OK-628-COMP-02

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Title : SW846 8260

Signal : TIC: VX042121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	34	rBV	131038	144670	7.54%	1.370%
2	2.386	207	213	230	rBV	39342	69051	3.60%	0.654%
3	2.788	273	279	294	rVB	13722	28763	1.50%	0.272%
4	3.581	401	409	424	rBV	21400	53040	2.76%	0.502%
5	5.385	694	705	721	rBV2	78688	233116	12.15%	2.208%
6	5.550	721	732	749	rVV	130262	367788	19.17%	3.483%
7	5.958	787	799	819	rBV	75092	203816	10.62%	1.930%
8	6.348	853	863	885	rBV	71918	192481	10.03%	1.823%
9	6.763	921	931	945	rBV	196994	482207	25.13%	4.567%
10	7.641	1066	1075	1081	rBV	41393	82570	4.30%	0.782%
11	7.696	1081	1084	1094	rVV	15540	29012	1.51%	0.275%
12	7.799	1094	1101	1123	rVV	1108591	1919041	100.00%	18.174%
13	8.549	1217	1224	1234	rBV	220863	359248	18.72%	3.402%
14	8.647	1234	1240	1251	rBV	432806	682858	35.58%	6.467%
15	8.958	1284	1291	1308	rBV	298465	454970	23.71%	4.309%
16	9.244	1331	1338	1345	rBV	314600	439694	22.91%	4.164%
17	9.311	1345	1349	1351	rVV	29217	42068	2.19%	0.398%
18	9.342	1351	1354	1356	rVV	48253	66077	3.44%	0.626%
19	9.378	1356	1360	1369	rVV	123527	192921	10.05%	1.827%
20	9.482	1372	1377	1384	rVV	586126	769112	40.08%	7.284%
21	9.580	1388	1393	1412	rVB	407127	527734	27.50%	4.998%
22	9.915	1442	1448	1464	rBV	1018852	1300043	67.74%	12.312%
23	10.055	1464	1471	1478	rBV	452472	652149	33.98%	6.176%
24	10.281	1504	1508	1517	rBV2	12541	20984	1.09%	0.199%
25	10.506	1541	1545	1555	rBV	13075	19985	1.04%	0.189%
26	10.640	1562	1567	1579	rBV	84012	109910	5.73%	1.041%
27	11.079	1634	1639	1652	rBV	387457	508668	26.51%	4.817%
28	12.024	1788	1794	1810	rBV	454328	607204	31.64%	5.750%


Sum of corrected areas: 10559180

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070124\
Data File : VX042121.D
Acq On : 01 Jul 2024 17:52
Operator : JC/MD
Sample : P3135-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OK-628-COMP-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

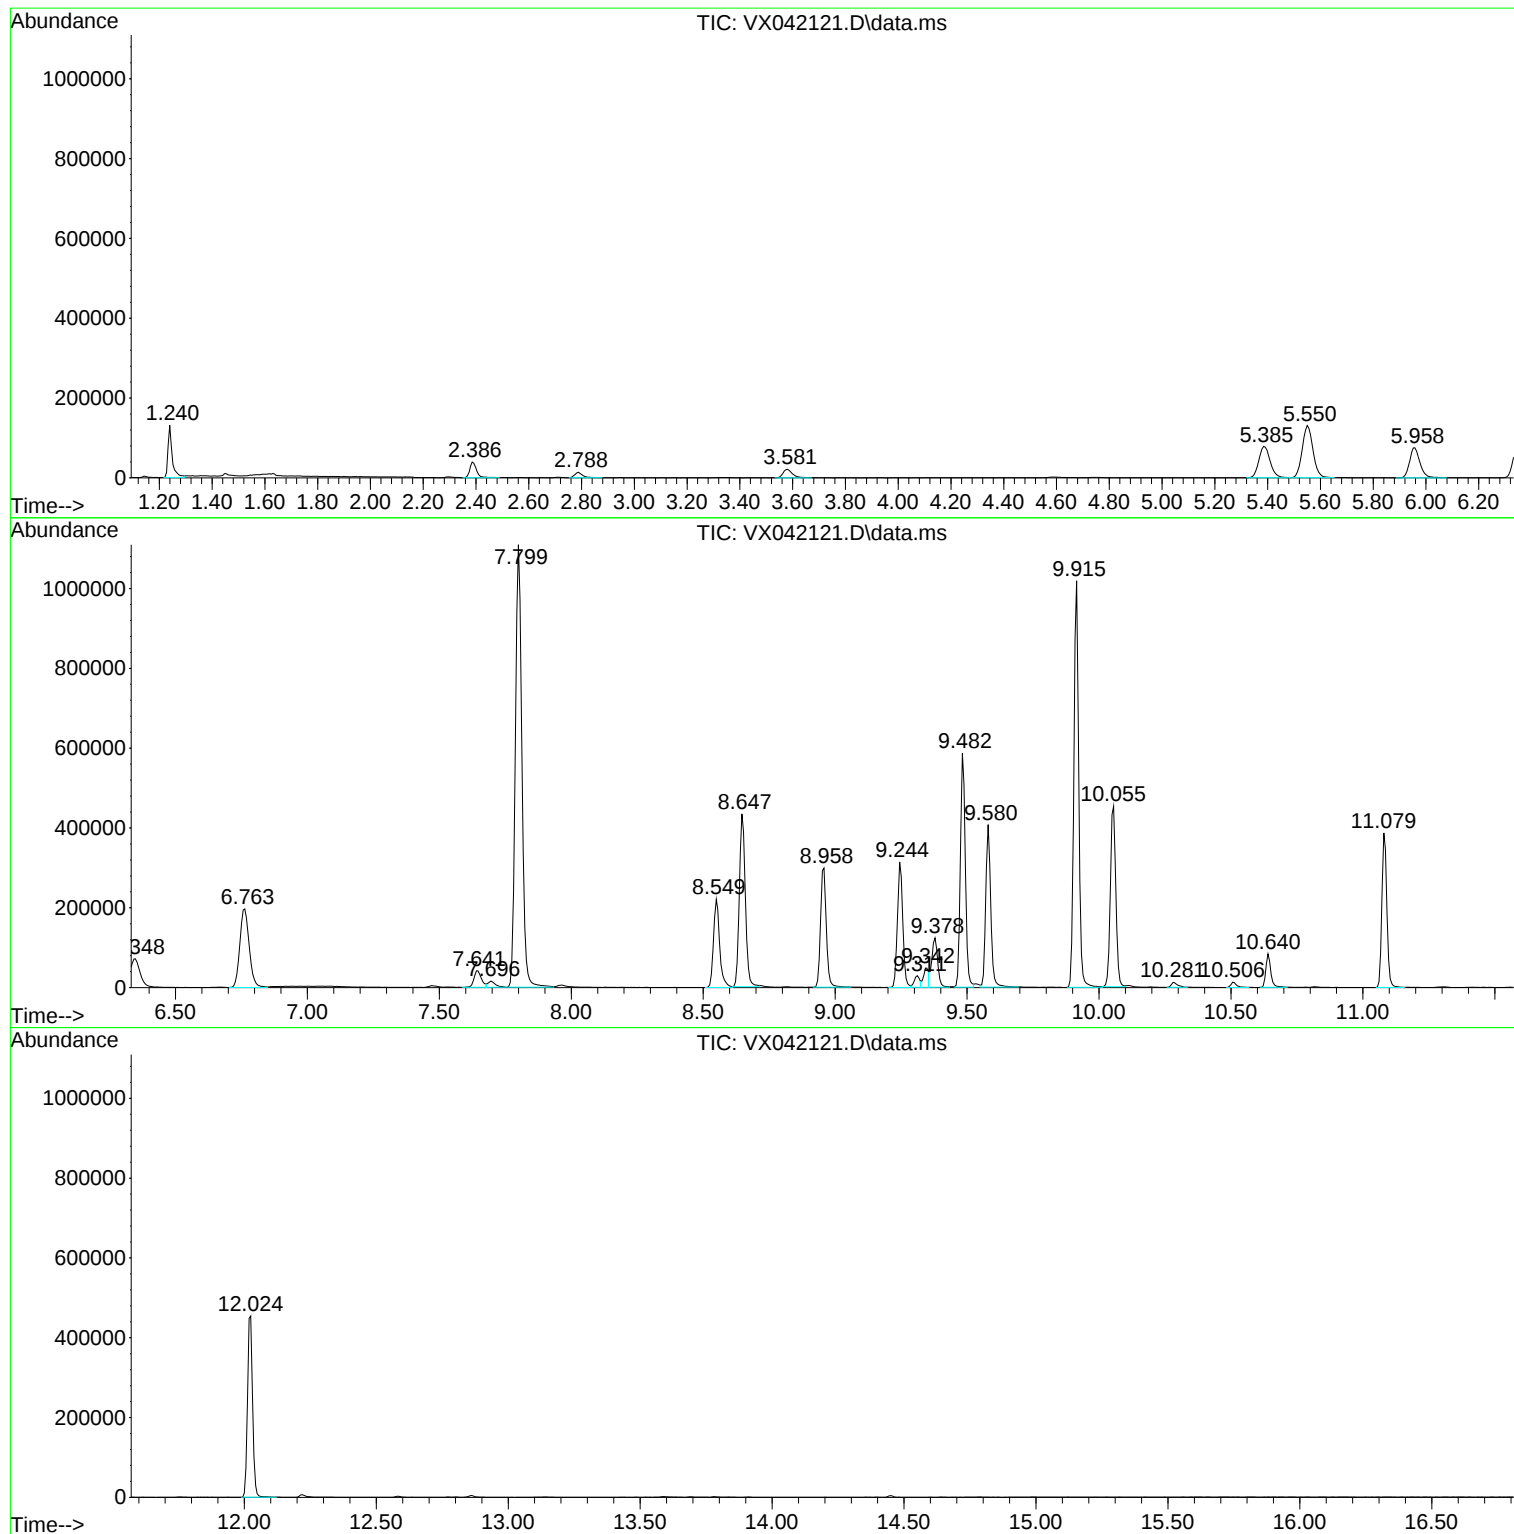

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070124\
Data File : VX042121.D
Acq On : 01 Jul 2024 17:52
Operator : JC/MD
Sample : P3135-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OK-628-COMP-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070124\
Data File : VX042121.D
Acq On : 01 Jul 2024 17:52
Operator : JC/MD
Sample : P3135-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OK-628-COMP-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc