


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX070218\
 Data File : VX003119.D
 Acq On : 02 Jul 2018 09:30
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260
 Last Update : Mon Jun 25 14:38:05 2018

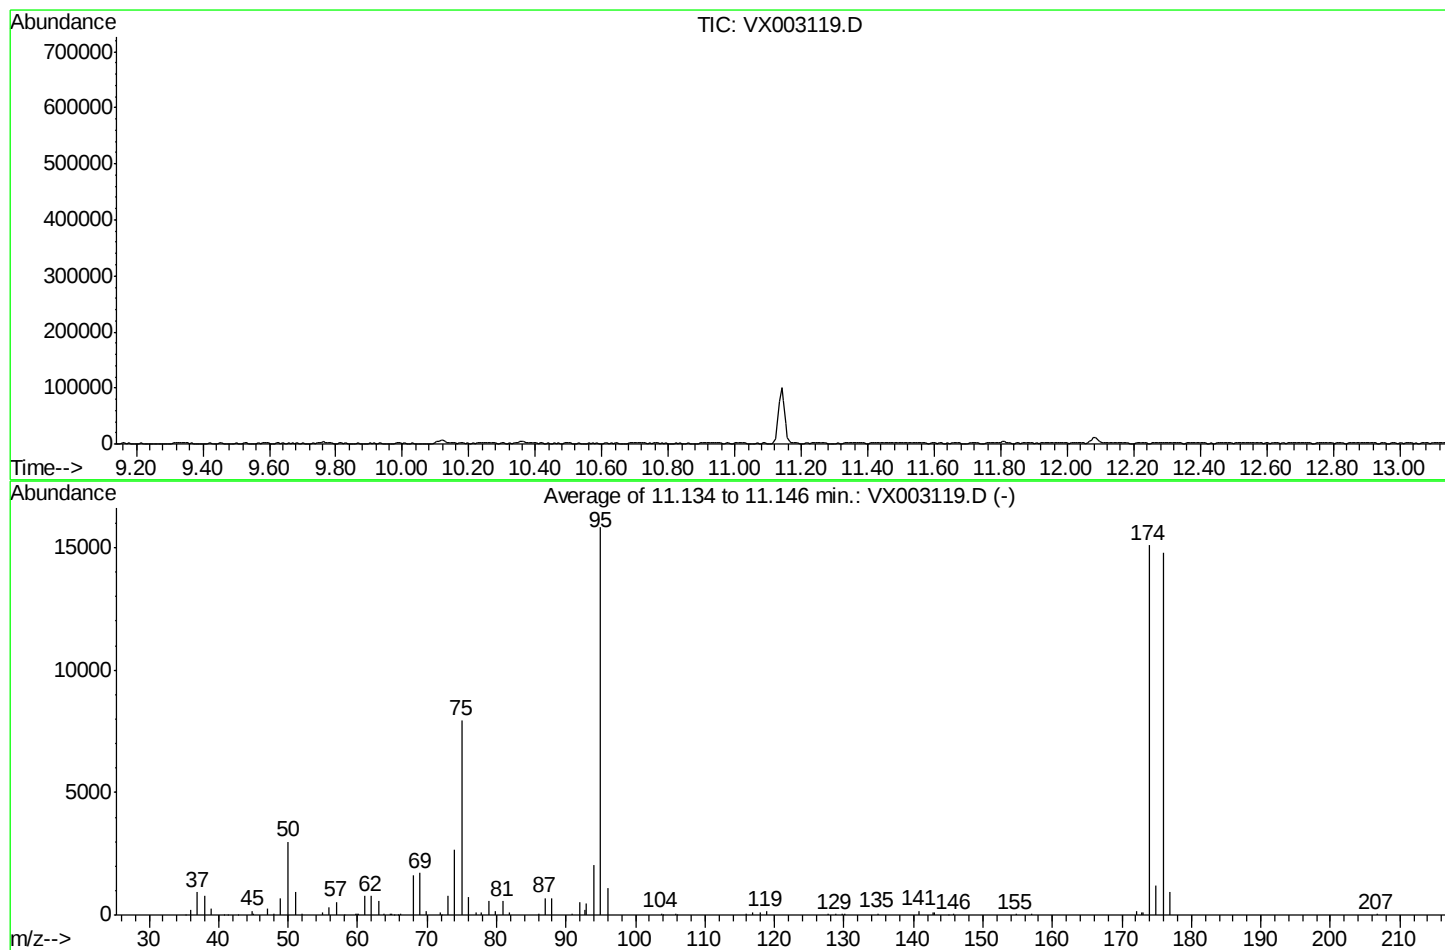

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	2999	PASS
75	95	30	60	50.1	7936	PASS
95	95	100	100	100.0	15831	PASS
96	95	5	9	6.9	1087	PASS
173	174	0.00	2	0.7	103	PASS
174	95	50	100	95.4	15100	PASS
175	174	5	9	8.0	1210	PASS
176	174	95	101	97.9	14778	PASS
177	176	5	9	6.5	963	PASS