

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX070219\  
Data File : VX010624.D  
Acq On : 02 Jul 2019 17:57  
Operator : JC/SP  
Sample : K3636-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SP19-MMW0002

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.276       | 16            | 20          | 31           | rBV      | 118701         | 150749        | 13.43%          | 2.485%        |
| 2         | 5.500       | 702           | 713         | 726          | rBV2     | 135274         | 384761        | 34.28%          | 6.343%        |
| 3         | 5.665       | 728           | 740         | 753          | rVB      | 228087         | 644176        | 57.39%          | 10.619%       |
| 4         | 6.061       | 793           | 805         | 818          | rBV      | 131051         | 342907        | 30.55%          | 5.653%        |
| 5         | 6.860       | 924           | 936         | 948          | rBV      | 340035         | 806839        | 71.88%          | 13.301%       |
| 6         | 8.713       | 1232          | 1240        | 1255         | rBV      | 736023         | 1122526       | 100.00%         | 18.505%       |
| 7         | 10.109      | 1460          | 1469        | 1478         | rBV      | 711731         | 962905        | 85.78%          | 15.874%       |
| 8         | 11.134      | 1631          | 1637        | 1649         | rBV      | 592002         | 759047        | 67.62%          | 12.513%       |
| 9         | 12.079      | 1786          | 1792        | 1799         | rBV      | 679166         | 892162        | 79.48%          | 14.707%       |


Sum of corrected areas: 6066072

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX070219\  
Data File : VX010624.D  
Acq On : 02 Jul 2019 17:57  
Operator : JC/SP  
Sample : K3636-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SP19-MMW0002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

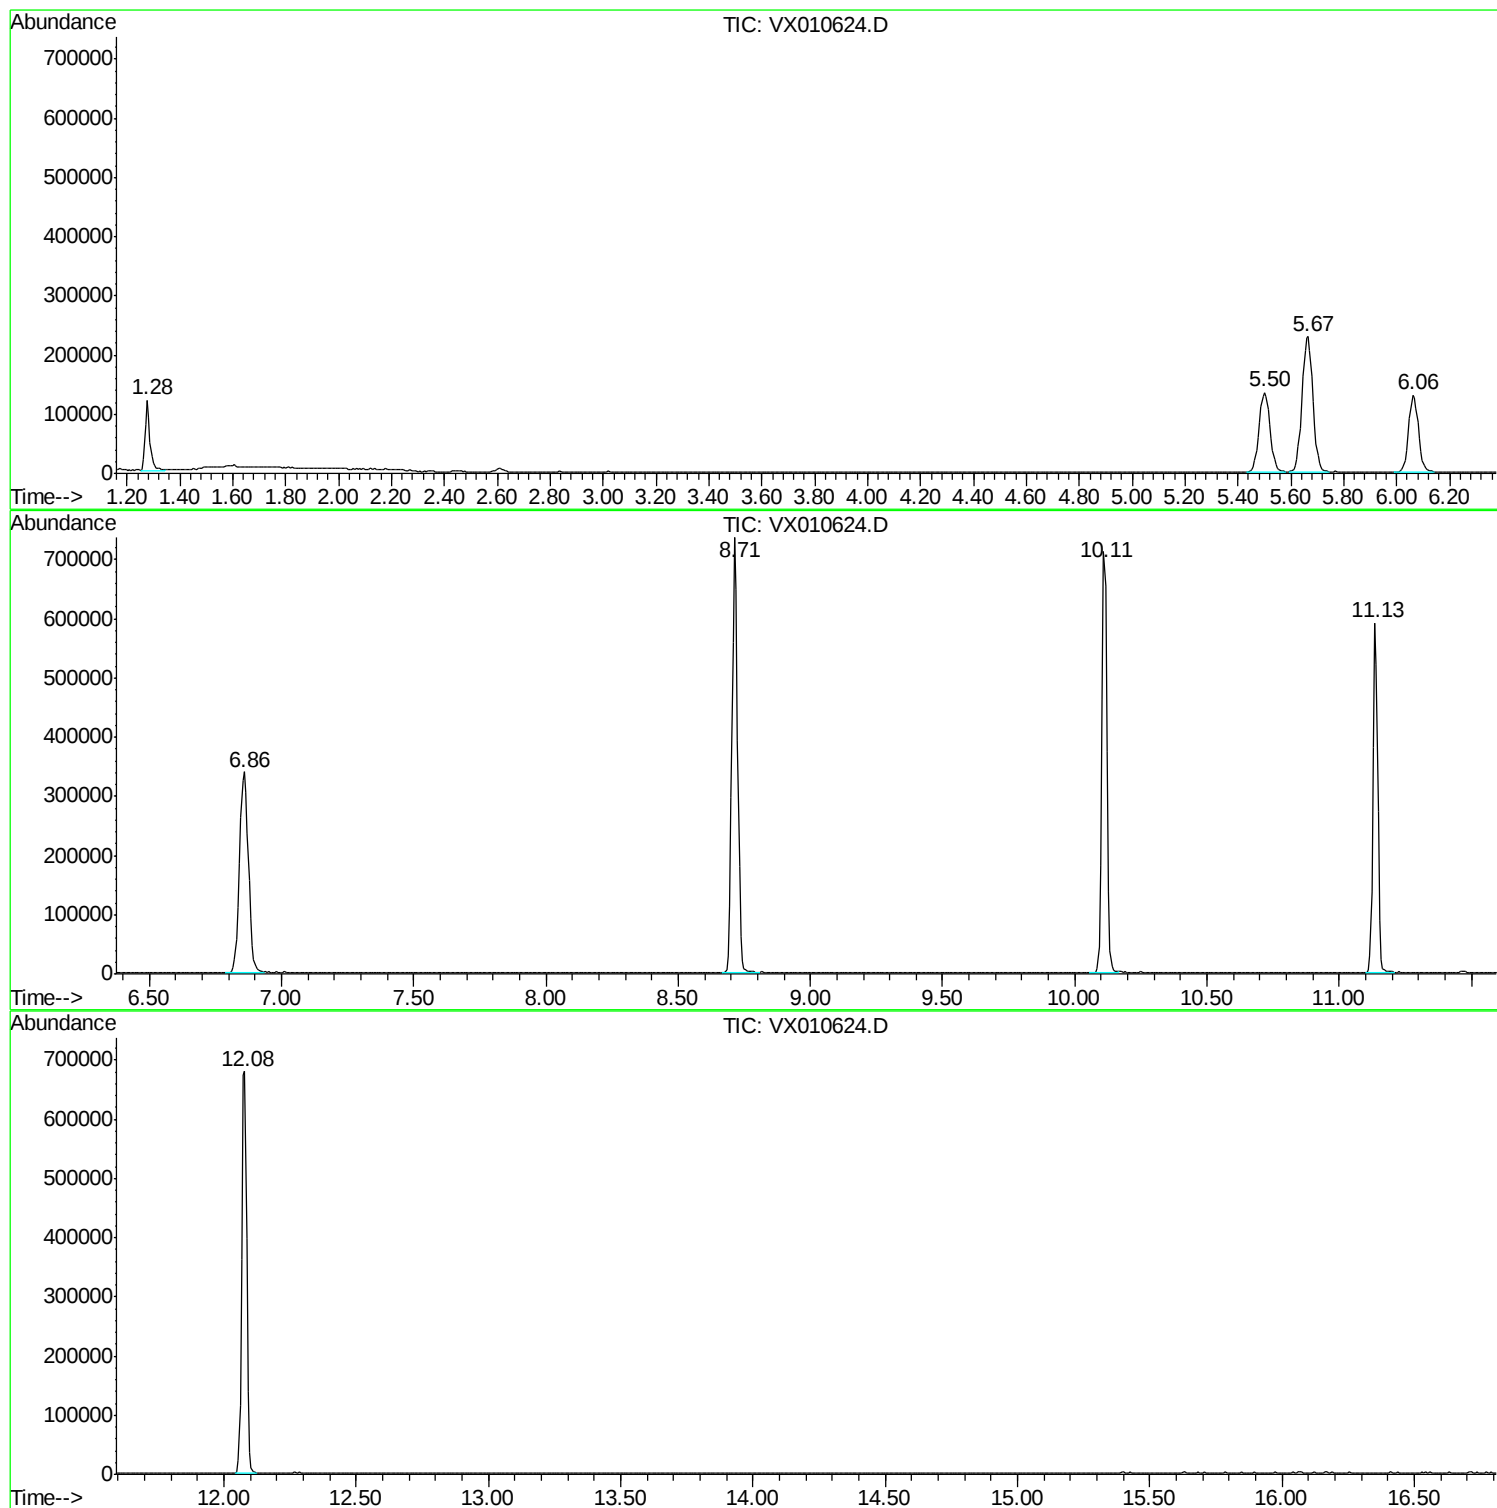

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX070219\  
Data File : VX010624.D  
Acq On : 02 Jul 2019 17:57  
Operator : JC/SP  
Sample : K3636-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SP19-MMW0002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX070219\  
Data File : VX010624.D  
Acq On : 02 Jul 2019 17:57  
Operator : JC/SP  
Sample : K3636-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SP19-MMW0002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X061919W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |