

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
 Data File : VX023126.D
 Acq On : 02 Jul 2021 22:37
 Operator : JC/MD
 Sample : M2907-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-063021

Quant Time: Jul 05 02:59:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 02 14:29:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	235457	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	387614	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	344226	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	141786	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	165324	52.243	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	104.480%
35) Dibromofluoromethane	5.397	113	122554	48.962	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.920%
50) Toluene-d8	8.653	98	457232	48.970	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.940%
62) 4-Bromofluorobenzene	11.085	95	161626	44.839	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.680%
Target Compounds						
16) Acetone	2.386	43	2611	2.085	ug/l	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023126.D
Acq On : 02 Jul 2021 22:37
Operator : JC/MD
Sample : M2907-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-063021

Quant Time: Jul 05 02:59:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 02 14:29:42 2021
Response via : Initial Calibration




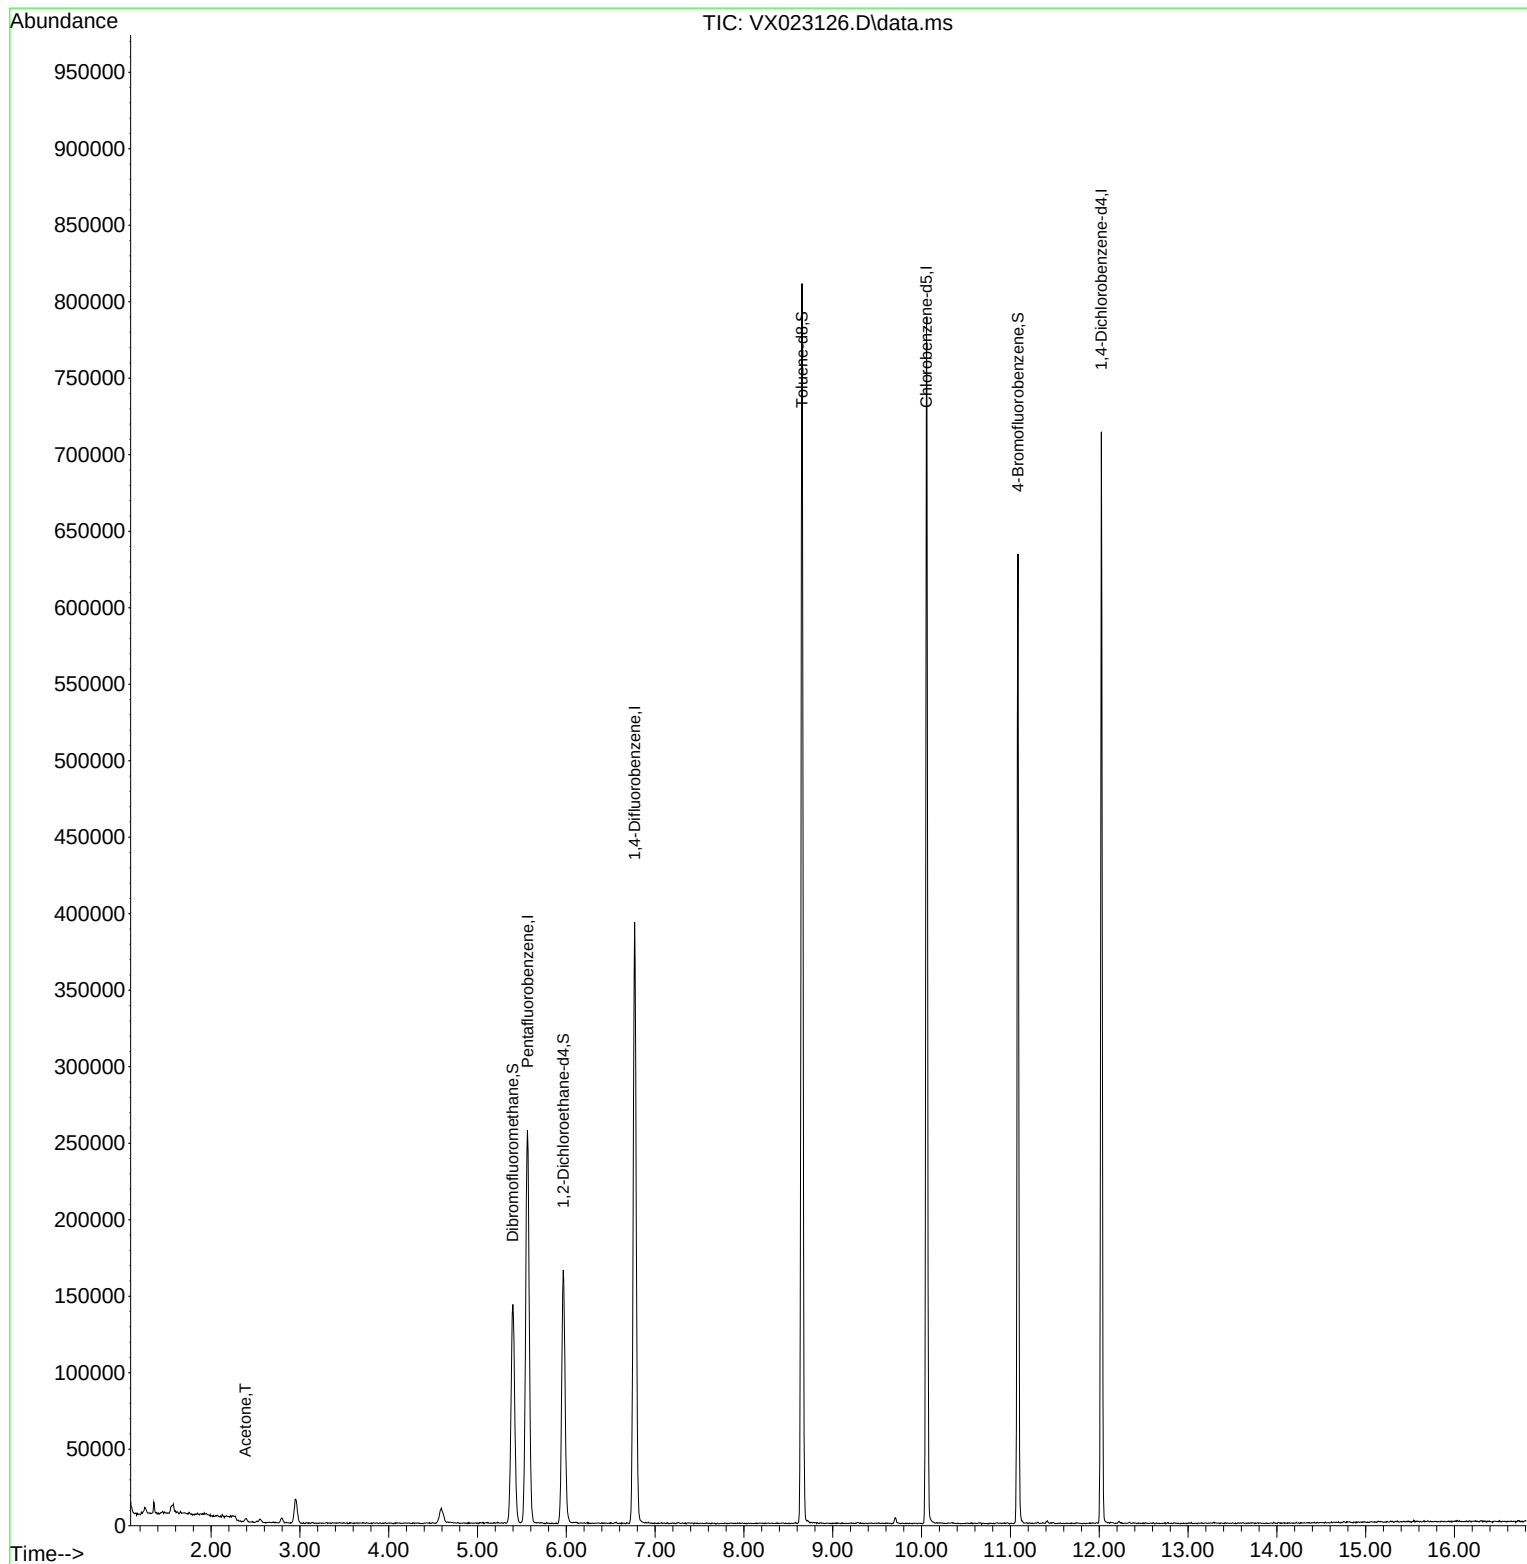


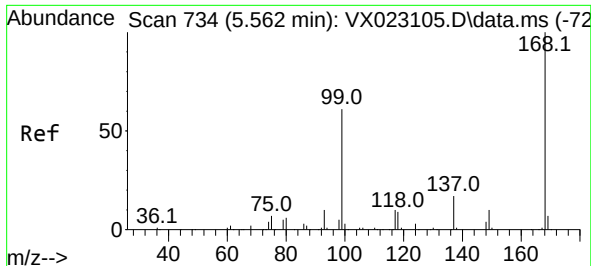

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX023126.D
Acq: 02 Jul 2021 22:37




Instrument :
MSVOA_X
ClientSampled :
TB-01-063021


Tgt Ion:168 Resp: 235457
Ion Ratio Lower Upper
168 100
99 59.7 45.8 68.6

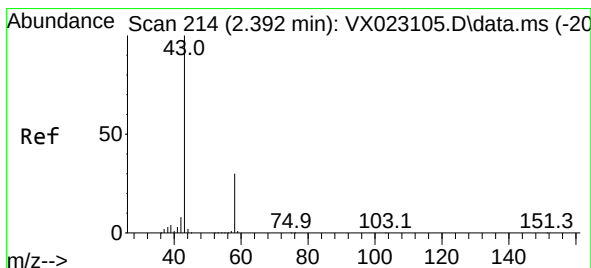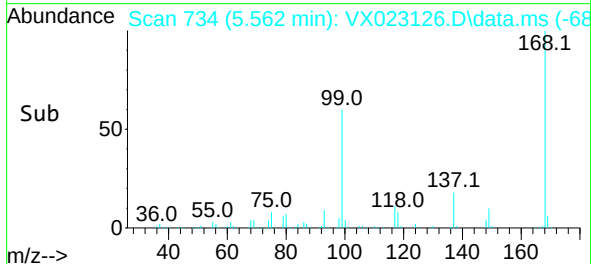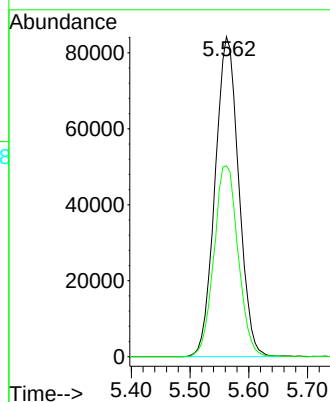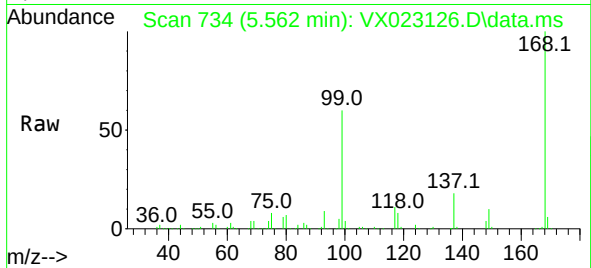

#16
Acetone
Concen: 2.085 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX023126.D
Acq: 02 Jul 2021 22:37

Tgt Ion: 43 Resp: 2611
Ion Ratio Lower Upper
43 100
58 29.9 27.8 41.8


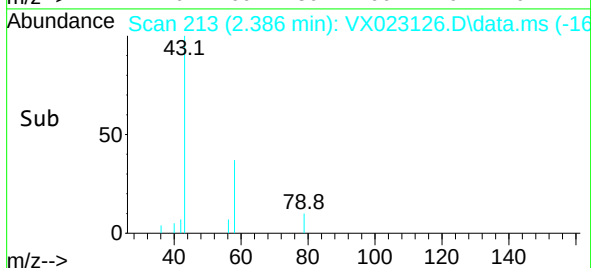
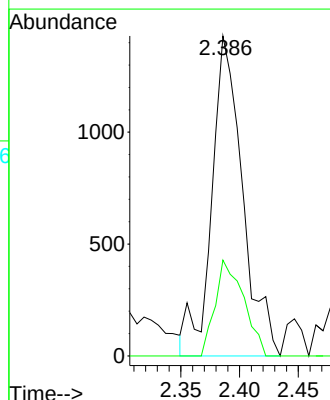
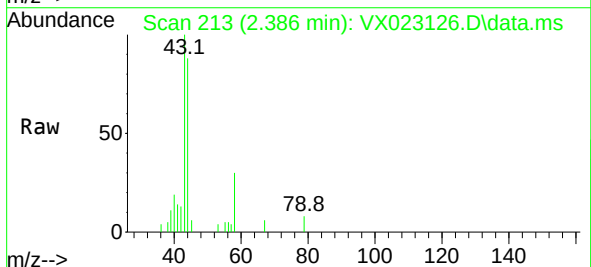


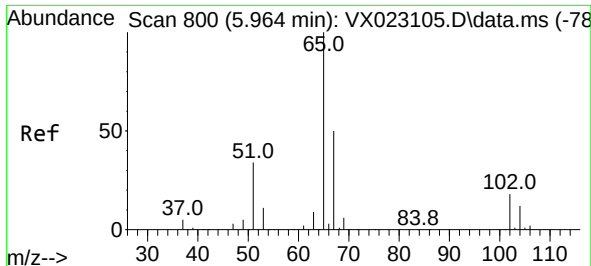

#33
1,2-Dichloroethane-d4
Concen: 52.243 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023126.D
Acq: 02 Jul 2021 22:37




Instrument :
MSVOA_X
ClientSampleId :
TB-01-063021


Tgt Ion: 65 Resp: 165324
Ion Ratio Lower Upper
65 100
67 51.1 0.0 105.4

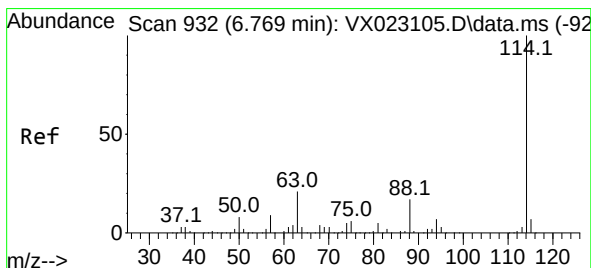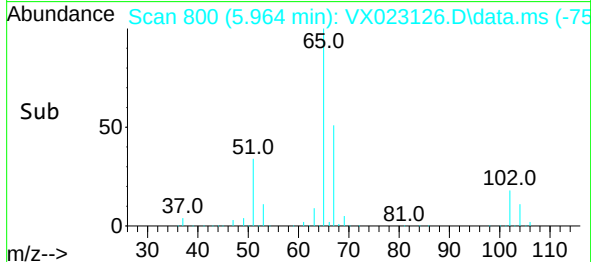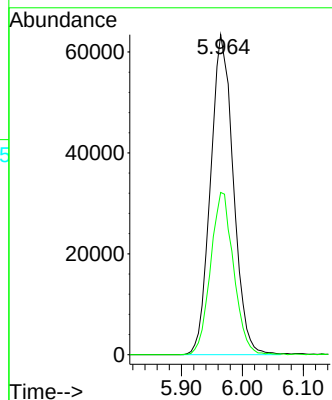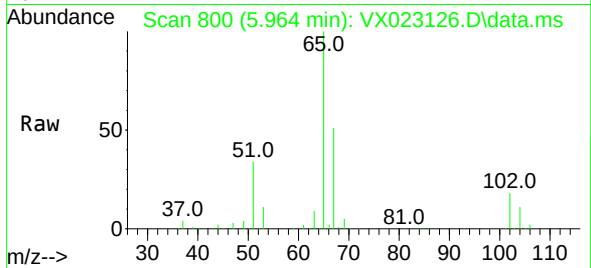

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023126.D
Acq: 02 Jul 2021 22:37

Tgt Ion: 114 Resp: 387614
Ion Ratio Lower Upper
114 100
63 20.1 0.0 40.8
88 15.2 0.0 32.8


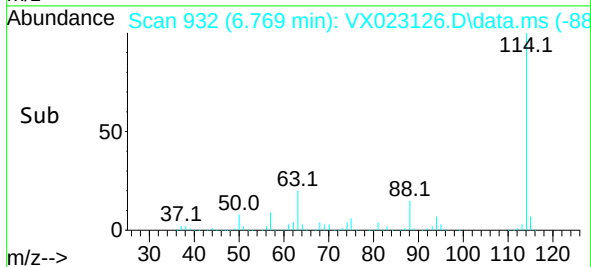
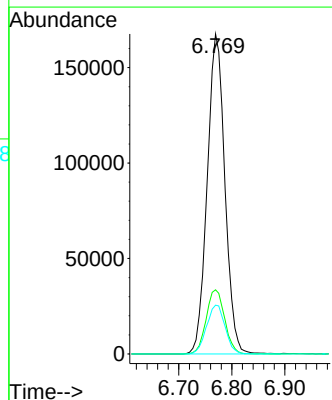
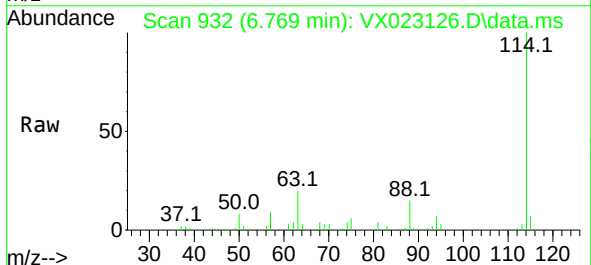


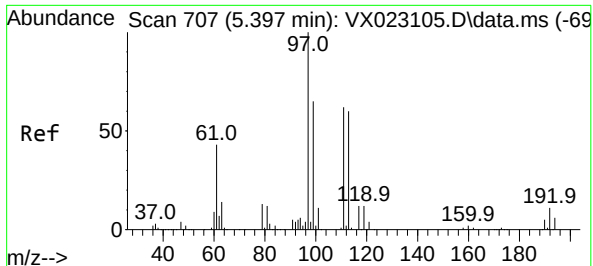

#35
Dibromofluoromethane
Concen: 48.962 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023126.D
Acq: 02 Jul 2021 22:37




Instrument :
MSVOA_X
ClientSampleId :
TB-01-063021


Tgt Ion:113 Resp: 122554
Ion Ratio Lower Upper
113 100
111 102.8 81.9 122.9
192 18.6 16.7 25.1

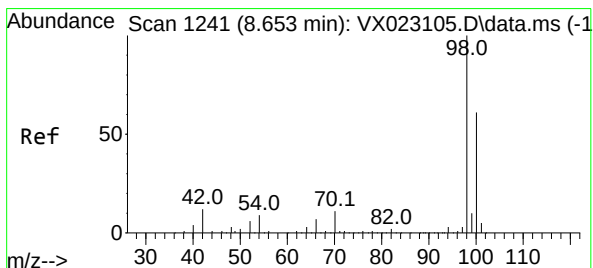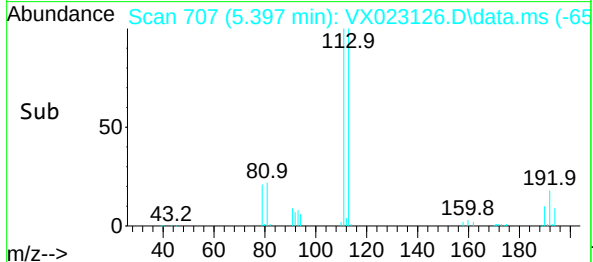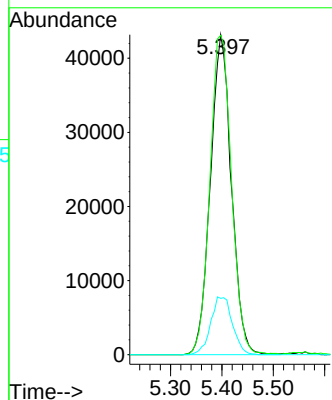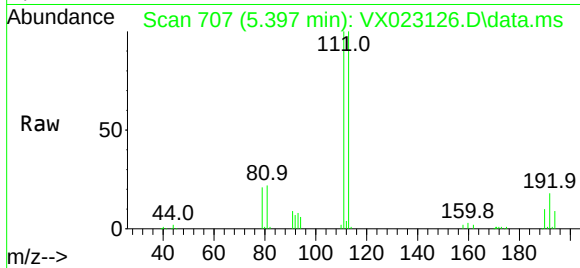

#50
Toluene-d8
Concen: 48.970 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023126.D
Acq: 02 Jul 2021 22:37

Tgt Ion: 98 Resp: 457232
Ion Ratio Lower Upper
98 100
100 64.0 51.9 77.9


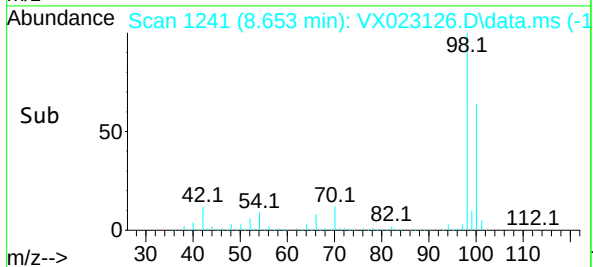
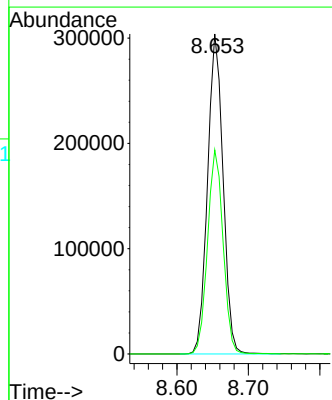
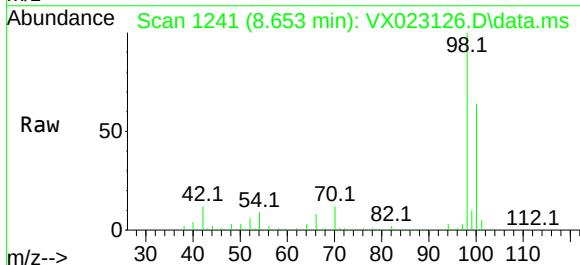


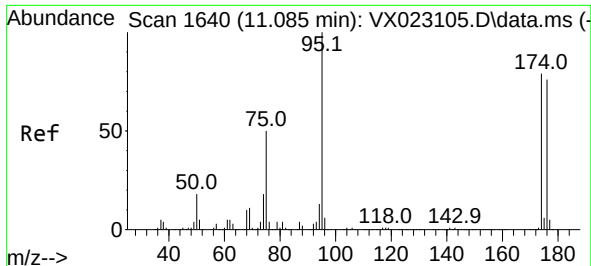

#62
4-Bromofluorobenzene
Concen: 44.839 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023126.D
Acq: 02 Jul 2021 22:37




Instrument :
MSVOA_X
ClientSampleId :
TB-01-063021


Tgt Ion: 95 Resp: 161626
Ion Ratio Lower Upper
95 100
174 76.2 0.0 154.6
176 74.3 0.0 155.8

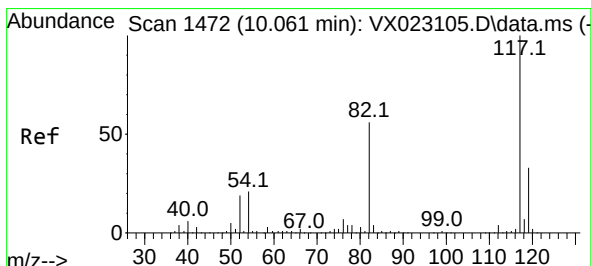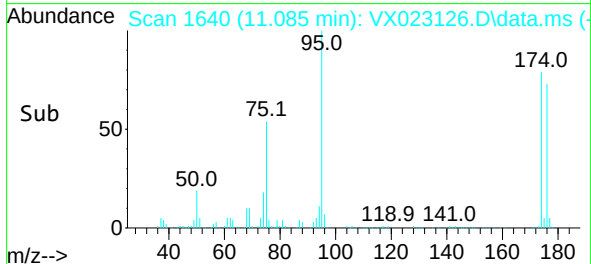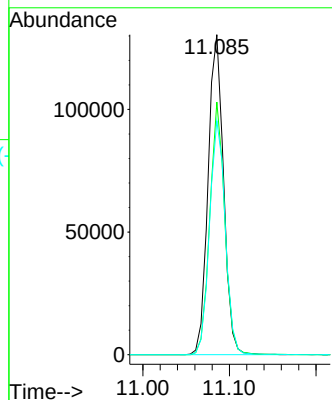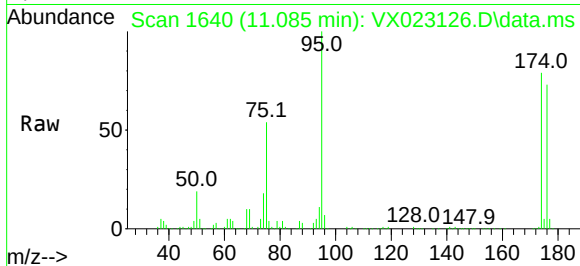

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023126.D
Acq: 02 Jul 2021 22:37

Tgt Ion: 117 Resp: 344226
Ion Ratio Lower Upper
117 100
82 58.6 47.4 71.2
119 32.1 26.6 39.8

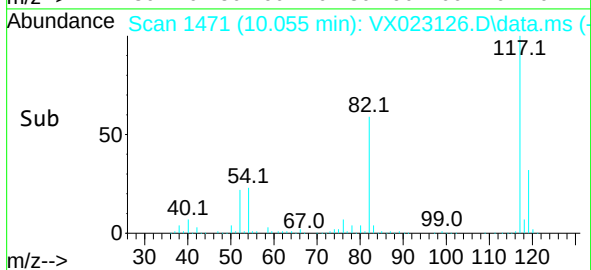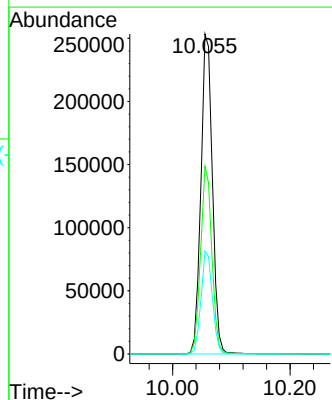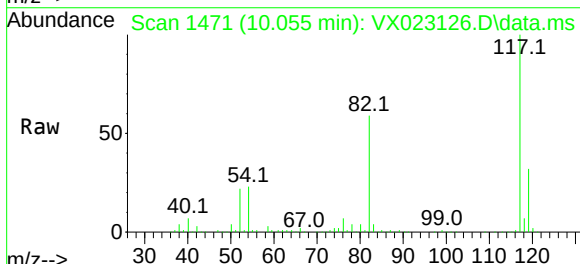

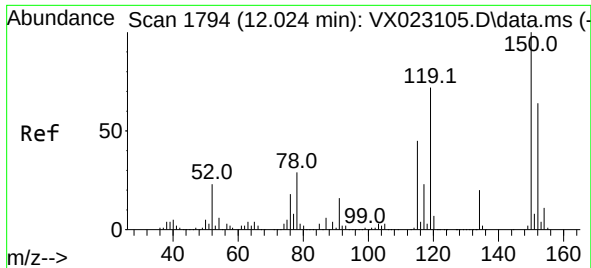

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: VX023126.D
 Acq: 02 Jul 2021 22:37

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-063021

Tgt Ion:152 Resp: 141786
 Ion Ratio Lower Upper
 152 100
 115 61.4 41.1 123.3
 150 157.1 0.0 349.0

