

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
 Data File : VX023120.D
 Acq On : 02 Jul 2021 20:16
 Operator : JC/MD
 Sample : M2924-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M

Title : SW846 8260

Signal : TIC: VX023120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rBV	56261	54650	4.47%	0.835%
2	1.569	72	79	84	rVB5	6085	13501	1.10%	0.206%
3	2.550	234	240	246	rVB	16261	27431	2.24%	0.419%
4	4.580	566	573	583	rBV3	6754	22028	1.80%	0.336%
5	5.397	692	707	723	rBV	143842	412104	33.67%	6.294%
6	5.562	723	734	748	rVV	250453	705854	57.68%	10.780%
7	5.964	789	800	815	rBV	161483	431362	35.25%	6.588%
8	6.769	922	932	948	rBV	383519	906537	74.07%	13.845%
9	8.653	1234	1241	1253	rBV	776216	1223816	100.00%	18.690%
10	10.055	1465	1471	1489	rBV	760356	1058391	86.48%	16.164%
11	11.085	1634	1640	1653	rBV	629163	798593	65.25%	12.196%
12	12.024	1789	1794	1805	rVB	721461	893621	73.02%	13.647%




Sum of corrected areas: 6547888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023120.D
Acq On : 02 Jul 2021 20:16
Operator : JC/MD
Sample : M2924-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

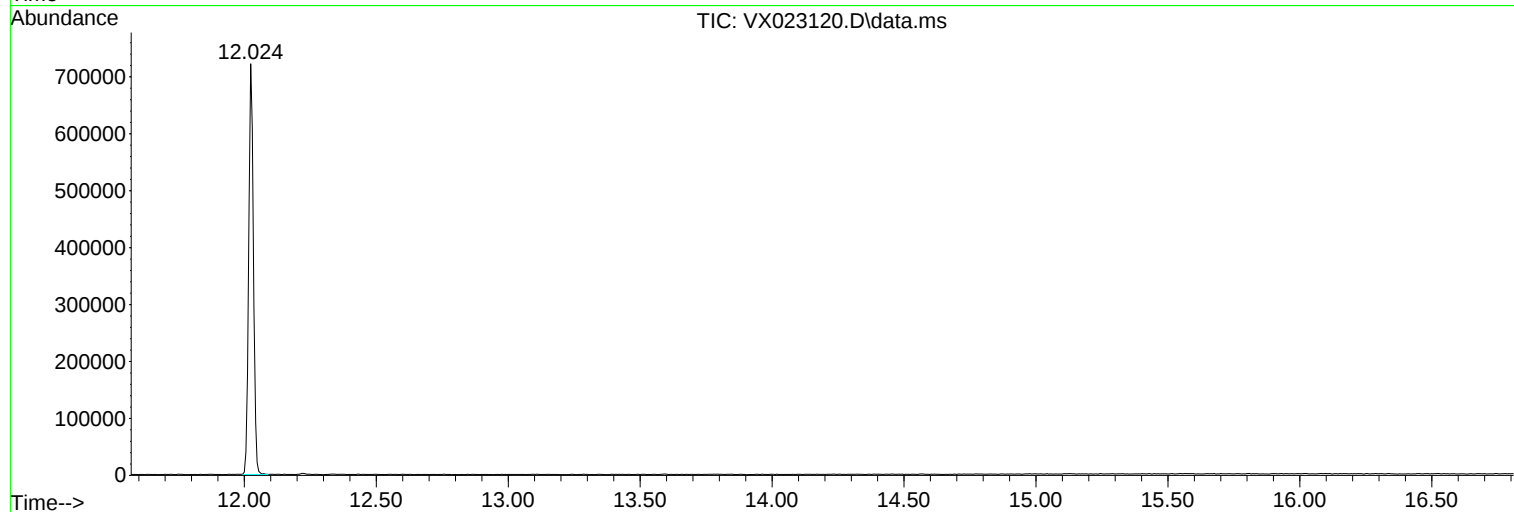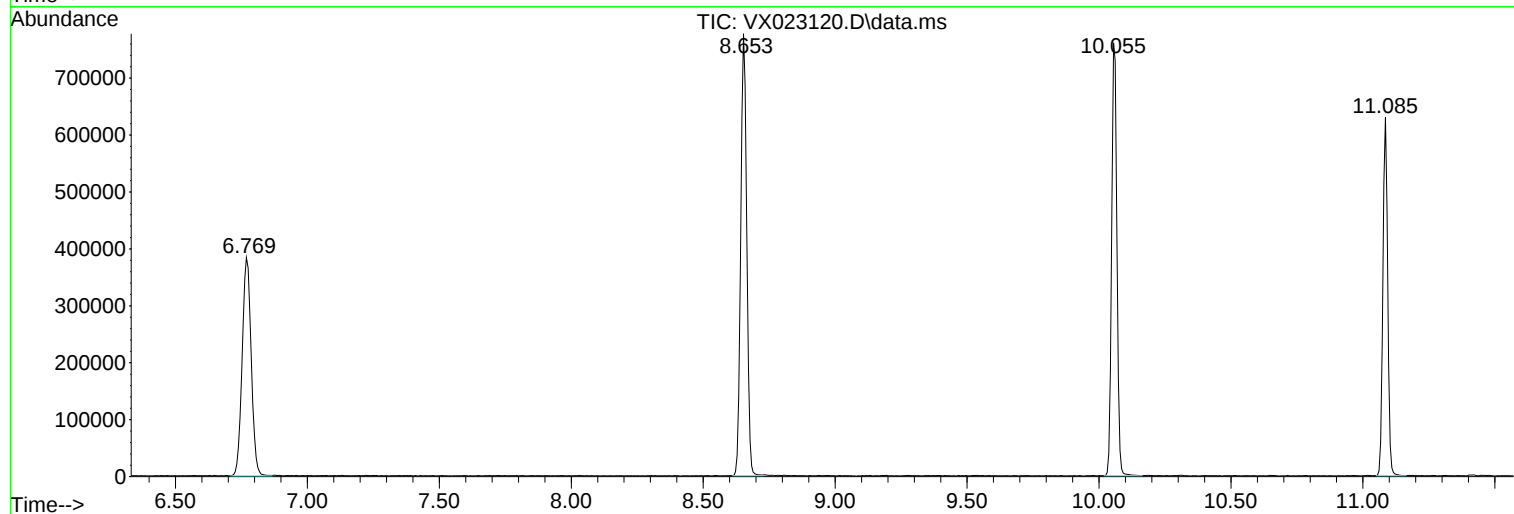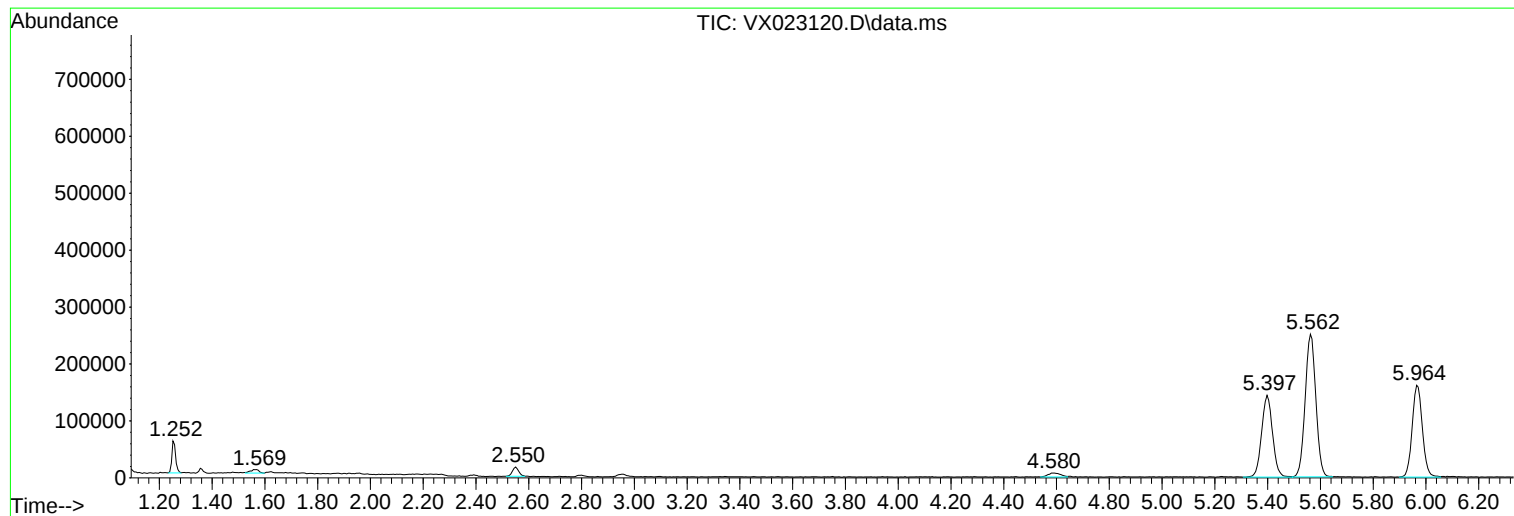

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023120.D
Acq On : 02 Jul 2021 20:16
Operator : JC/MD
Sample : M2924-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023120.D
Acq On : 02 Jul 2021 20:16
Operator : JC/MD
Sample : M2924-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
