

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
 Data File : VX023122.D
 Acq On : 02 Jul 2021 21:03
 Operator : JC/MD
 Sample : M2898-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-07-1.5-6.5-062921

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M

Title : SW846 8260

Signal : TIC: VX023122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	27	31	43	rBV2	70025	197474	15.30%	2.816%
2	2.550	231	240	245	rBV2	9858	24353	1.89%	0.347%
3	5.397	696	707	723	rBV	149097	434983	33.70%	6.202%
4	5.562	723	734	746	rBV	267579	743451	57.59%	10.601%
5	5.964	790	800	817	rBV	171694	455755	35.31%	6.498%
6	6.769	922	932	942	rBV2	408561	962452	74.56%	13.723%
7	8.653	1234	1241	1255	rVB	833982	1290845	100.00%	18.406%
8	10.055	1465	1471	1482	rBV	808890	1112064	86.15%	15.856%
9	11.085	1634	1640	1651	rBV	665855	837041	64.84%	11.935%
10	12.024	1788	1794	1802	rBV	757374	954901	73.97%	13.616%




Sum of corrected areas: 7013319

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023122.D
Acq On : 02 Jul 2021 21:03
Operator : JC/MD
Sample : M2898-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07-1.5-6.5-062921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

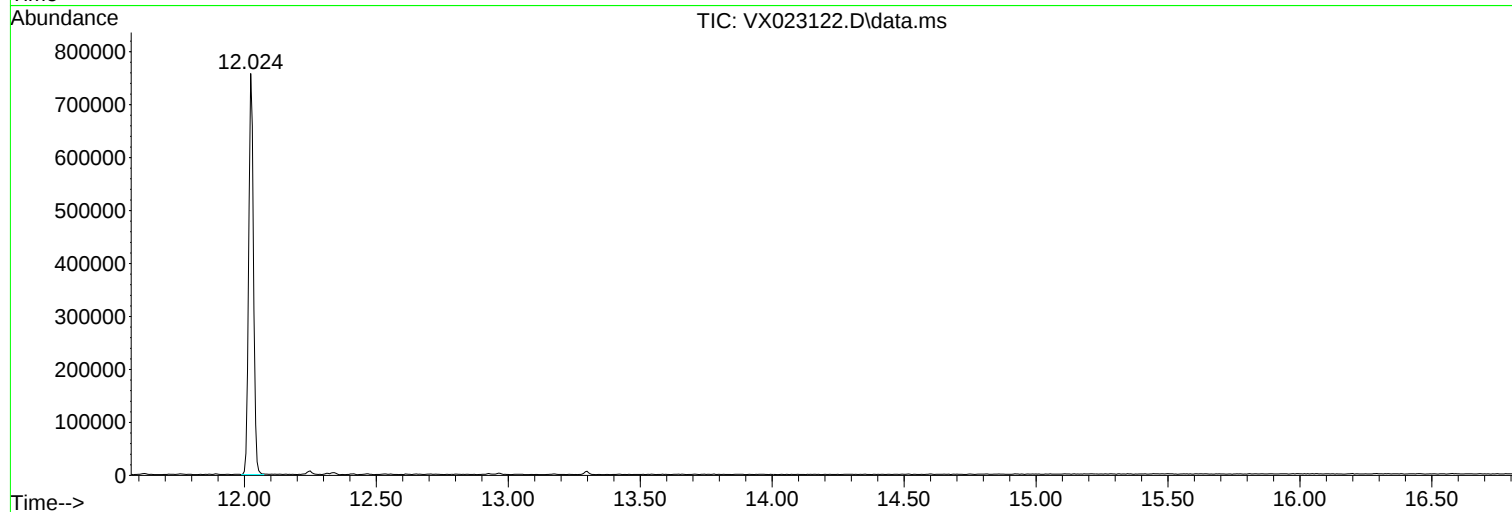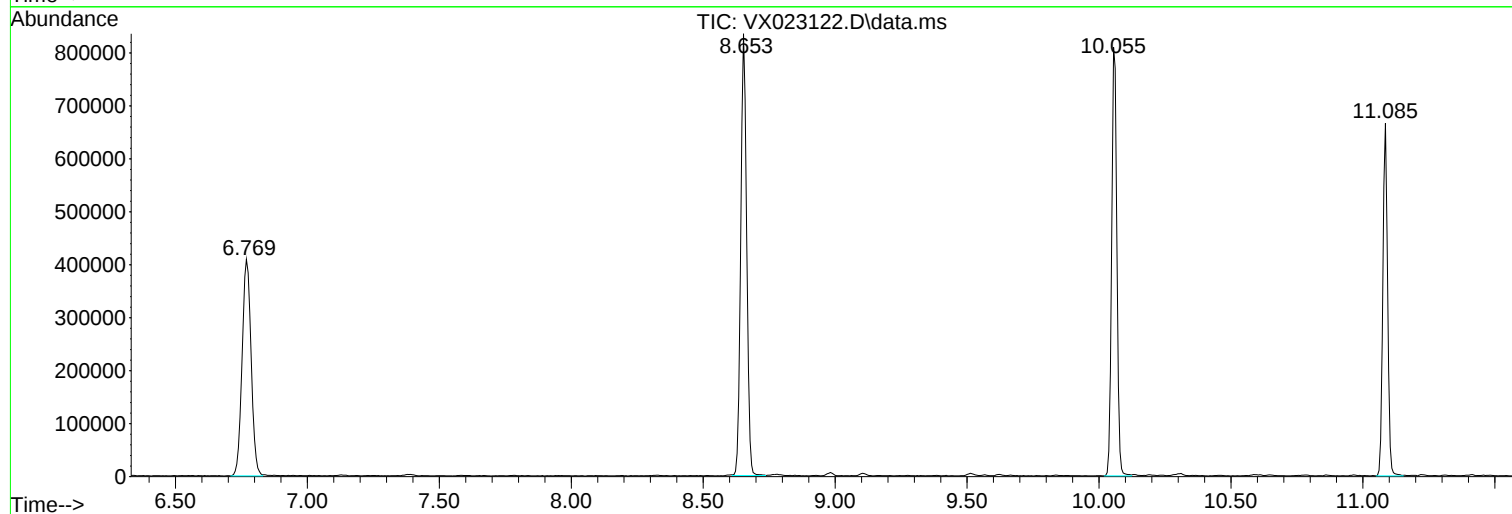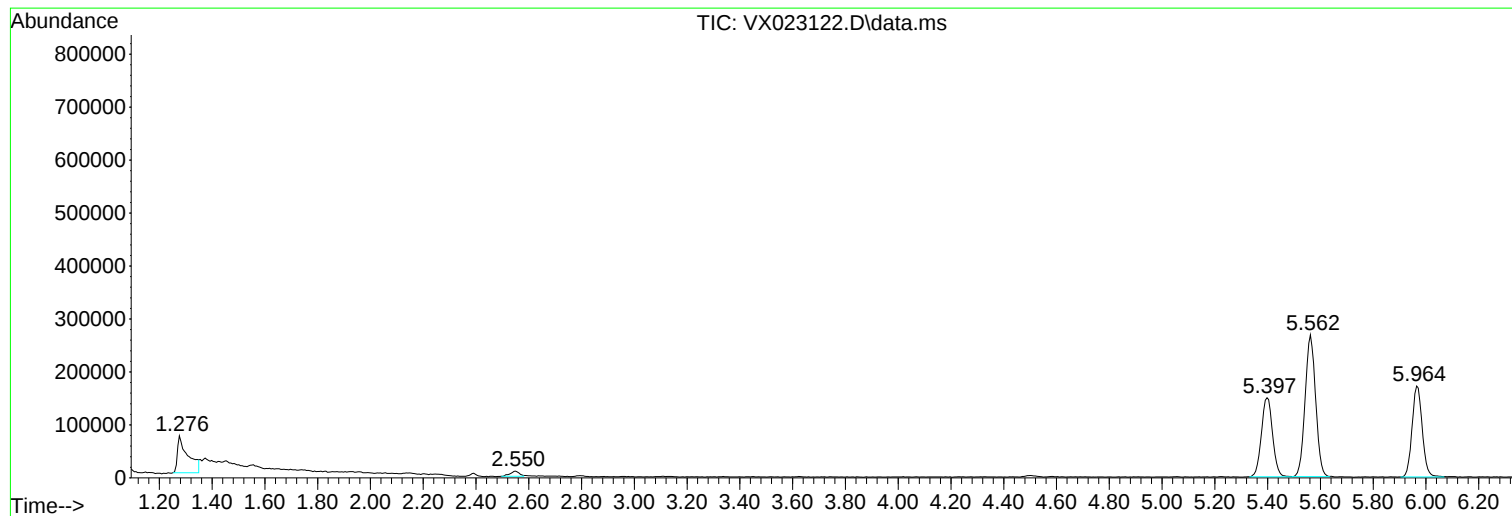

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023122.D
Acq On : 02 Jul 2021 21:03
Operator : JC/MD
Sample : M2898-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07-1.5-6.5-062921










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.276 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.276	13.28 ug/l	197474	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	40
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	33
3			Ethane, 1-chloro-1,1-difluoro-	100	C2H3ClF2	000075-68-3	22
4			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
5			2-Aminoethyl hydrogen sulfate	141	C2H7NO4S	000926-39-6	9

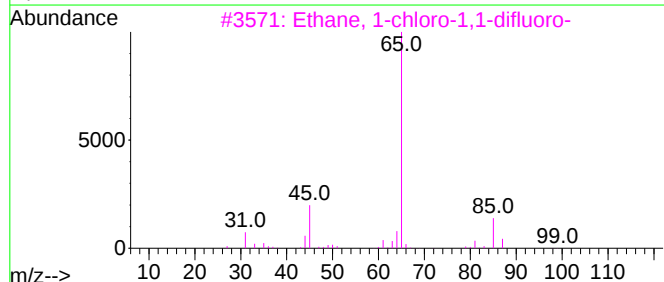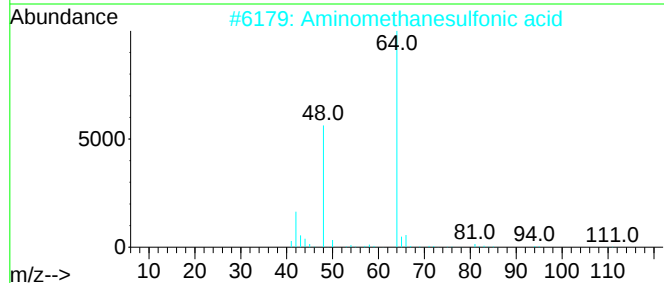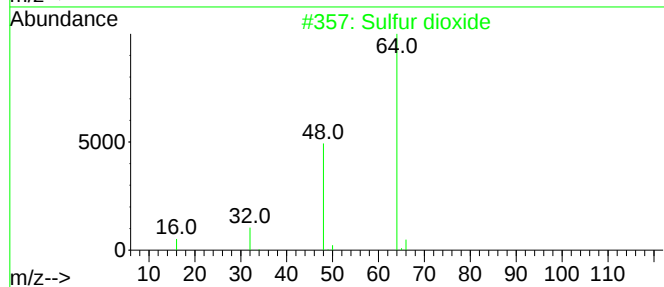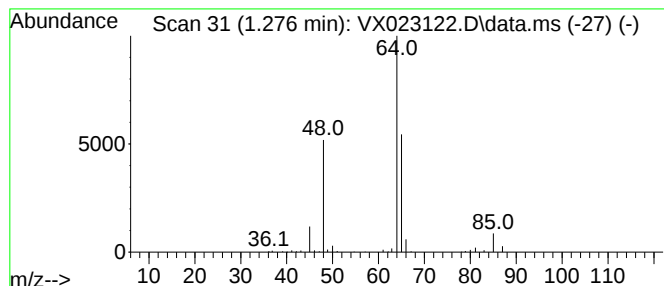

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023122.D
Acq On : 02 Jul 2021 21:03
Operator : JC/MD
Sample : M2898-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07-1.5-6.5-062921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.276	1.276	13.3	ug/l	197474	1	5.562	743451	50.0