

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
 Data File : VX023124.D
 Acq On : 02 Jul 2021 21:50
 Operator : JC/MD
 Sample : M2898-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-07-6.5-11.5-062921

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M

Title : SW846 8260

Signal : TIC: VX023124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	27	31	44	rBV2	86522	267904	21.93%	3.999%
2	2.550	231	240	247	rBV2	7488	18884	1.55%	0.282%
3	5.397	695	707	722	rBV3	140496	408381	33.43%	6.096%
4	5.562	723	734	747	rVB	251272	702324	57.50%	10.484%
5	5.971	790	801	813	rBV	154616	426216	34.90%	6.362%
6	6.769	920	932	948	rBV	381048	907916	74.33%	13.553%
7	8.653	1234	1241	1250	rBV	789950	1221419	100.00%	18.233%
8	10.055	1466	1471	1480	rBV	784939	1055273	86.40%	15.752%
9	11.085	1634	1640	1650	rBV	625622	791153	64.77%	11.810%
10	12.024	1788	1794	1806	rBV	724065	899615	73.65%	13.429%




Sum of corrected areas: 6699085

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023124.D
Acq On : 02 Jul 2021 21:50
Operator : JC/MD
Sample : M2898-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07-6.5-11.5-062921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

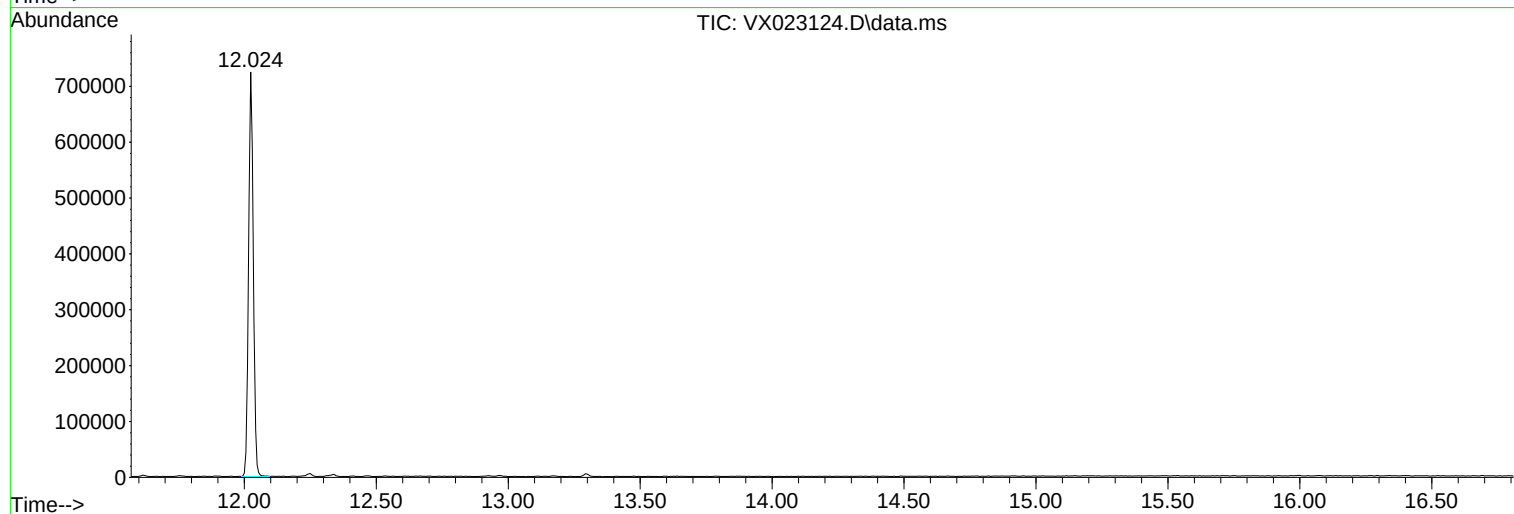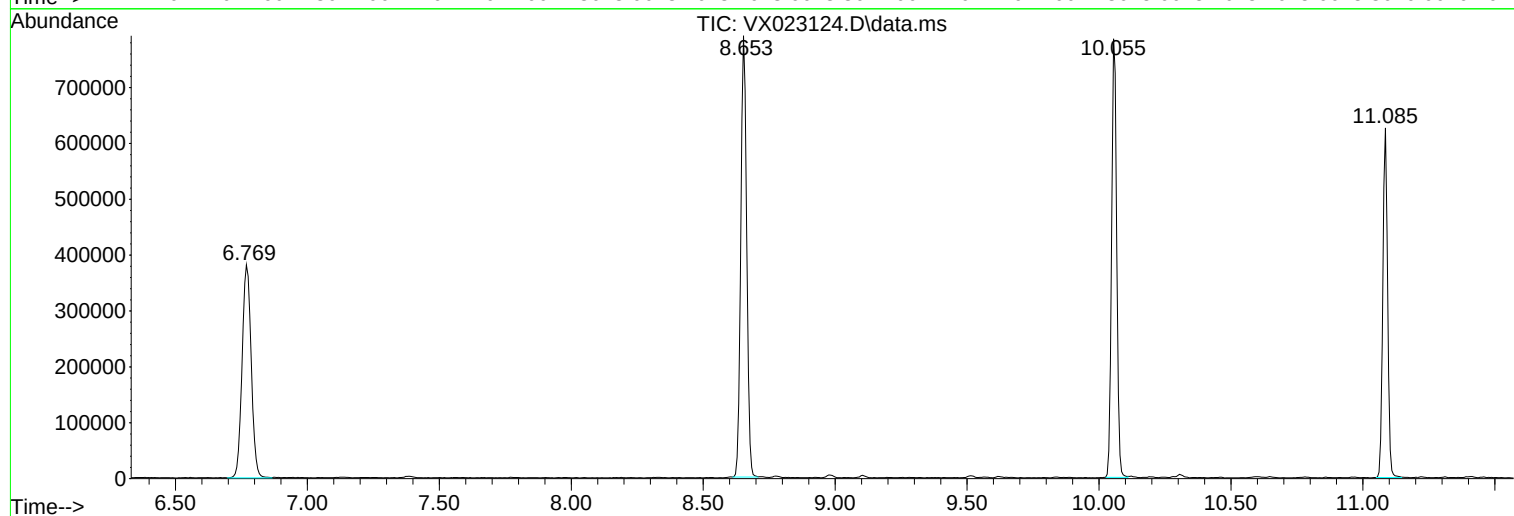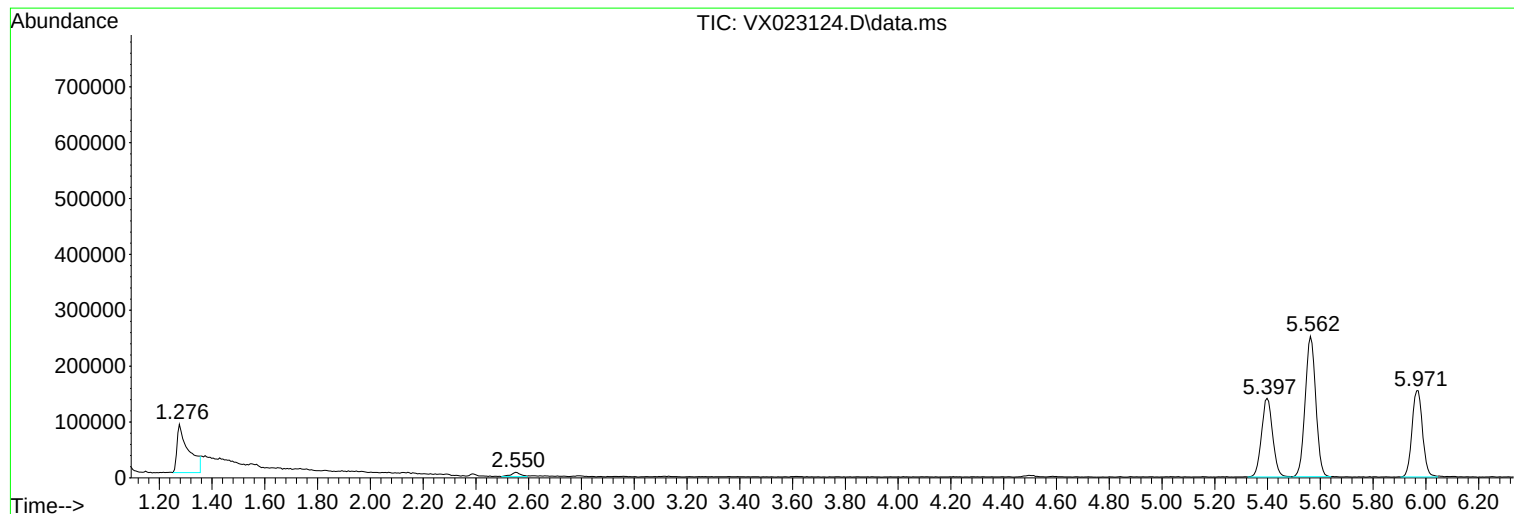

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023124.D
Acq On : 02 Jul 2021 21:50
Operator : JC/MD
Sample : M2898-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07-6.5-11.5-062921










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.276	19.07 ug/l	267904	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	86
2			2-Aminoethyl hydrogen sulfate	141	C2H7N04S	000926-39-6	74
3			Aminomethanesulfonic acid	111	CH5N03S	013881-91-9	43
4			L-Alanine, 3-sulfo-	169	C3H7N05S	000498-40-8	9
5			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4

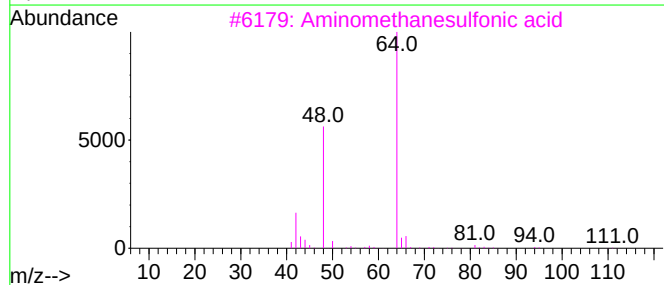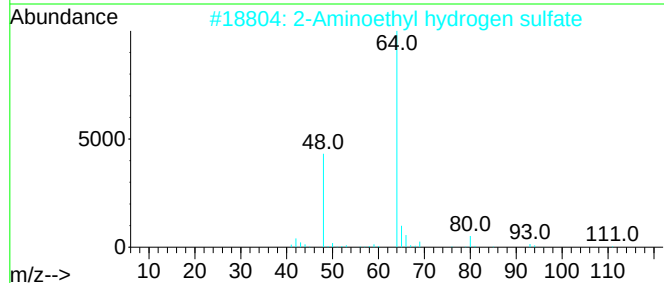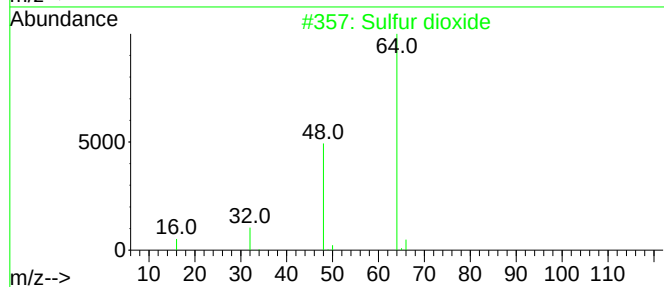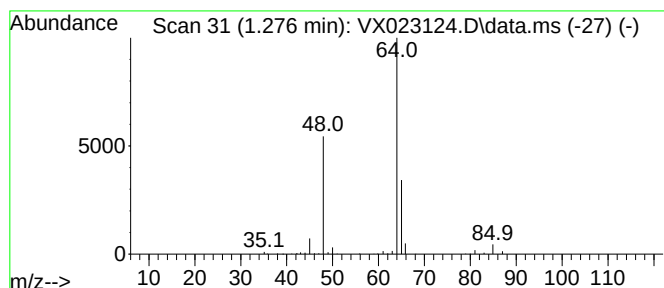

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023124.D
Acq On : 02 Jul 2021 21:50
Operator : JC/MD
Sample : M2898-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-07-6.5-11.5-062921

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.276	19.1	ug/l	267904	1	5.562	702324	50.0