
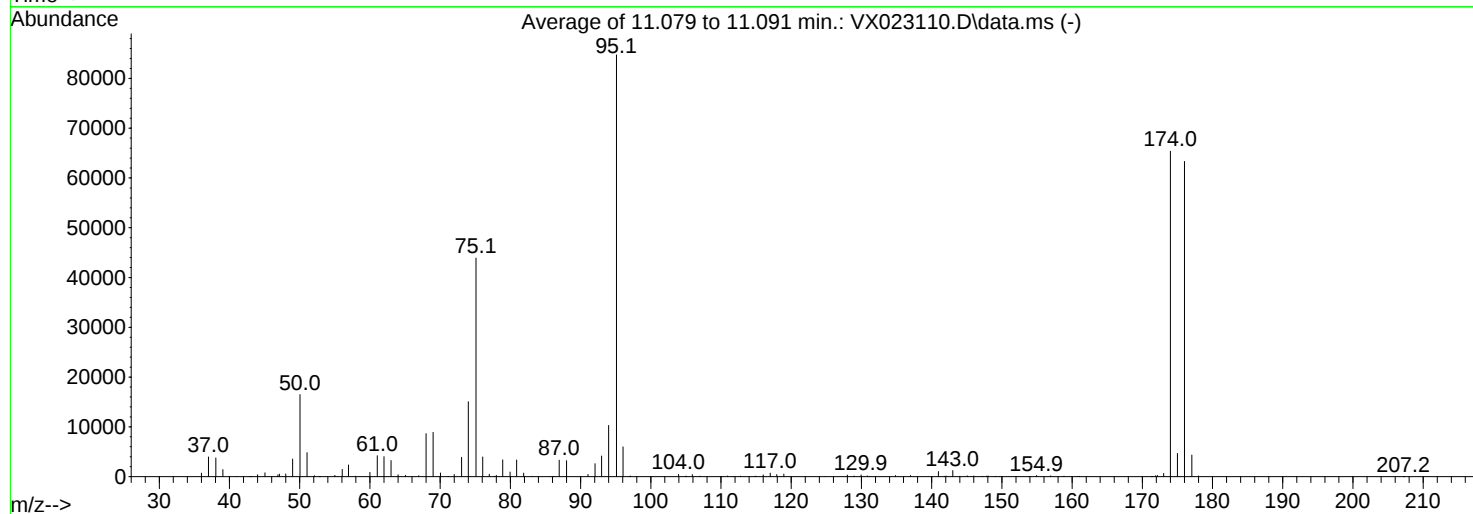


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070221\
Data File : VX023110.D
Acq On : 02 Jul 2021 15:44
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Title : SW846 8260
Last Update : Fri Jul 02 14:29:42 2021

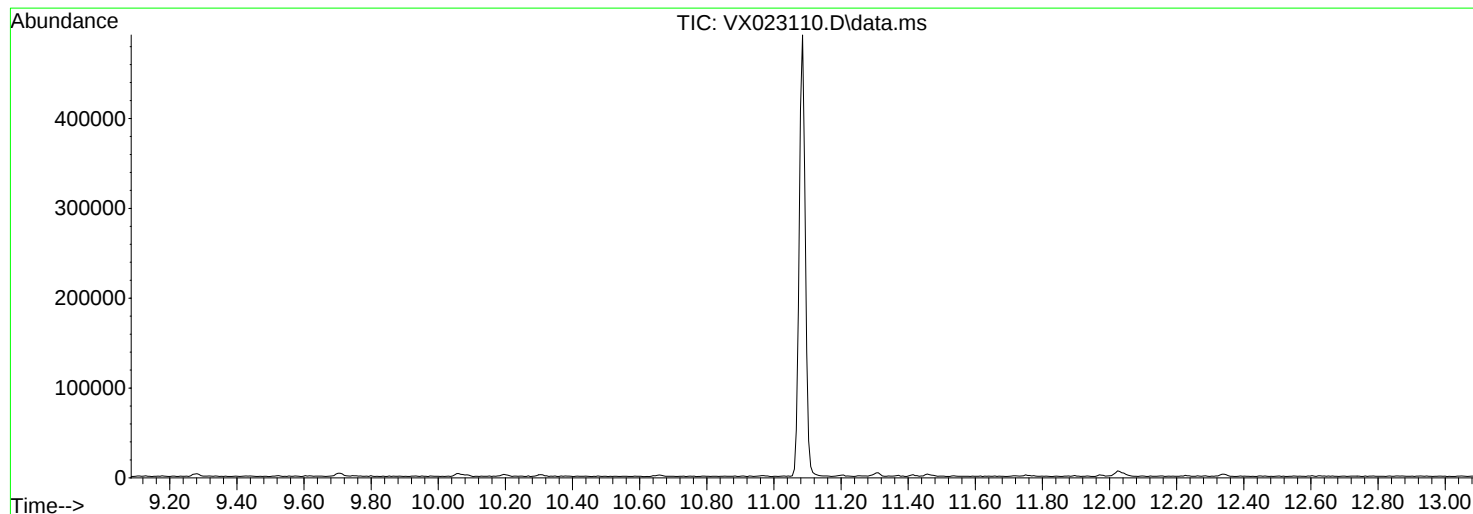

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	16499	PASS
75	95	30	60	51.8	43901	PASS
95	95	100	100	100.0	84733	PASS
96	95	5	9	7.1	5986	PASS
173	174	0.00	2	1.0	633	PASS
174	95	50	100	77.2	65395	PASS
175	174	5	9	7.1	4649	PASS
176	174	95	101	96.8	63323	PASS
177	176	5	9	6.8	4328	PASS