

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070224\
 Data File : VX042129.D
 Acq On : 02 Jul 2024 11:02
 Operator : JC/MD
 Sample : VX0702MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0702MBL01

Quant Time: Jul 03 03:29:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 23:51:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	154793	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	237444	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	226989	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	108376	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	75709	42.415	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	84.820%		
35) Dibromofluoromethane	5.385	113	74888	44.450	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	88.900%		
50) Toluene-d8	8.647	98	273447	46.200	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	92.400%		
62) 4-Bromofluorobenzene	11.079	95	99059	45.402	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.800%		
Target Compounds						
						Qvalue
3) Chloromethane	1.294	50	421	0.285	ug/l	99
5) Bromomethane	1.599	94	765	1.045	ug/l	93
6) Chloroethane	1.660	64	273	Below Cal		89
10) Methyl Iodide	2.447	142	617	0.371	ug/l	# 60
11) Tert butyl alcohol	2.953	59	3428	10.119	ug/l	# 78
12) 1,1-Dichloroethene	2.312	96	268	0.201	ug/l	# 78
13) Acrolein	2.239	56	551	1.451	ug/l	94
15) Acrylonitrile	3.081	53	474	0.536	ug/l	# 90
16) Acetone	2.386	43	799	1.019	ug/l	97
17) Carbon Disulfide	2.508	76	2236	0.821	ug/l	# 93
20) Methylene Chloride	2.782	84	894	0.521	ug/l	91
21) trans-1,2-Dichloroethene	3.093	96	444	0.328	ug/l	# 69
25) 2-Butanone	4.635	43	296	0.243	ug/l	# 51
29) Tetrahydrofuran	5.056	42	186	0.236	ug/l	# 61
31) Cyclohexane	5.550	56	2034	0.974	ug/l	# 1
38) Carbon Tetrachloride	5.550	117	12764	6.457	ug/l	# 15
44) Trichloroethene	7.135	130	347	0.215	ug/l	66
49) 1,4-Dioxane	7.702	88	51	21.038	ug/l	# 60
53) t-1,3-Dichloropropene	9.000	75	228	1.001	ug/l	# 43
68) m/p-Xylenes	10.305	106	681	0.228	ug/l	96
71) Bromoform	10.811	173	24	0.891	ug/l	# 29
76) 1,2,3-Trichloropropane	11.079	75	44674	22.706	ug/l	# 39
81) trans-1,4-Dichloro-2-b...	11.079	75	44674	64.484	ug/l	# 5
82) 4-Chlorotoluene	11.463	91	1058	0.208	ug/l	98
87) 1,3-Dichlorobenzene	11.975	146	867	0.251	ug/l	96
88) 1,4-Dichlorobenzene	11.975	146	867	0.245	ug/l	97
93) 1,2,4-Trichlorobenzene	13.591	180	1222	0.528	ug/l	99
94) Hexachlorobutadiene	13.725	225	274	0.234	ug/l	88
95) Naphthalene	13.774	128	5832	1.487	ug/l	97
96) 1,2,3-Trichlorobenzene	13.963	180	1547	0.634	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070224\
Data File : VX042129.D
Acq On : 02 Jul 2024 11:02
Operator : JC/MD
Sample : VX0702MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01

Quant Time: Jul 03 03:29:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration

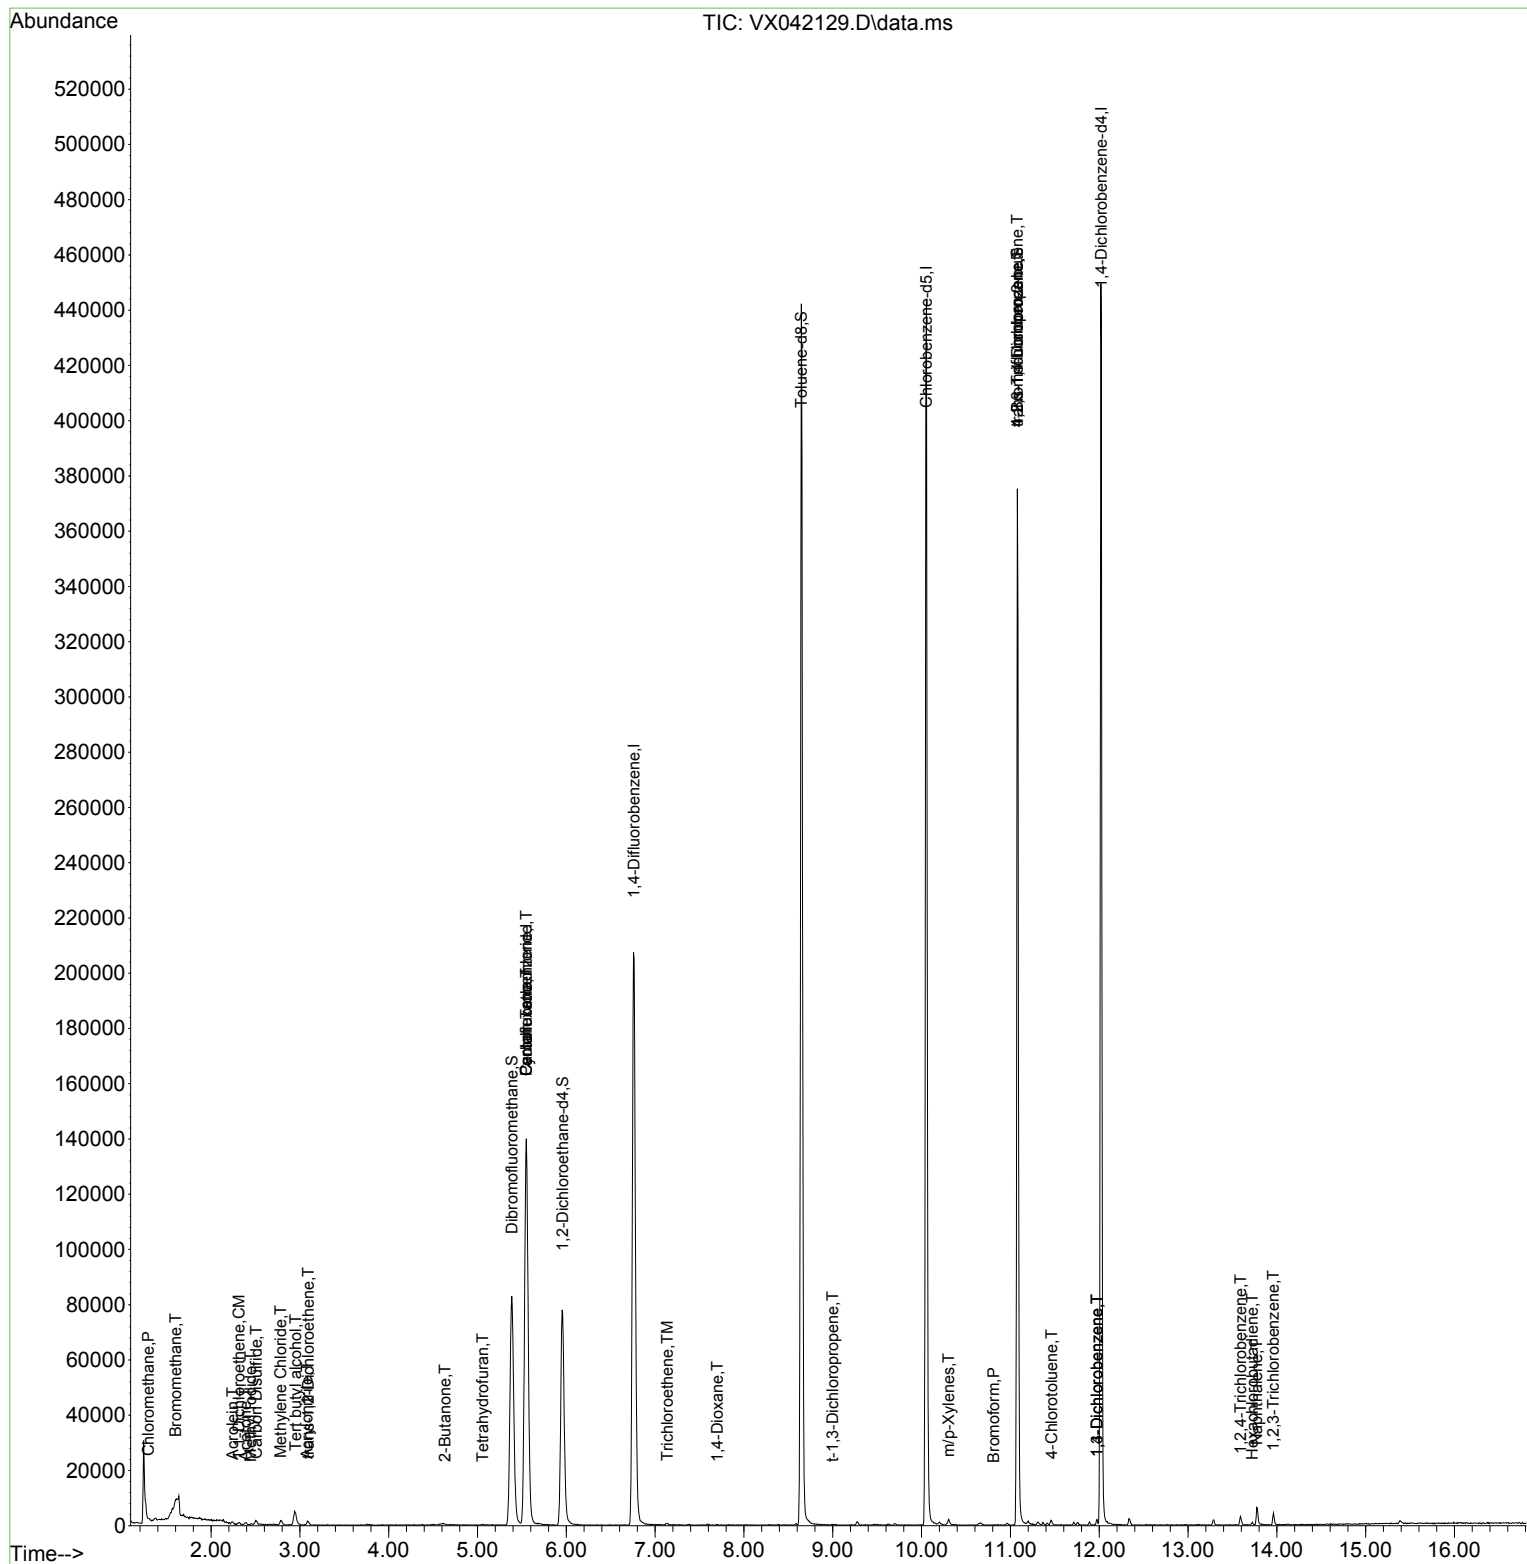



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02

Instrument :

MSVOA_X

ClientSampleId :





VX0702MBL01

Tgt Ion:168 Resp: 154793

Ion Ratio Lower Upper

168 100

99 45.7 56.6 85.0#

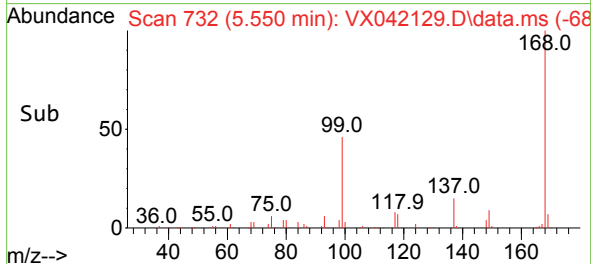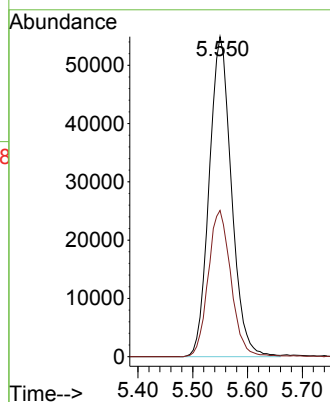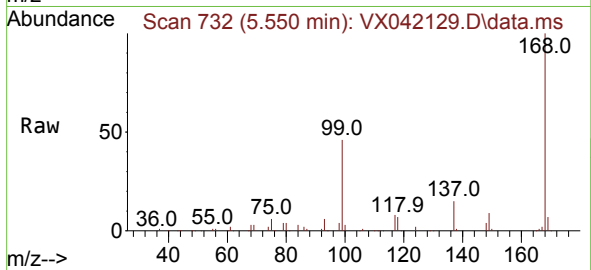

#3

Chloromethane

Concen: 0.285 ug/l

RT: 1.294 min Scan# 34

Delta R.T. -0.012 min

Lab File: VX042129.D




Acq: 02 Jul 2024 11:02


Tgt Ion: 50 Resp: 421

Ion Ratio Lower Upper

50 100

52 32.2 25.5 38.3


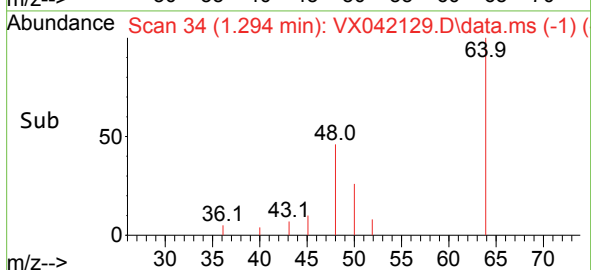




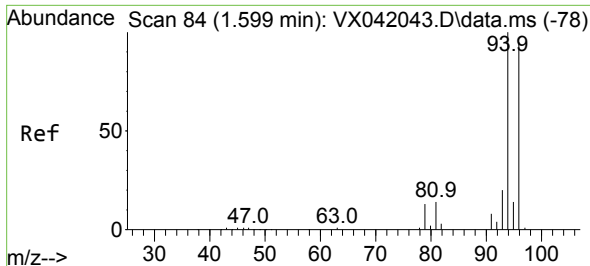

#5
Bromomethane
Concen: 1.045 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion: 94 Resp: 765
Ion Ratio Lower Upper
94 100
96 86.8 74.6 111.8

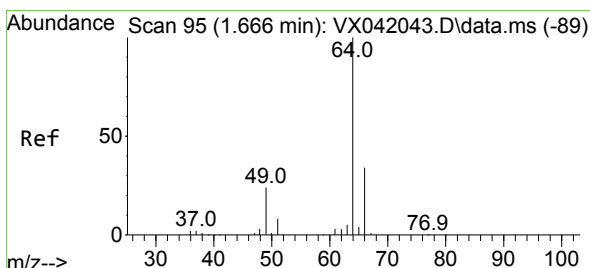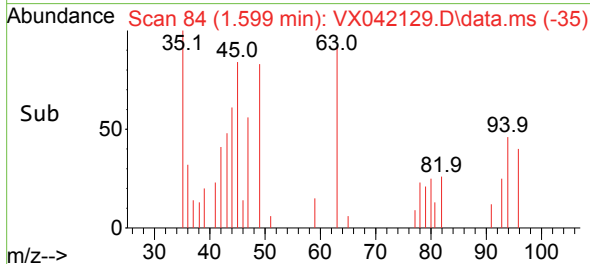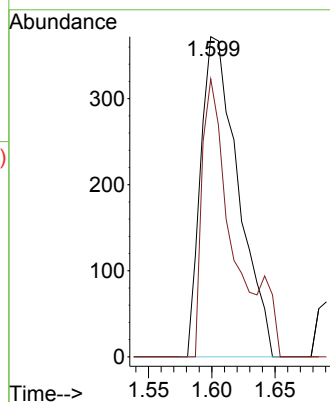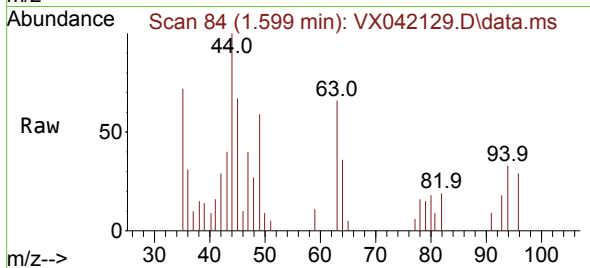

#6
Chloroethane
Concen: Below Cal
RT: 1.660 min Scan# 94
Delta R.T. 0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02


Tgt Ion: 64 Resp: 273
Ion Ratio Lower Upper
64 100
66 37.5 25.1 37.7

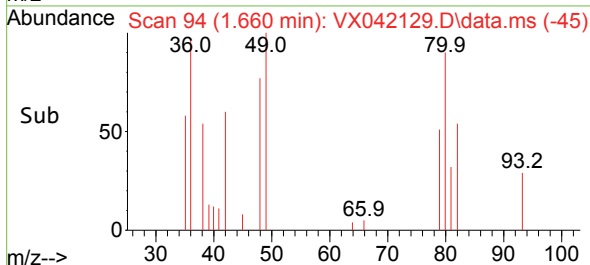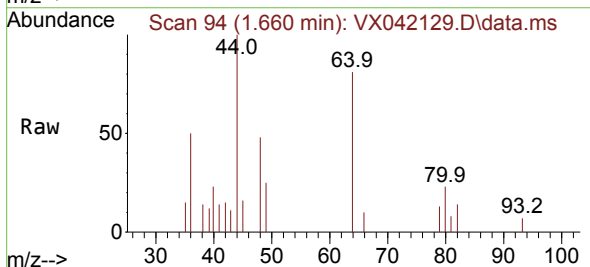






#10
Methyl Iodide
Concen: 0.371 ug/l
RT: 2.447 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01







Tgt Ion:142 Resp: 617
Ion Ratio Lower Upper
142 100
127 22.9 41.6 62.4#
141 0.0 11.6 17.4#

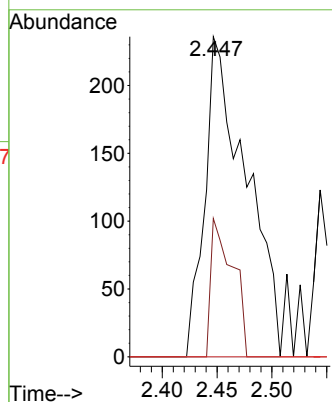

#11
Tert butyl alcohol
Concen: 10.119 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.055 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 59 Resp: 3428
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#

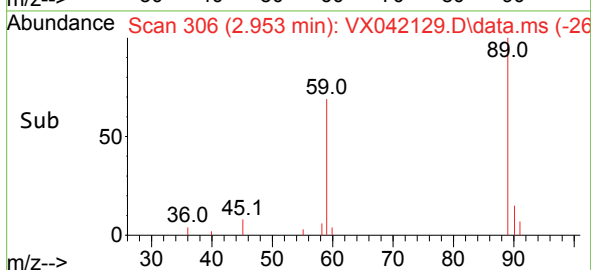

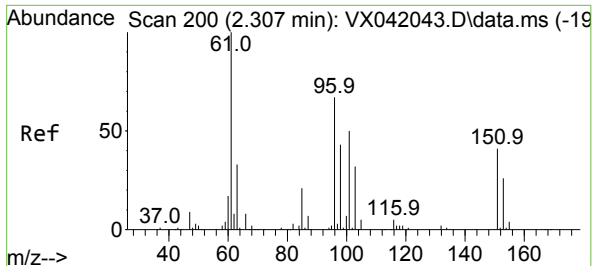

#12

1,1-Dichloroethene

Concen: 0.201 ug/l

RT: 2.312 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02

Instrument :

MSVOA_X

ClientSampleId :

VX0702MBL01





Tgt Ion: 96 Resp: 268

Ion Ratio Lower Upper

96 100

61 148.6 144.6 216.8

98 47.0 50.4 75.6#

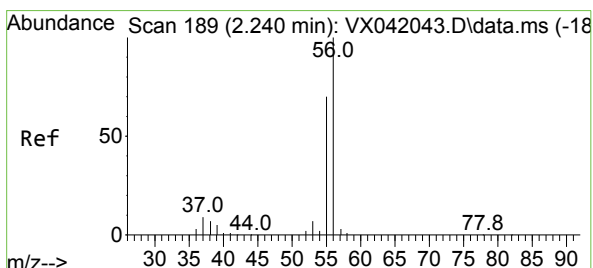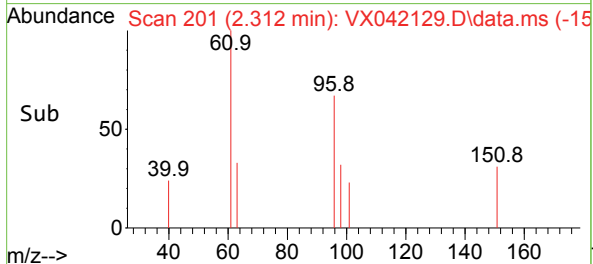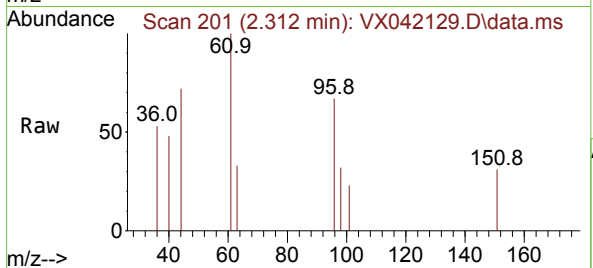

#13

Acrolein

Concen: 1.451 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.000 min

Lab File: VX042129.D




Acq: 02 Jul 2024 11:02


Tgt Ion: 56 Resp: 551

Ion Ratio Lower Upper

56 100


55 66.4 57.1 85.7

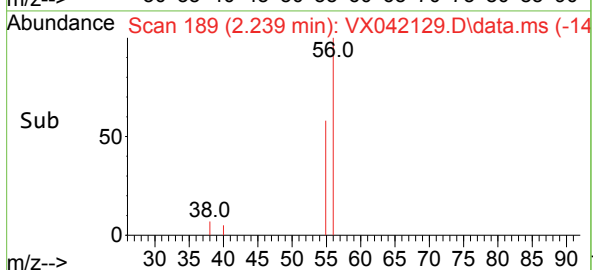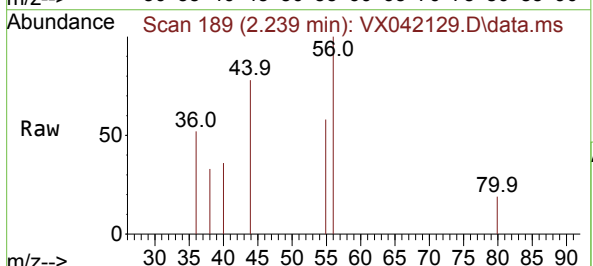






#15
Acrylonitrile
Concen: 0.536 ug/l
RT: 3.081 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01







Tgt Ion: 53 Resp: 474
Ion Ratio Lower Upper
53 100
52 82.9 66.0 99.0
51 18.4 29.8 44.6#

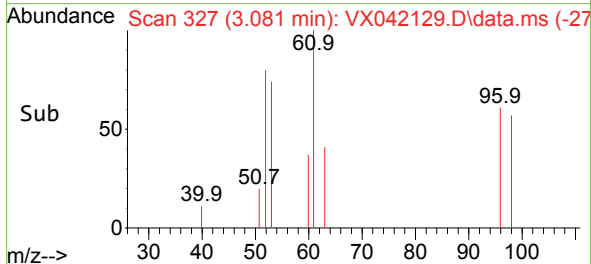

#16
Acetone
Concen: 1.019 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.012 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 43 Resp: 799
Ion Ratio Lower Upper
43 100
58 28.8 21.9 32.9


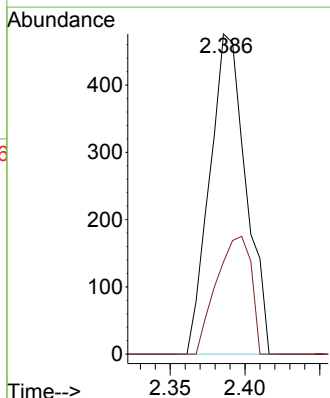
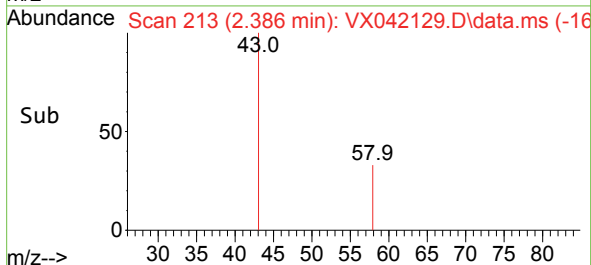
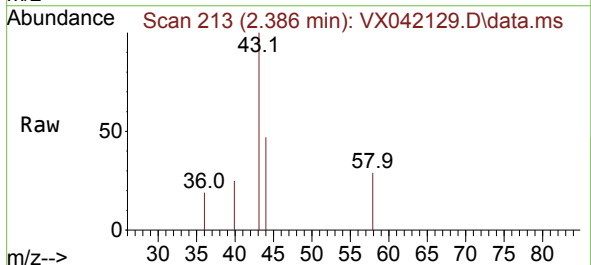




#17
Carbon Disulfide
Concen: 0.821 ug/l
RT: 2.508 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion: 76 Resp: 2236
Ion Ratio Lower Upper
76 100
78 11.2 7.0 10.6#

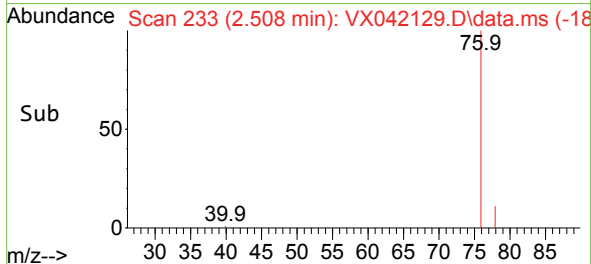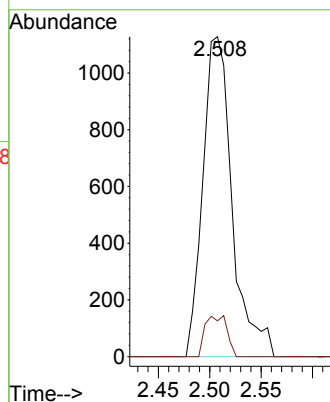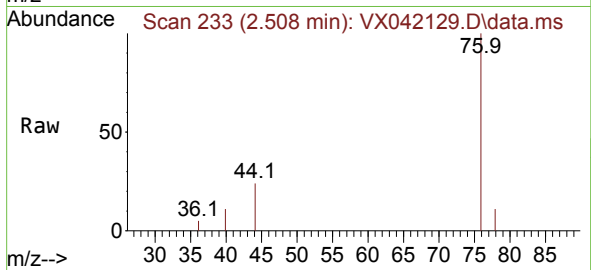

#20
Methylene Chloride
Concen: 0.521 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 84 Resp: 894
Ion Ratio Lower Upper
84 100
49 118.7 103.6 155.4
51 39.4 33.8 50.6
86 71.4 49.4 74.0




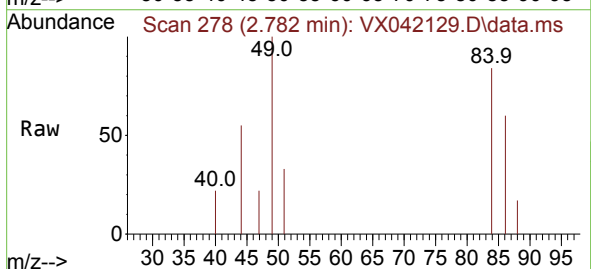




#21
trans-1,2-Dichloroethene
Concen: 0.328 ug/l
RT: 3.093 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion: 96 Resp: 444
Ion Ratio Lower Upper
96 100
61 98.1 119.2 178.8#
98 54.1 48.7 73.1

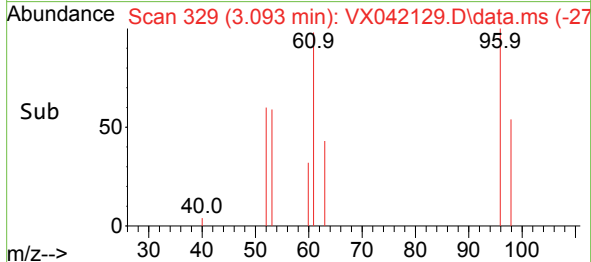

#25
2-Butanone
Concen: 0.243 ug/l
RT: 4.635 min Scan# 582
Delta R.T. 0.061 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 43 Resp: 296
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.2#

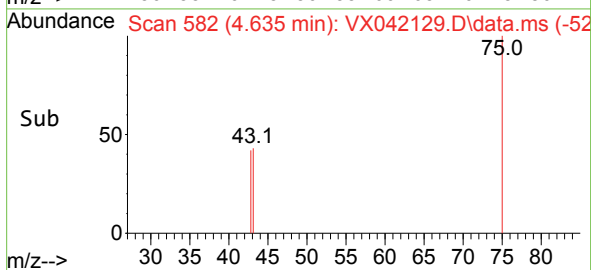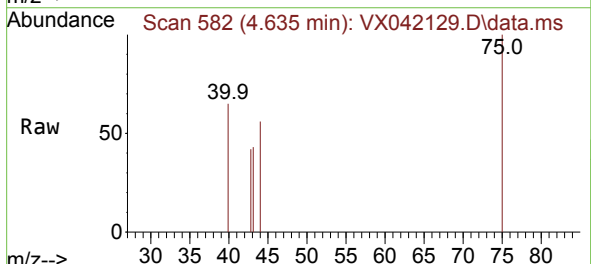



#29

Tetrahydrofuran

Concen: 0.236 ug/l

RT: 5.056 min Scan# 61

Delta R.T. 0.037 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02

Instrument :

MSVOA_X

ClientSampleId :

VX0702MBL01





Tgt Ion: 42 Resp: 186

Ion Ratio Lower Upper

42 100

72 23.7 34.2 51.4#

71 10.8 32.2 48.2#

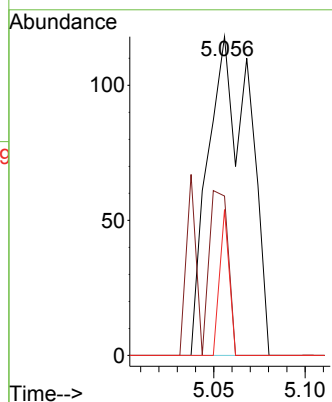

#31

Cyclohexane

Concen: 0.974 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.085 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02




Tgt Ion: 56 Resp: 2034


Ion Ratio Lower Upper

56 100

69 196.3 23.4 35.2#

84 172.3 65.9 98.9#


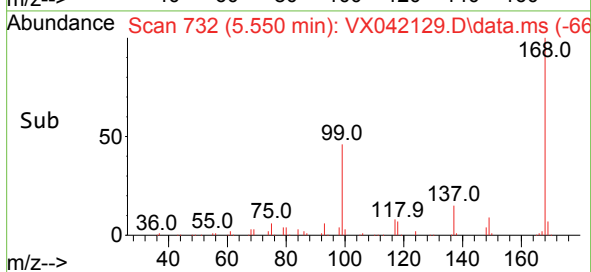
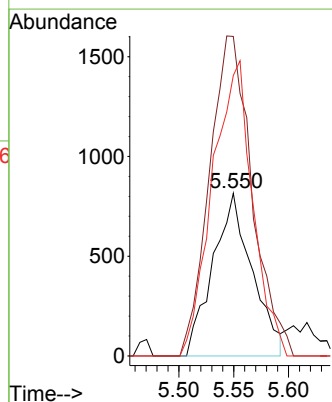





#33
1,2-Dichloroethane-d4
Concen: 42.415 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion: 65 Resp: 75709
Ion Ratio Lower Upper
65 100
67 53.5 0.0 100.2

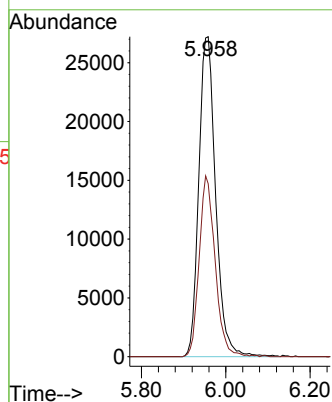

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 114 Resp: 237444
Ion Ratio Lower Upper
114 100
63 17.6 0.0 45.0
88 14.3 0.0 36.6


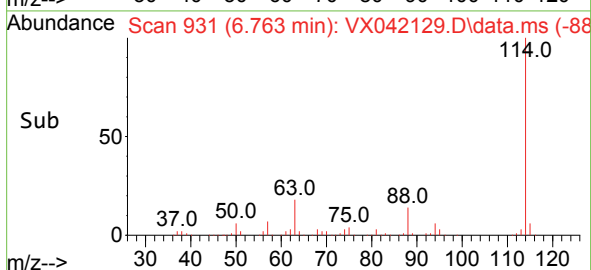






#35
Dibromofluoromethane
Concen: 44.450 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion:113 Resp: 74888
Ion Ratio Lower Upper
113 100
111 101.8 82.9 124.3
192 25.1 13.3 19.9#

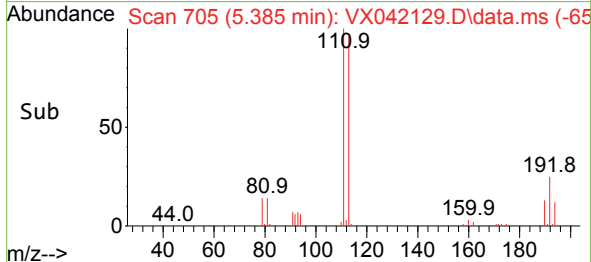

#38
Carbon Tetrachloride
Concen: 6.457 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion:117 Resp: 12764
Ion Ratio Lower Upper
117 100
119 5.5 78.2 117.2#
121 0.0 24.4 36.6#


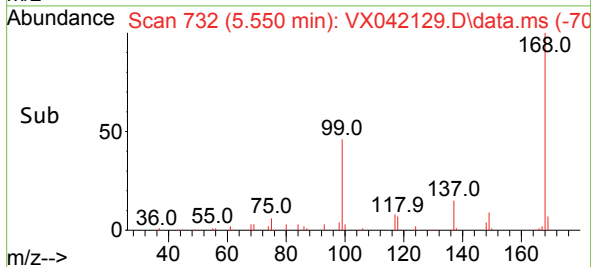

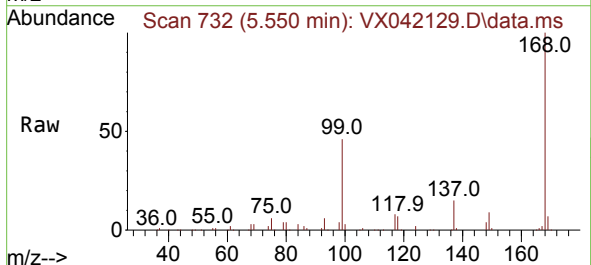




#44
Trichloroethene
Concen: 0.215 ug/l
RT: 7.135 min Scan# 990
Delta R.T. 0.006 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion:130 Resp: 347
Ion Ratio Lower Upper
130 100
95 67.6 0.0 204.4

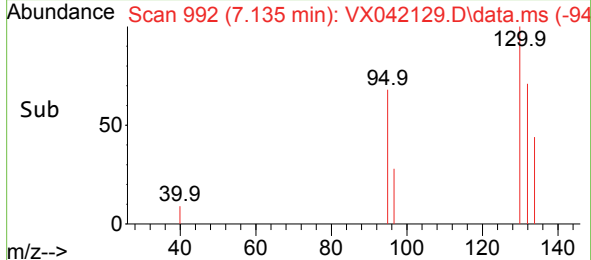

#49
1,4-Dioxane
Concen: 21.038 ug/l
RT: 7.702 min Scan# 1085
Delta R.T. 0.037 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 88 Resp: 51
Ion Ratio Lower Upper
88 100
43 0.0 0.0 0.0
58 41.2 60.1 90.1#


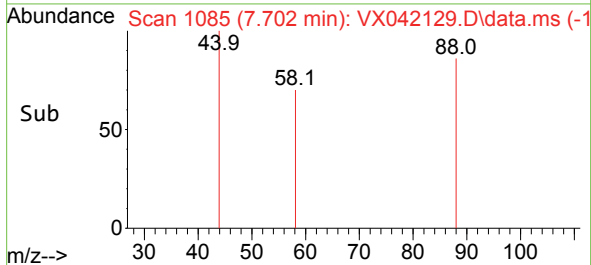

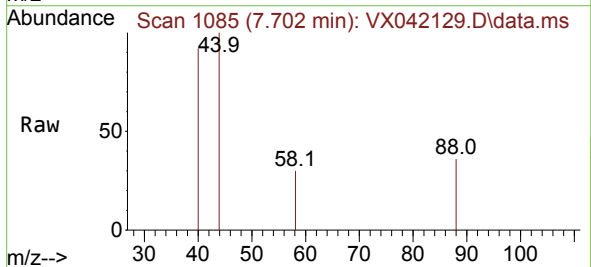




#50
Toluene-d8
Concen: 46.200 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion: 98 Resp: 273447
Ion Ratio Lower Upper
98 100
100 66.9 53.1 79.7



#53
t-1,3-Dichloropropene
Concen: 1.001 ug/l
RT: 9.000 min Scan# 1298
Delta R.T. 0.018 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 75 Resp: 228
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#


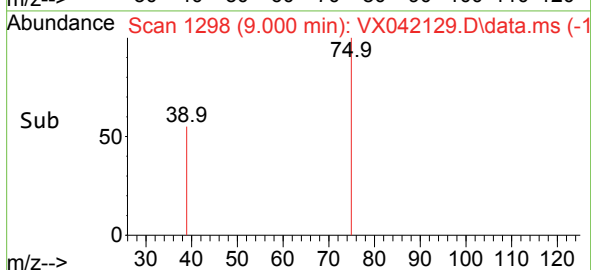






#62
4-Bromofluorobenzene
Concen: 45.402 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion: 95 Resp: 99059
Ion Ratio Lower Upper
95 100
174 98.3 0.0 135.6
176 96.4 0.0 131.0

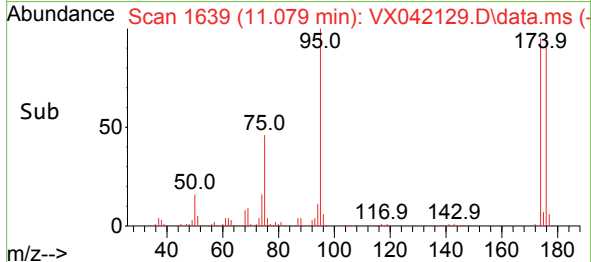

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 117 Resp: 226989
Ion Ratio Lower Upper
117 100
82 49.7 46.2 69.4
119 31.8 25.5 38.3

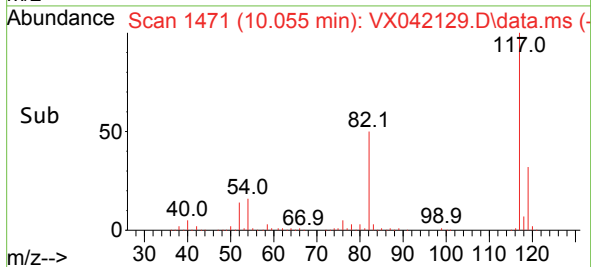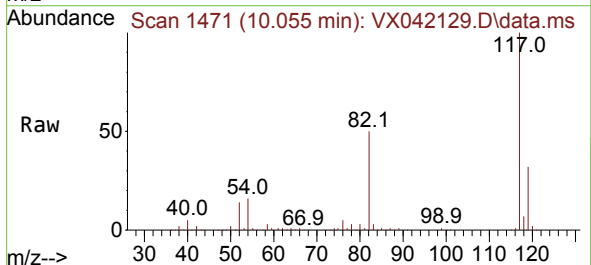



#68

m/p-Xylenes

Concen: 0.228 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.006 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02

Instrument :

MSVOA_X

ClientSampleId :





VX0702MBL01

Tgt Ion:106 Resp: 681

Ion Ratio Lower Upper

106 100

91 200.3 165.5 248.3

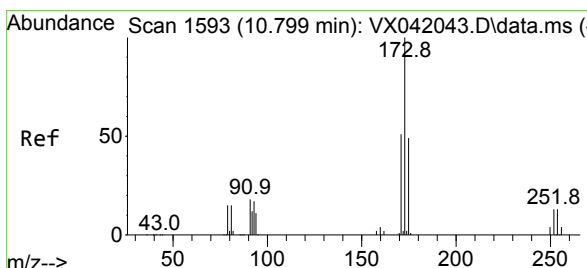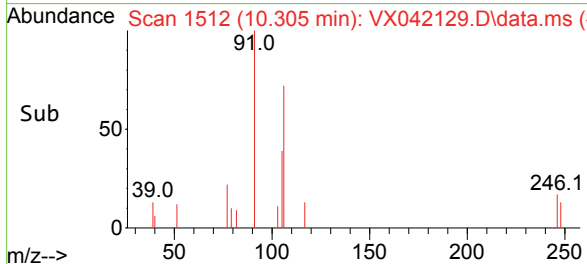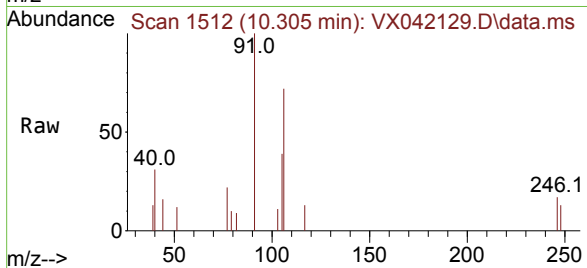

#71

Bromoform

Concen: 0.891 ug/l

RT: 10.811 min Scan# 1595

Delta R.T. 0.012 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02




Tgt Ion:173 Resp: 24


Ion Ratio Lower Upper

173 100

175 0.0 24.1 72.4#

254 0.0 0.0 0.0


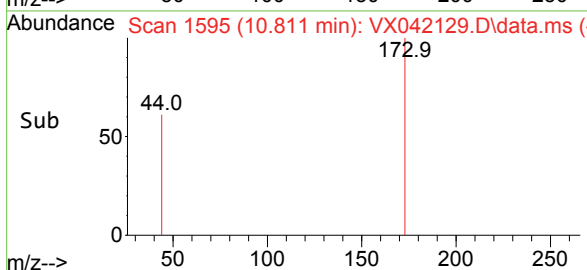

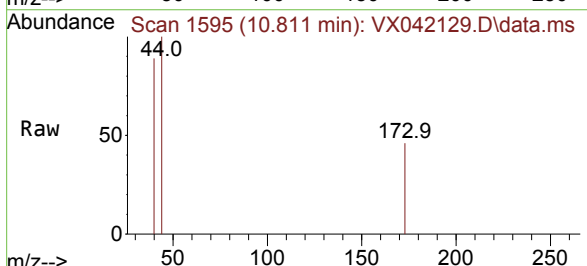




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX042129.D
 Acq: 02 Jul 2024 11:02




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0702MBL01


Tgt Ion:152 Resp: 108376
 Ion Ratio Lower Upper
 152 100
 115 53.0 43.3 129.9
 150 154.5 0.0 345.0

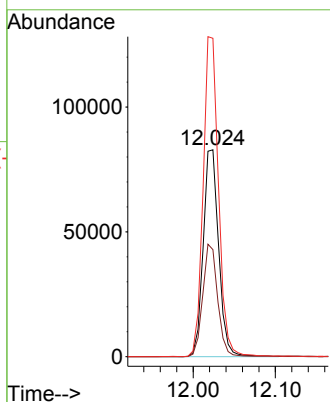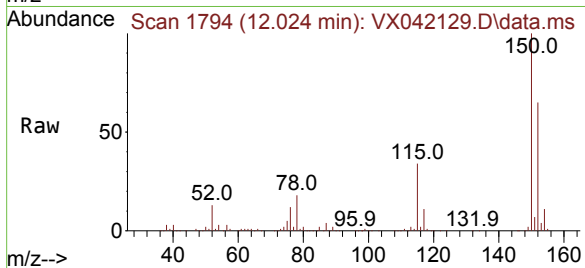

#76
 1,2,3-Trichloropropane
 Concen: 22.706 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX042129.D
 Acq: 02 Jul 2024 11:02

Tgt Ion: 75 Resp: 44674
 Ion Ratio Lower Upper
 75 100
 77 1.3 19.1 57.5#


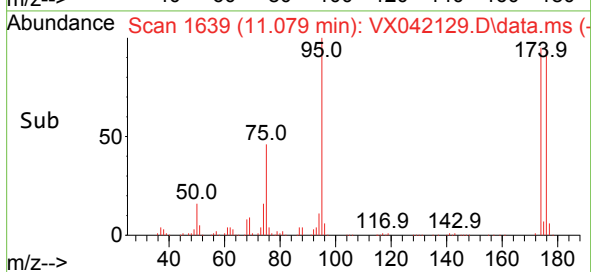
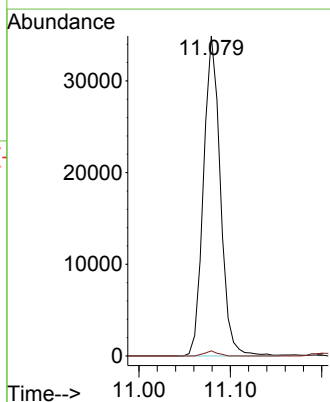
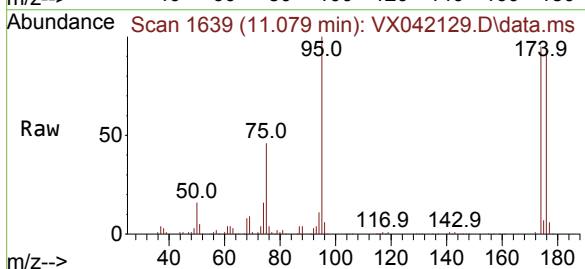




#81
trans-1,4-Dichloro-2-butene
Concen: 64.484 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02




Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01


Tgt Ion: 75 Resp: 44674
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

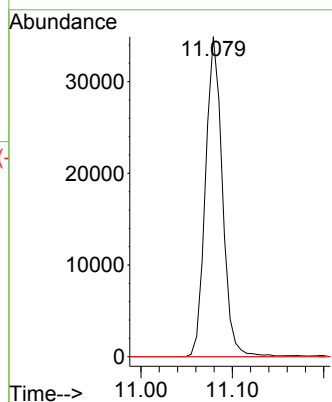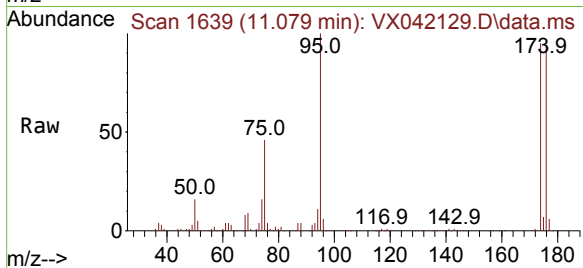

#82
4-Chlorotoluene
Concen: 0.208 ug/l
RT: 11.463 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion: 91 Resp: 1058
Ion Ratio Lower Upper
91 100
126 27.5 14.2 42.6

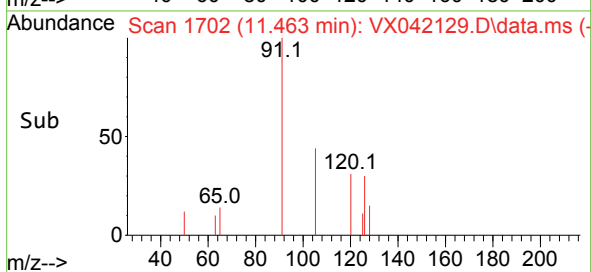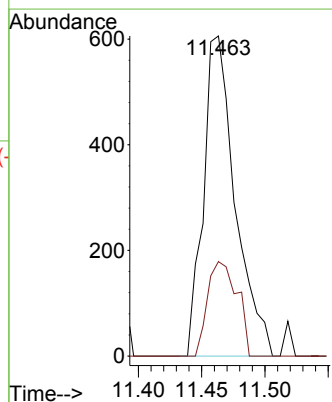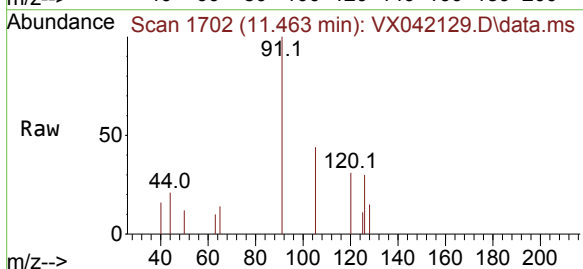



#87

1,3-Dichlorobenzene

Concen: 0.251 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. 0.006 min

Lab File: VX042129.D


Acq: 02 Jul 2024 11:02

Instrument :

MSVOA_X

ClientSampleId :

VX0702MBL01

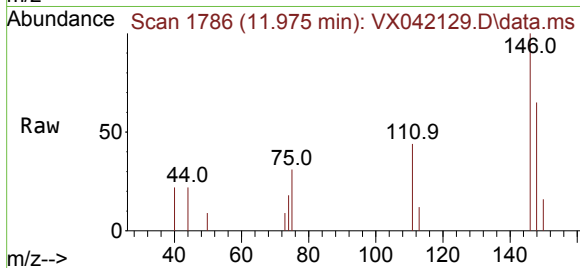




Tgt Ion:146 Resp: 867

Ion Ratio Lower Upper

146 100

111 41.6 22.1 66.1

148 66.2 31.8 95.3

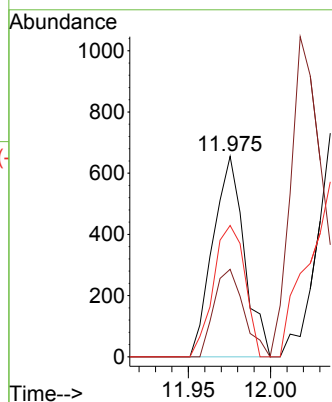

#88

1,4-Dichlorobenzene

Concen: 0.245 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. -0.067 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02




Tgt Ion:146 Resp: 867


Ion Ratio Lower Upper

146 100

111 41.6 21.3 63.7

148 66.2 31.8 95.4

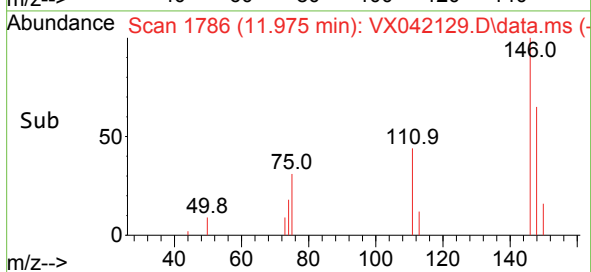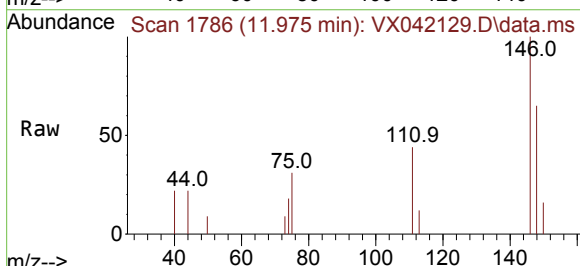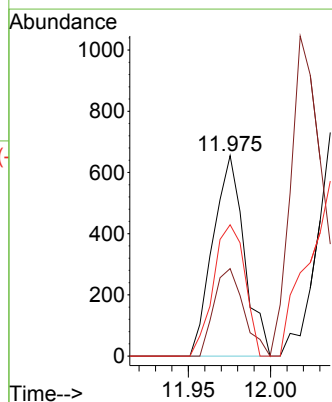



#93

1,2,4-Trichlorobenzene

Concen: 0.528 ug/l

RT: 13.591 min Scan# 2050

Delta R.T. 0.006 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02

Instrument :

MSVOA_X

ClientSampleId :

VX0702MBL01





Tgt Ion:180 Resp: 1222

Ion Ratio Lower Upper

180 100

182 96.0 48.3 144.8

145 35.4 18.0 54.0

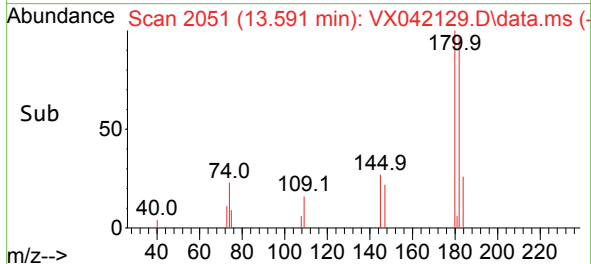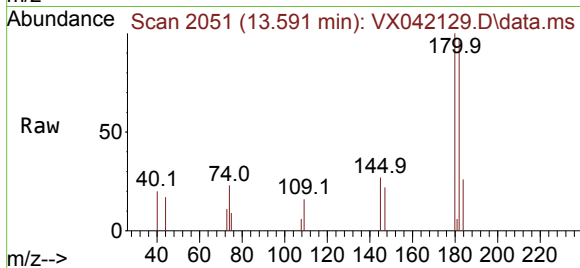

#94

Hexachlorobutadiene

Concen: 0.234 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. -0.000 min

Lab File: VX042129.D

Acq: 02 Jul 2024 11:02




Tgt Ion:225 Resp: 274


Ion Ratio Lower Upper

225 100

223 49.6 31.1 93.2

227 58.0 32.5 97.5


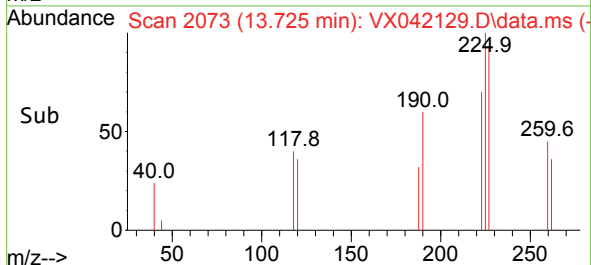

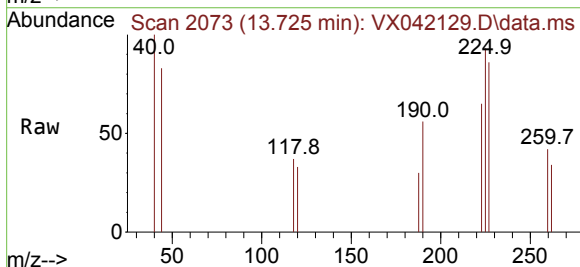


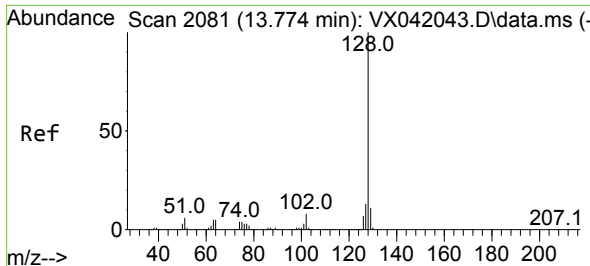

#95
Naphthalene
Concen: 1.487 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Instrument :
MSVOA_X
ClientSampleId :
VX0702MBL01

Tgt Ion:	128	Resp:	5832
Ion	Ratio	Lower	Upper
128	100		
127	12.0	10.3	15.5
129	9.2	8.8	13.2

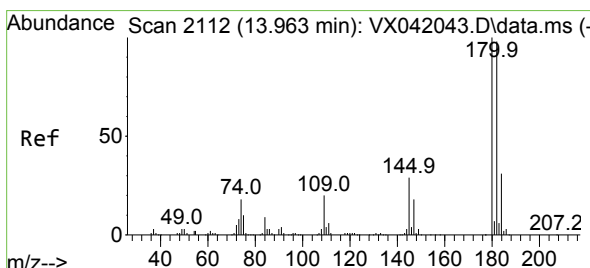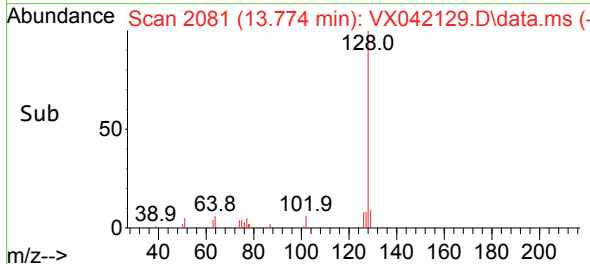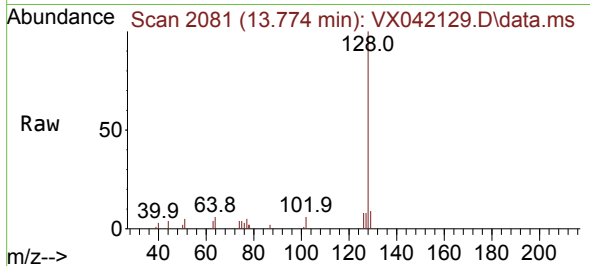

#96
1,2,3-Trichlorobenzene
Concen: 0.634 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.000 min
Lab File: VX042129.D
Acq: 02 Jul 2024 11:02

Tgt Ion:	180	Resp:	1547
Ion	Ratio	Lower	Upper
180	100		
182	87.1	46.9	140.6
145	29.8	17.8	53.5

