

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070224\
 Data File : VX042152.D
 Acq On : 02 Jul 2024 20:03
 Operator : JC/MD
 Sample : P3106-04 20X
 Misc : 5.05g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FILTER-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Title : SW846 8260

Signal : TIC: VX042152.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	28	rBV	13638	16155	2.66%	0.405%
2	1.599	66	84	85	rBV6	6732	20822	3.43%	0.522%
3	1.648	90	92	95	rVB3	6283	6956	1.15%	0.174%
4	2.947	298	305	316	rBV3	2647	7199	1.19%	0.180%
5	4.245	509	518	540	rBV3	7331	30222	4.98%	0.757%
6	5.385	694	705	721	rBV2	72329	212939	35.05%	5.335%
7	5.550	721	732	746	rVV	120651	339819	55.94%	8.515%
8	5.952	789	798	819	rBV	67597	186146	30.64%	4.664%
9	6.763	922	931	950	rBV	180657	440266	72.48%	11.031%
10	7.232	1001	1008	1027	rBV2	14445	48519	7.99%	1.216%
11	8.647	1234	1240	1250	rBV	392814	607450	100.00%	15.220%
12	10.055	1465	1471	1486	rBV	410422	557895	91.84%	13.979%
13	10.299	1506	1511	1517	rBV2	5354	8726	1.44%	0.219%
14	11.079	1634	1639	1654	rBV	340275	452724	74.53%	11.344%
15	12.018	1788	1793	1803	rBV	414236	546791	90.01%	13.701%
16	12.219	1822	1826	1833	rBV3	6100	10081	1.66%	0.253%
17	12.420	1854	1859	1864	rBV2	10293	13246	2.18%	0.332%
18	12.914	1931	1940	1946	rVV8	3708	11806	1.94%	0.296%
19	12.975	1946	1950	1957	rVB5	4091	6638	1.09%	0.166%
20	13.268	1993	1998	2001	rBV	20109	25828	4.25%	0.647%
21	13.603	2047	2053	2060	rBV10	3402	8024	1.32%	0.201%
22	13.682	2060	2066	2068	rBV4	4361	8131	1.34%	0.204%
23	13.737	2071	2075	2077	rVV3	6100	8648	1.42%	0.217%
24	13.774	2077	2081	2088	rVV	33861	54930	9.04%	1.376%
25	13.841	2088	2092	2099	rVB6	9461	17048	2.81%	0.427%
26	14.036	2118	2124	2128	rBV2	35173	44282	7.29%	1.110%
27	14.225	2150	2155	2159	rVB7	6171	10058	1.66%	0.252%
28	14.432	2180	2189	2193	rBV9	8510	19972	3.29%	0.500%
29	14.475	2193	2196	2198	rBV4	4737	6423	1.06%	0.161%
30	14.505	2198	2201	2206	rVB4	7762	12753	2.10%	0.320%
31	14.560	2206	2210	2215	rBV4	5064	9175	1.51%	0.230%
32	14.633	2215	2222	2227	rBV2	18956	38226	6.29%	0.958%
33	14.755	2238	2242	2244	rBV	45504	48918	8.05%	1.226%
34	14.780	2244	2246	2251	rVB	20866	27831	4.58%	0.697%
35	15.097	2293	2298	2302	rBV5	6018	12405	2.04%	0.311%
36	15.213	2313	2317	2323	rVV2	13731	19176	3.16%	0.480%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070224\
Data File : VX042152.D
Acq On : 02 Jul 2024 20:03
Operator : JC/MD
Sample : P3106-04 20X
Misc : 5.05g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FILTER-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Title : SW846 8260

37	15.274	2324	2327	2331	rVB5	5739	6295	1.04%	0.158%
38	15.377	2340	2344	2348	rBV6	4872	9053	1.49%	0.227%
39	15.487	2357	2362	2367	rBV4	13871	21075	3.47%	0.528%
40	15.560	2370	2374	2378	rVB2	7445	11652	1.92%	0.292%
41	15.615	2378	2383	2387	rBV2	10317	17187	2.83%	0.431%
42	15.920	2430	2433	2439	rVB5	6645	11069	1.82%	0.277%
43	16.097	2456	2462	2466	rBV9	4422	10546	1.74%	0.264%
44	16.377	2502	2508	2512	rVB9	3547	7916	1.30%	0.198%




Sum of corrected areas: 3991021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070224\
Data File : VX042152.D
Acq On : 02 Jul 2024 20:03
Operator : JC/MD
Sample : P3106-04 20X
Misc : 5.05g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FILTER-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

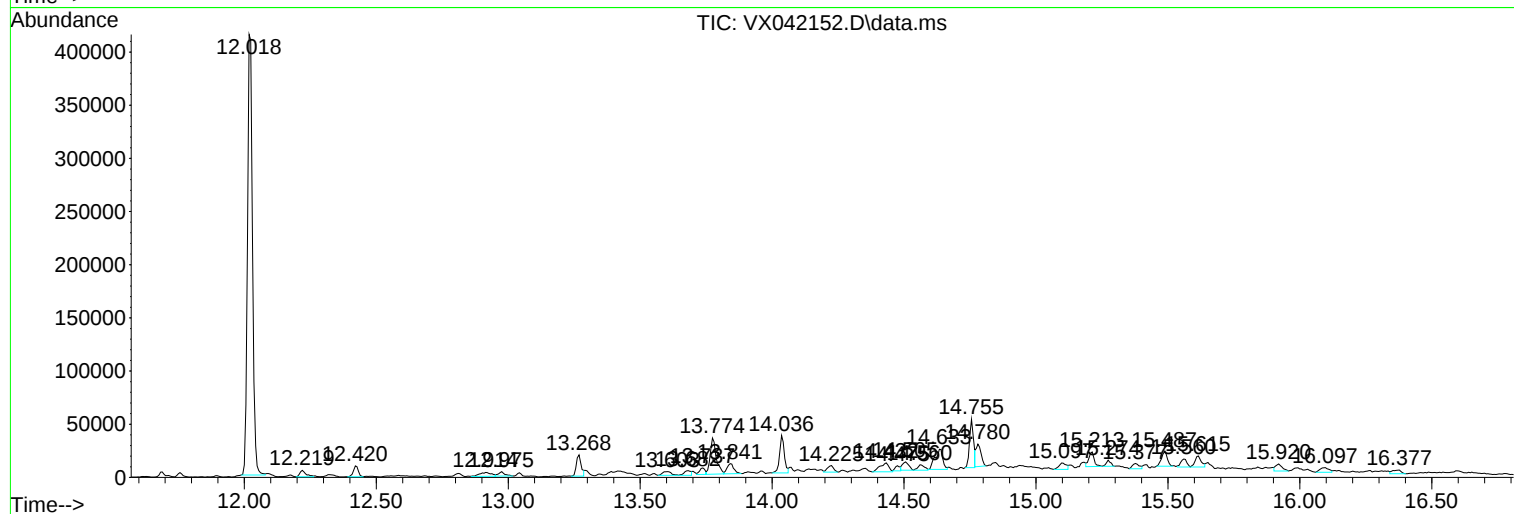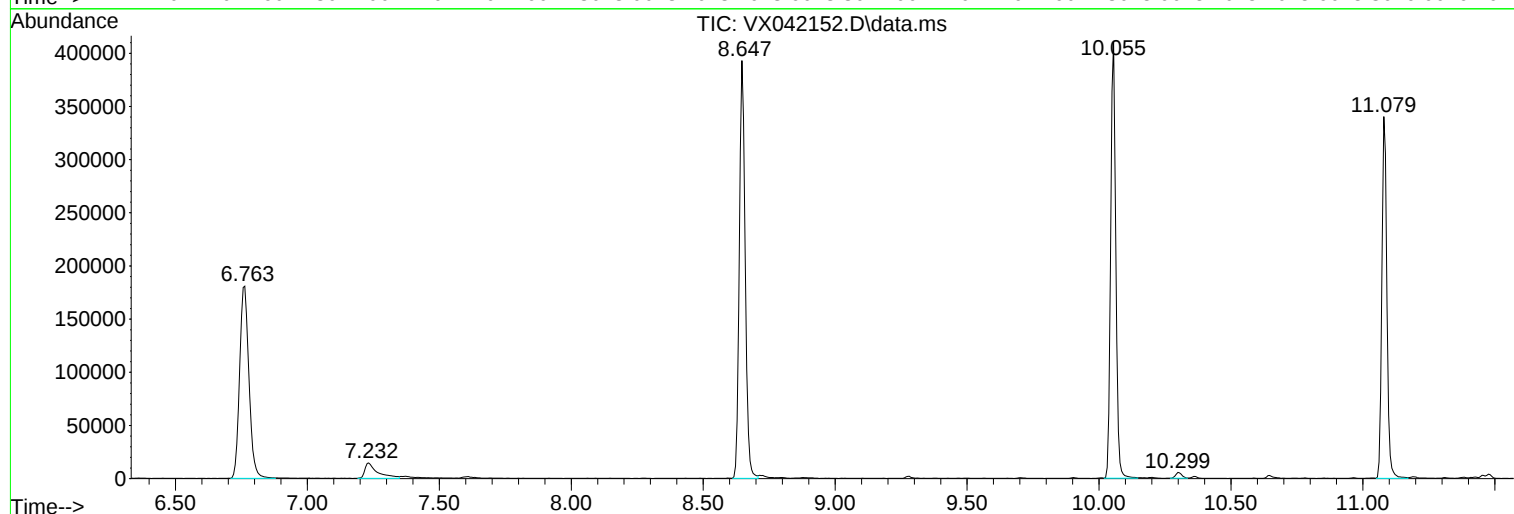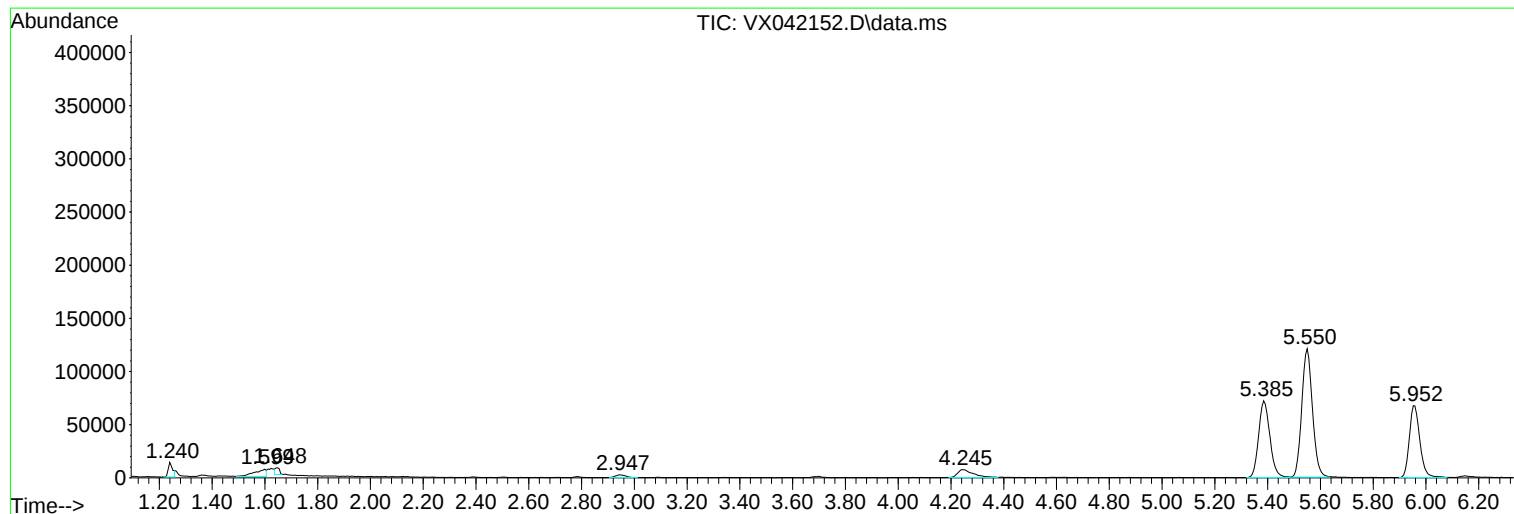

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070224\
Data File : VX042152.D
Acq On : 02 Jul 2024 20:03
Operator : JC/MD
Sample : P3106-04 20X
Misc : 5.05g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FILTER-1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Butanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.232	5.51 ug/l	48519	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Butanol	74	C4H10O	000071-36-3	78
2			Butane, 1-chloro-	92	C4H9Cl	000109-69-3	45
3			3,4-Dimethyldihydrofuran-2,5-dione	128	C6H8O3	007475-92-5	40
4			Propane, 2-cyclopropyl-	84	C6H12	003638-35-5	36
5			Oxetane, 3,3-dimethyl-	86	C5H10O	006921-35-3	36

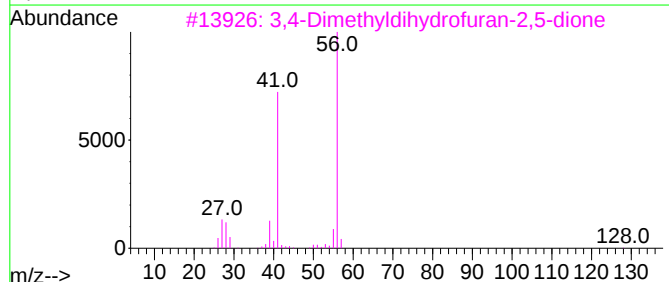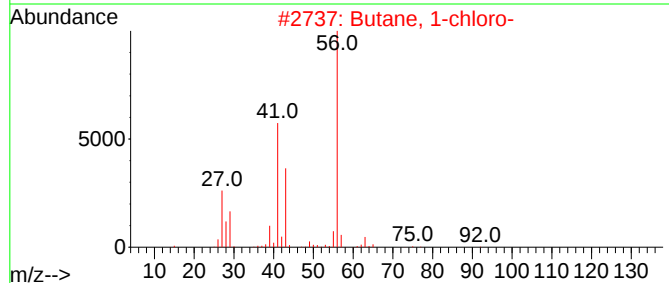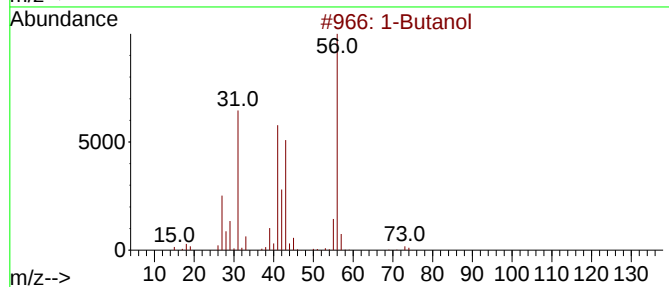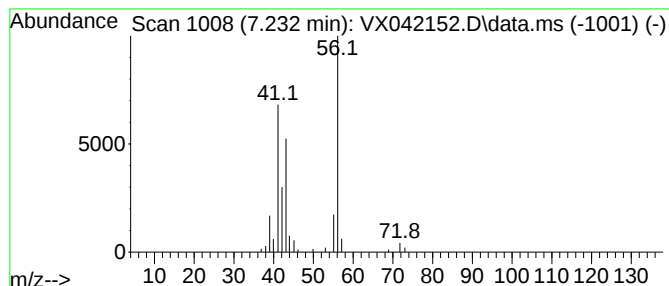

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070224\
Data File : VX042152.D
Acq On : 02 Jul 2024 20:03
Operator : JC/MD
Sample : P3106-04 20X
Misc : 5.05g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FILTER-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Butanol	7.232	5.5	ug/l	48519	2	6.763	440266	50.0