



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070224\
Data File : VX042127.D
Acq On : 02 Jul 2024 09:10
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Title : SW846 8260
Last Update : Fri Jun 21 23:51:58 2024

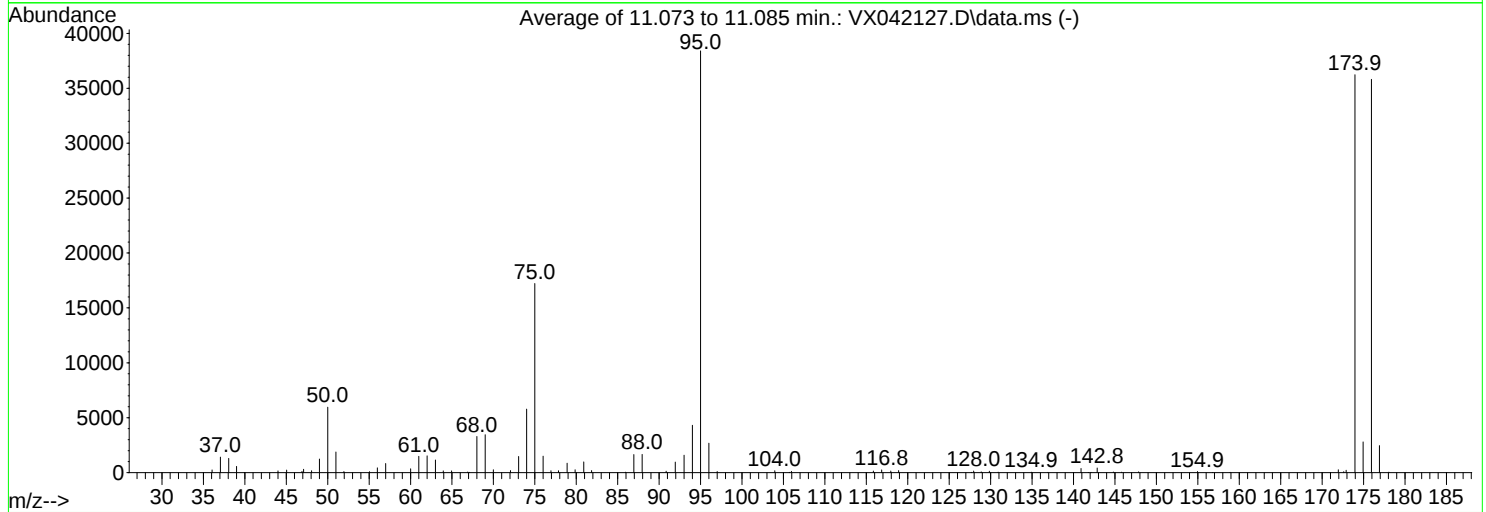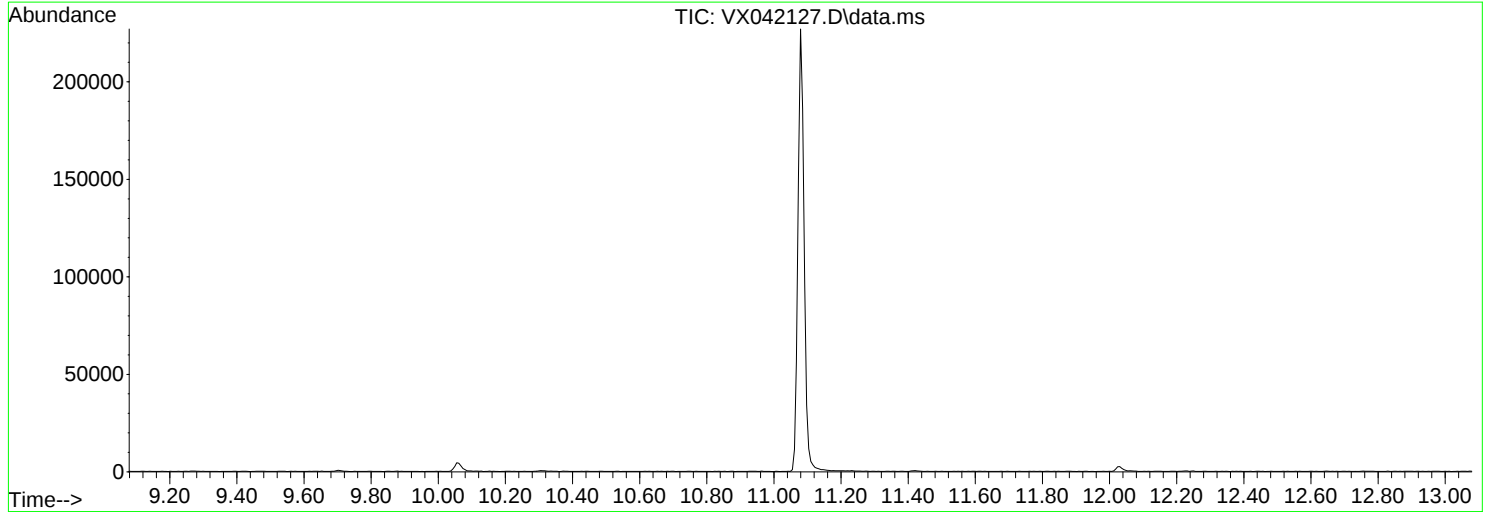

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.5	5959	PASS
75	95	30	60	44.8	17220	PASS
95	95	100	100	100.0	38408	PASS
96	95	5	9	7.0	2682	PASS
173	174	0.00	2	0.6	219	PASS
174	95	50	100	94.3	36229	PASS
175	174	5	9	7.7	2793	PASS
176	174	95	101	98.8	35811	PASS
177	176	5	9	6.9	2468	PASS