

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070225\
 Data File : VX046866.D
 Acq On : 02 Jul 2025 14:53
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Title : SW846 8260

Signal : TIC: VX046866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.397	695	707	723	rBV3	219303	695492	32.79%	5.855%
2	5.562	723	734	756	rVB	372074	1173363	55.32%	9.878%
3	5.964	790	800	825	rBV	247472	720171	33.95%	6.063%
4	6.763	921	931	950	rBV	591383	1543425	72.76%	12.993%
5	8.647	1234	1240	1258	rBV	1305705	2121181	100.00%	17.857%
6	10.055	1465	1471	1487	rBV	1292466	1866247	87.98%	15.710%
7	11.079	1633	1639	1653	rBV	1136252	1437626	67.77%	12.102%
8	11.457	1697	1701	1707	rVB3	16228	25094	1.18%	0.211%
9	11.890	1764	1772	1777	rBV	23669	28503	1.34%	0.240%
10	12.018	1788	1793	1812	rVB	1570794	1940316	91.47%	16.334%
11	12.335	1840	1845	1856	rBV2	38744	57594	2.72%	0.485%
12	13.286	1992	2001	2006	rBV2	20202	29044	1.37%	0.244%
13	13.585	2046	2050	2062	rBV3	26139	38575	1.82%	0.325%
14	13.719	2068	2072	2078	rBV2	118126	141452	6.67%	1.191%
15	13.780	2078	2082	2090	rVB	14883	23455	1.11%	0.197%
16	13.963	2106	2112	2119	rBV	25328	37461	1.77%	0.315%




Sum of corrected areas: 11878999

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070225\
Data File : VX046866.D
Acq On : 02 Jul 2025 14:53
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

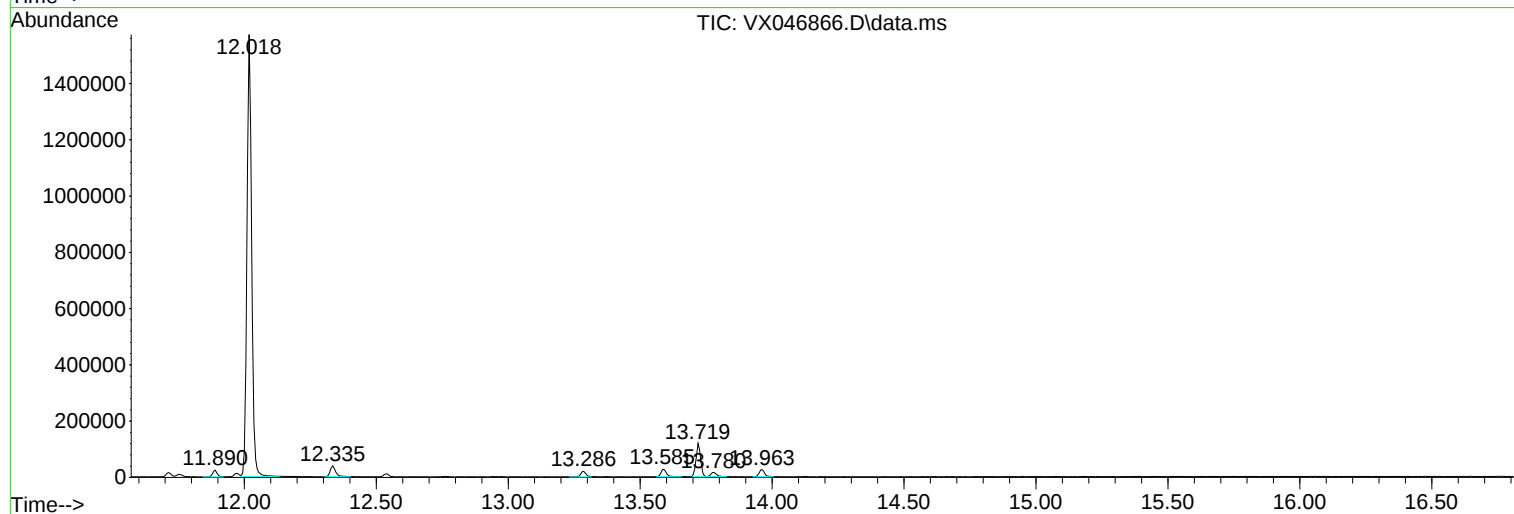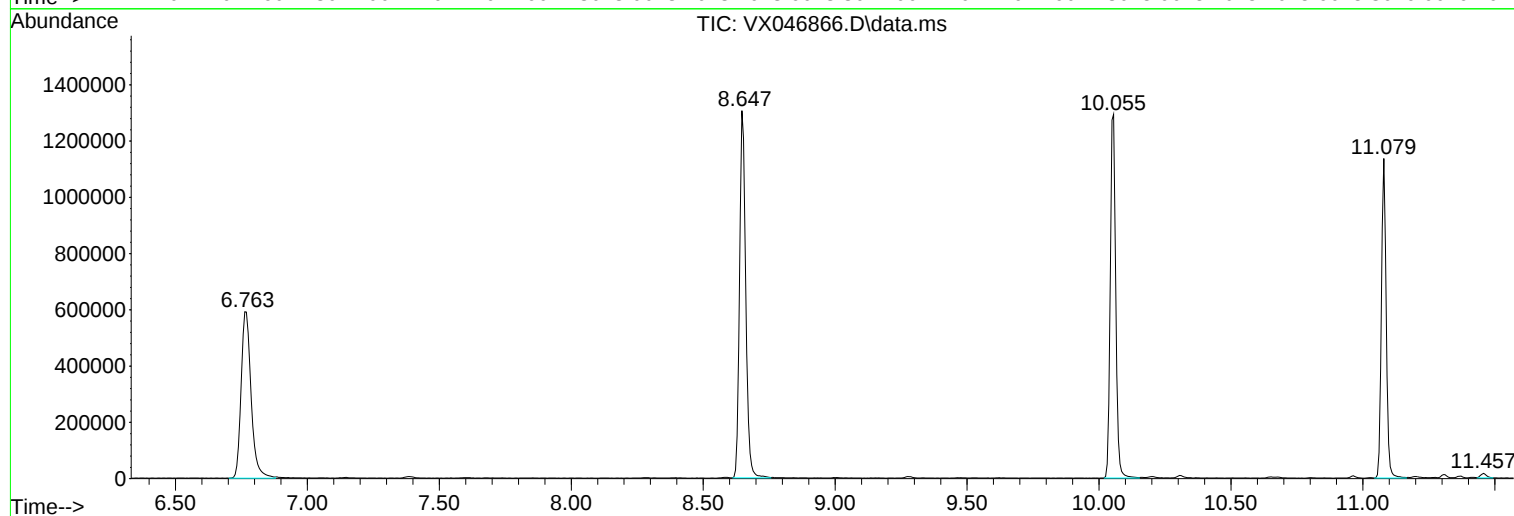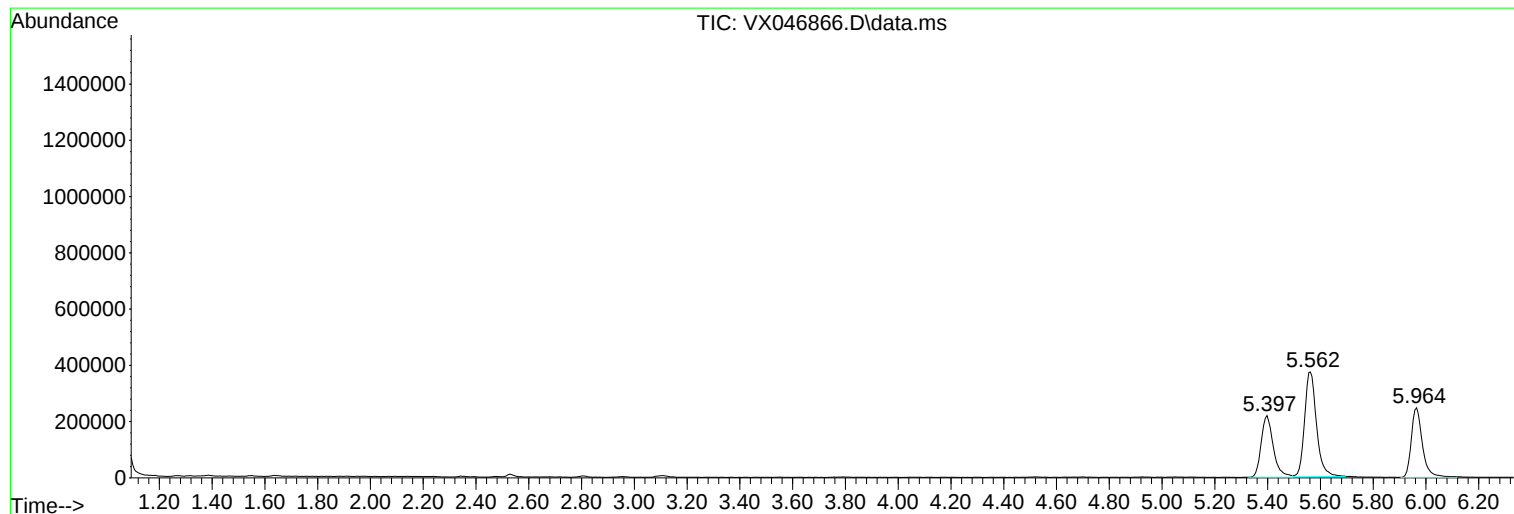

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070225\
Data File : VX046866.D
Acq On : 02 Jul 2025 14:53
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070225\
Data File : VX046866.D
Acq On : 02 Jul 2025 14:53
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc