

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070318\
 Data File : VX003156.D
 Acq On : 03 Jul 2018 18:33
 Operator : JC/MD
 Sample : J3754-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S10-0146

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	76	80	93	rBV	601784	890273	39.05%	5.818%
2	1.788	192	197	206	rVB	47177	65673	2.88%	0.429%
3	2.623	328	334	340	rVB	23830	41471	1.82%	0.271%
4	2.843	361	370	380	rBV	145083	320429	14.06%	2.094%
5	3.075	400	408	418	rVB2	44063	100052	4.39%	0.654%
6	4.300	598	609	621	rBV	54307	164908	7.23%	1.078%
7	4.550	636	650	660	rBV4	13349	54136	2.37%	0.354%
8	5.507	794	807	822	rBV	181238	509120	22.33%	3.327%
9	5.672	822	834	859	rVB2	265102	1006967	44.17%	6.581%
10	6.074	888	900	905	rBV	183000	471368	20.68%	3.080%
11	6.147	905	912	928	rVB	898940	2279696	100.00%	14.898%
12	6.348	934	945	964	rVB	85545	279224	12.25%	1.825%
13	6.867	1020	1030	1048	rBV	380259	890811	39.08%	5.822%
14	7.683	1159	1164	1173	rVB	11931	26082	1.14%	0.170%
15	7.994	1209	1215	1220	rBV	23044	46994	2.06%	0.307%
16	8.055	1220	1225	1235	rVB	73134	147272	6.46%	0.962%
17	8.183	1236	1246	1255	rBV	200138	408770	17.93%	2.671%
18	8.519	1293	1301	1312	rBV	189090	318860	13.99%	2.084%
19	8.720	1326	1334	1350	rBV	901620	1433779	62.89%	9.370%
20	9.317	1426	1432	1440	rBV	21030	33832	1.48%	0.221%
21	9.445	1447	1453	1459	rBV	49226	74345	3.26%	0.486%
22	9.525	1459	1466	1473	rBV	362816	547909	24.03%	3.581%
23	9.866	1518	1522	1527	rVB	16947	25576	1.12%	0.167%
24	10.012	1541	1546	1551	rBV	22128	31888	1.40%	0.208%
25	10.073	1551	1556	1559	rBV	259290	354303	15.54%	2.315%
26	10.116	1559	1563	1569	rVB	781262	1041550	45.69%	6.807%
27	10.366	1597	1604	1609	rVB	40424	58892	2.58%	0.385%
28	10.439	1611	1616	1621	rBV	38292	51802	2.27%	0.339%
29	11.024	1706	1712	1716	rBV	229678	300851	13.20%	1.966%
30	11.079	1716	1721	1726	rVV	108586	139175	6.10%	0.910%
31	11.140	1726	1731	1740	rVV	825500	1068458	46.87%	6.983%
32	11.219	1740	1744	1748	rBV2	17876	24589	1.08%	0.161%
33	11.366	1764	1768	1771	rVV	115592	141009	6.19%	0.922%
34	11.671	1807	1818	1822	rBV	141448	194271	8.52%	1.270%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070318\
Data File : VX003156.D
Acq On : 03 Jul 2018 18:33
Operator : JC/MD
Sample : J3754-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S10-0146

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Title : SW846 8260

35	11.768	1828	1834	1838	rVV6	11198	24987	1.10%	0.163%
36	11.811	1838	1841	1845	rVB	22392	24673	1.08%	0.161%
37	11.951	1852	1864	1872	rVB3	21992	49131	2.16%	0.321%
38	12.030	1872	1877	1880	rBV2	26743	36409	1.60%	0.238%
39	12.079	1880	1885	1892	rVB	921551	1178816	51.71%	7.704%
40	12.305	1914	1922	1930	rBV	79699	121487	5.33%	0.794%
41	12.658	1976	1980	1985	rBV2	65085	93859	4.12%	0.613%
42	12.713	1985	1989	1993	rVV4	12430	29345	1.29%	0.192%
43	12.756	1993	1996	2002	rVV2	34731	59459	2.61%	0.389%
44	12.993	2027	2035	2043	rVB4	12367	27757	1.22%	0.181%
45	13.365	2089	2096	2100	rBV7	10207	24902	1.09%	0.163%
46	13.481	2111	2115	2122	rVB	23061	30371	1.33%	0.198%
47	13.835	2168	2173	2180	rVB	41570	56376	2.47%	0.368%


Sum of corrected areas: 15301907

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070318\
Data File : VX003156.D
Acq On : 03 Jul 2018 18:33
Operator : JC/MD
Sample : J3754-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S10-0146

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

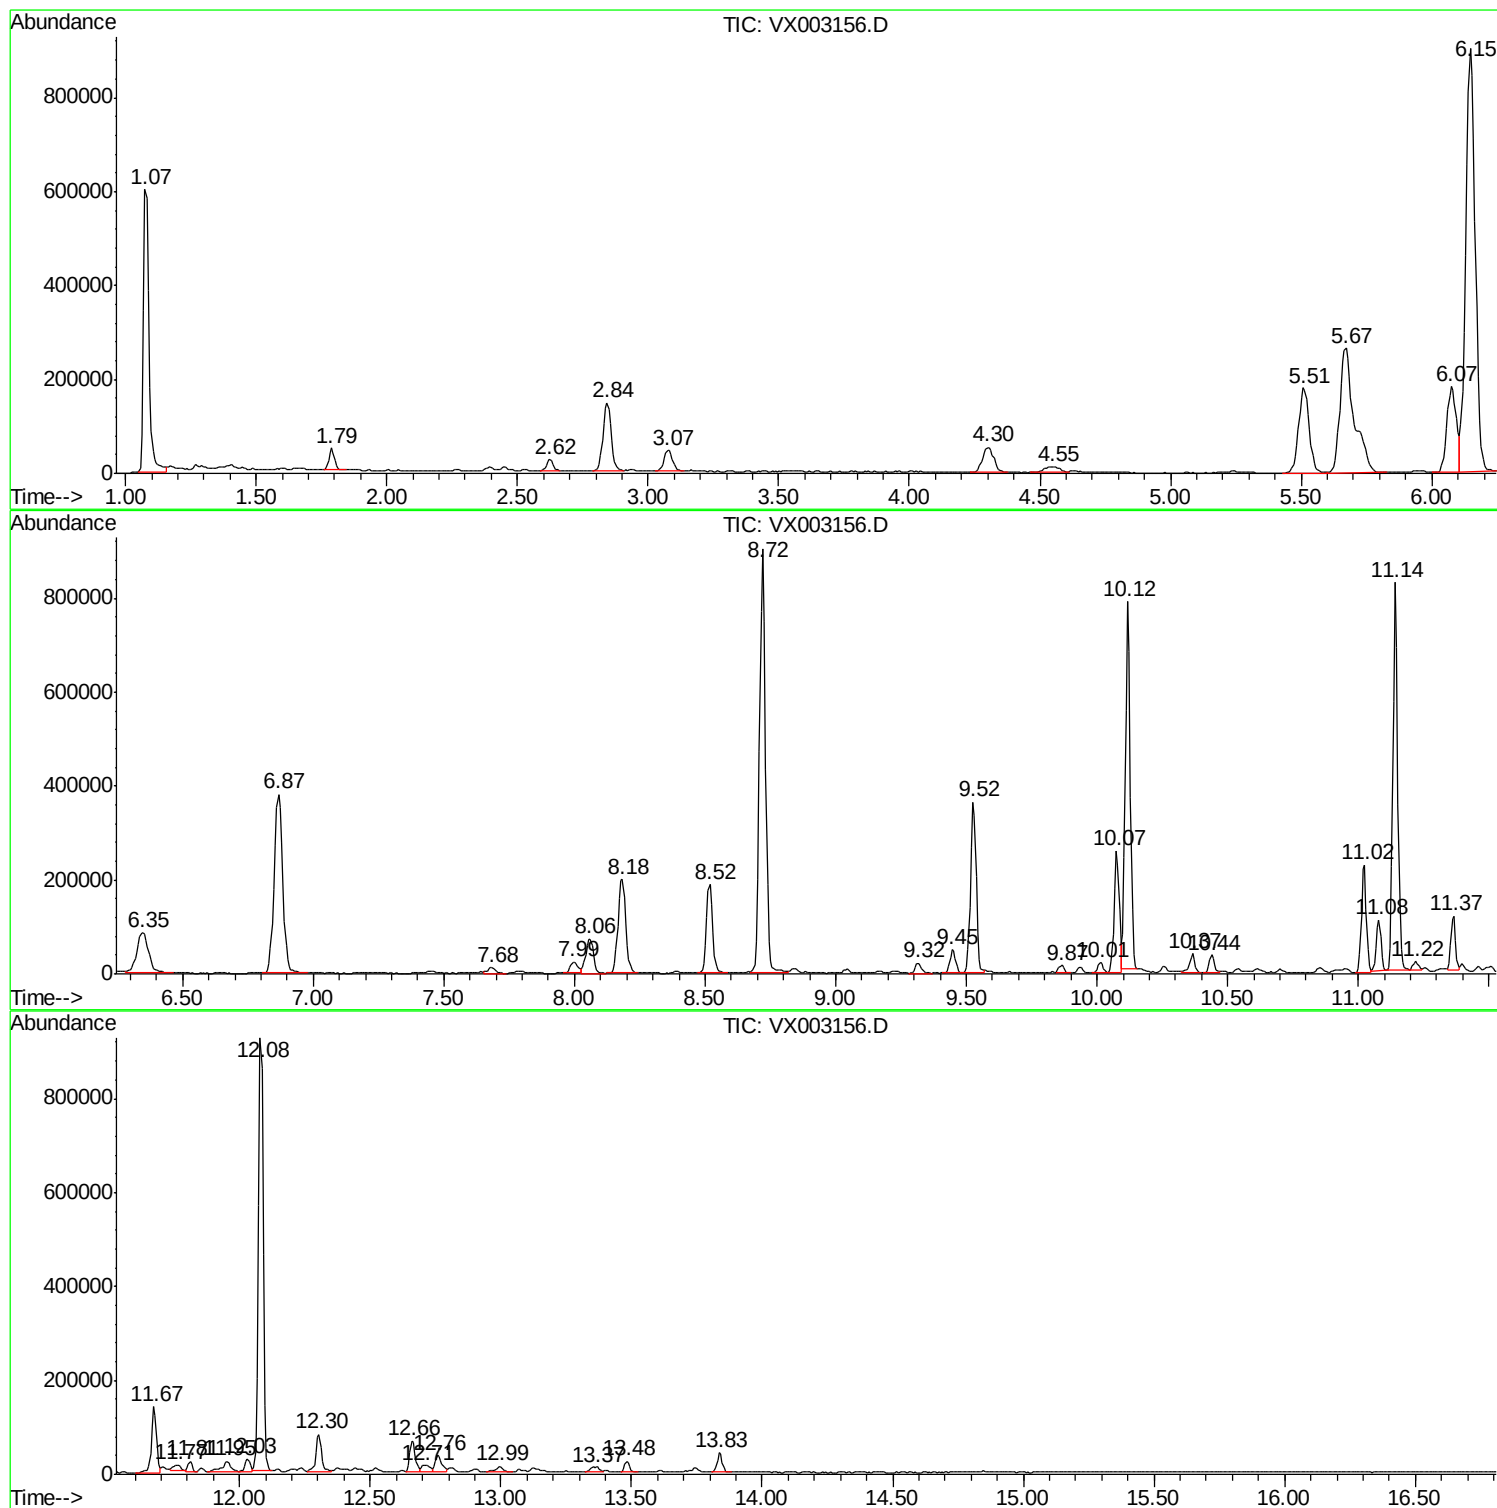

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070318\
Data File : VX003156.D
Acq On : 03 Jul 2018 18:33
Operator : JC/MD
Sample : J3754-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S10-0146

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX070318\
Data File : VX003156.D
Acq On : 03 Jul 2018 18:33
Operator : JC/MD
Sample : J3754-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S10-0146

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062518W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc