


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX070319\
Data File : VX010661.D
Acq On : 04 Jul 2019 00:38
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Title : SW846 8260
Last Update : Thu Jun 20 03:31:56 2019

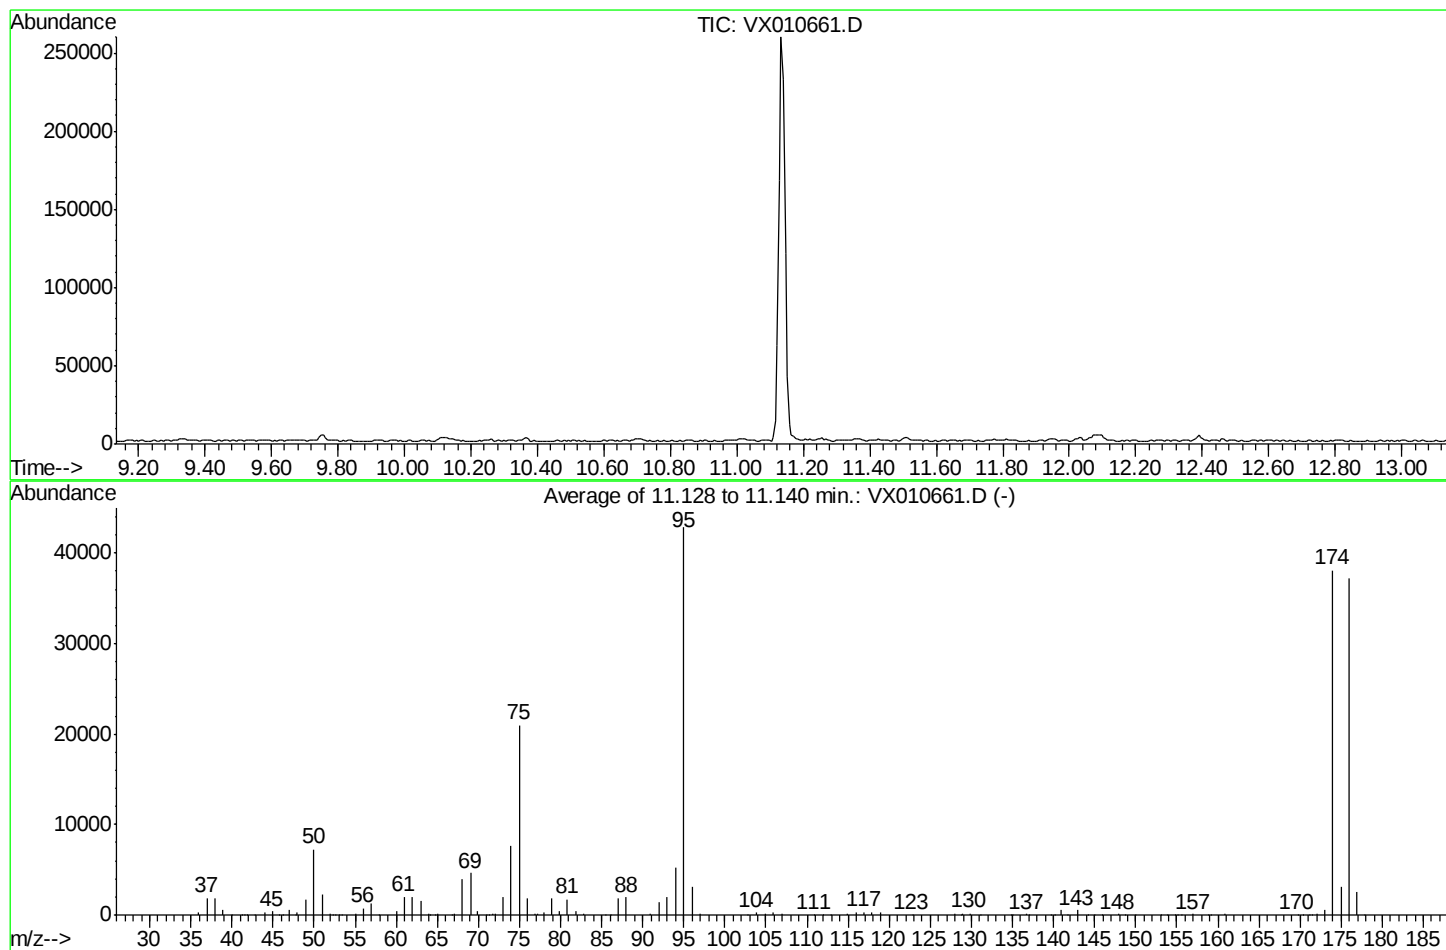

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	7256	PASS
75	95	30	60	49.0	20984	PASS
95	95	100	100	100.0	42853	PASS
96	95	5	9	7.3	3125	PASS
173	174	0.00	2	1.4	550	PASS
174	95	50	100	88.9	38090	PASS
175	174	5	9	8.3	3166	PASS
176	174	95	101	97.9	37277	PASS
177	176	5	9	6.8	2528	PASS